

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060617\
 Data File : BF095701.D
 Acq On : 6 Jun 2017 10:51
 Operator : SJ/MA
 Sample : I3441-08
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-RO-6710-060117

Quant Time: Jun 06 16:29:42 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:15:31 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	84737	20.00	ng	-0.02
21) Naphthalene-d8	9.41	136	349740	20.00	ng	-0.02
38) Acenaphthene-d10	12.23	164	164923	20.00	ng	-0.02
63) Phenanthrene-d10	14.63	188	320167	20.00	ng	-0.02
75) Chrysene-d12	18.34	240	281739	20.00	ng	-0.02
86) Perylene-d12	20.01	264	200033	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	772961	145.35	ng	0.00
7) Phenol-d6	6.94	99	752585	118.21	ng	-0.02
23) Nitrobenzene-d5	8.30	82	491317	87.25	ng	-0.02
41) 2,4,6-Tribromophenol	13.53	330	203375	139.38	ng	-0.02
44) 2-Fluorobiphenyl	11.19	172	994581	83.92	ng	-0.02
78) Terphenyl-d14	17.01	244	960491	84.61	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	8.30	70	62208	15.42	ng	# 73
31) Naphthalene	9.44	128	194167	11.06	ng	99
32) Benzoic acid	9.44	122	499	5.26	ng	# 1
33) 4-Chloroaniline	9.44	127	25929	3.78	ng	# 31
37) 2-Methylnaphthalene	10.58	142	24688	2.08	ng	96
50) 2,6-Dinitrotoluene	12.23	165	21735	7.96	ng	# 31
55) 4-Nitrophenol	12.60	139	1164	5.22	ng	# 25

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060617\
Data File : BF095701.D
Acq On : 6 Jun 2017 10:51
Operator : SJ/MA
Sample : I3441-08
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-RO-6710-060117

Quant Time: Jun 06 16:29:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

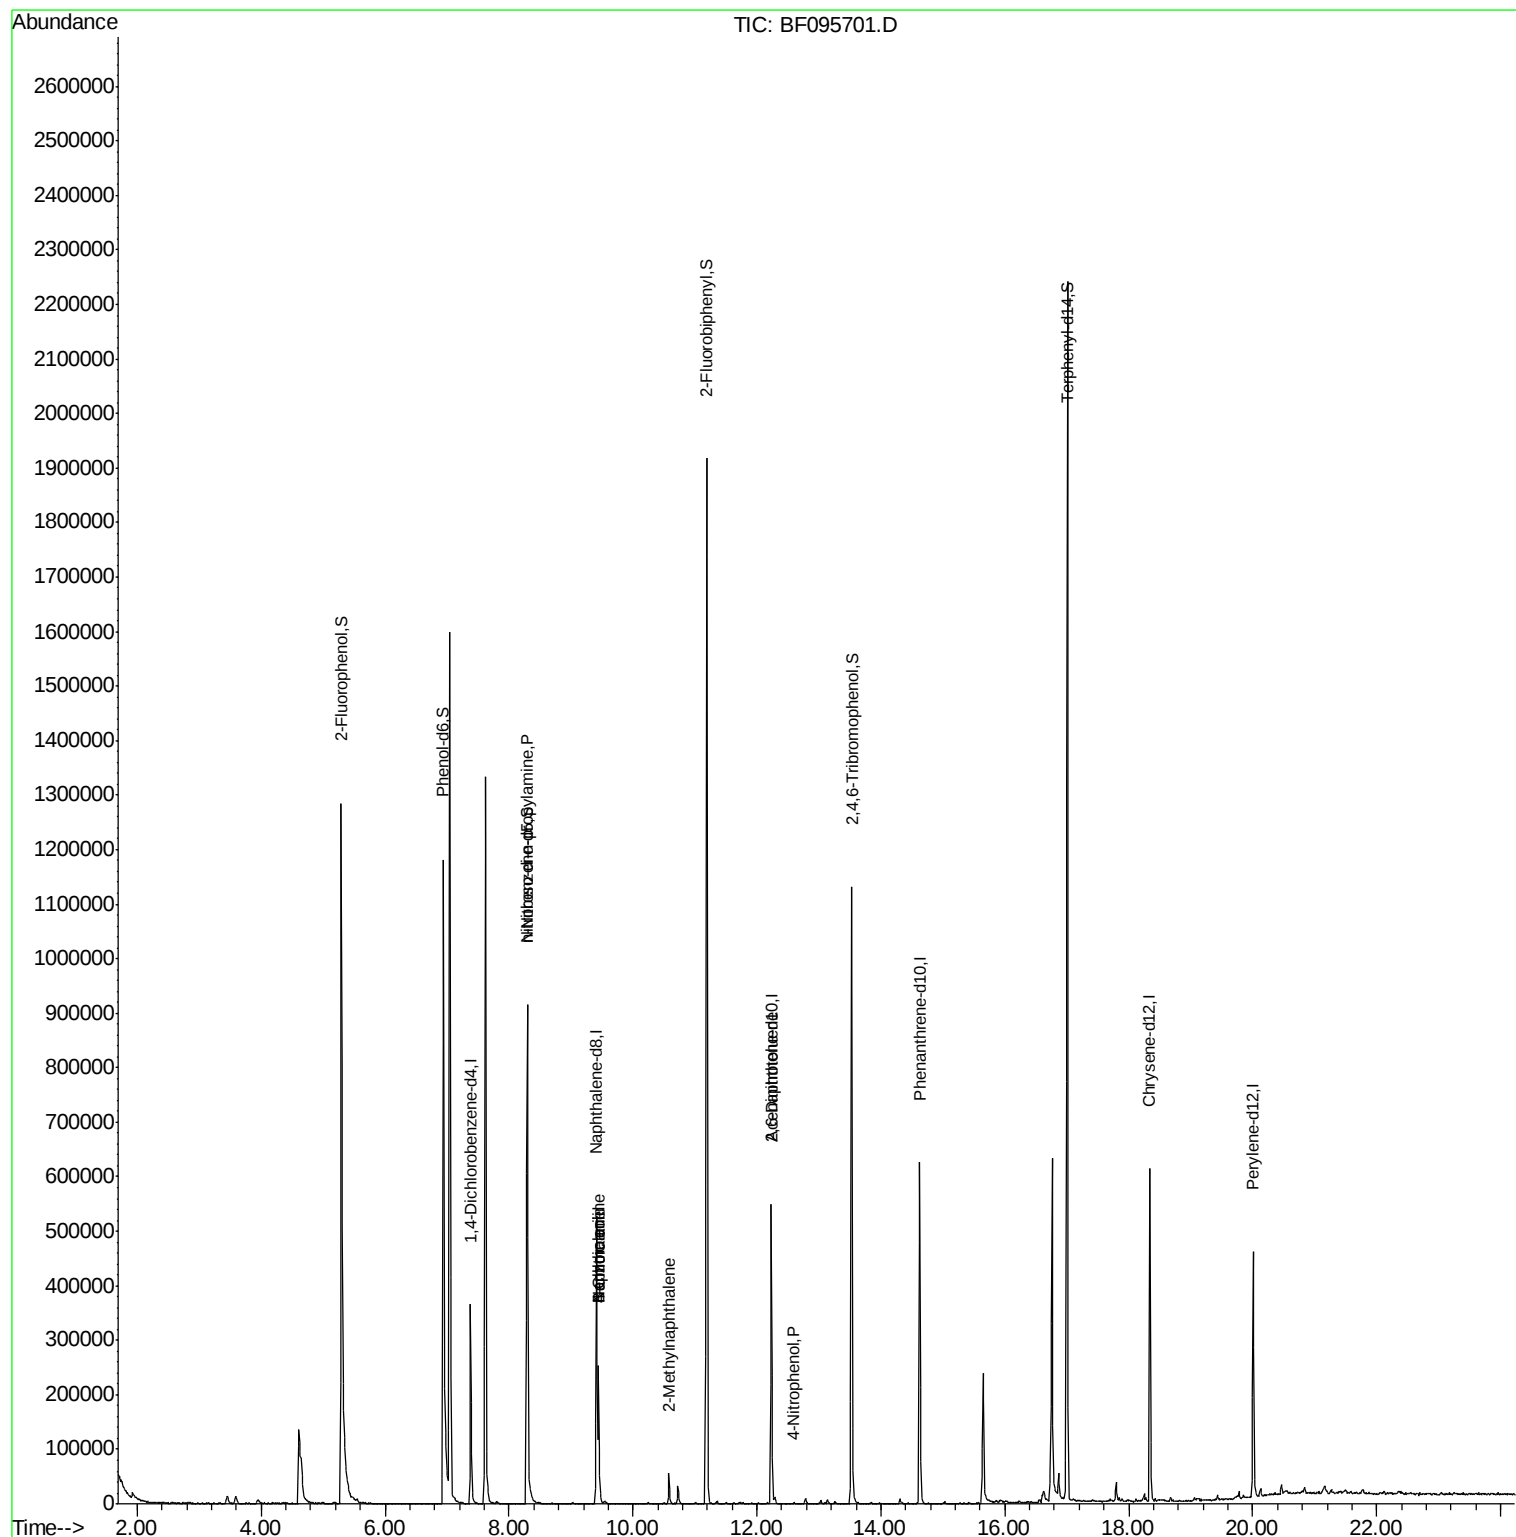




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.38 min Scan# 968
Delta R.T. -0.02 min
Lab File: BF095701.D
Acq: 6 Jun 2017 10:51

Instrument :
BNA_F
ClientSampleId :
OR-RO-6710-060117

Tot Ion:152 Resp: 84737
Ion Ratio Lower Upper
152 100
150 165.0 126.2 189.2
115 64.3 52.2 78.2

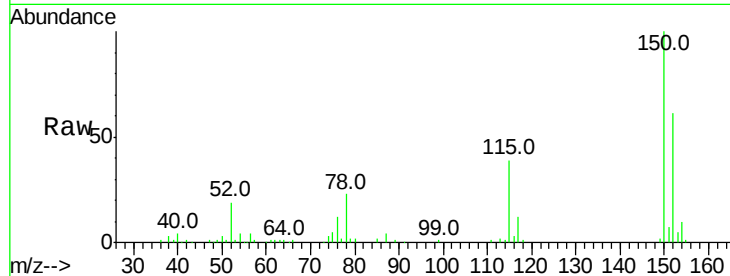


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

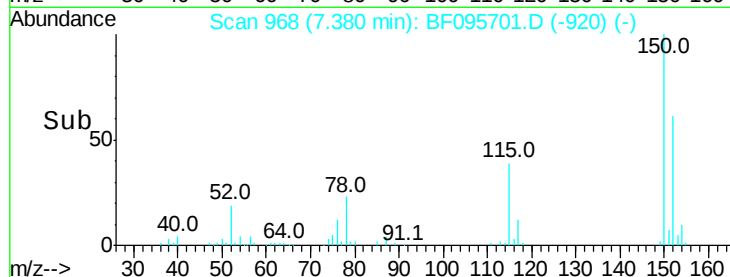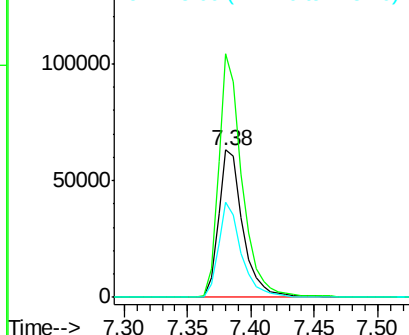



#5


2-Fluorophenol
Concen: 145.35 ng
RT: 5.29 min Scan# 613
Delta R.T. 0.01 min
Lab File: BF095701.D
Acq: 6 Jun 2017 10:51

Tgt Ion:112 Resp: 772961
Ion Ratio Lower Upper
112 100
64 56.3 46.0 69.0
63 27.1 23.4 35.0

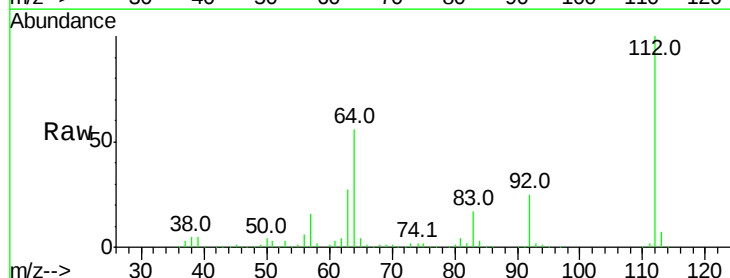

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

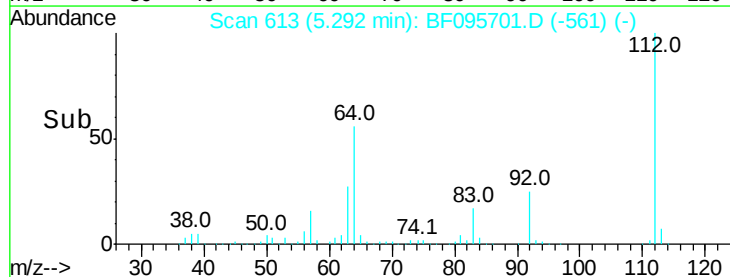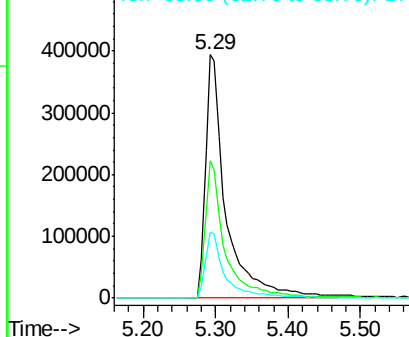

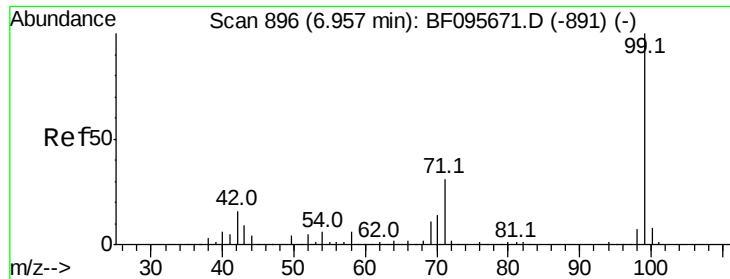

#7

Phenol-d6

Concen: 118.21 ng

RT: 6.94 min Scan# 893

Delta R.T. -0.02 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51

Instrument :

BNA_F

ClientSampleId :

OR-RO-6710-060117


Tot Ion: 99 Resp: 752585

Ion Ratio Lower Upper

99 100

42 16.0 13.5 20.3




71 32.5 24.5 36.7

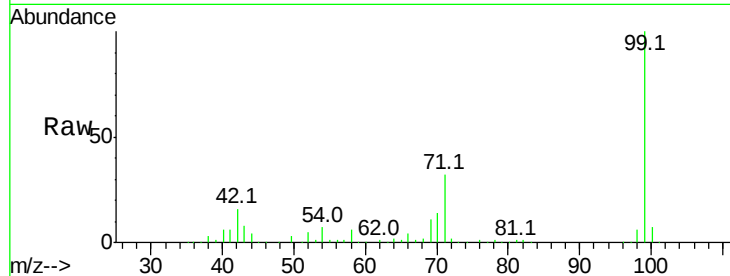

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

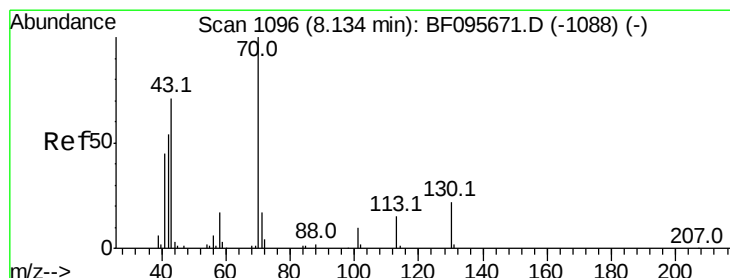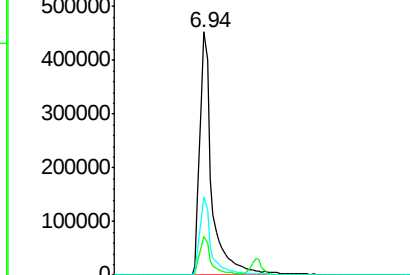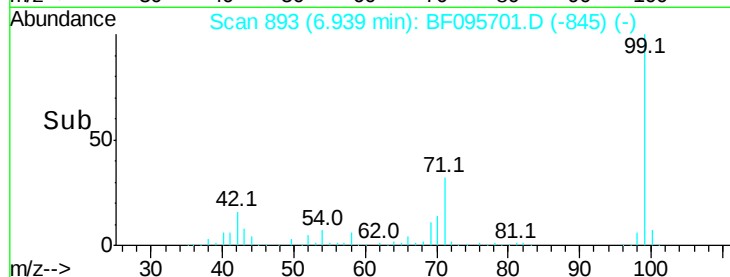

#19

n-Nitroso-di-n-propylamine

Concen: 15.42 ng

RT: 8.30 min Scan# 1124

Delta R.T. 0.16 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51

Tgt Ion: 70 Resp: 62208


Ion Ratio Lower Upper

70 100

42 41.4 47.2 70.8#

101 0.0 7.2 10.8#

130 1.9 15.9 23.9#


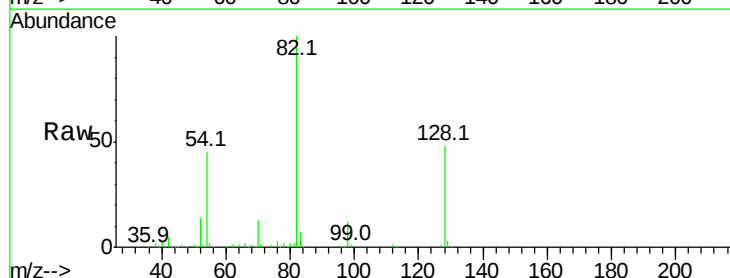


Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

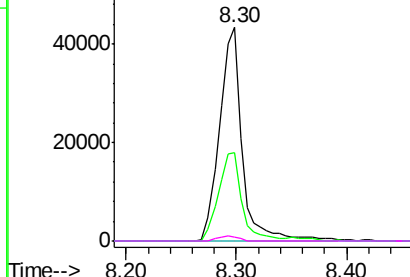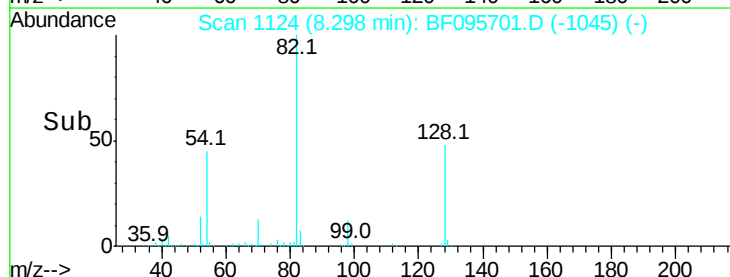



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.41 min Scan# 1313

Delta R.T. -0.02 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51

Instrument :

BNA_F

ClientSampleId :

OR-RO-6710-060117

Tot Ion:136 Resp: 349740


Ion Ratio Lower Upper

136 100

137 11.4 8.5 12.7

54 6.8 4.9 7.3

68 5.6 4.1 6.1



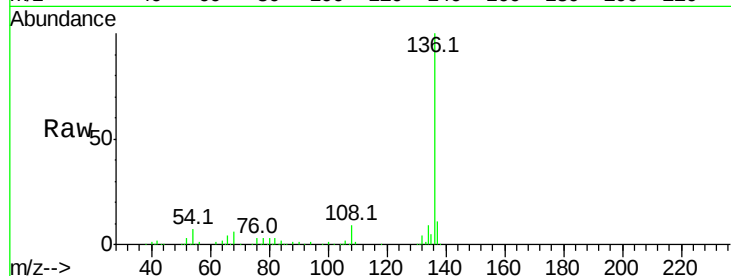


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

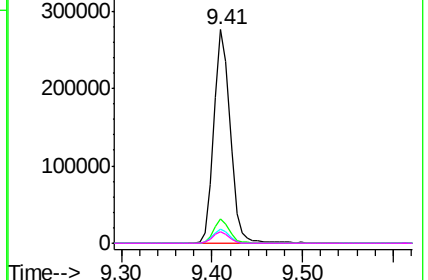

#23

Nitrobenzene-d5

Concen: 87.25 ng

RT: 8.30 min Scan# 1124

Delta R.T. -0.02 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51


Tgt Ion: 82 Resp: 491317

Ion Ratio Lower Upper

82 100

128 48.5 34.0 51.0



54 45.0 42.2 63.2




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

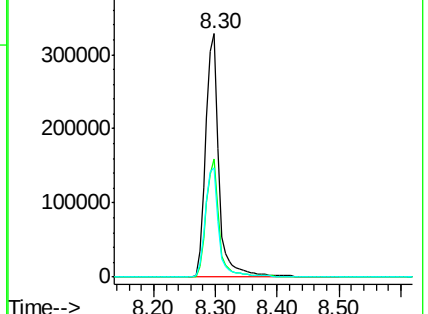


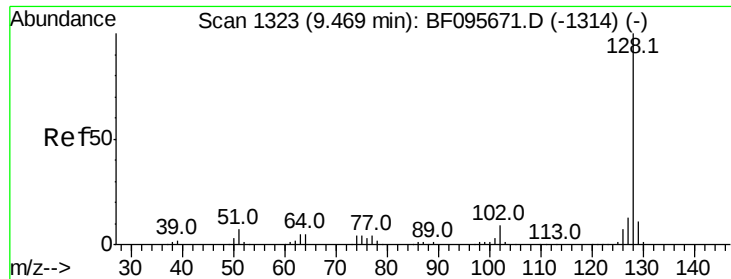




#31
Naphthalene
Concen: 11.06 ng
RT: 9.44 min Scan# 1319
Delta R.T. -0.02 min
Lab File: BF095701.D
Acq: 6 Jun 2017 10:51

Instrument :
BNA_F
ClientSampleId :
OR-RO-6710-060117

Tot Ion:128 Resp: 194167
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.6
127 13.1 10.8 16.2

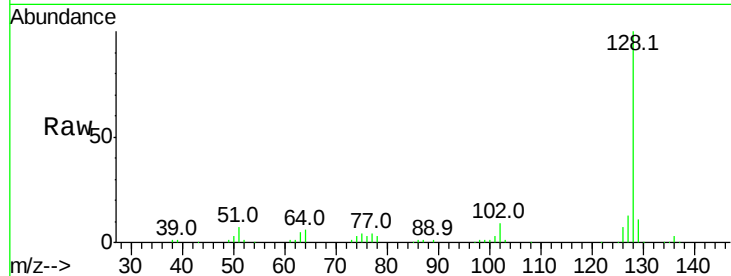


Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

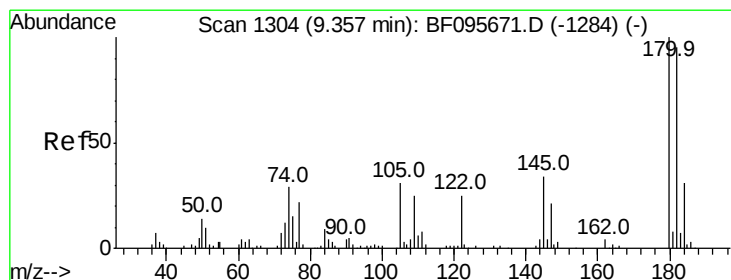
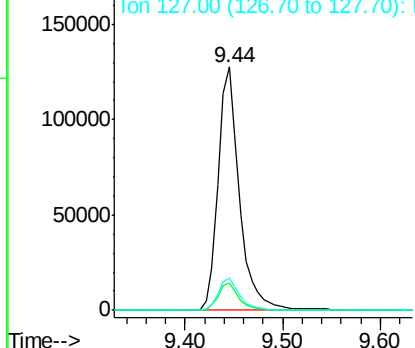



#32
Benzoic acid
Concen: 5.26 ng
RT: 9.44 min Scan# 1318
Delta R.T. 0.08 min
Lab File: BF095701.D
Acq: 6 Jun 2017 10:51

Tgt Ion:122 Resp: 499
Ion Ratio Lower Upper
122 100
105 0.0 103.3 143.3#
77 1175.5 73.7 113.7#



Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF0



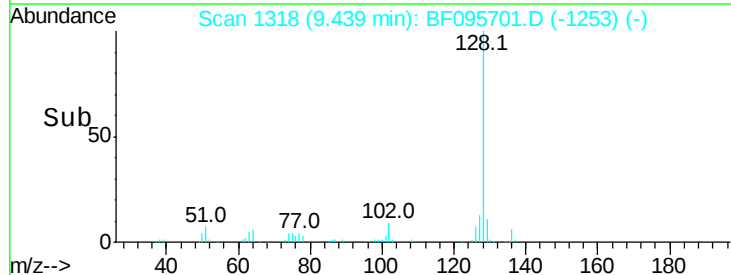
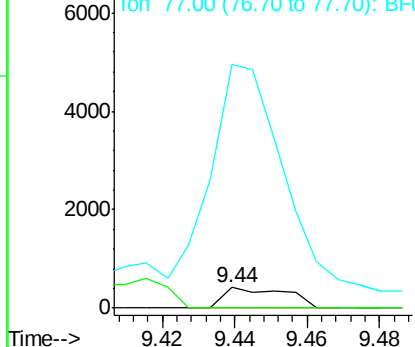


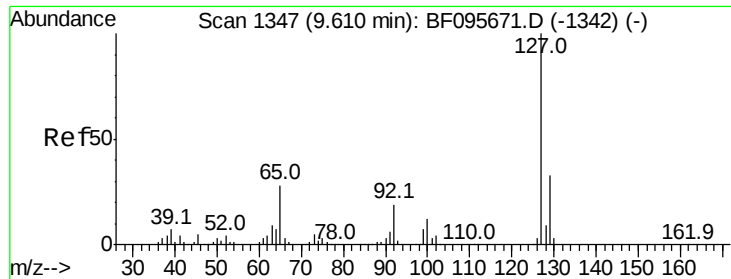

#33
4-Chloroaniline
Concen: 3.78 ng
RT: 9.44 min Scan# 1319
Delta R.T. -0.16 min
Lab File: BF095701.D
Acq: 6 Jun 2017 10:51




Instrument :
BNA_F
ClientSampleId :
OR-RO-6710-060117


Tot Ion:127 Resp: 25929
Ion Ratio Lower Upper
127 100
129 85.2 26.2 39.2#
65 0.0 27.8 41.8#
92 0.0 16.8 25.2#

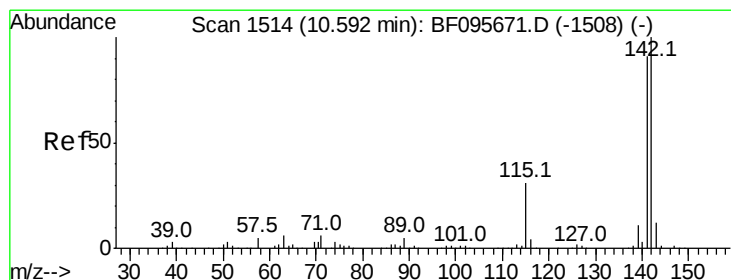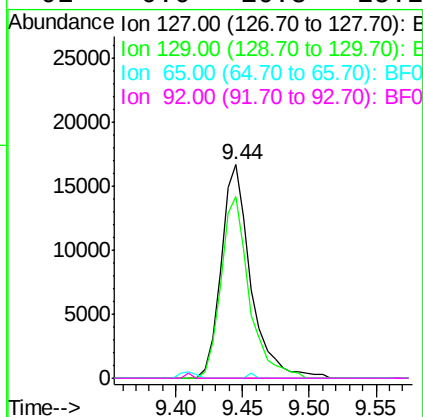

#37
2-Methylnaphthalene
Concen: 2.08 ng
RT: 10.58 min Scan# 1512
Delta R.T. -0.01 min
Lab File: BF095701.D
Acq: 6 Jun 2017 10:51

Tgt Ion:142 Resp: 24688
Ion Ratio Lower Upper
142 100
141 86.2 71.3 106.9
115 30.3 27.1 40.7

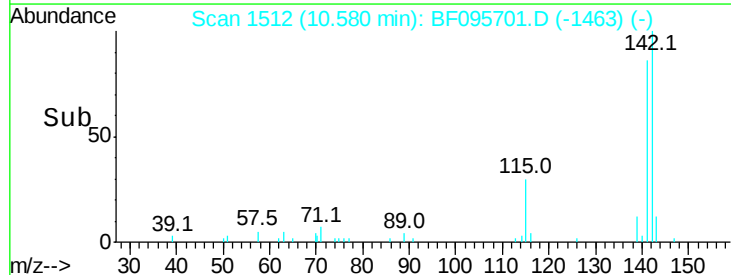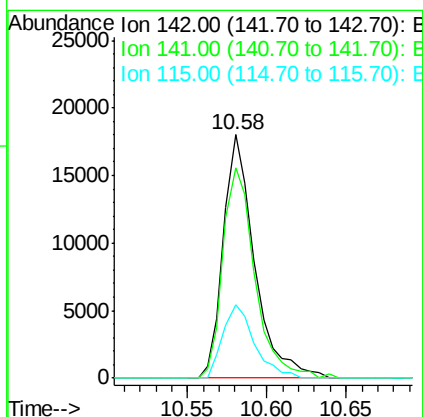

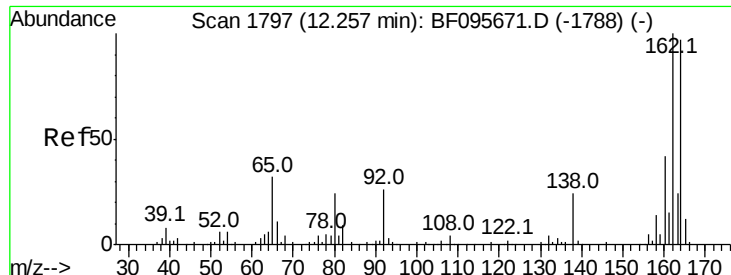

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.23 min Scan# 1793

Delta R.T. -0.02 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51

Instrument :

BNA_F

ClientSampleId :

OR-RO-6710-060117


Tot Ion:164 Resp: 164923

Ion Ratio Lower Upper

164 100

162 103.9 82.6 123.8




160 44.2 36.2 54.2

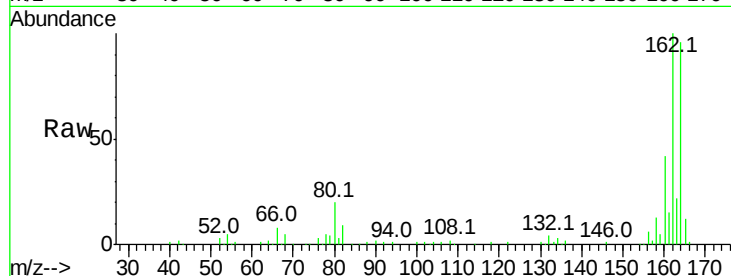

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

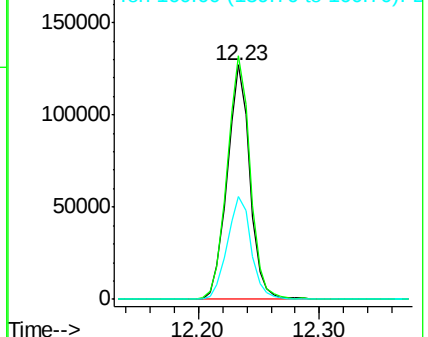

#41

2,4,6-Tribromophenol

Concen: 139.38 ng

RT: 13.53 min Scan# 2014

Delta R.T. -0.02 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51


Tgt Ion:330 Resp: 203375

Ion Ratio Lower Upper

330 100

332 96.0 76.6 115.0



141 38.0 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



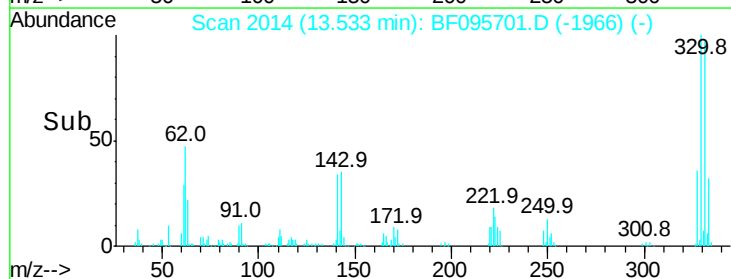
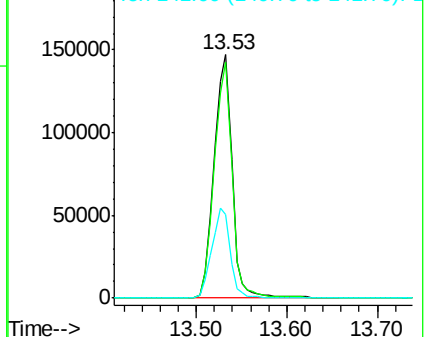


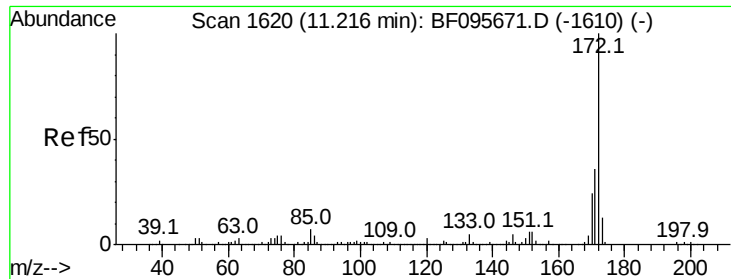

#44
 2-Fluorobiphenyl
 Concen: 83.92 ng
 RT: 11.19 min Scan# 1616
 Delta R.T. -0.02 min
 Lab File: BF095701.D
 Acq: 6 Jun 2017 10:51




Instrument :
 BNA_F
 ClientSampleId :
 OR-RO-6710-060117


Tot Ion:172 Resp: 994581
 Ion Ratio Lower Upper
 172 100
 171 35.8 29.6 44.4
 170 23.5 19.8 29.8

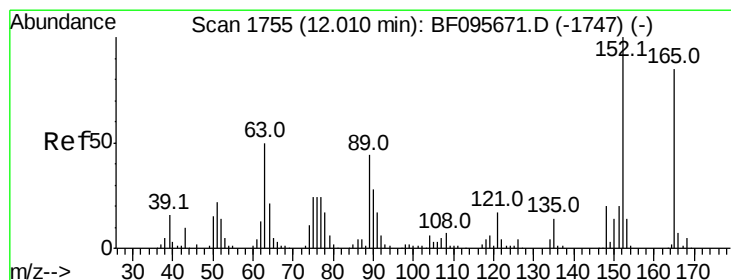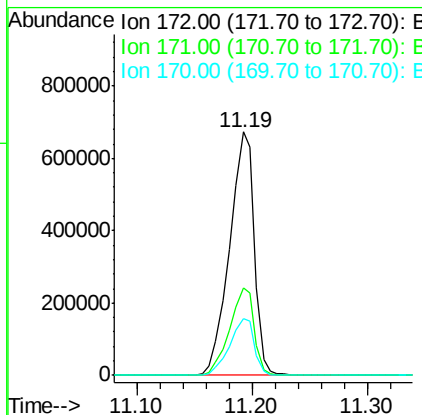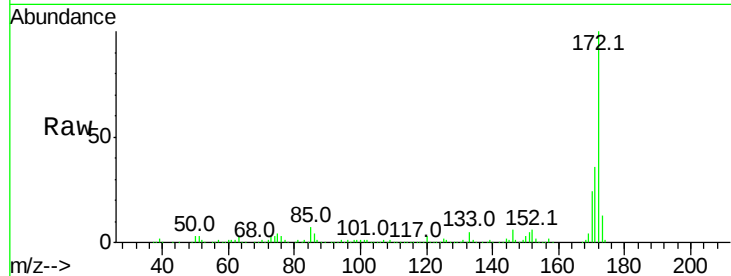

#50
 2,6-Dinitrotoluene
 Concen: 7.96 ng
 RT: 12.23 min Scan# 1793
 Delta R.T. 0.22 min
 Lab File: BF095701.D
 Acq: 6 Jun 2017 10:51

Tgt Ion:165 Resp: 21735
 Ion Ratio Lower Upper
 165 100
 63 0.0 34.3 51.5#
 89 0.0 37.1 55.7#

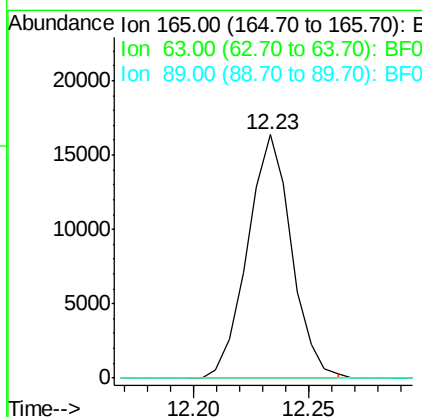

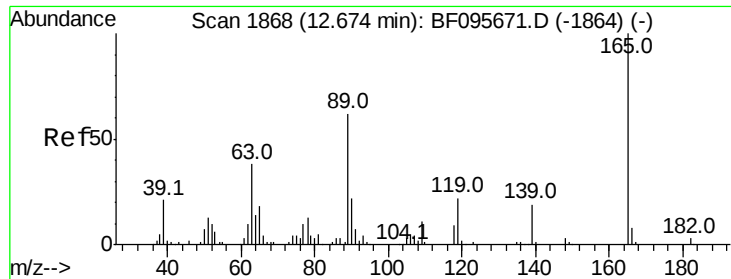

#55

4-Nitrophenol

Concen: 5.22 ng

RT: 12.60 min Scan# 1855

Delta R.T. -0.08 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51

Instrument :

BNA_F

ClientSampleId :

OR-RO-6710-060117


Tot Ion:139 Resp: 1164

Ion Ratio Lower Upper

139 100

109 0.0 34.1 74.1#


65 0.0 31.4 71.4#

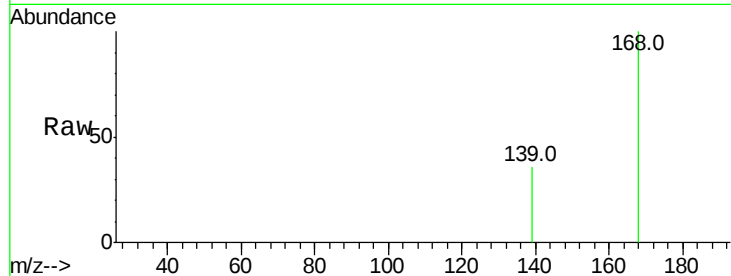



Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BF0

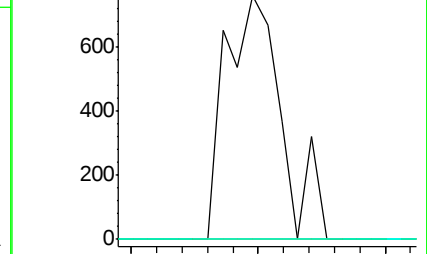

Time-->



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.63 min Scan# 2200

Delta R.T. -0.02 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51


Tgt Ion:188 Resp: 320167

Ion Ratio Lower Upper

188 100

94 10.2 9.4 14.2


80 10.5 10.2 15.2




Abundance Ion 188.00 (187.70 to 188.70): E


Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

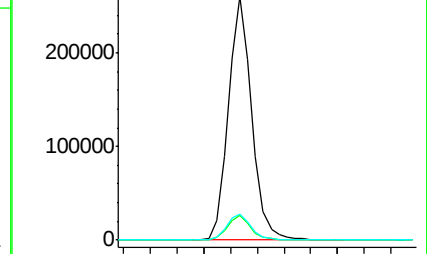

Time-->



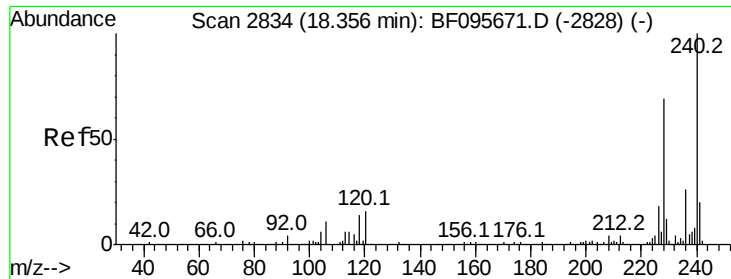

#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.34 min Scan# 2831

Delta R.T. -0.02 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51

Instrument :

BNA_F

ClientSampleId :

OR-RO-6710-060117


Tot Ion:240 Resp: 281739

Ion Ratio Lower Upper

240 100

120 14.5 5.8 8.8#




236 25.1 20.5 30.7

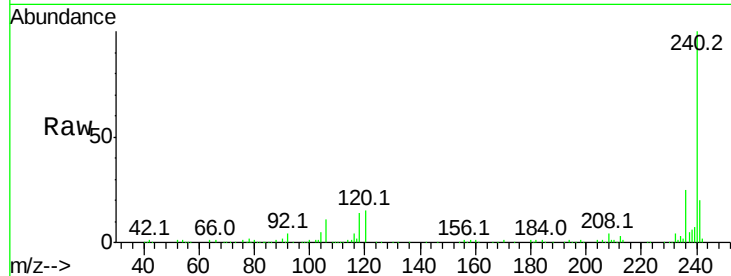

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

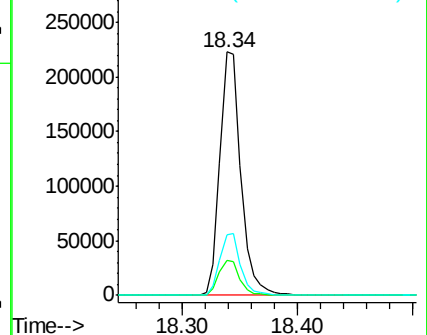

#78

Terphenyl-d14

Concen: 84.61 ng

RT: 17.01 min Scan# 2605

Delta R.T. -0.01 min

Lab File: BF095701.D

Acq: 6 Jun 2017 10:51


Tgt Ion:244 Resp: 960491

Ion Ratio Lower Upper

244 100

212 6.9 6.0 9.0



122 14.4 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

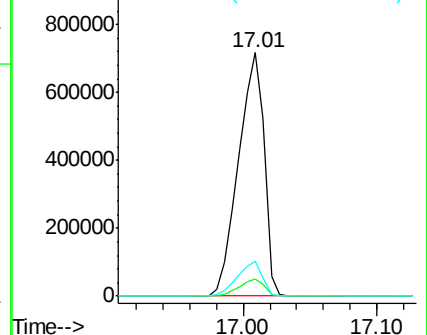

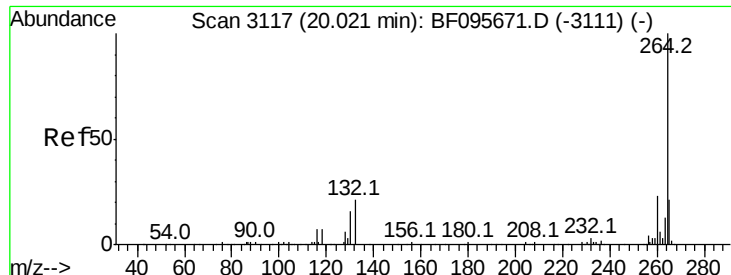

#86

Pervlene-d12

Concen: 20.00 ng

RT: 20.01 min Scan# 3115

Delta R.T. -0.01 min

Lab File: BF095701.D


Acq: 6 Jun 2017 10:51

Instrument :

BNA_F

ClientSampleId :

OR-RO-6710-060117




Tot Ion:264 Resp: 200033

Ion Ratio Lower Upper

264 100

260 22.7 19.5 29.3

265 20.8 17.2 25.8

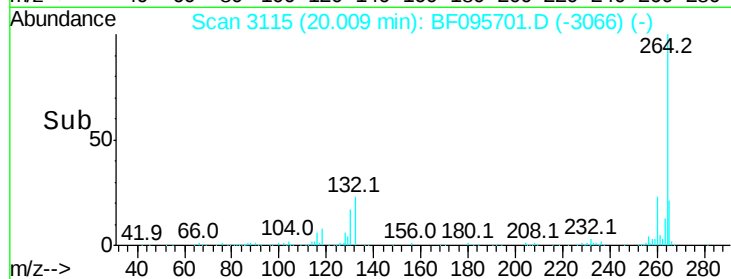

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

