

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060617\
 Data File : BF095707.D
 Acq On : 6 Jun 2017 14:04
 Operator : SJ/MA
 Sample : I3444-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jun 06 16:30:41 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:15:31 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	88345	20.00	ng	-0.01
21) Naphthalene-d8	9.41	136	373615	20.00	ng	-0.02
38) Acenaphthene-d10	12.23	164	168496	20.00	ng	-0.02
63) Phenanthrene-d10	14.63	188	326975	20.00	ng	-0.02
75) Chrysene-d12	18.34	240	337933	20.00	ng	-0.02
86) Perylene-d12	20.01	264	237771	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	798069	143.95	ng	0.00
7) Phenol-d6	6.94	99	797477	120.15	ng	-0.02
23) Nitrobenzene-d5	8.30	82	554999	92.26	ng	-0.02
41) 2,4,6-Tribromophenol	13.53	330	222782	149.44	ng	-0.02
44) 2-Fluorobiphenyl	11.19	172	1272193	105.07	ng	-0.02
78) Terphenyl-d14	17.01	244	1089184	79.99	ng	0.00
Target Compounds						
15) Benzyl Alcohol	7.62	79	10239	2.25	ng	# 41
19) n-Nitroso-di-n-propylamine	8.30	70	68981	16.40	ng	# 75
50) 2,6-Dinitrotoluene	12.23	165	21264	7.62	ng	# 31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060617\
Data File : BF095707.D
Acq On : 6 Jun 2017 14:04
Operator : SJ/MA
Sample : I3444-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jun 06 16:30:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

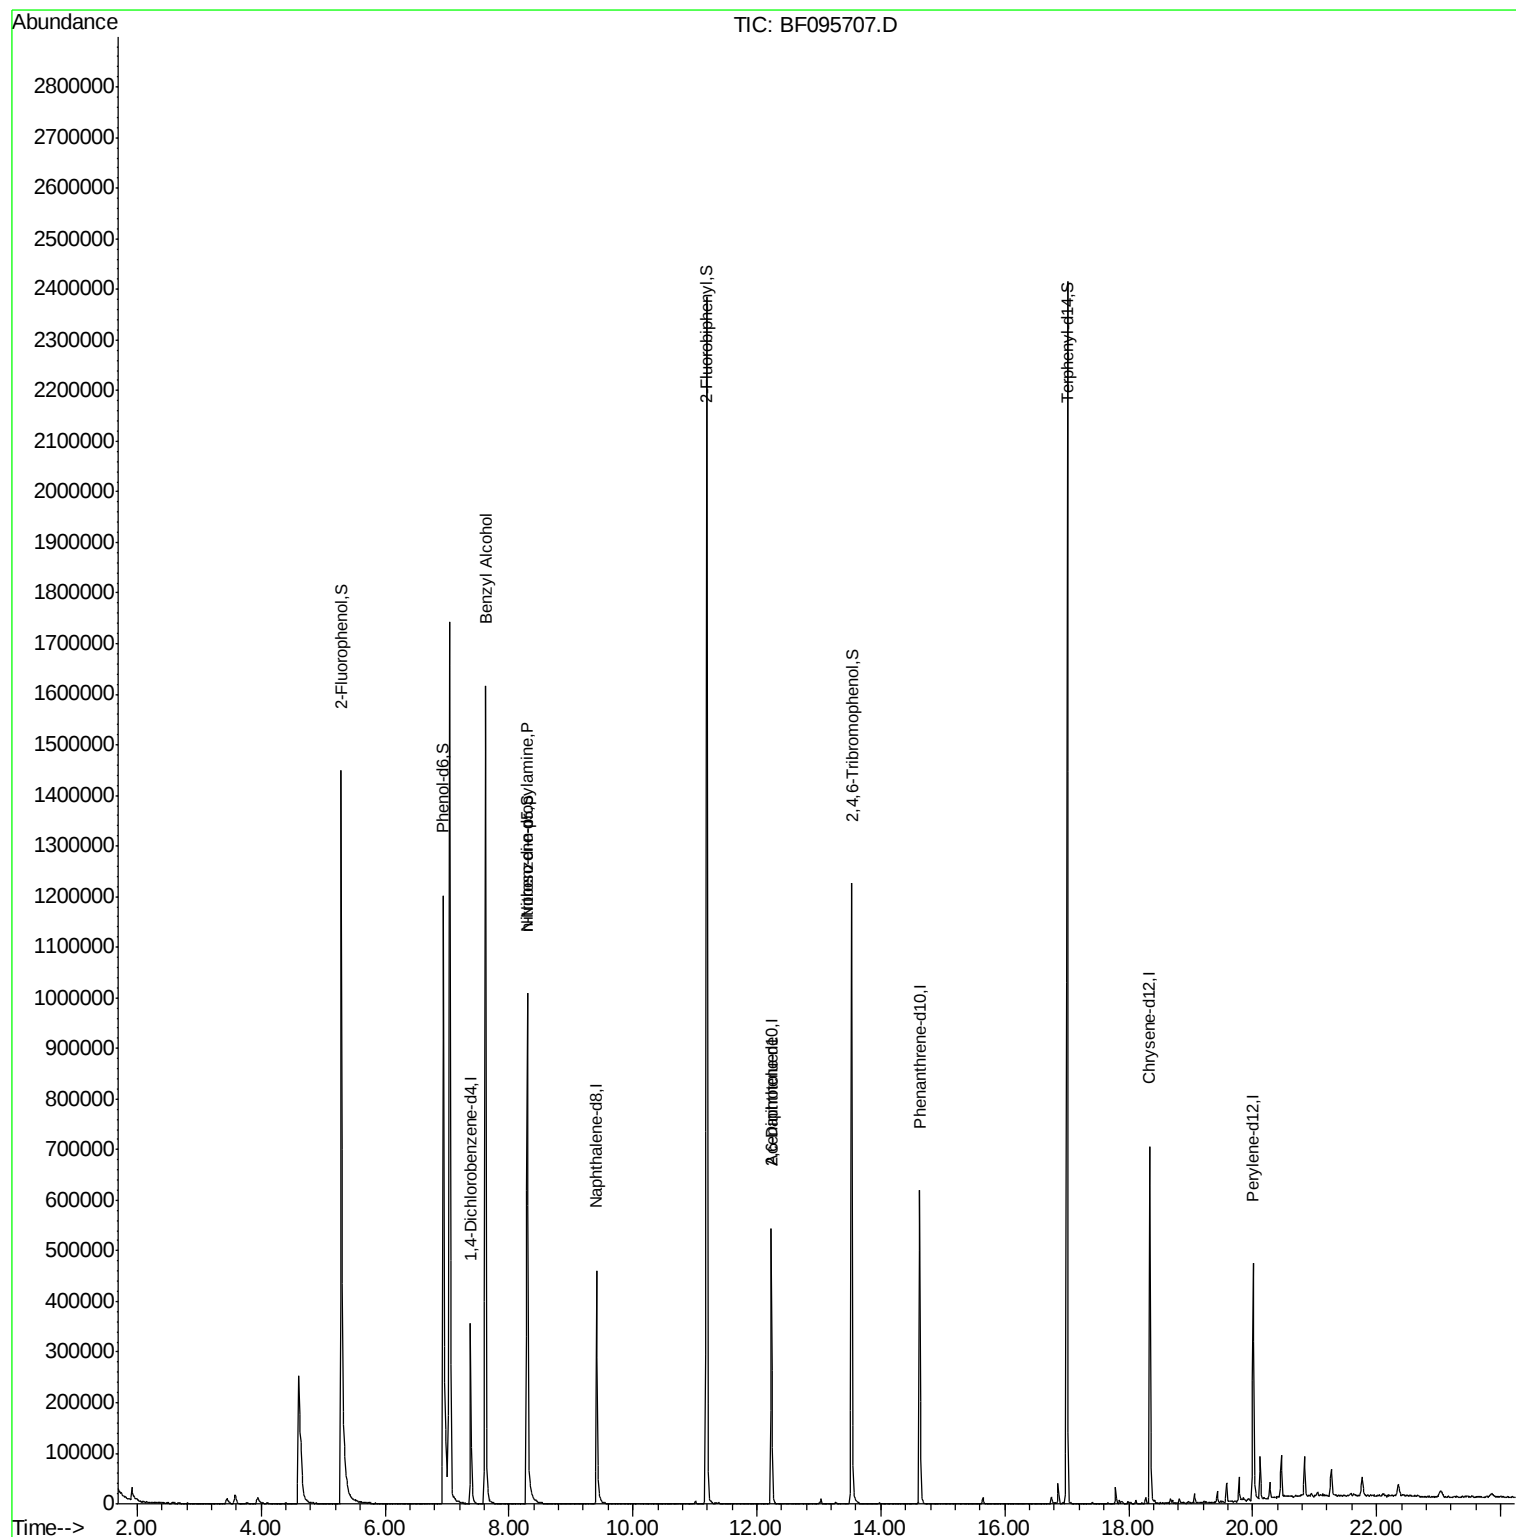

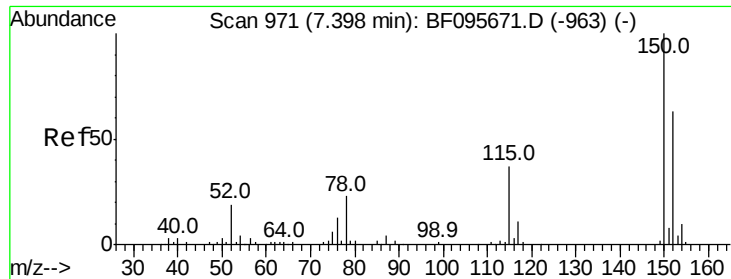


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.39 min Scan# 969
Delta R.T. -0.01 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 88345
Ion Ratio Lower Upper
152 100
150 156.9 126.2 189.2
115 59.7 52.2 78.2

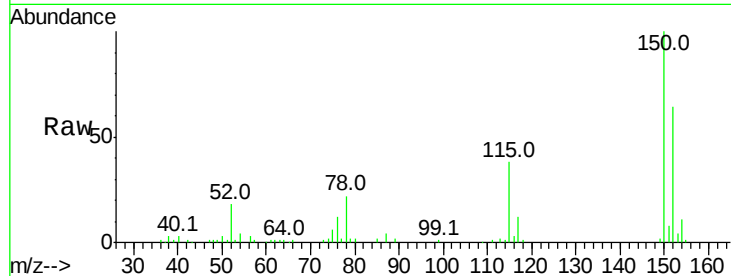


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

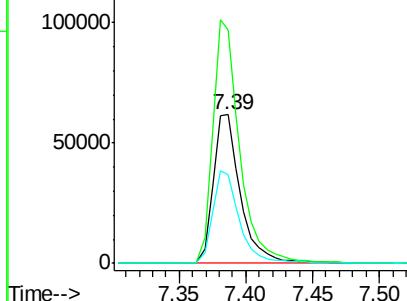



#5

2-Fluorophenol
Concen: 143.95 ng
RT: 5.29 min Scan# 613
Delta R.T. 0.01 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04

Tgt Ion:112 Resp: 798069
Ion Ratio Lower Upper
112 100
64 55.7 46.0 69.0
63 27.5 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

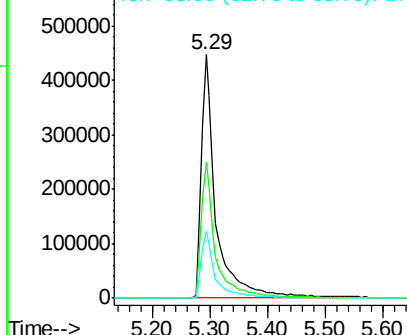



#7

Phenol-d6

Concen: 120.15 ng

RT: 6.94 min Scan# 893

Delta R.T. -0.02 min

Lab File: BF095707.D

Acq: 6 Jun 2017 14:04

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 797477

Ion Ratio Lower Upper

99 100

42 15.6 13.5 20.3

71 31.6 24.5 36.7

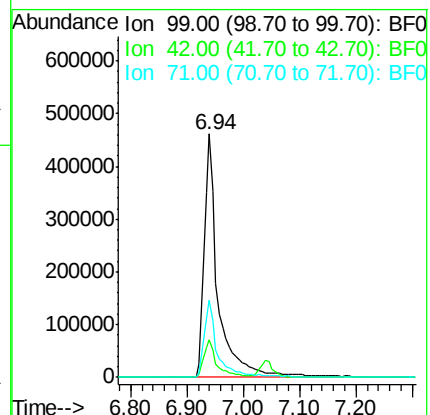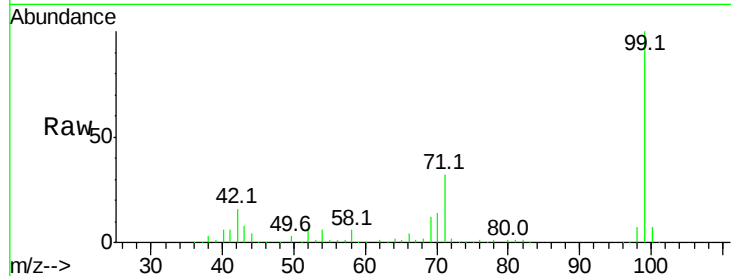

#15

Benzyl Alcohol

Concen: 2.25 ng

RT: 7.62 min Scan# 1008

Delta R.T. -0.08 min

Lab File: BF095707.D

Acq: 6 Jun 2017 14:04




Tgt Ion: 79 Resp: 10239


Ion Ratio Lower Upper

79 100

108 23.1 63.4 95.0#

77 101.8 49.2 73.8#



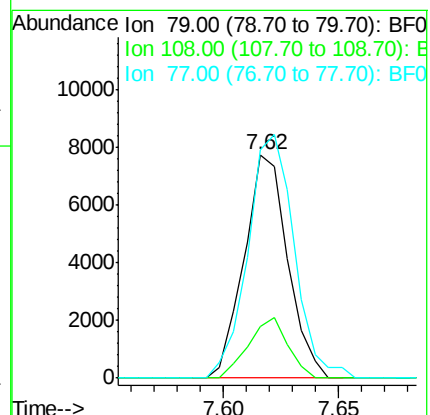





#19
n-Nitroso-di-n-propylamine
Concen: 16.40 ng
RT: 8.30 min Scan# 1124
Delta R.T. 0.16 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 70 Resp: 68981
Ion Ratio Lower Upper
70 100
42 43.8 47.2 70.8#
101 0.0 7.2 10.8#
130 2.5 15.9 23.9#

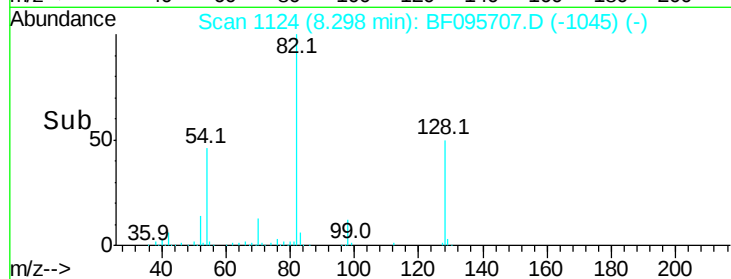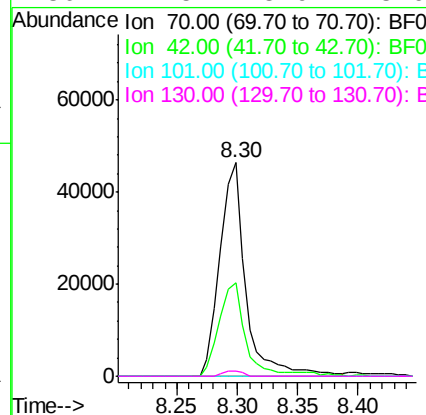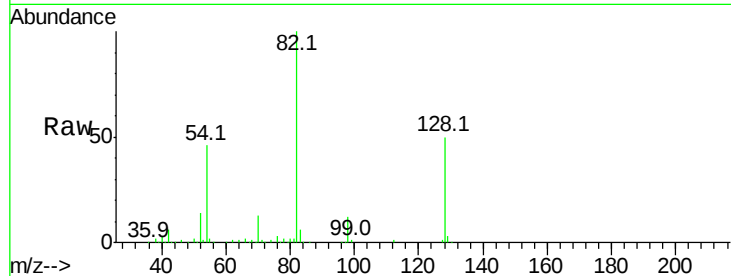

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 9.41 min Scan# 1313
Delta R.T. -0.02 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04

Tgt Ion: 136 Resp: 373615
Ion Ratio Lower Upper
136 100
137 10.8 8.5 12.7
54 7.1 4.9 7.3
68 5.7 4.1 6.1


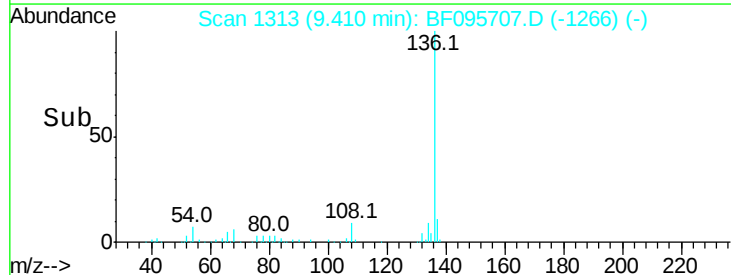

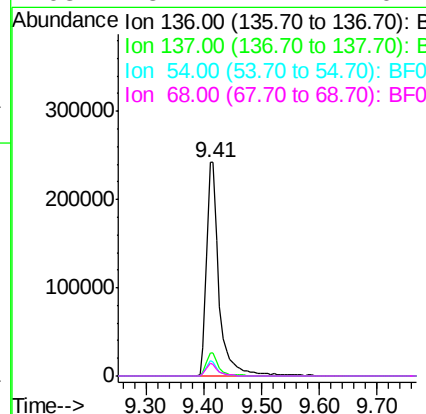




#23
Nitrobenzene-d5
Concen: 92.26 ng
RT: 8.30 min Scan# 1124
Delta R.T. -0.02 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04




Instrument :
BNA_F
ClientSampled :


Tot Ion: 82 Resp: 554999
Ion Ratio Lower Upper
82 100
128 50.1 34.0 51.0
54 46.3 42.2 63.2

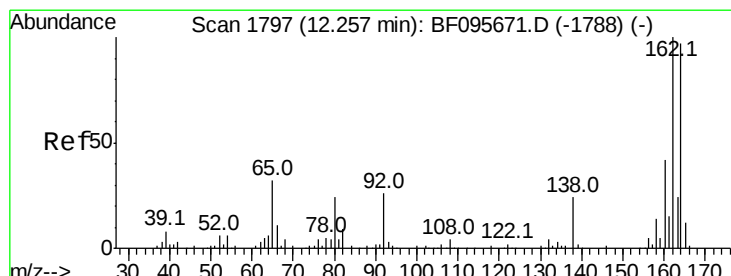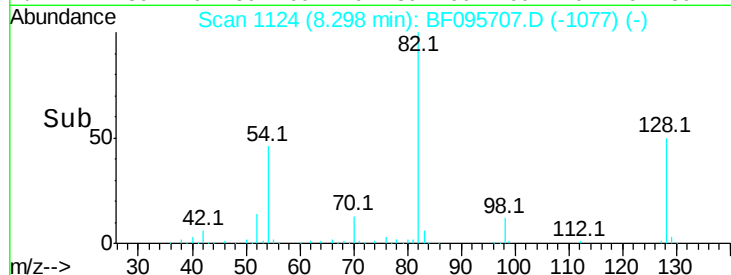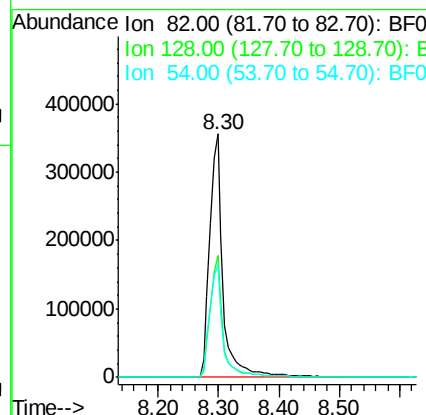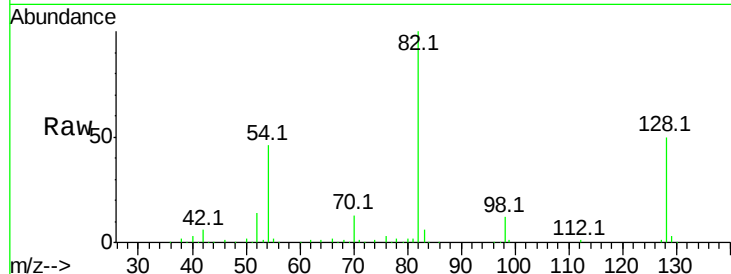

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.23 min Scan# 1793
Delta R.T. -0.02 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04

Tgt Ion:164 Resp: 168496
Ion Ratio Lower Upper
164 100
162 103.2 82.6 123.8
160 43.8 36.2 54.2

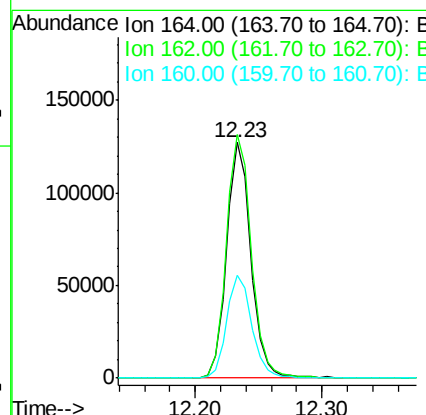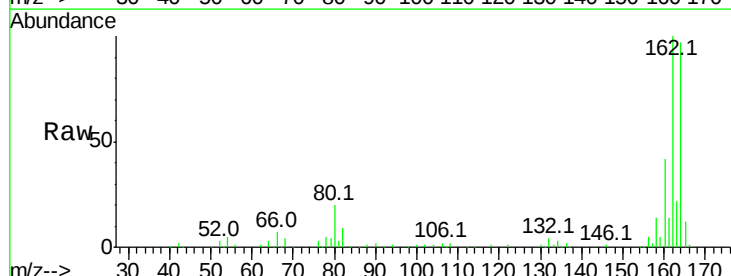


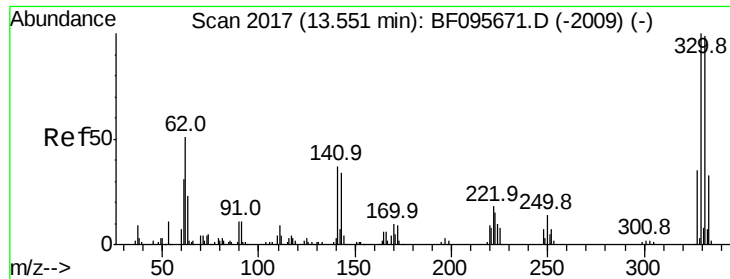




#41
 2,4,6-Tribromophenol
 Concen: 149.44 ng
 RT: 13.53 min Scan# 2014
 Delta R.T. -0.02 min
 Lab File: BF095707.D
 Acq: 6 Jun 2017 14:04

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 222782
 Ion Ratio Lower Upper
 330 100
 332 96.5 76.6 115.0
 141 37.8 31.4 47.2

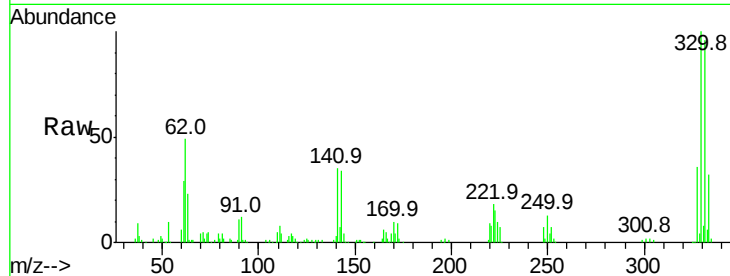


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

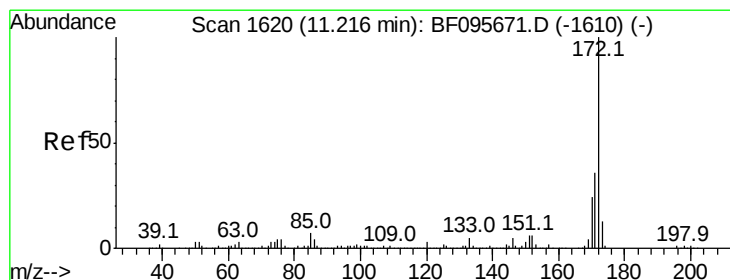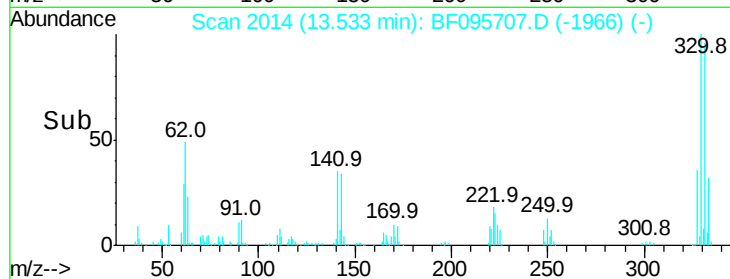
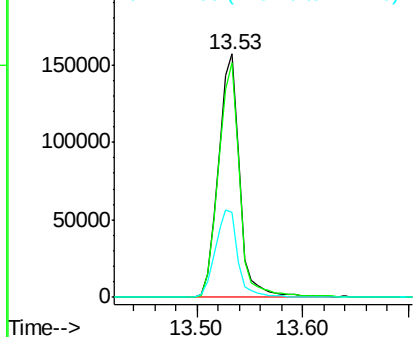



#44
 2-Fluorobiphenyl
 Concen: 105.07 ng
 RT: 11.19 min Scan# 1616
 Delta R.T. -0.02 min
 Lab File: BF095707.D
 Acq: 6 Jun 2017 14:04

Tgt Ion:172 Resp: 1272193
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.6 44.4
 170 23.8 19.8 29.8

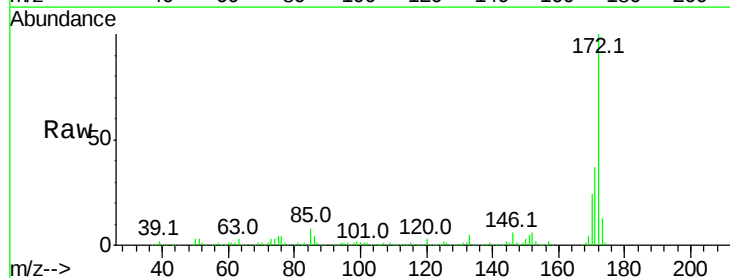

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

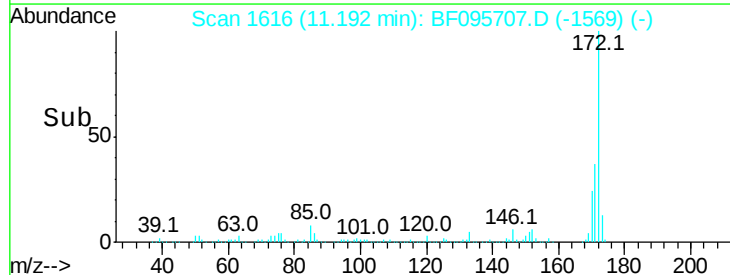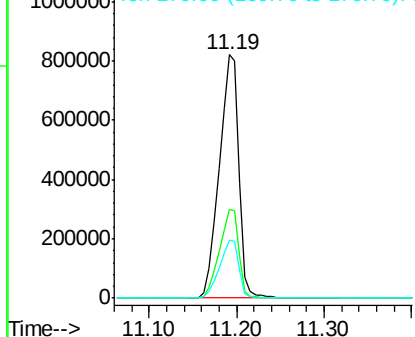


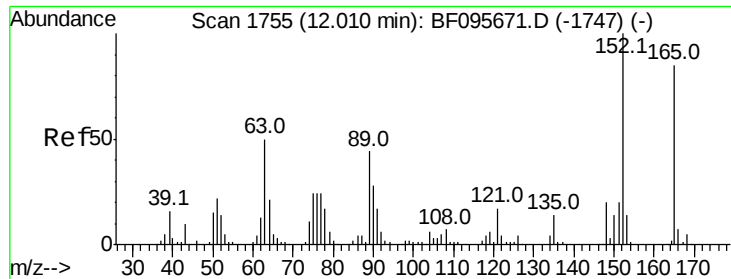




#50
2,6-Dinitrotoluene
Concen: 7.62 ng
RT: 12.23 min Scan# 1793
Delta R.T. 0.22 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04

Instrument :
BNA_F
ClientSampleId :

Tot Ion:165 Resp: 21264
Ion Ratio Lower Upper
165 100
63 0.0 34.3 51.5#
89 0.0 37.1 55.7#




Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0

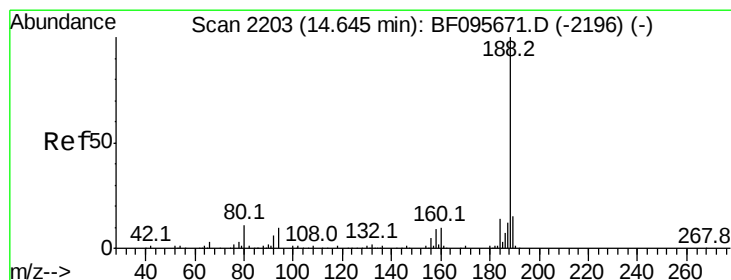
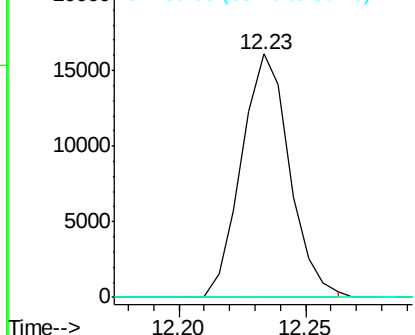



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.63 min Scan# 2200
Delta R.T. -0.02 min
Lab File: BF095707.D
Acq: 6 Jun 2017 14:04

Tgt Ion:188 Resp: 326975
Ion Ratio Lower Upper
188 100
94 10.1 9.4 14.2
80 11.1 10.2 15.2



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

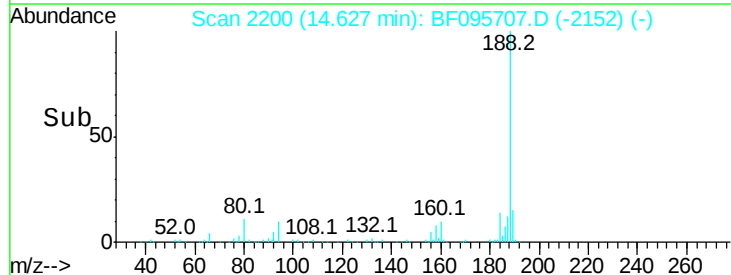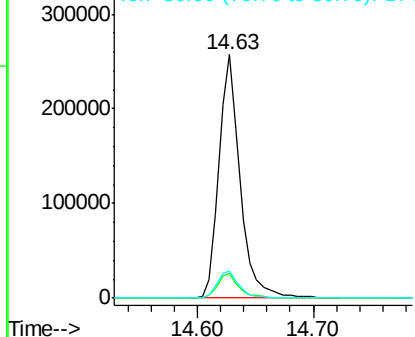

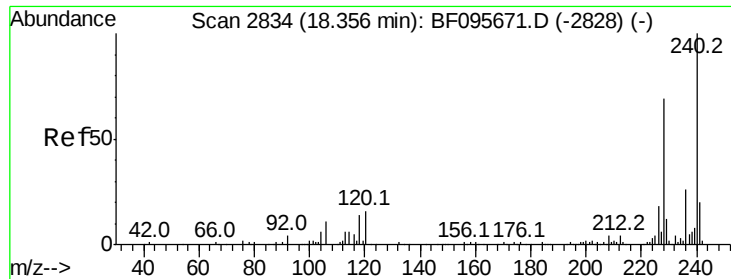

#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.34 min Scan# 2831

Delta R.T. -0.02 min

Lab File: BF095707.D

Acq: 6 Jun 2017 14:04

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 337933

Ion Ratio Lower Upper

240 100

120 14.4 5.8 8.8#




236 24.8 20.5 30.7

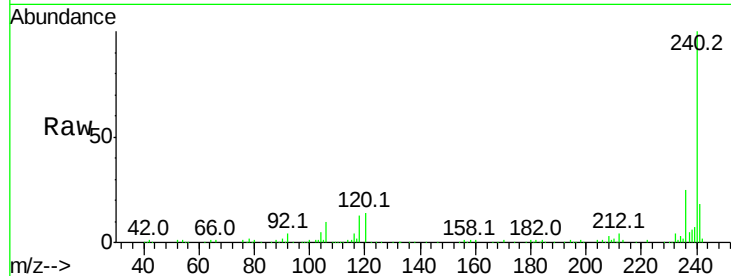

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

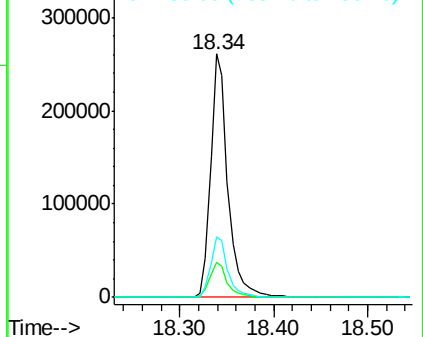

#78

Terphenyl-d14

Concen: 79.99 ng

RT: 17.01 min Scan# 2605

Delta R.T. -0.01 min

Lab File: BF095707.D

Acq: 6 Jun 2017 14:04


Tgt Ion:244 Resp: 1089184

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0



122 14.2 10.3 15.5






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

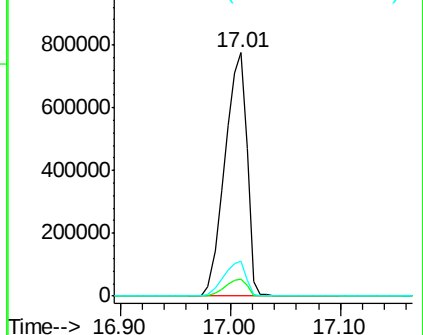

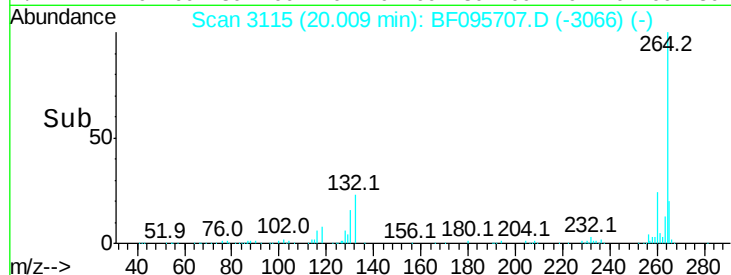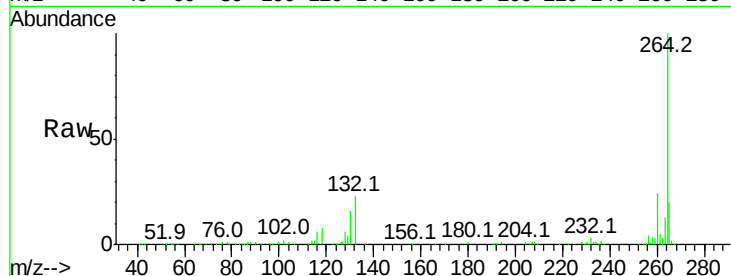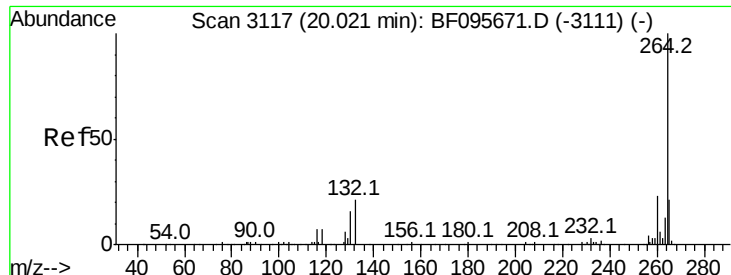

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 20.01 min Scan# 3115
 Delta R.T. -0.01 min
 Lab File: BF095707.D
 Acq: 6 Jun 2017 14:04

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:264	Resp:	237771
Ion Ratio	Lower	Upper
264	100	
260	23.9	19.5 29.3
265	20.0	17.2 25.8

