
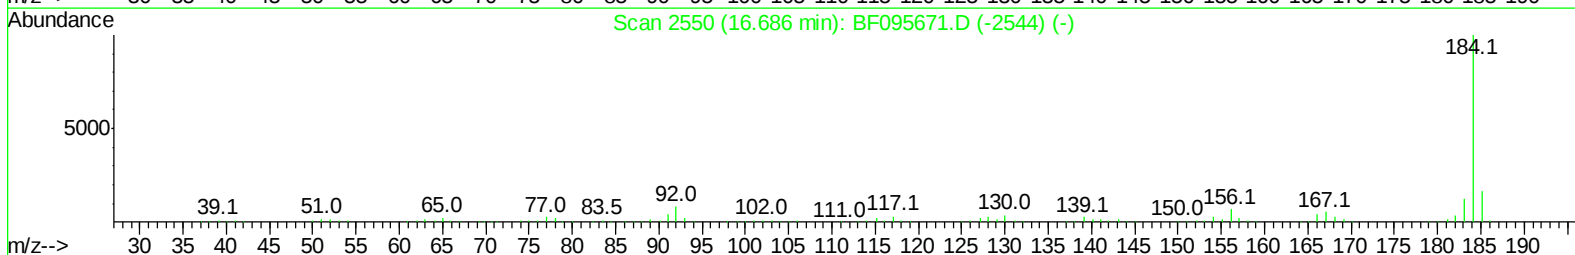
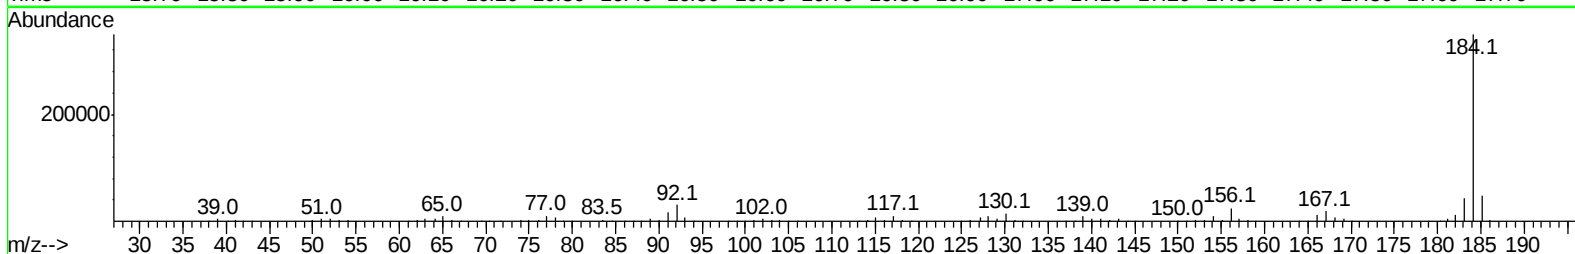


Data Path : Z:\HPCHEM1\BNA F\Data\BF060617\
 Data File : BF095699.D
 Acq On : 6 Jun 2017 9:39
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 17:44:18 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:15:31 2017
 Response via : Initial Calibration

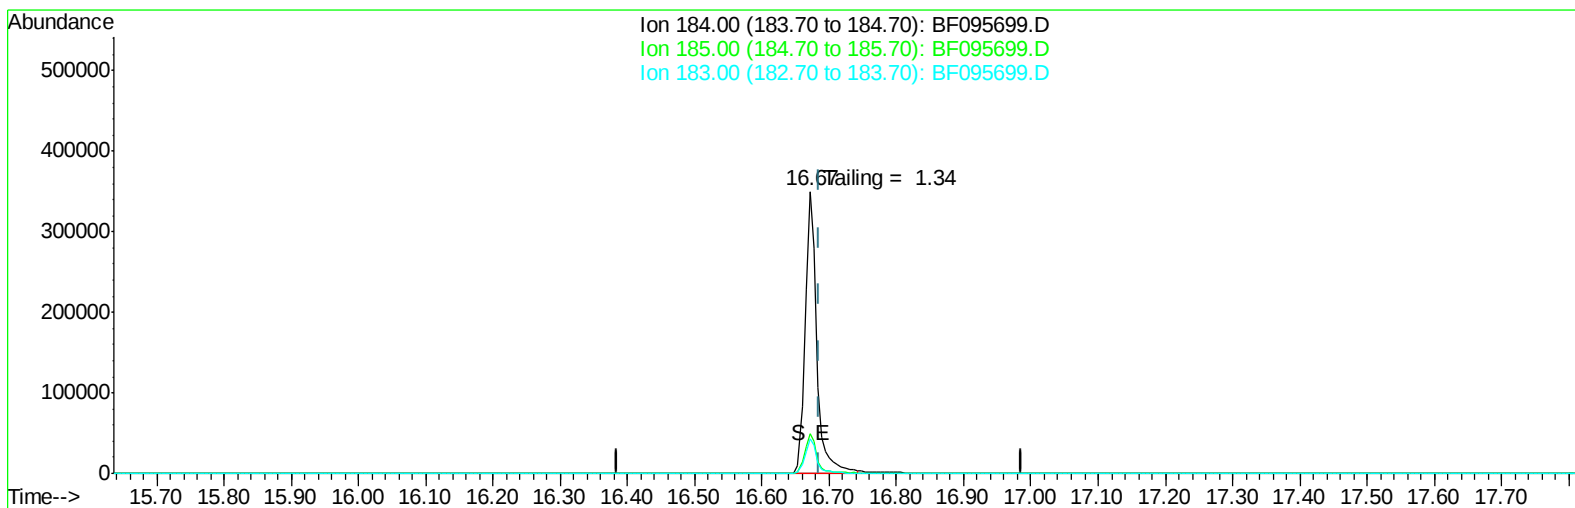

TIC: BF095699.D

(76) Benzidine




16.671min (-0.015) 0.00ng

response 431459

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.97#
183.00	12.20	12.16
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF060617\
Data File : BF095699.D
Acq On : 6 Jun 2017 9:39
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 17:44:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

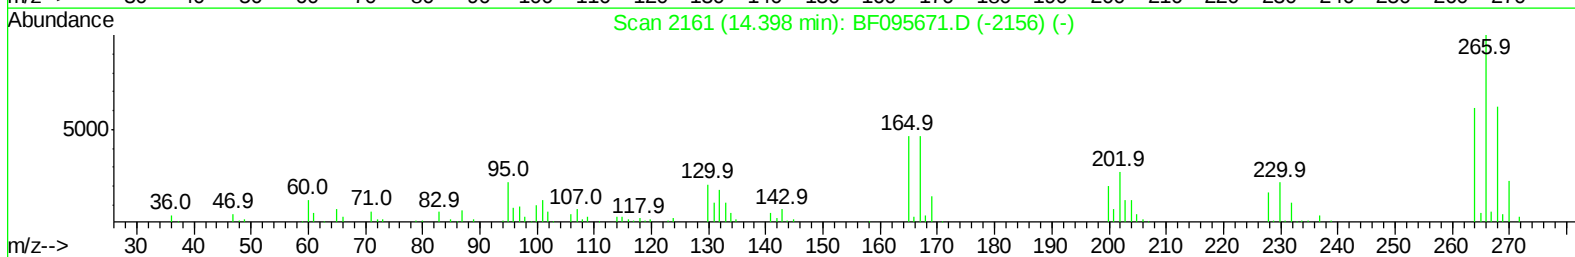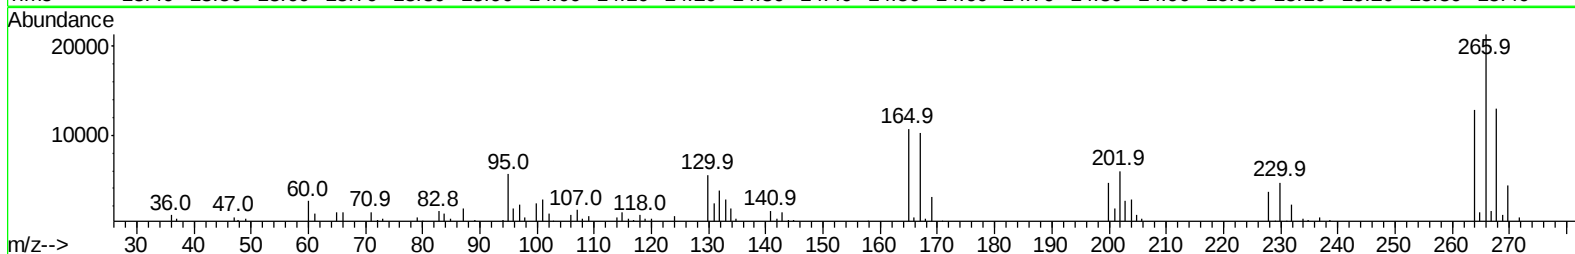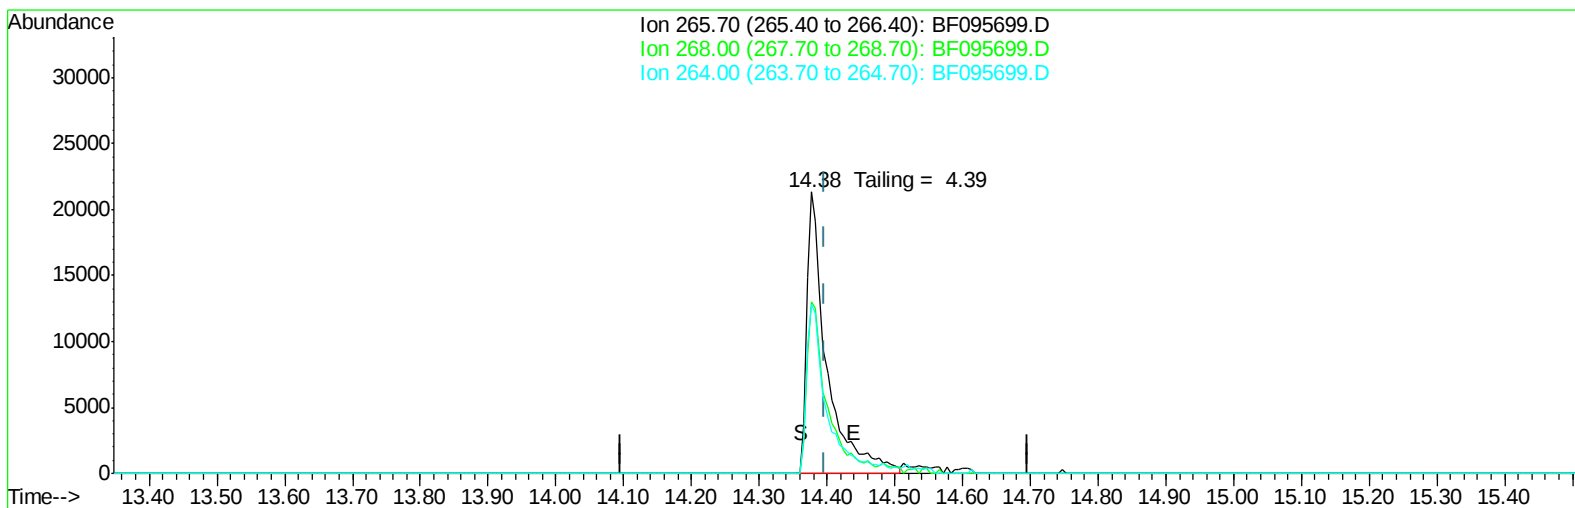

TIC: BF095699.D

(69) Pentachlorophenol (C)

14.377min (-0.020) 0.00ng

response 43845

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.01
264.00	64.60	59.99
0.00	0.00	0.00