


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060617\
 Data File : BF095711.D
 Acq On : 6 Jun 2017 16:12
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

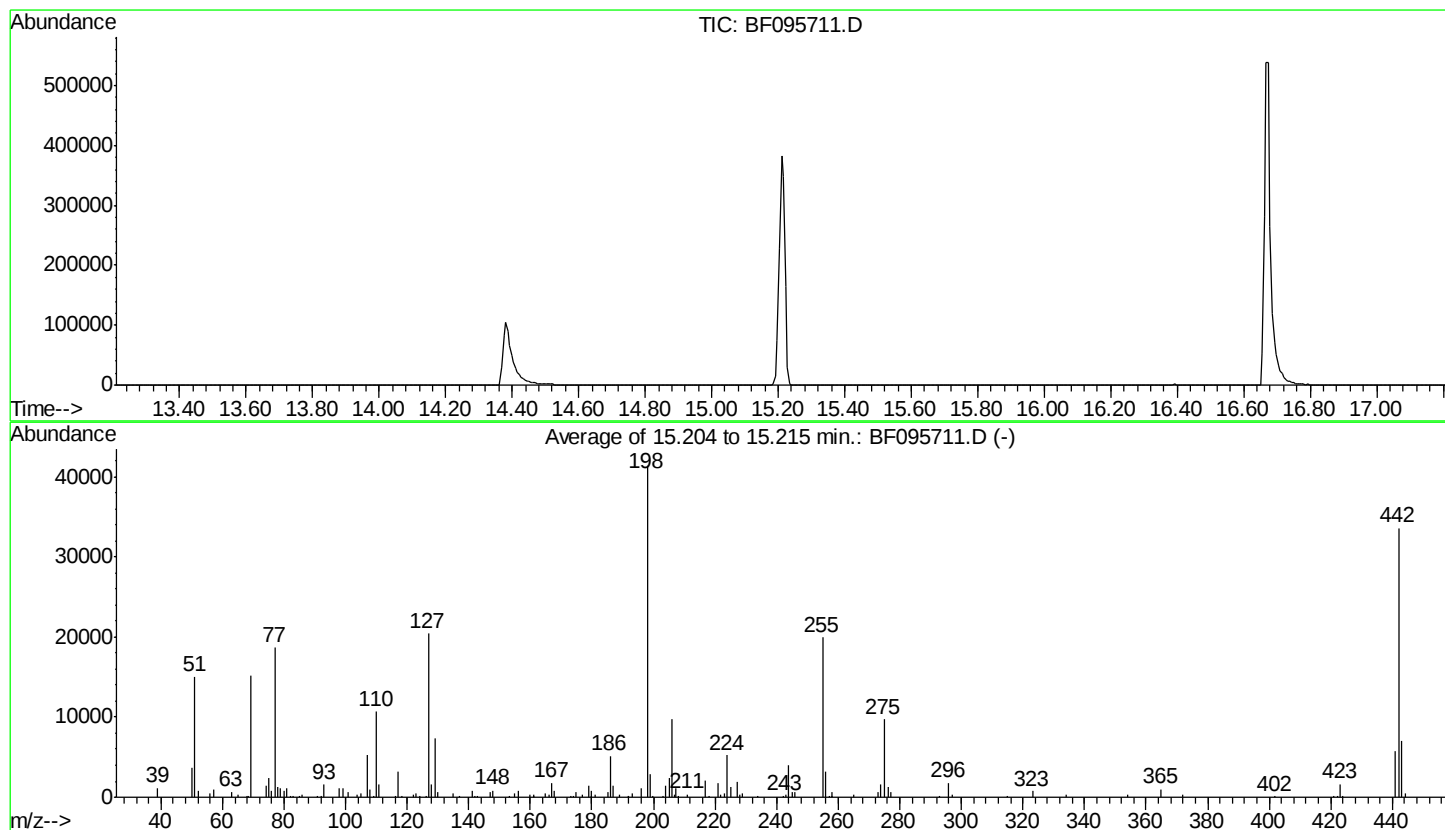

AutoFind: Scans 2298, 2299, 2300; Background Corrected with Scan 2292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	15069	PASS
68	69	0.00	2	0.9	138	PASS
69	198	0.00	100	36.6	15144	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	20450	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41400	PASS
199	198	5	9	6.8	2807	PASS
275	198	10	60	23.5	9733	PASS
365	198	1	100	2.5	1022	PASS
441	442	0.01	24	17.0	5702	PASS
442	198	50	100	81.2	33626	PASS
443	442	15	24	20.8	6987	PASS