

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
 Data File : BF128698.D
 Acq On : 06 Jun 2022 16:00
 Operator : CG\JU
 Sample : N3189-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20220419-COMPOSITE-H

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	539	542	558	rBV	2393629	2555679	94.89%	15.399%
2	6.469	707	711	712	rBV	31275	32219	1.20%	0.194%
3	6.493	712	715	724	rVB	2729640	2532028	94.01%	15.256%
4	6.822	767	771	774	rBV	595223	454505	16.88%	2.739%
5	7.387	861	867	870	rBV	1662079	1735625	64.44%	10.458%
6	8.104	985	989	992	rBV	722349	568230	21.10%	3.424%
7	9.187	1167	1173	1176	rBV	3012347	2693219	100.00%	16.228%
8	9.863	1284	1288	1291	rBV	833635	680210	25.26%	4.099%
9	10.657	1418	1423	1426	rBV	2032755	1826086	67.80%	11.003%
10	11.345	1537	1540	1544	rBV	667006	574943	21.35%	3.464%
11	11.416	1548	1552	1555	rVB3	41878	33799	1.25%	0.204%
12	11.880	1627	1631	1636	rBV	27542	31508	1.17%	0.190%
13	12.939	1807	1811	1814	rBV	2109180	1726117	64.09%	10.401%
14	13.869	1966	1969	1981	rVB7	15197	37432	1.39%	0.226%
15	13.992	1986	1990	1993	rBV	476339	423733	15.73%	2.553%
16	14.086	2002	2006	2015	rBV	225842	238910	8.87%	1.440%
17	15.457	2234	2239	2243	rBV	381714	452170	16.79%	2.725%




Sum of corrected areas: 16596413

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
Data File : BF128698.D
Acq On : 06 Jun 2022 16:00
Operator : CG\JU
Sample : N3189-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220419-COMPOSITE-H

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

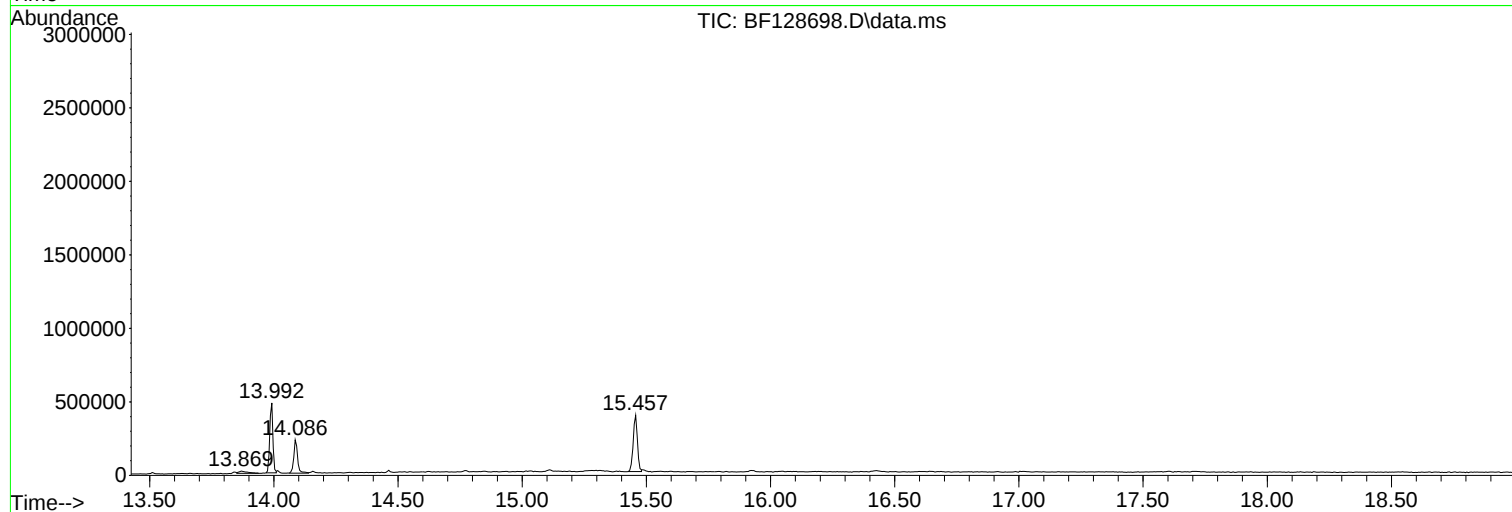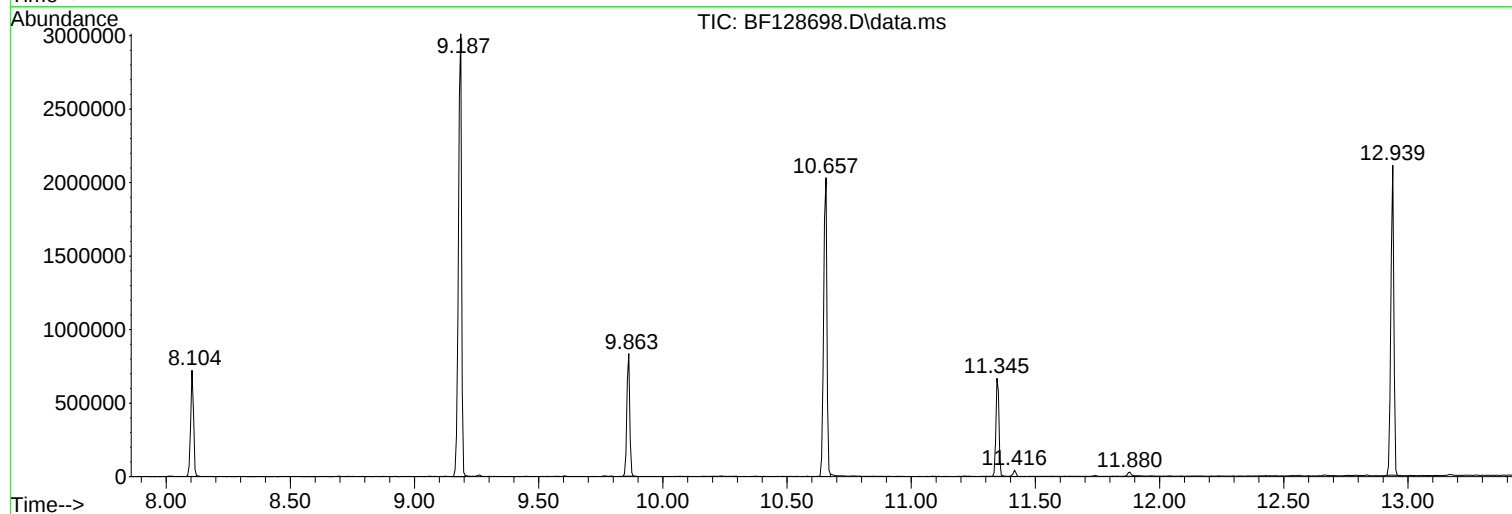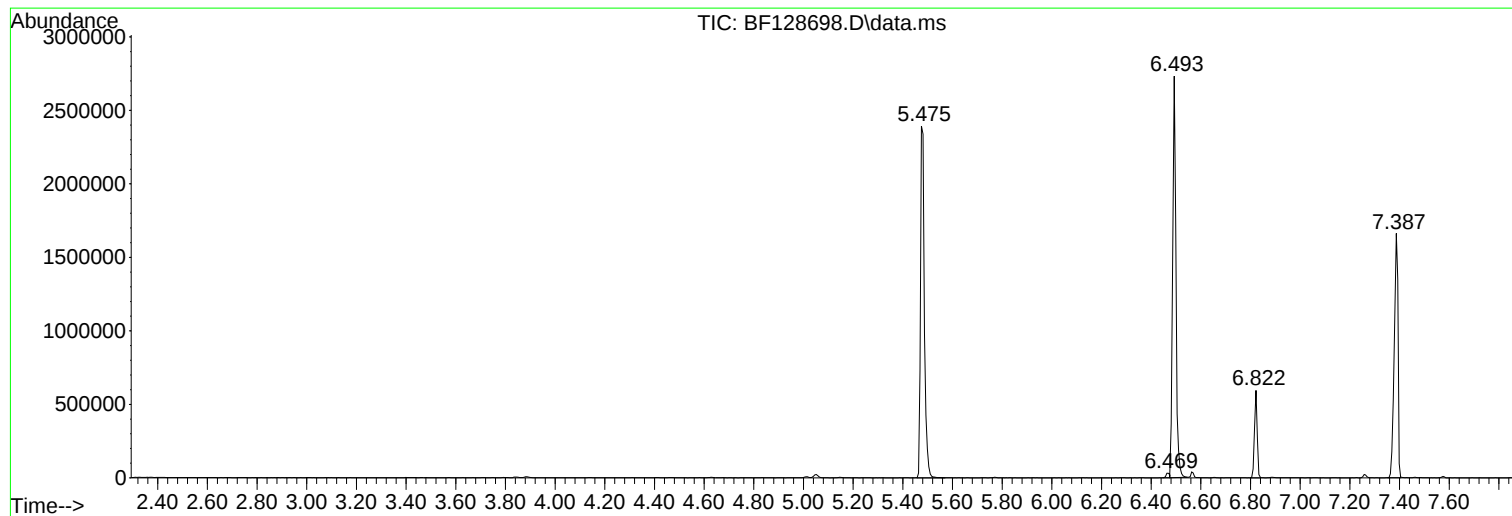

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
Data File : BF128698.D
Acq On : 06 Jun 2022 16:00
Operator : CG\JU
Sample : N3189-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220419-COMPOSITE-H










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.086	11.28 ng	238910	Chrysene-d12	13.992

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	87
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	38
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	37

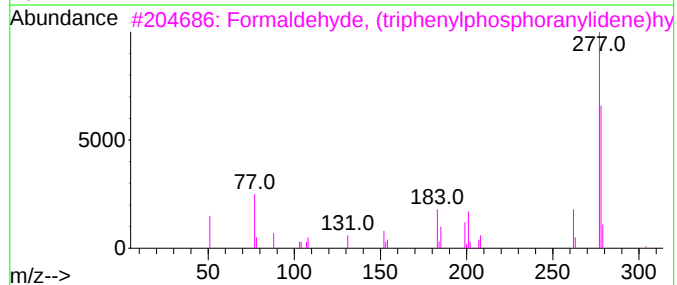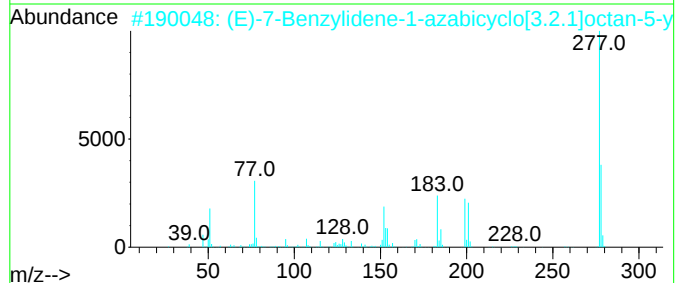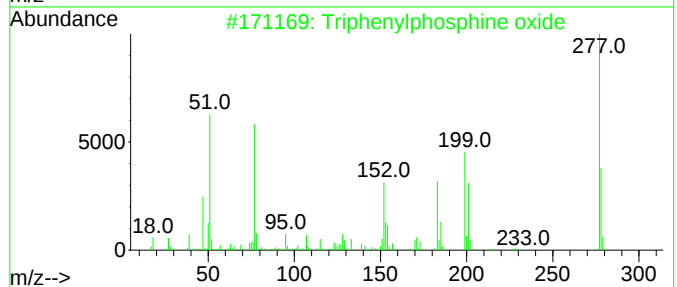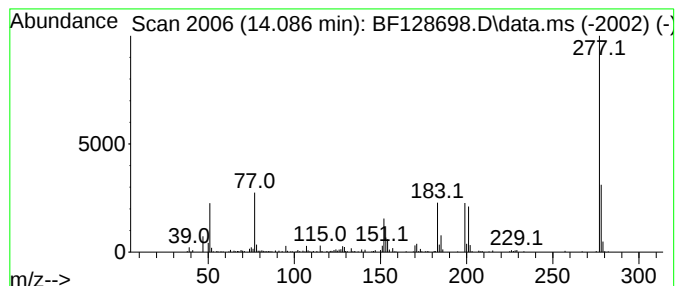

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
Data File : BF128698.D
Acq On : 06 Jun 2022 16:00
Operator : CG\JU
Sample : N3189-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220419-COMPOSITE-H

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.086	11.3	ng	238910	5	13.992	423733	20.0