

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
 Data File : BF128701.D
 Acq On : 06 Jun 2022 17:29
 Operator : CG\JU
 Sample : N3189-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20220414-COMPOSITE-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.045	466	469	476	rVB	23766	32194	1.12%	0.190%
2	5.475	539	542	559	rBV	2584637	2693973	93.38%	15.880%
3	6.492	711	715	724	rVB	3084749	2697266	93.49%	15.899%
4	6.822	767	771	774	rBV	594084	455209	15.78%	2.683%
5	7.387	862	867	870	rBV	1810493	1861529	64.52%	10.973%
6	8.104	985	989	992	rBV	714147	567097	19.66%	3.343%
7	9.186	1167	1173	1176	rBV	3355195	2884983	100.00%	17.006%
8	9.863	1284	1288	1291	rVB	727715	613247	21.26%	3.615%
9	10.657	1418	1423	1426	rBV	2033715	1793599	62.17%	10.572%
10	11.345	1537	1540	1544	rBV	604696	535820	18.57%	3.158%
11	11.880	1627	1631	1636	rBV	39527	43842	1.52%	0.258%
12	12.939	1806	1811	1814	rBV	2108635	1756382	60.88%	10.353%
13	13.992	1985	1990	1993	rBV	460051	419758	14.55%	2.474%
14	14.086	2001	2006	2015	rBV	154244	163636	5.67%	0.965%
15	15.457	2234	2239	2243	rBV	375618	446237	15.47%	2.630%




Sum of corrected areas: 16964772

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
Data File : BF128701.D
Acq On : 06 Jun 2022 17:29
Operator : CG\JU
Sample : N3189-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220414-COMPOSITE-C

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

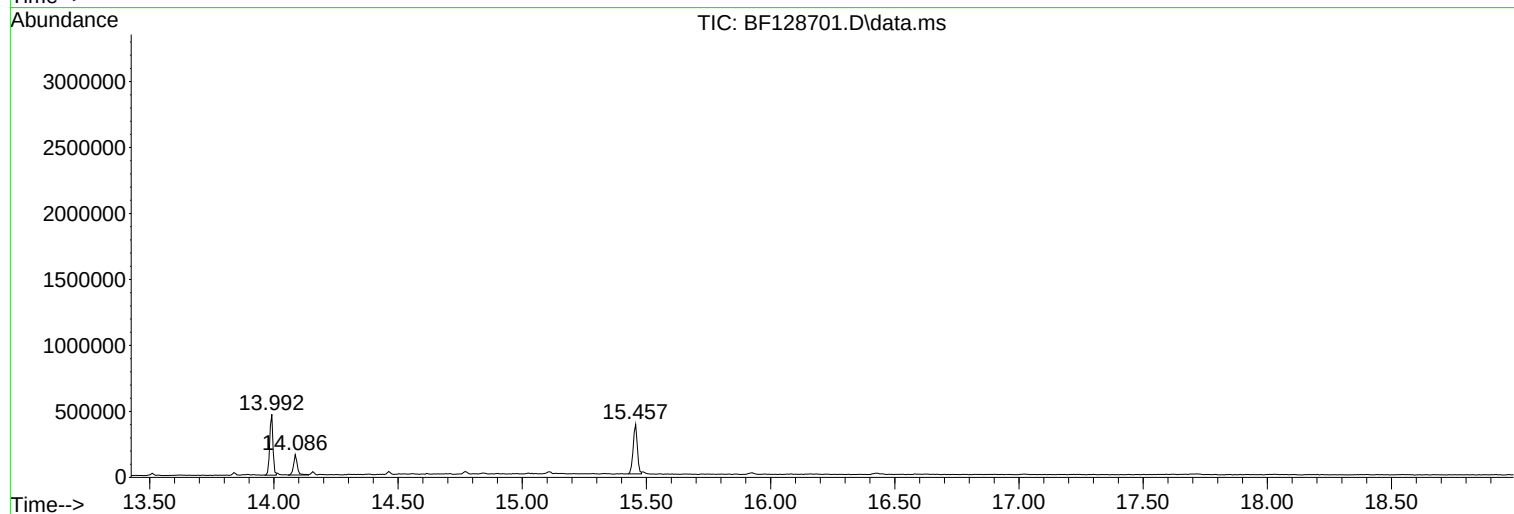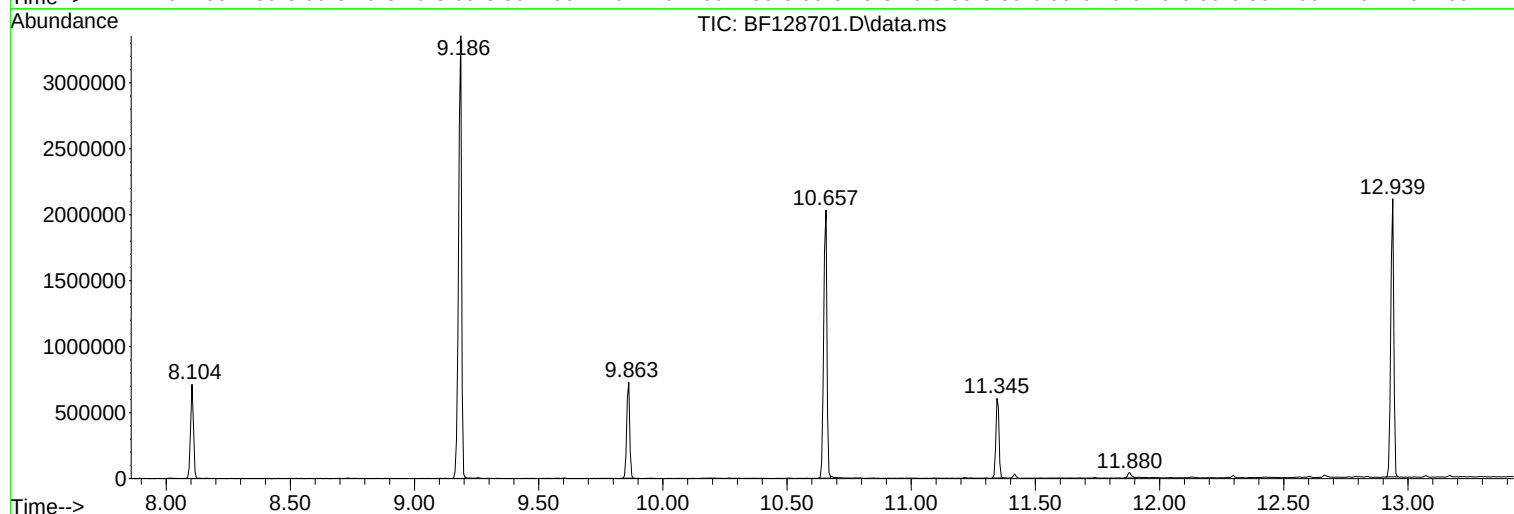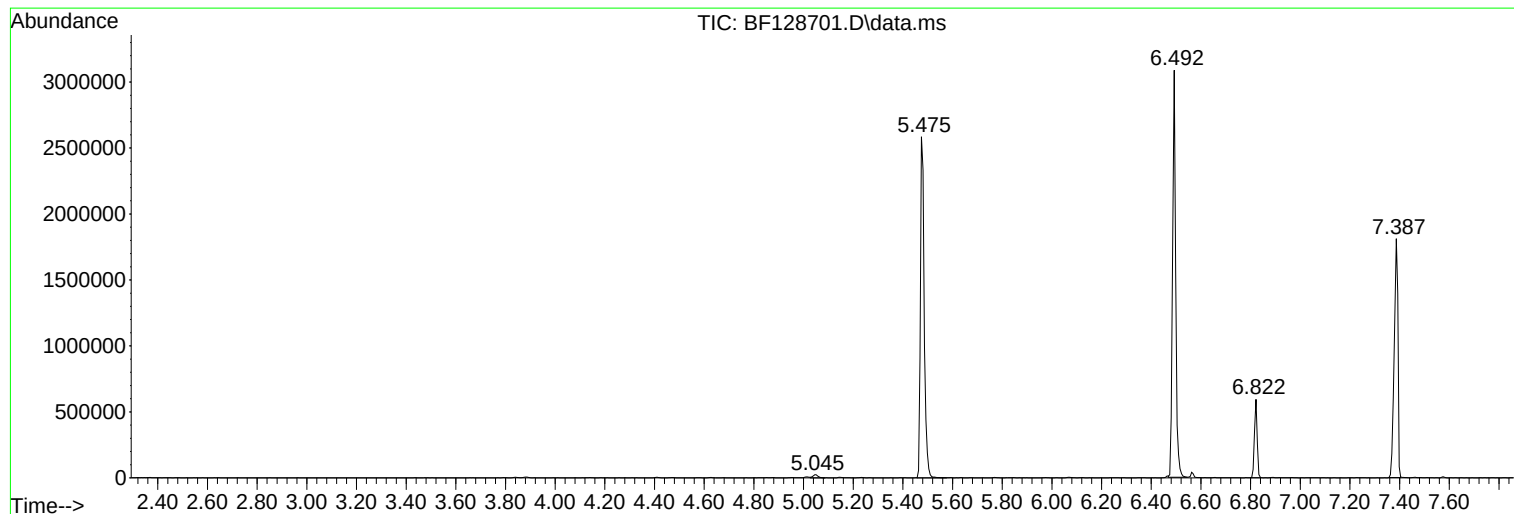

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
Data File : BF128701.D
Acq On : 06 Jun 2022 17:29
Operator : CG\JU
Sample : N3189-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220414-COMPOSITE-C










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.086	7.80 ng	163636	Chrysene-d12	13.992

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	90
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	72
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	38
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	23

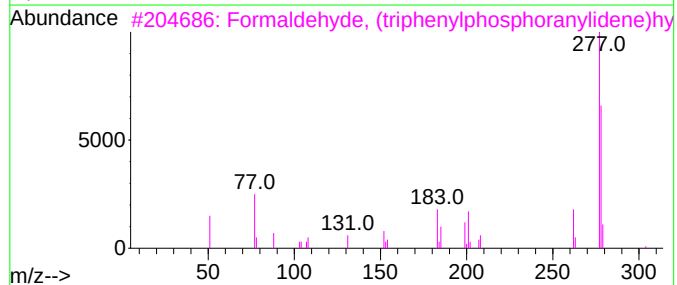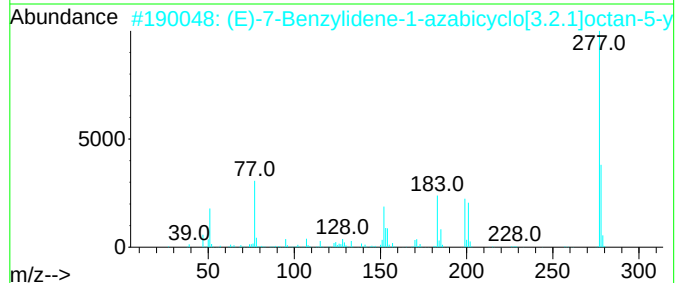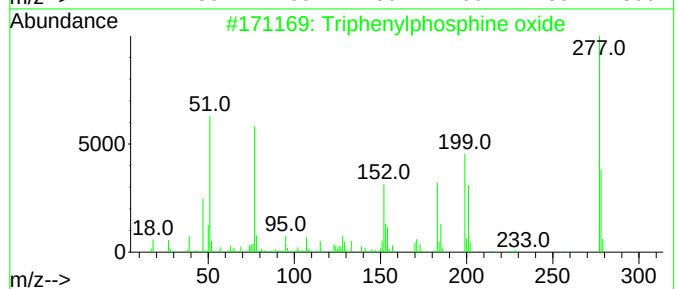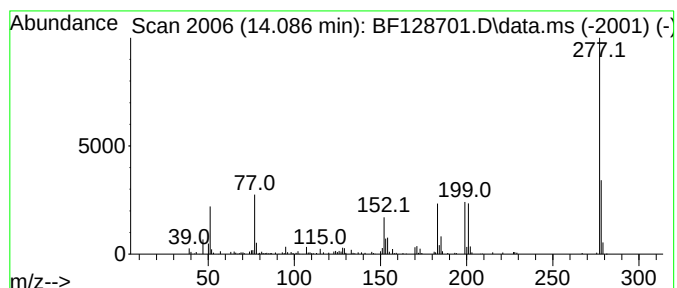

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
Data File : BF128701.D
Acq On : 06 Jun 2022 17:29
Operator : CG\JU
Sample : N3189-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220414-COMPOSITE-C

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.086	7.8	ng	163636	5	13.992	419758	20.0