


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
 Data File : BF128690.D
 Acq On : 06 Jun 2022 10:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 17:07:23 2022

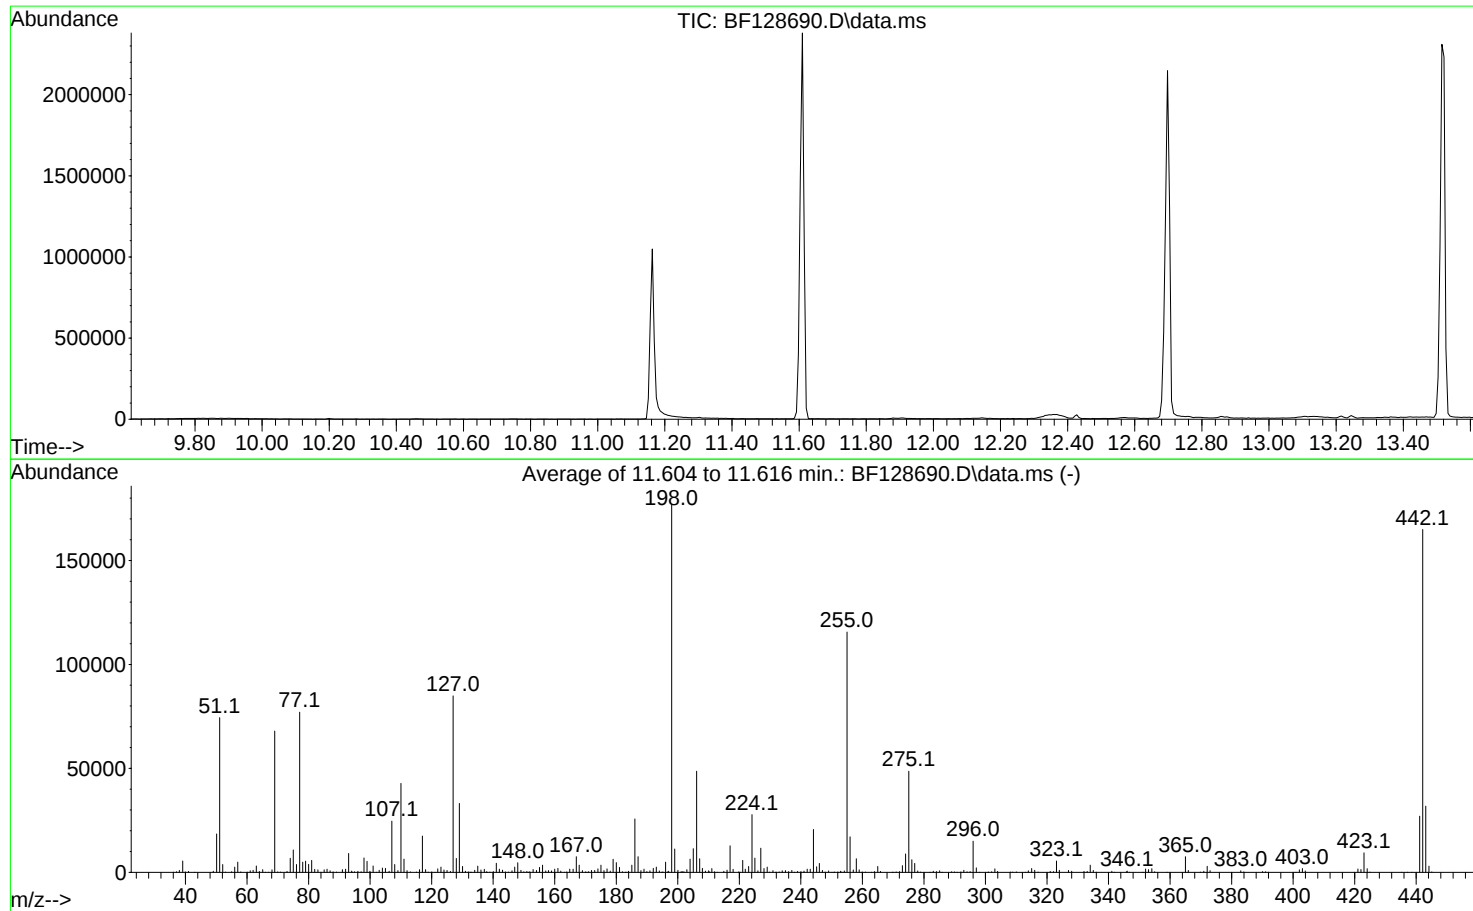




AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	74432	PASS
68	69	0.00	2	1.8	1210	PASS
69	198	0.00	100	38.4	67989	PASS
70	69	0.00	2	0.4	242	PASS
127	198	10	80	48.0	84872	PASS
197	198	0.00	2	0.3	512	PASS
198	198	100	100	100.0	176915	PASS
199	198	5	9	6.4	11274	PASS
275	198	10	60	27.5	48667	PASS
365	198	1	100	4.3	7575	PASS
441	198	0.01	100	15.3	27029	PASS
442	442	50	100	100.0	164917	PASS
443	442	15	24	19.3	31856	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
 Data File : BF128690.D
 Acq On : 06 Jun 2022 10:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 06:05:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 17:07:23 2022
 Response via : Initial Calibration

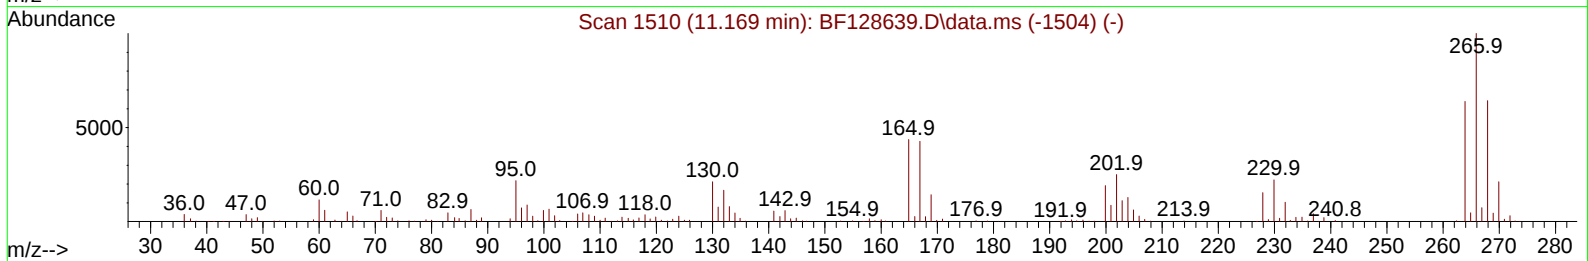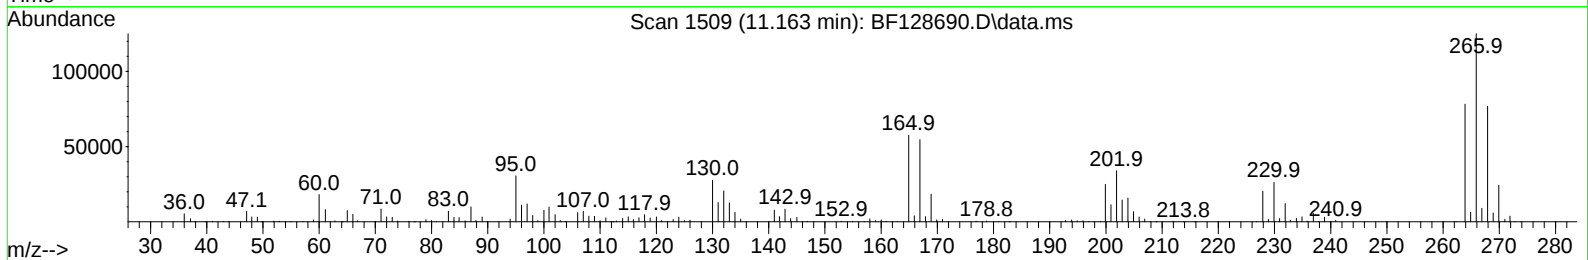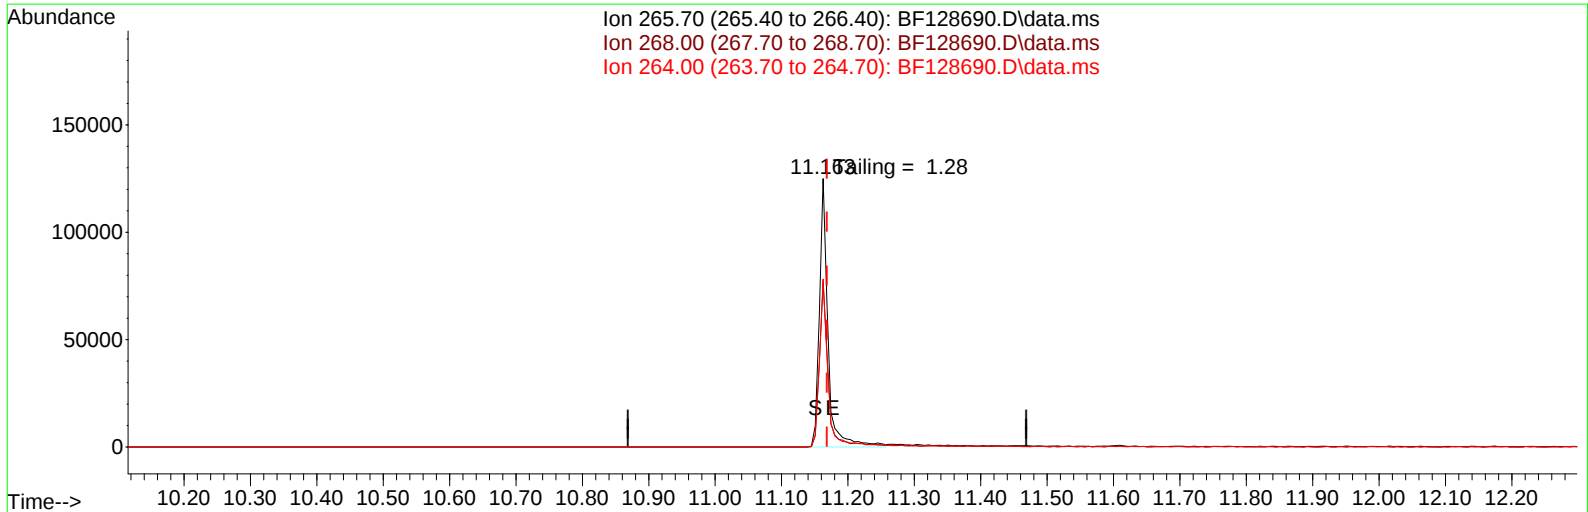

TIC: BF128690.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 20755.07 ng




response 115738

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	61.44
264.00	61.80	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060622\
Data File : BF128690.D
Acq On : 06 Jun 2022 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 07 06:05:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

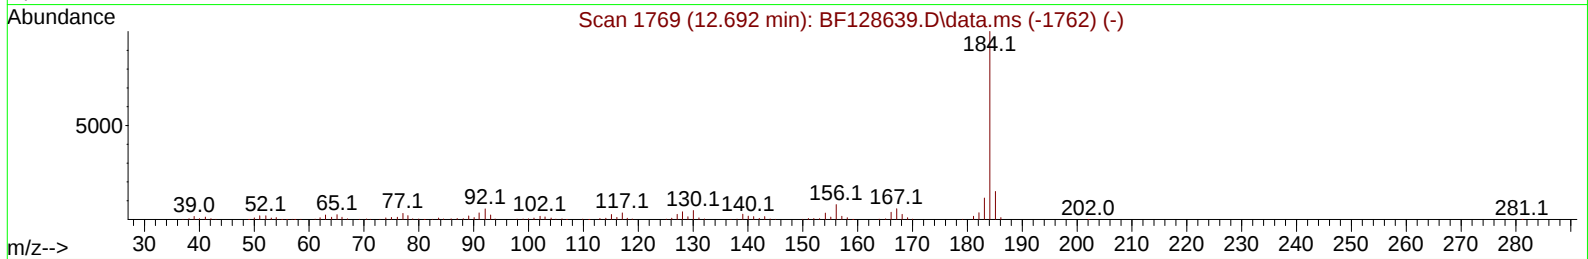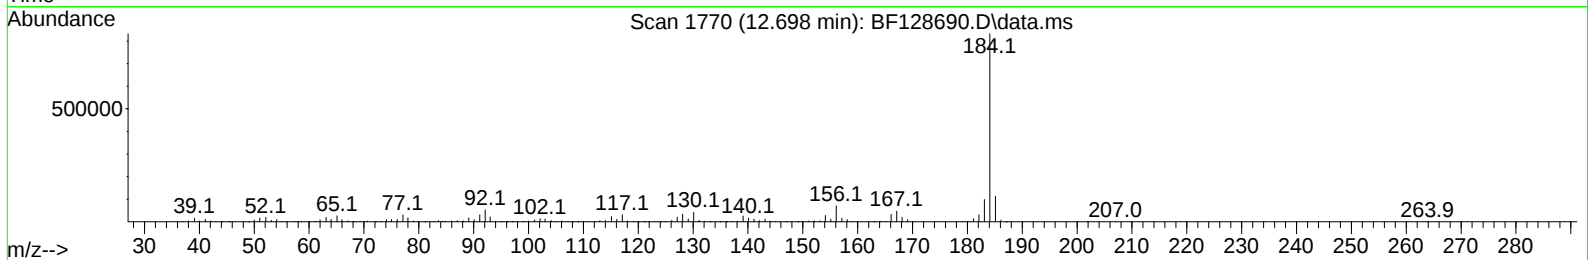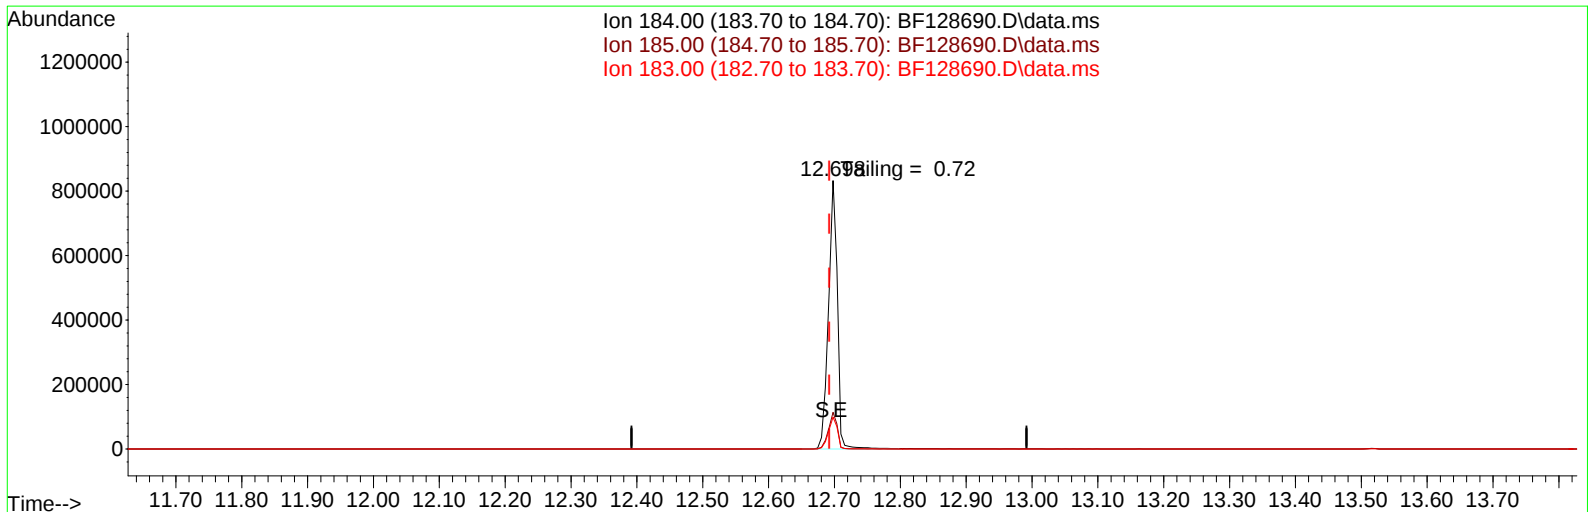

TIC: BF128690.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response 787831

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.66
183.00	11.60	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2022	BNA_F	<u>BF128690.D</u>
Compound Name	Response	Retention Time
DDT	413587	13.521
DDD	4316	13.245
DDE	681	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4997	418584	1.19

Instrument :
BNA_F
ClientSampleId :
DFTPP