

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060624\
 Data File : BF138144.D
 Acq On : 06 Jun 2024 20:45
 Operator : CG\JU
 Sample : P2718-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.222	16	23	28	rVB	9706589	13527586	100.00%	20.282%
2	5.122	513	516	520	rVB	173399	191664	1.42%	0.287%
3	5.522	579	584	587	rBV	4008935	3716429	27.47%	5.572%
4	6.516	749	753	756	rBV	2700581	2366098	17.49%	3.548%
5	6.904	815	819	822	rBV	2875841	2180831	16.12%	3.270%
6	7.469	909	915	918	rBV	5907339	5481729	40.52%	8.219%
7	8.187	1032	1037	1040	rBV	3527925	2896411	21.41%	4.343%
8	8.492	1085	1089	1098	rVB	196188	168842	1.25%	0.253%
9	9.263	1214	1220	1223	rBV	12143487	10906791	80.63%	16.353%
10	9.939	1331	1335	1338	rBV	4371342	3394866	25.10%	5.090%
11	10.728	1465	1469	1472	rBV	7135457	6149303	45.46%	9.220%
12	11.428	1584	1588	1591	rBV	3634042	3253905	24.05%	4.879%
13	11.945	1673	1676	1681	rBV	123619	136119	1.01%	0.204%
14	13.016	1853	1858	1861	rBV	10497089	9539194	70.52%	14.302%
15	14.063	2032	2036	2044	rBV	1643225	1481477	10.95%	2.221%
16	15.545	2282	2288	2300	rBV	998072	1306330	9.66%	1.959%




Sum of corrected areas: 66697575

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060624\
Data File : BF138144.D
Acq On : 06 Jun 2024 20:45
Operator : CG\JU
Sample : P2718-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

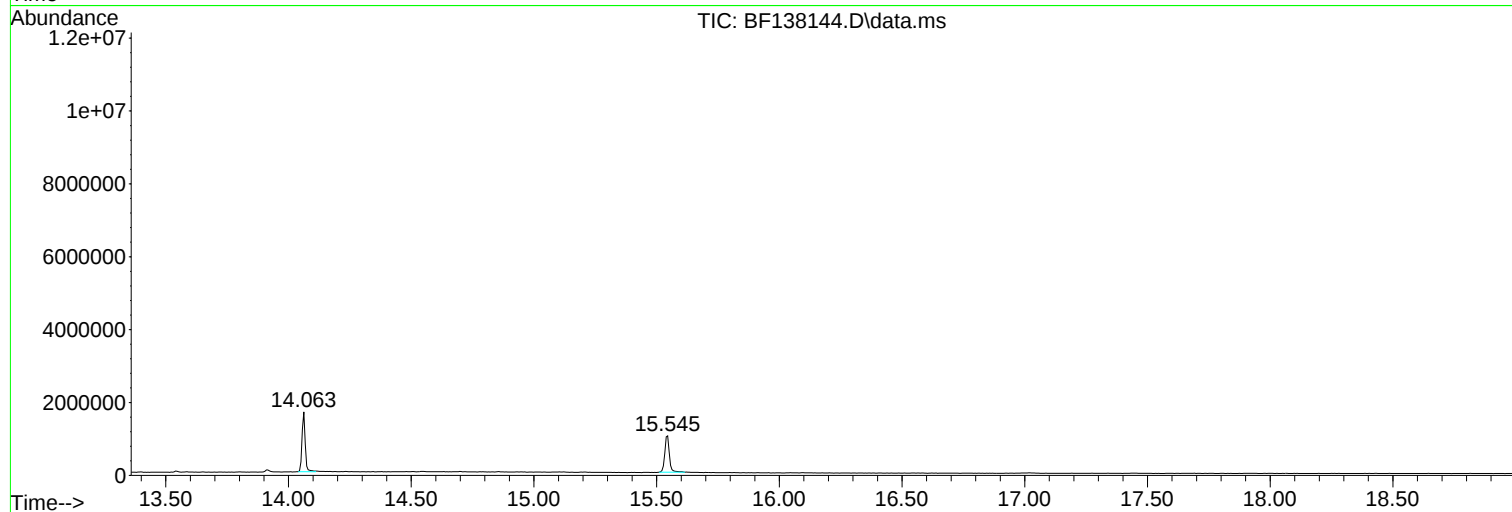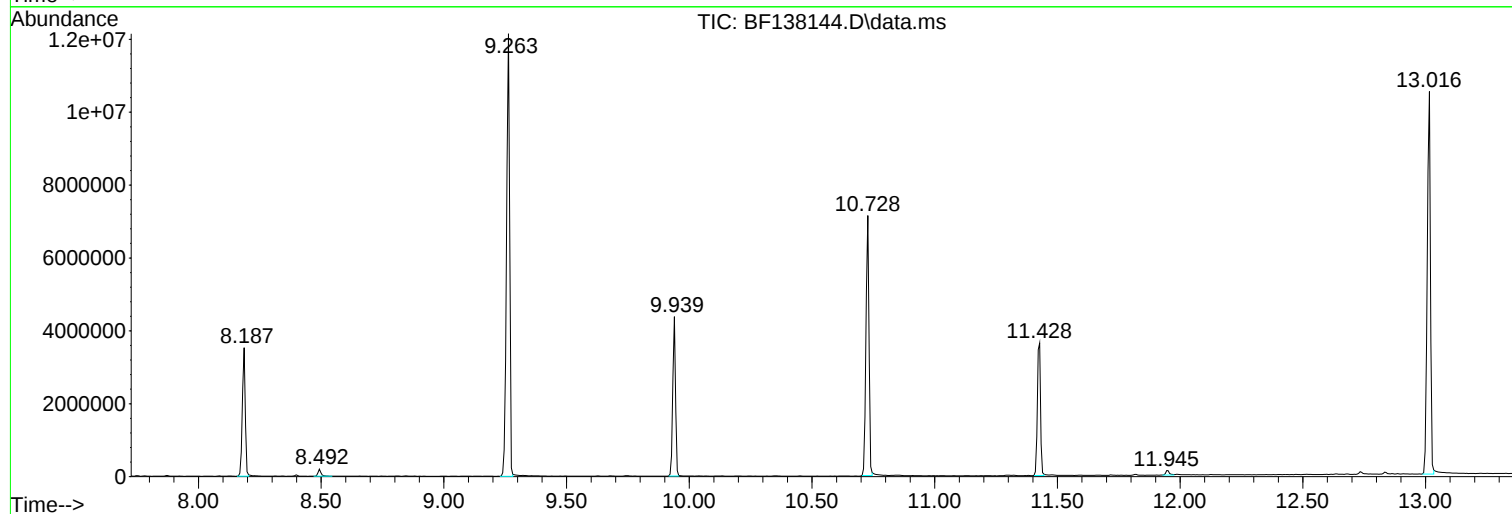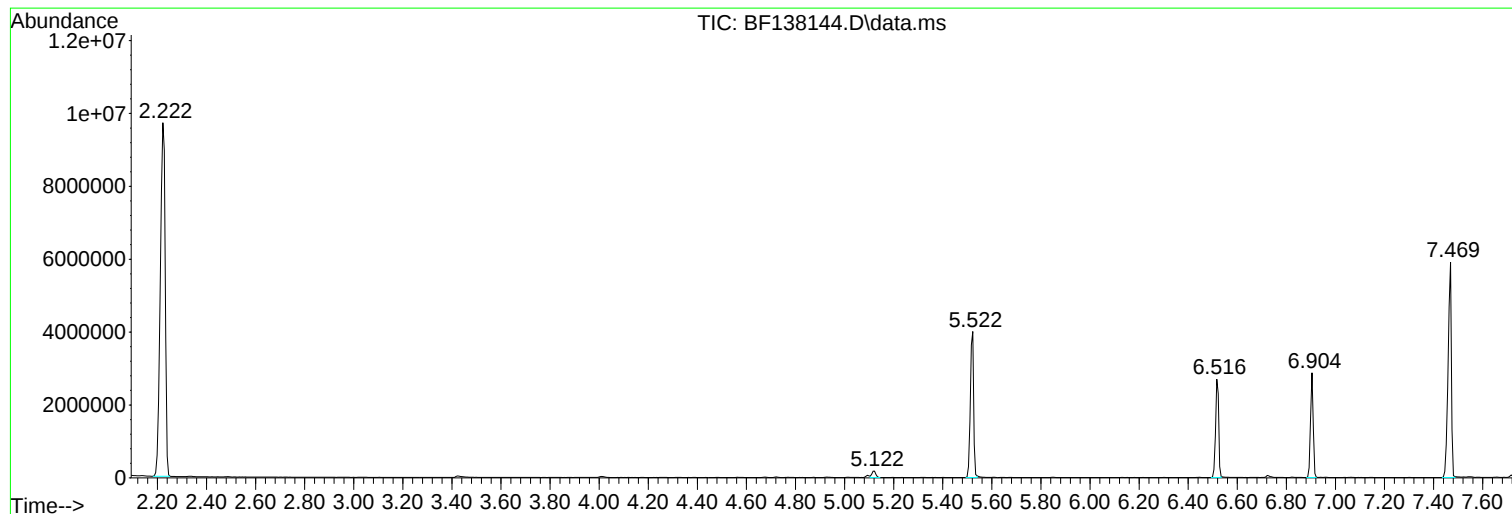

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060624\
Data File : BF138144.D
Acq On : 06 Jun 2024 20:45
Operator : CG\JU
Sample : P2718-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.222	124.06 ng	13527600	1,4-Dichlorobenzene-d4	6.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	27
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
5			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	17

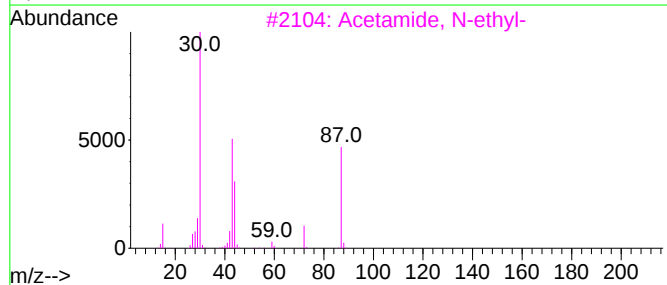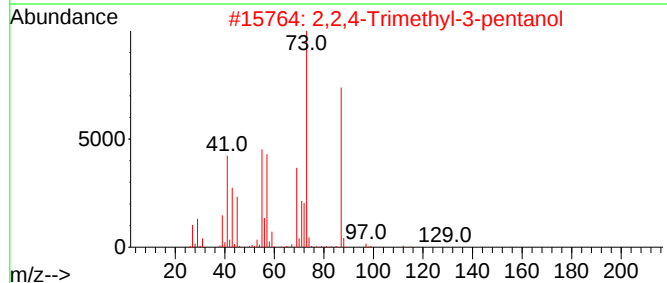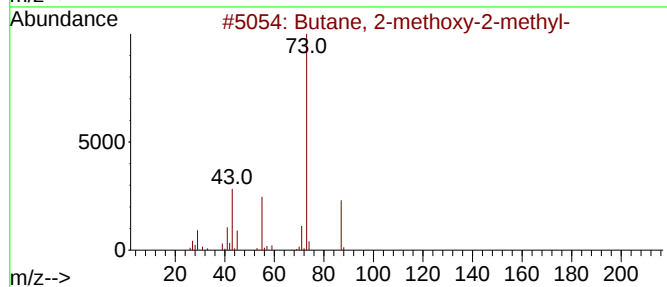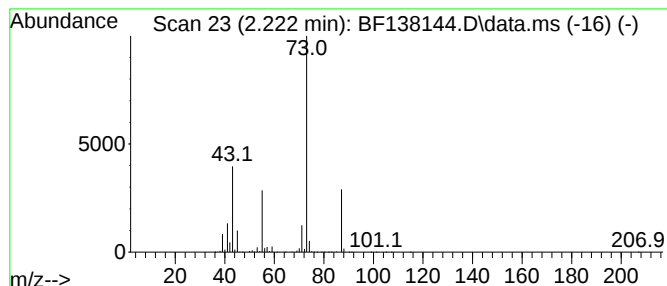

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060624\
Data File : BF138144.D
Acq On : 06 Jun 2024 20:45
Operator : CG\JU
Sample : P2718-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.222	124.1	ng	13527600	1	6.904	2180830	20.0