
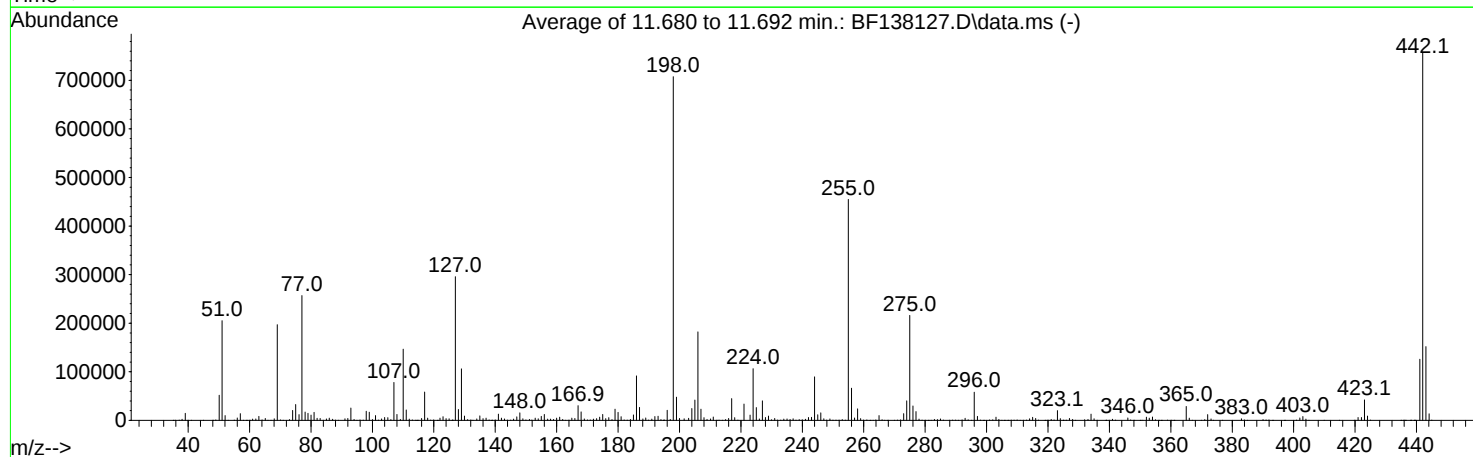


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060624\
Data File : BF138127.D
Acq On : 06 Jun 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 06 05:19:29 2024

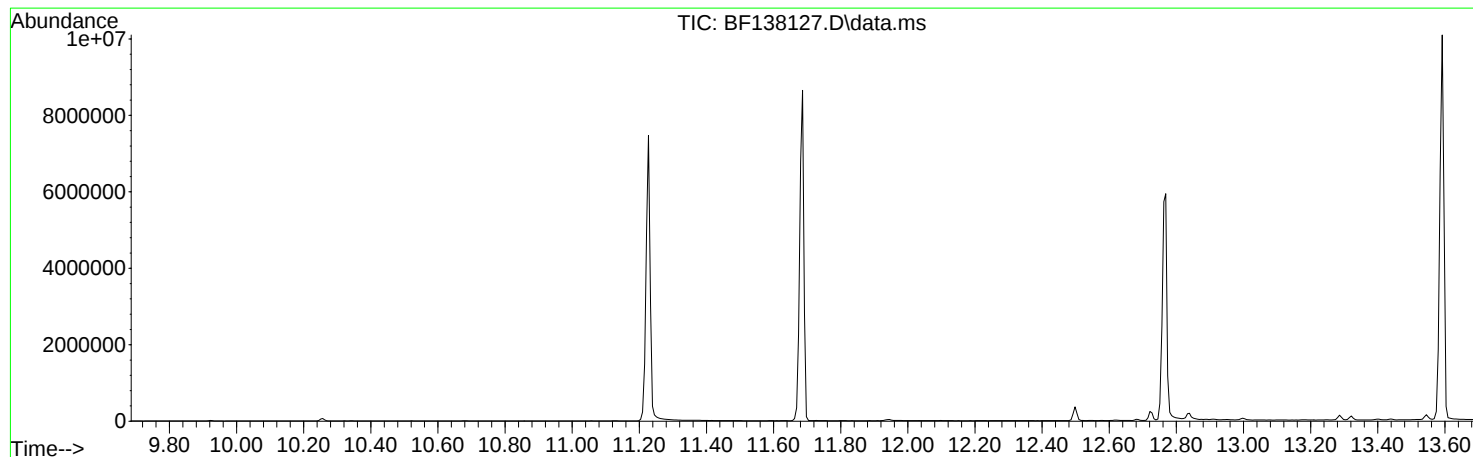




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	205341	PASS
68	69	0.00	2	1.7	3293	PASS
69	198	0.00	100	27.9	197085	PASS
70	69	0.00	2	0.4	864	PASS
127	198	10	80	41.8	295765	PASS
197	198	0.00	2	0.3	2090	PASS
198	198	100	100	100.0	707392	PASS
199	198	5	9	6.7	47718	PASS
275	198	10	60	30.5	215997	PASS
365	198	1	100	4.1	28723	PASS
441	198	0.01	100	17.8	126000	PASS
442	442	50	100	100.0	757248	PASS
443	442	15	24	20.1	151955	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060624\
Data File : BF138127.D
Acq On : 06 Jun 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 06 12:18:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

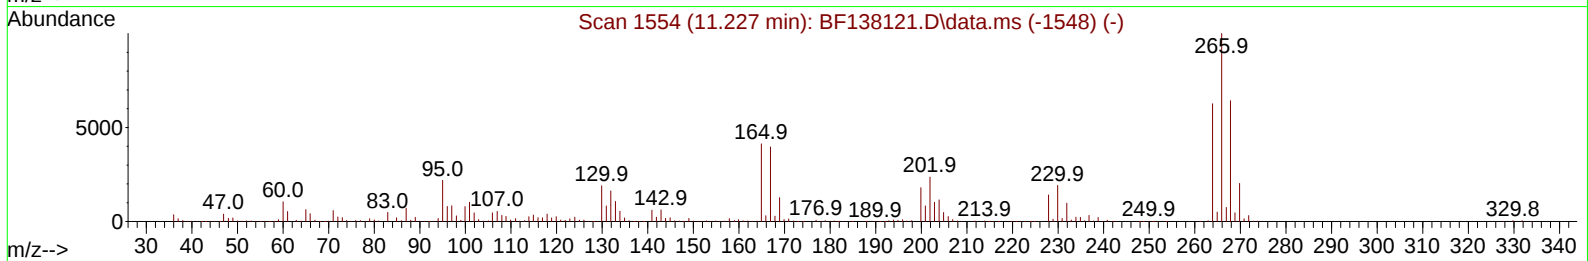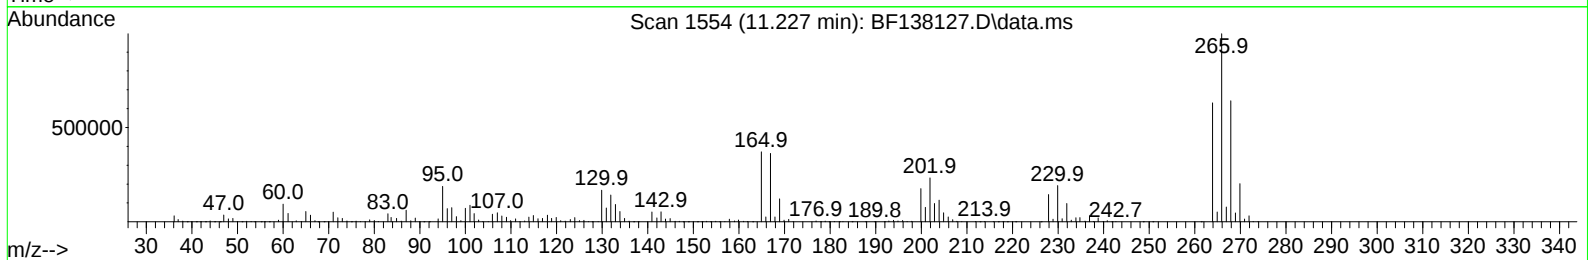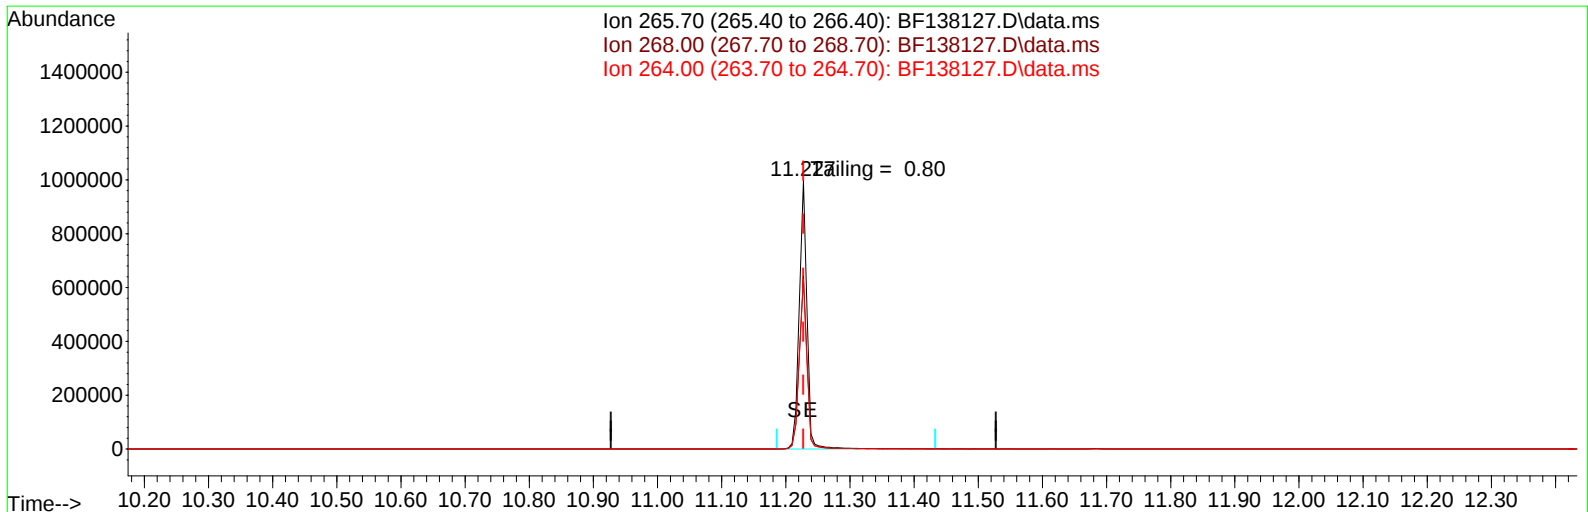

TIC: BF138127.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 412608.57 ng




response 847890

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.38
264.00	62.60	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060624\
Data File : BF138127.D
Acq On : 06 Jun 2024 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 06 12:18:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 06 05:19:29 2024
Response via : Initial Calibration

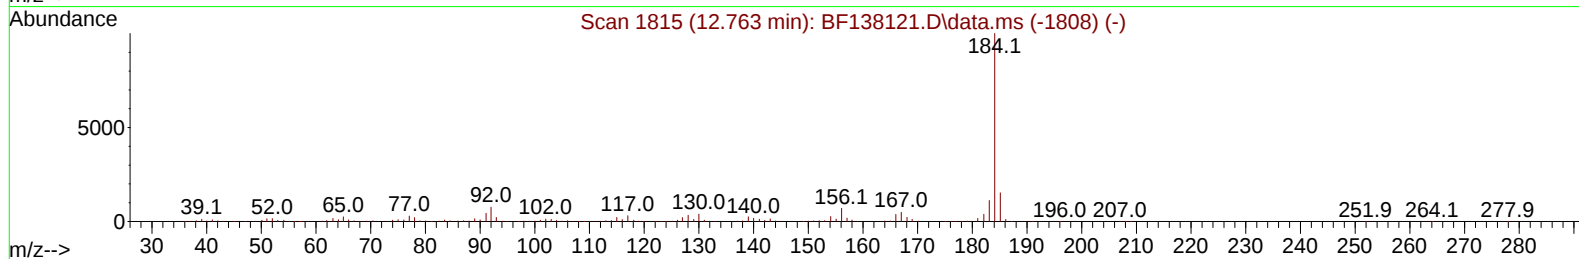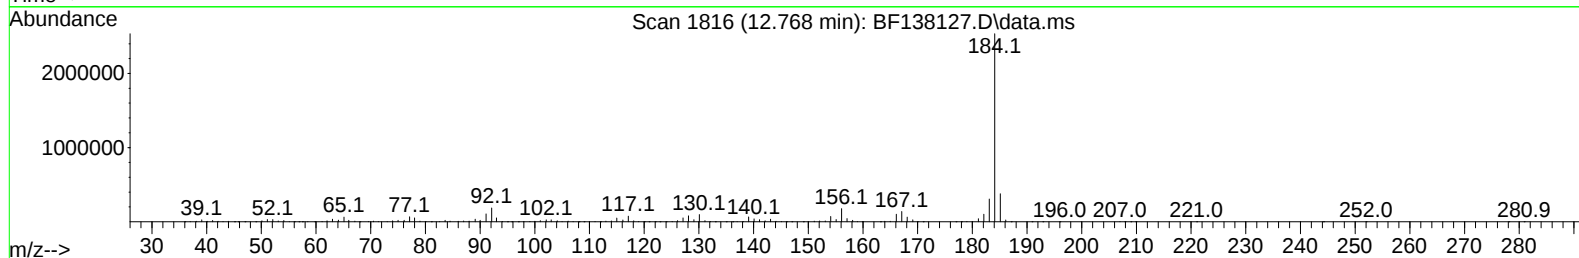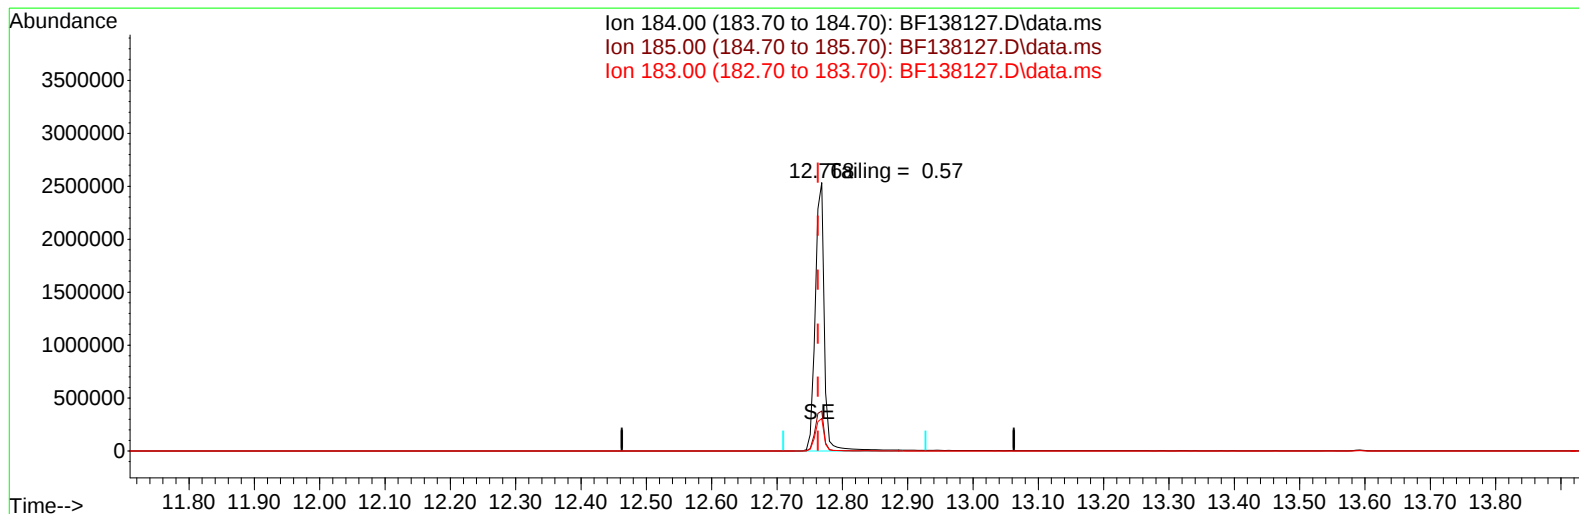

TIC: BF138127.D\data.ms

(77) Benzidine

12.768min (+ 0.006) 32220.96 ng

response 2461602

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.92
183.00	11.20	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2024	BNA_F	<u>BF138127.D</u>
Compound Name	Response	Retention Time
DDT	1687822	13.592
DDD	32580	13.286
DDE	1183	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33763	1721585	1.96

Instrument :
BNA_F
ClientSampleId :
DFTPP