

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060715\
 Data File : BF079813.D
 Acq On : 7 Jun 2015 14:26
 Operator : TP/IZ
 Sample : G2519-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 1505283163

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.347	13	14	16	rVB	16676709	11693804	100.00%	77.203%
2	1.472	20	25	27	rBV2	316435	678848	5.81%	4.482%
3	2.421	104	108	122	rVB2	366976	962543	8.23%	6.355%
4	7.473	548	550	553	rBV	256443	212793	1.82%	1.405%
5	8.765	661	663	666	rBV	316343	276962	2.37%	1.829%
6	10.536	816	818	821	rBV	260393	318494	2.72%	2.103%
7	12.045	948	950	953	rBV	285267	332830	2.85%	2.197%
8	14.994	1206	1208	1211	rBV	355145	356864	3.05%	2.356%
9	16.925	1374	1377	1382	rBV	201059	313636	2.68%	2.071%


Sum of corrected areas: 15146774

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060715\
Data File : BF079813.D
Acq On : 7 Jun 2015 14:26
Operator : TP/IZ
Sample : G2519-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1505283163

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

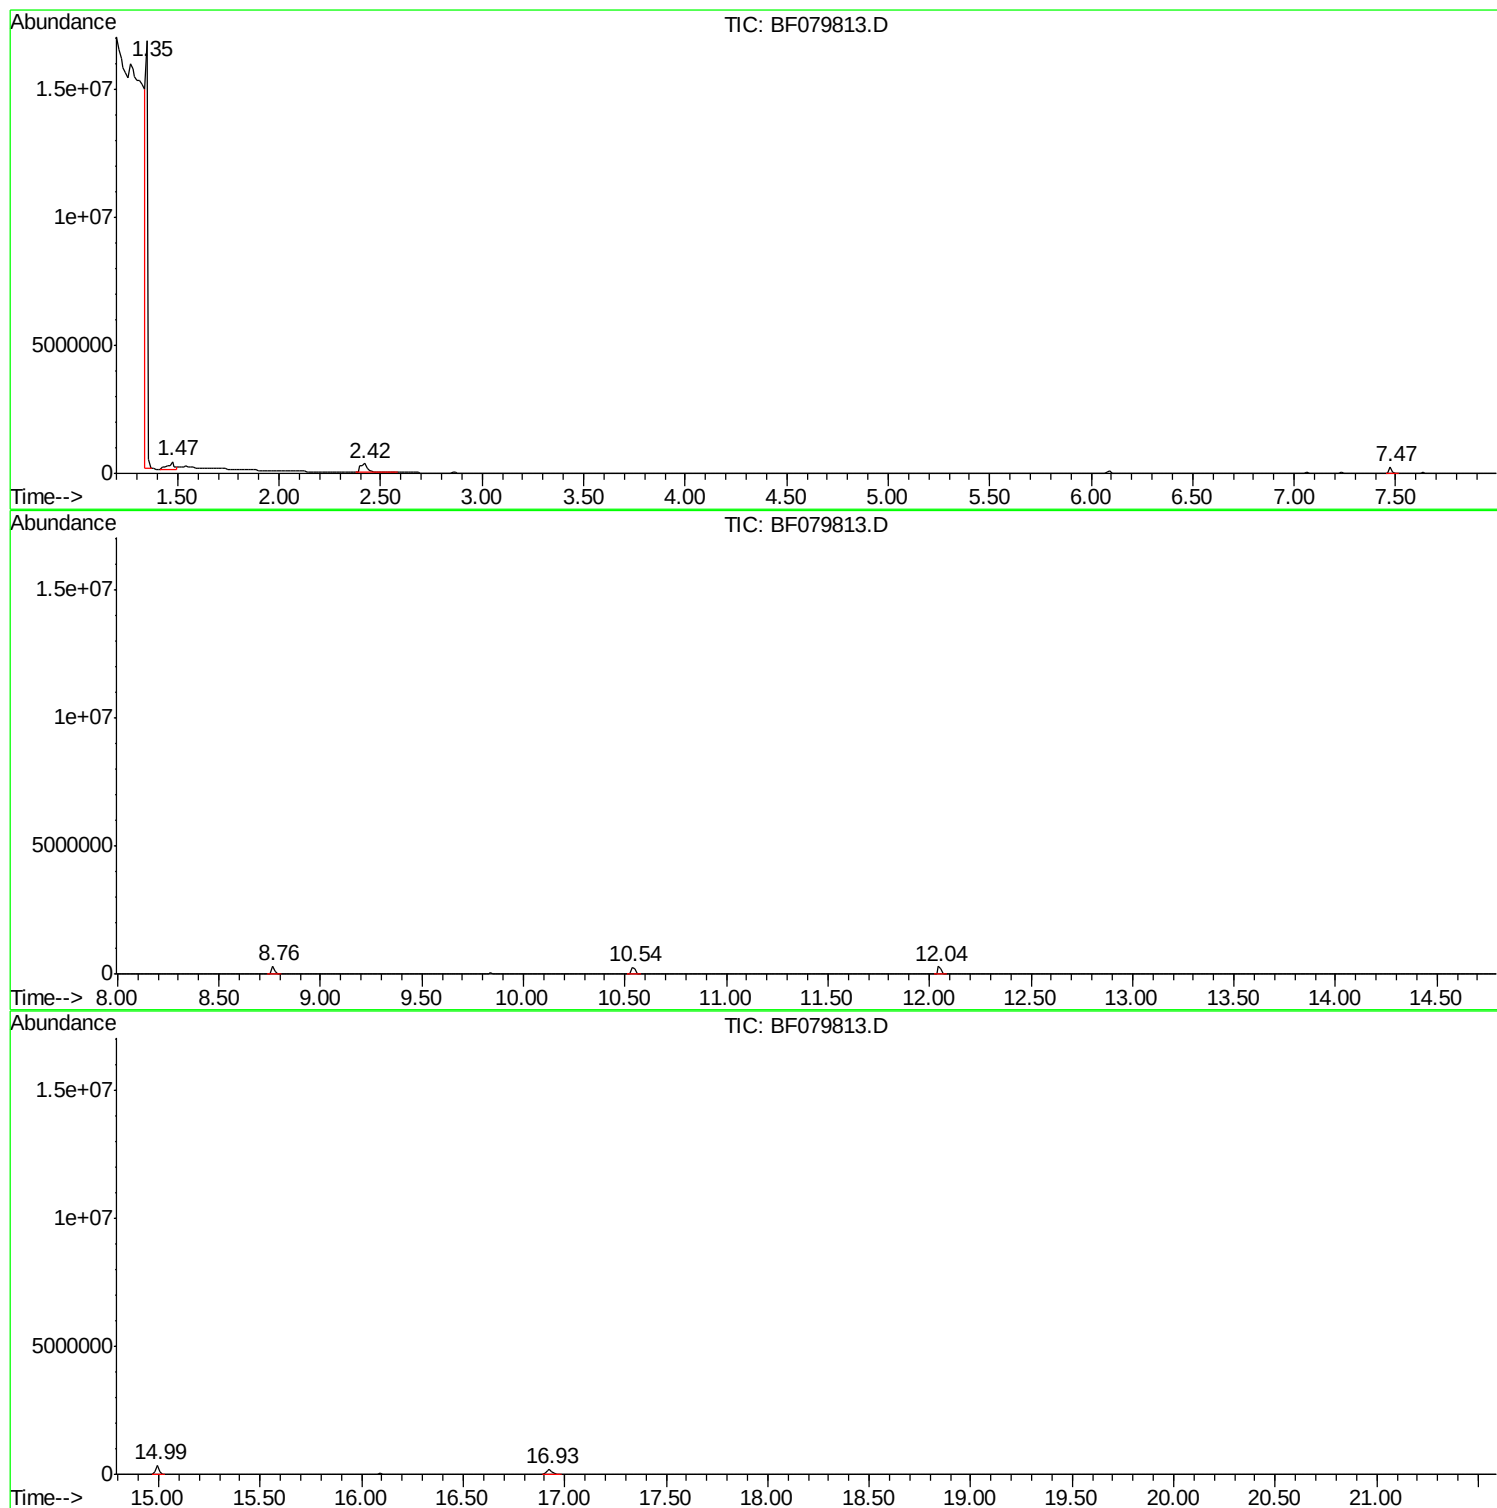

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060715\
Data File : BF079813.D
Acq On : 7 Jun 2015 14:26
Operator : TP/IZ
Sample : G2519-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1505283163










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethene, 1,2-dichloro-, (E)- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.47	63.80 ng	678848	1,4-Dichlorobenzene-d4	7.47

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethene, 1,2-dichloro-, (E)-	96	C2H2Cl2	000156-60-5	90
2			Ethene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	90
3			1,2-Dichloroethylene	96	C2H2Cl2	000540-59-0	50
4			Ethene, 1,1-dichloro-	96	C2H2Cl2	000075-35-4	49
5			Chloromethylmethyl sulfide	96	C2H5ClS	002373-51-5	25

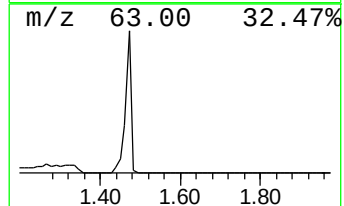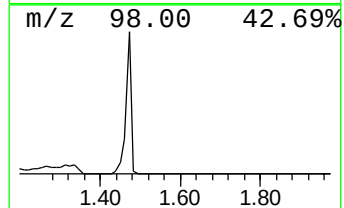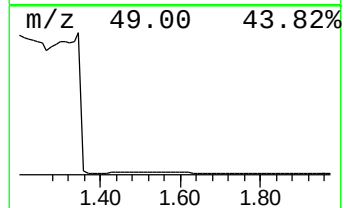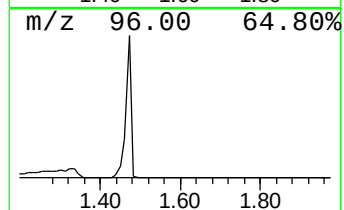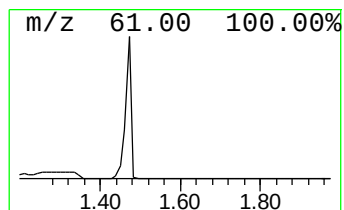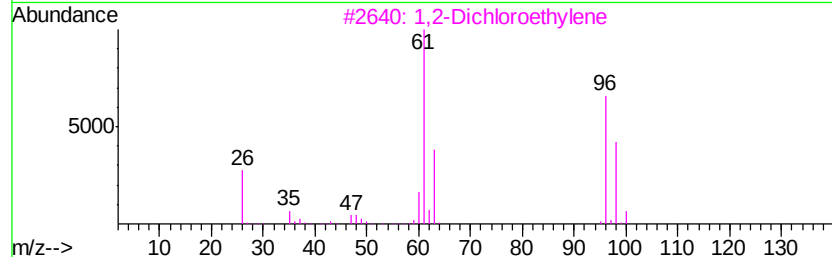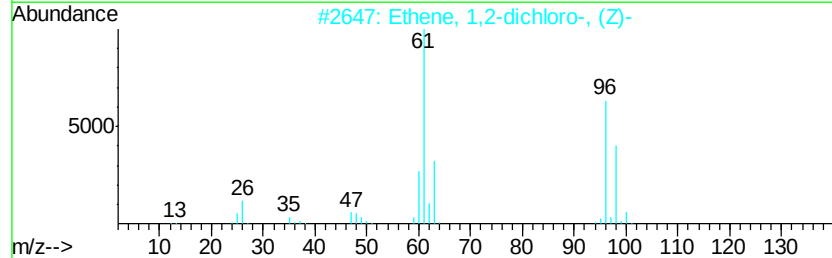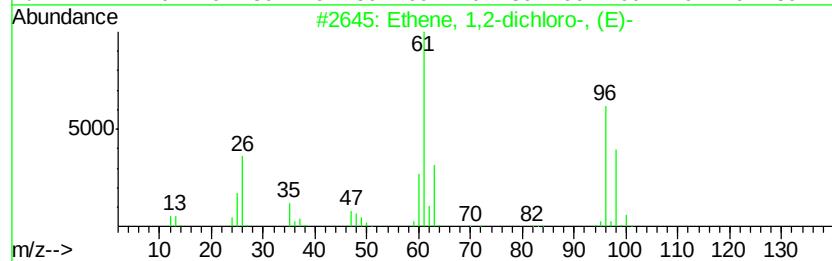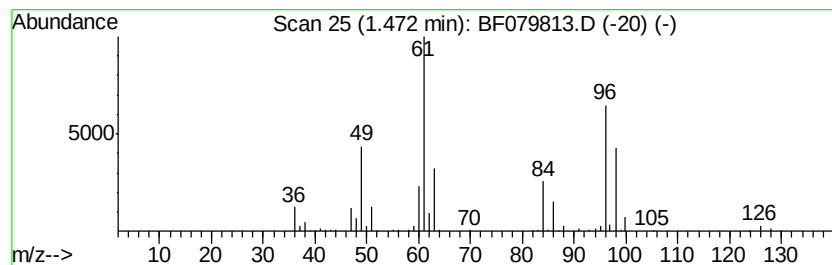

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060715\
Data File : BF079813.D
Acq On : 7 Jun 2015 14:26
Operator : TP/IZ
Sample : G2519-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1505283163

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, 1,2-dichl...	1.47	63.8	ng	678848	1	7.47	212793	20.0