


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060715\
 Data File : BF079791.D
 Acq On : 7 Jun 2015 3:20
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 18:33:51 2015

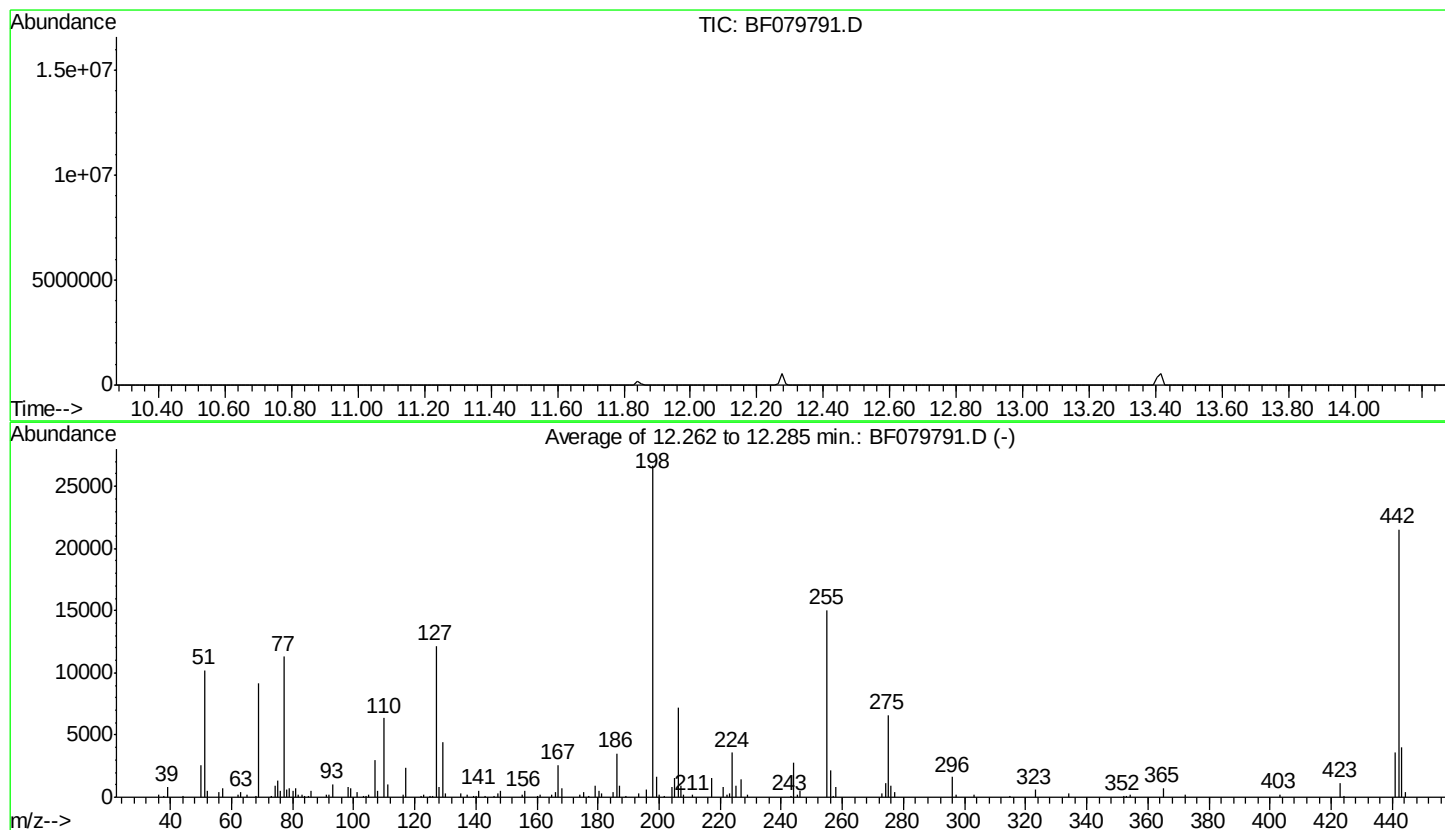

AutoFind: Scans 969, 970, 971; Background Corrected with Scan 966

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	10221	PASS
68	69	0.00	2	1.5	135	PASS
69	198	0.00	100	34.4	9174	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	12200	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26663	PASS
199	198	5	9	6.3	1685	PASS
275	198	10	60	24.9	6632	PASS
365	198	1	100	2.9	774	PASS
441	442	0.01	24	16.7	3592	PASS
442	198	50	100	80.7	21530	PASS
443	442	15	24	18.7	4033	PASS