



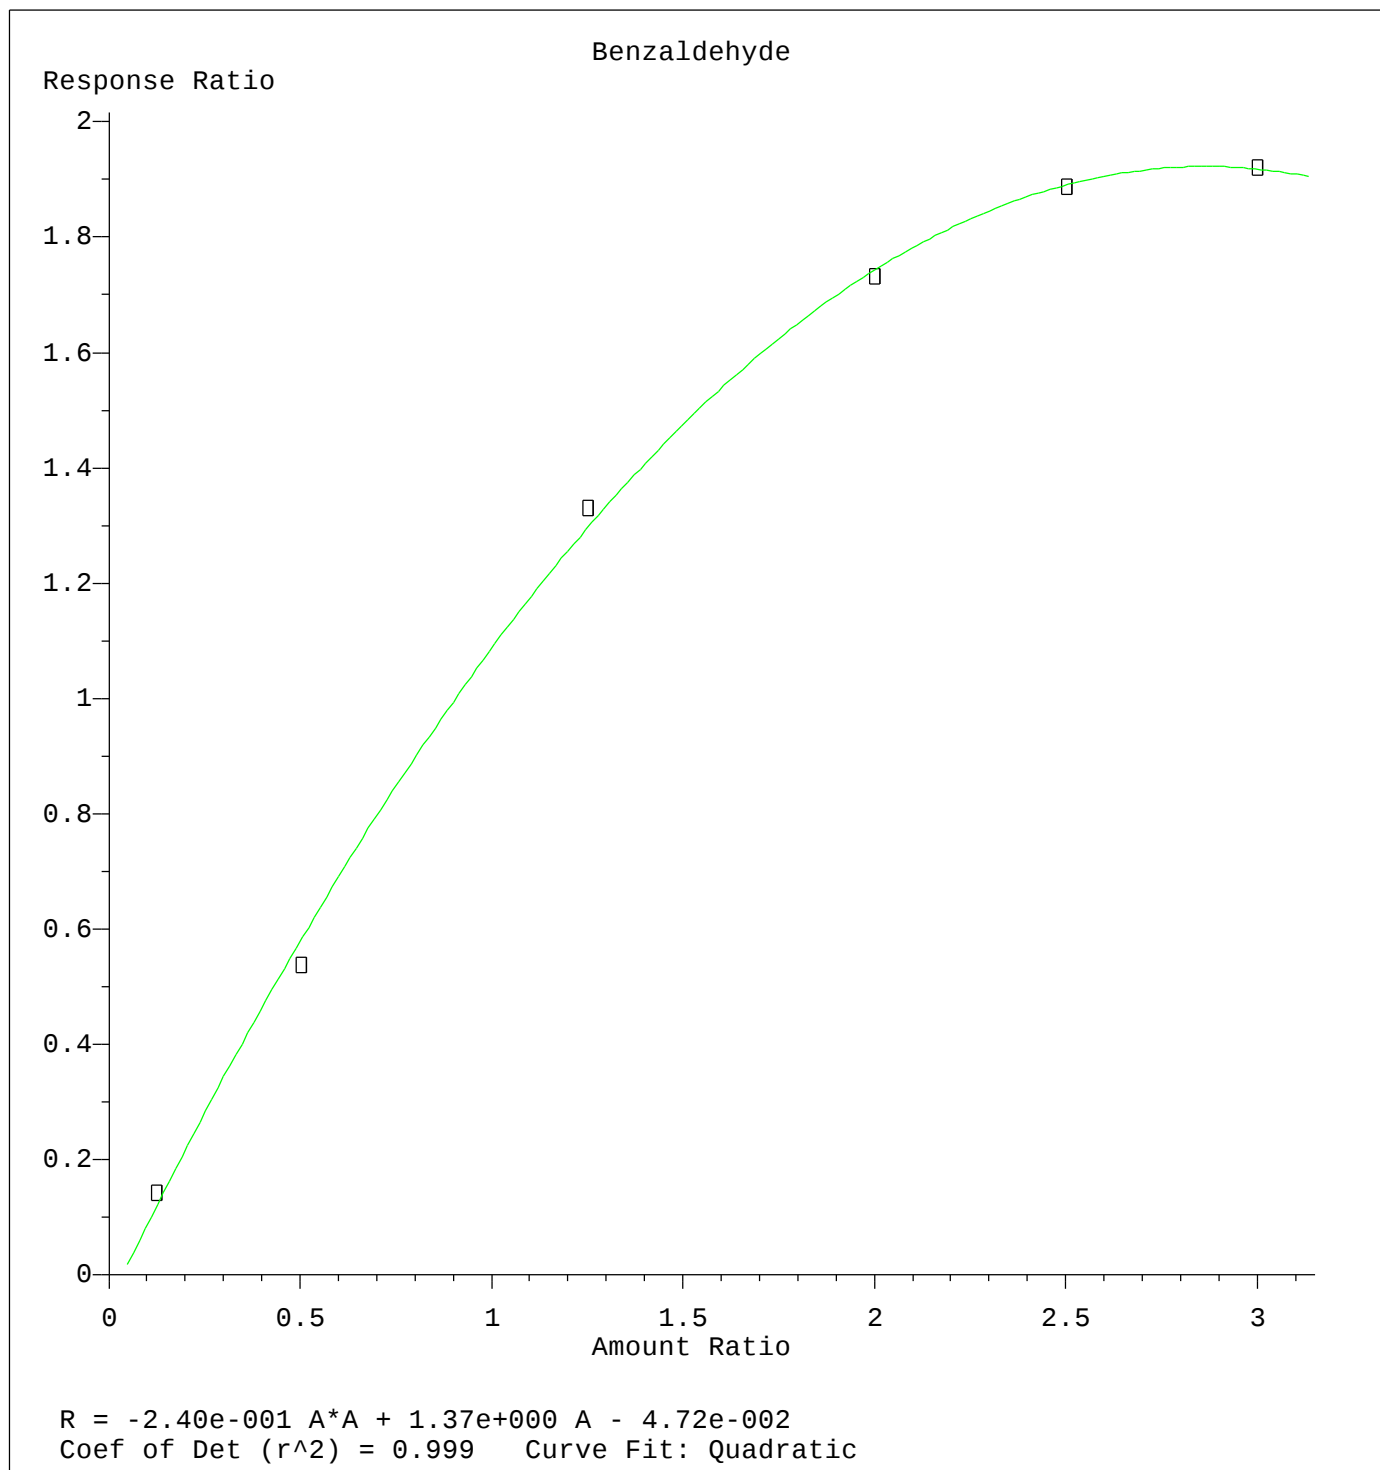


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016

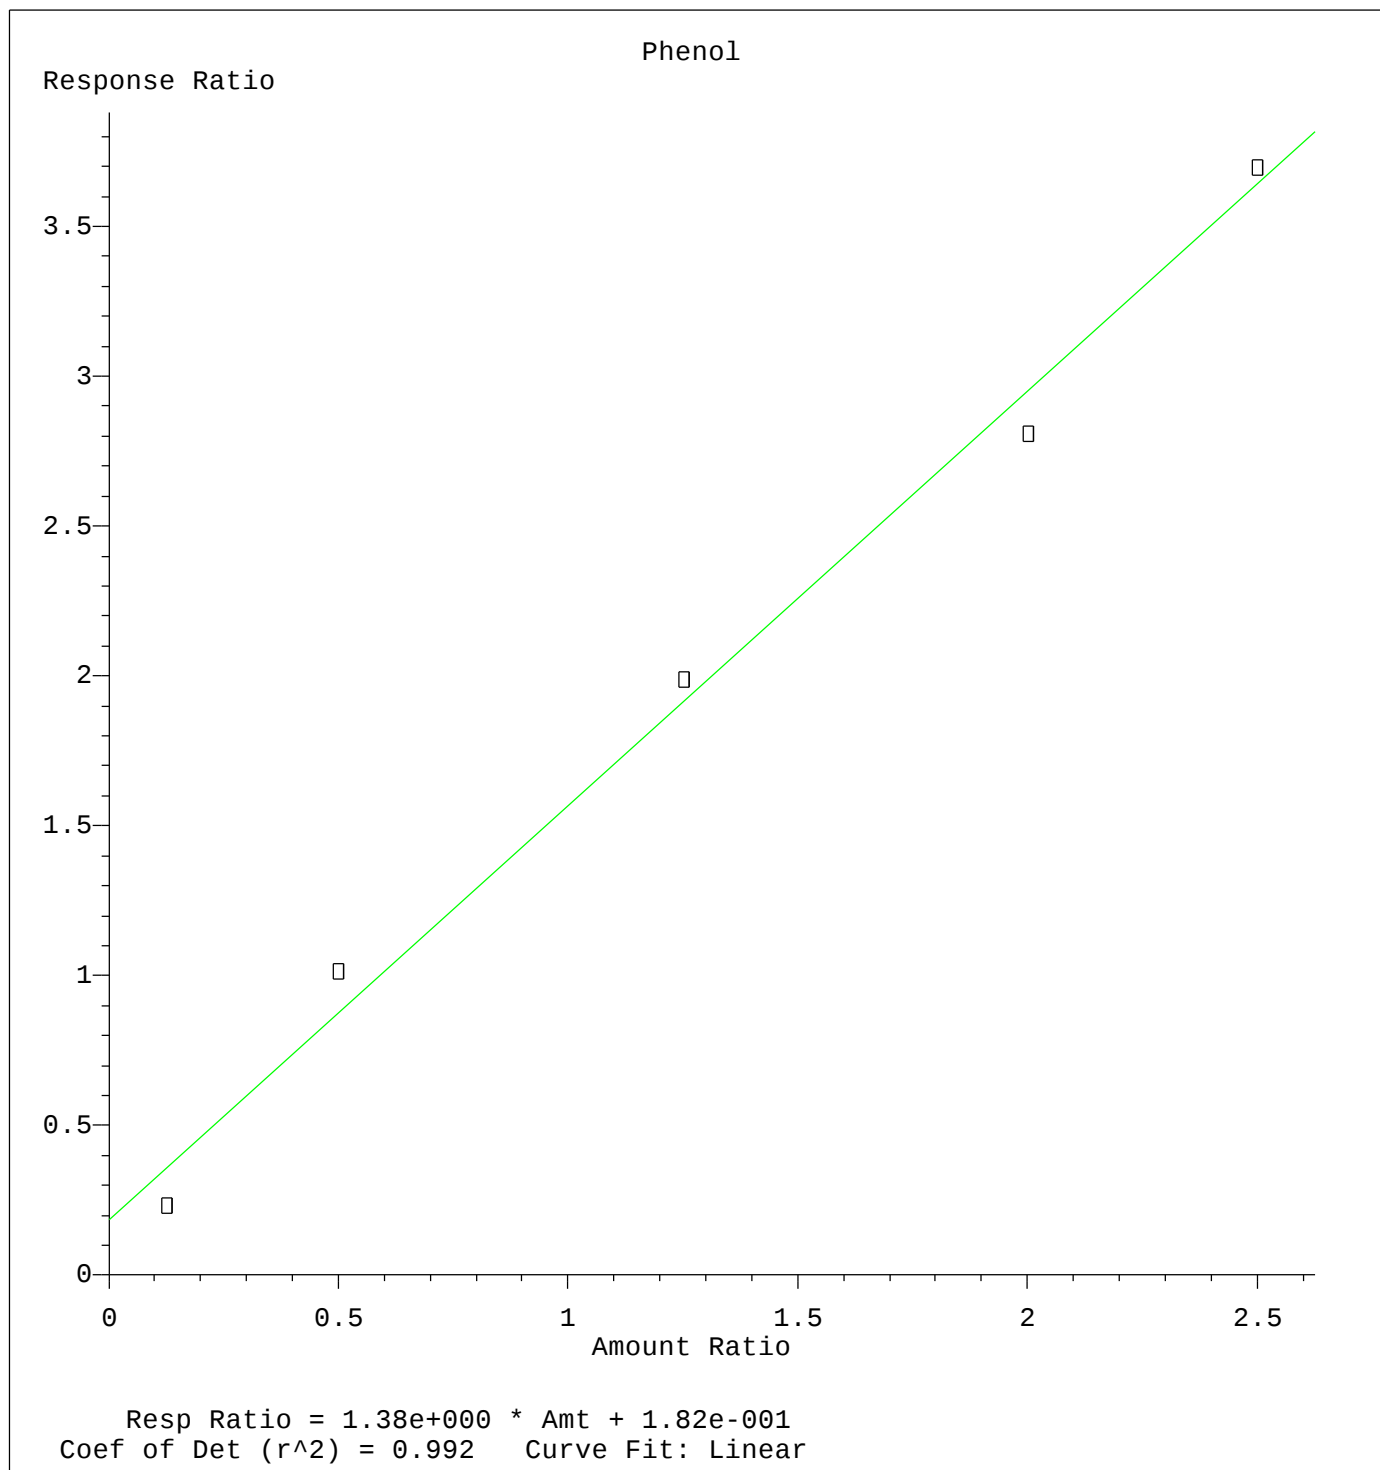

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016

1,2,4,5-Tetrachlorobenzene

Response Ratio

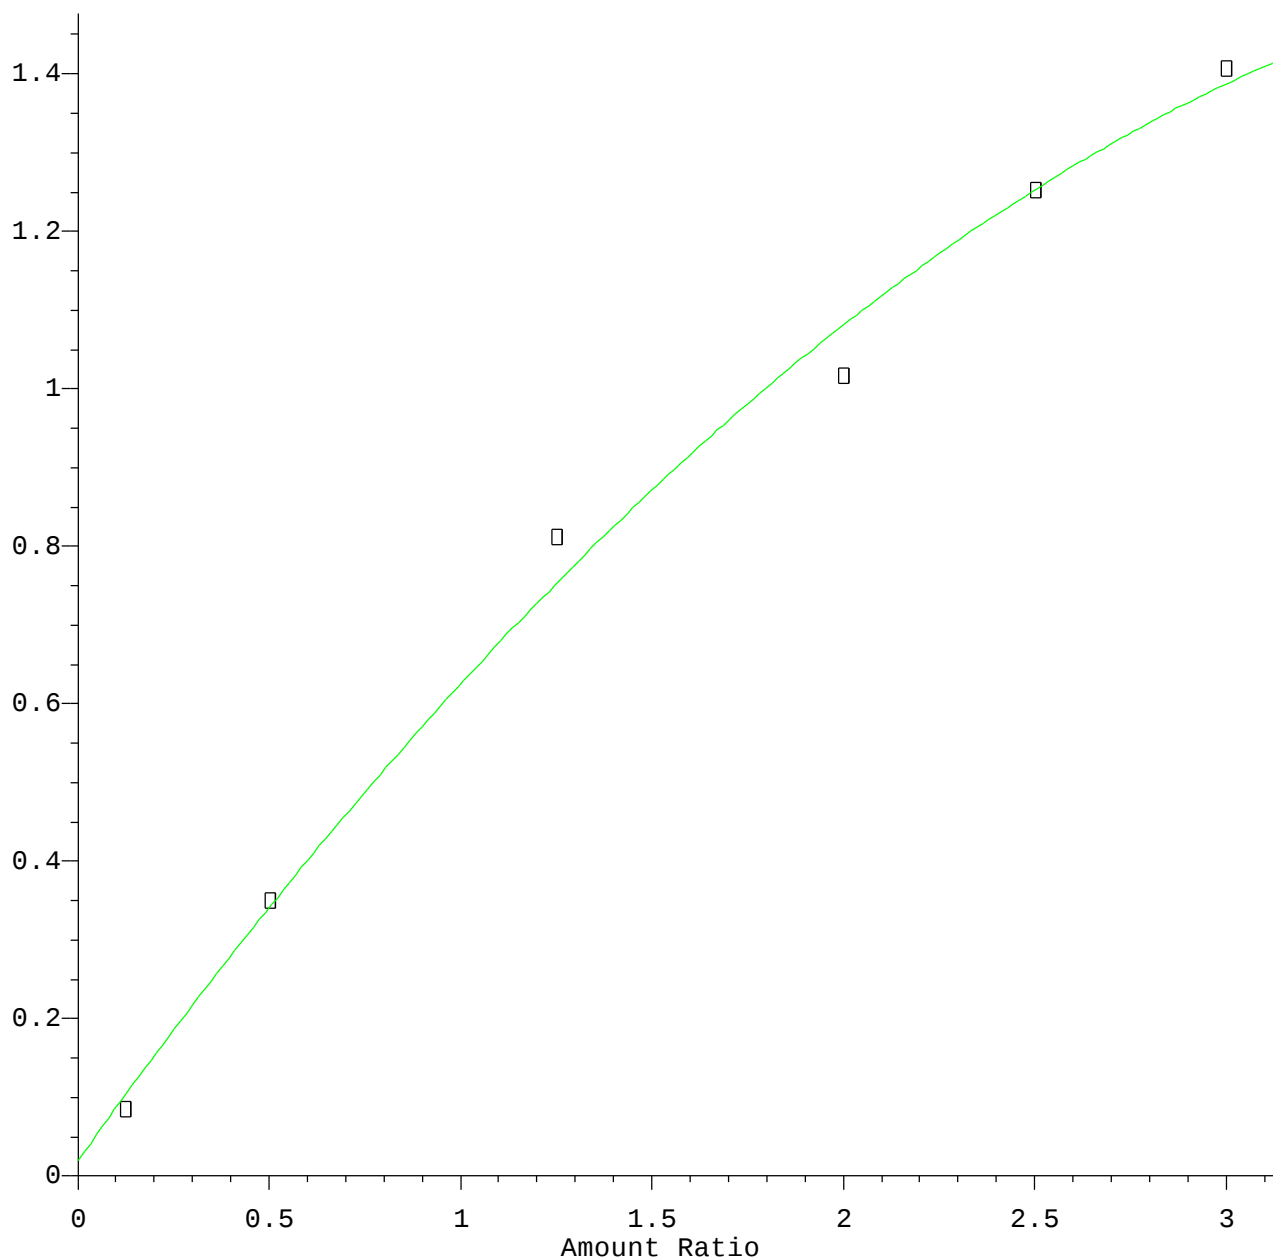


$R = -7.47e-002 A^2 + 6.80e-001 A + 2.02e-002$
Coef of Det (r^2) = 0.994 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016


2-Fluorobiphenyl

Response Ratio

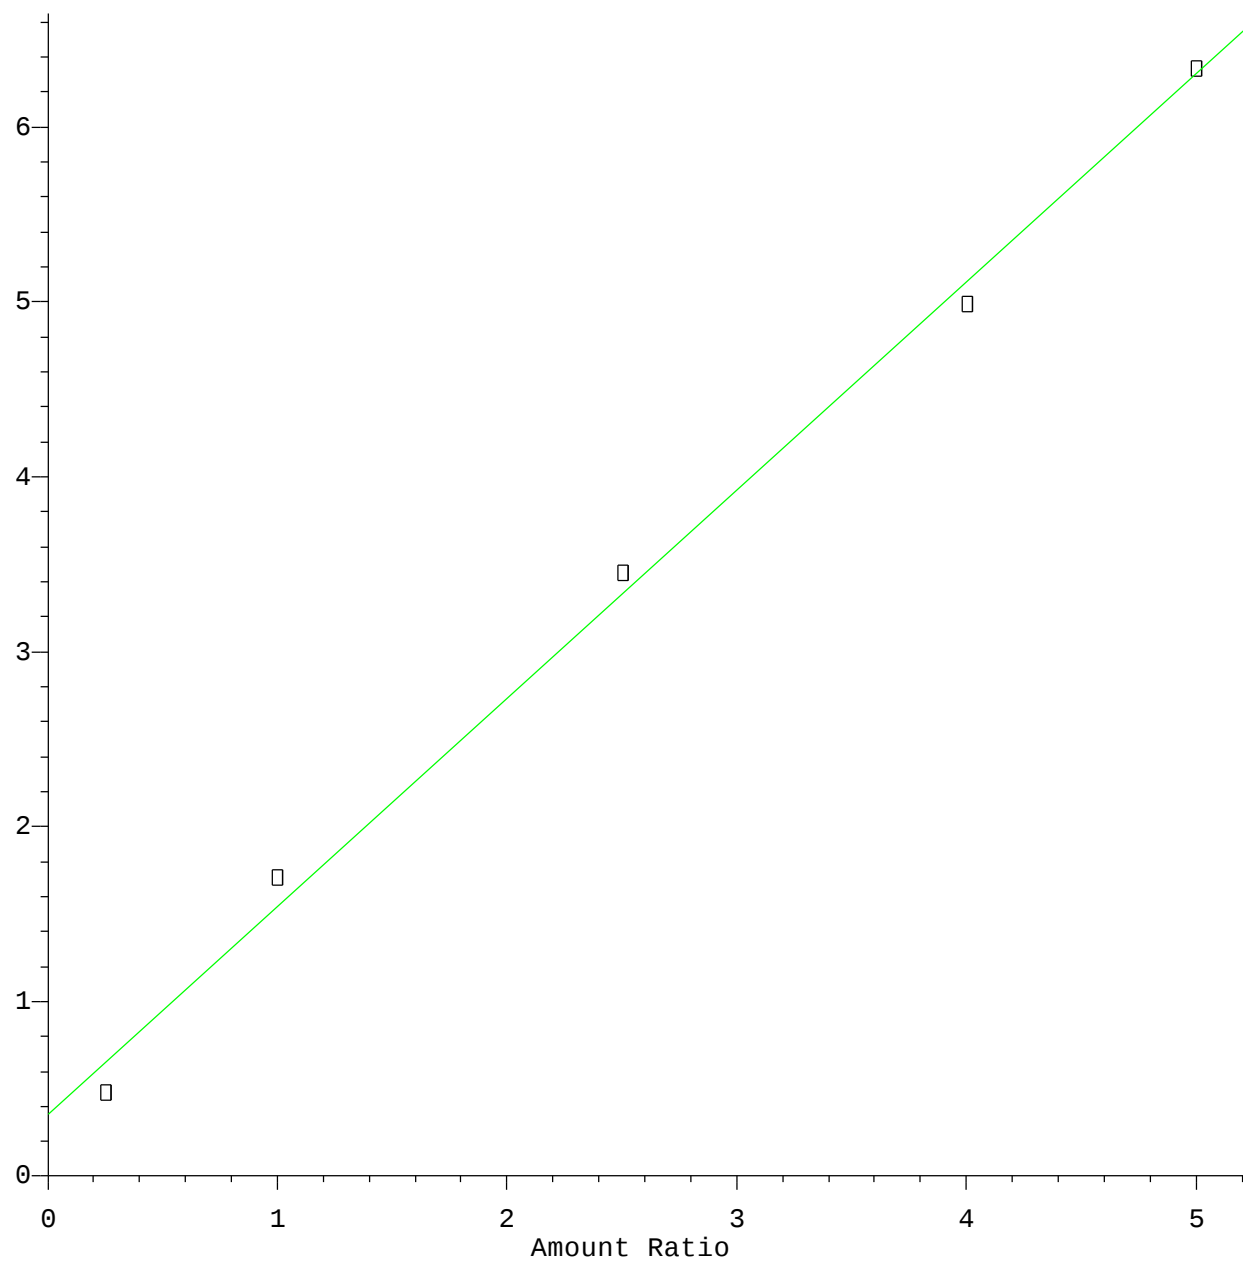


Resp Ratio = 1.19e+000 * Amt + 3.52e-001
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016

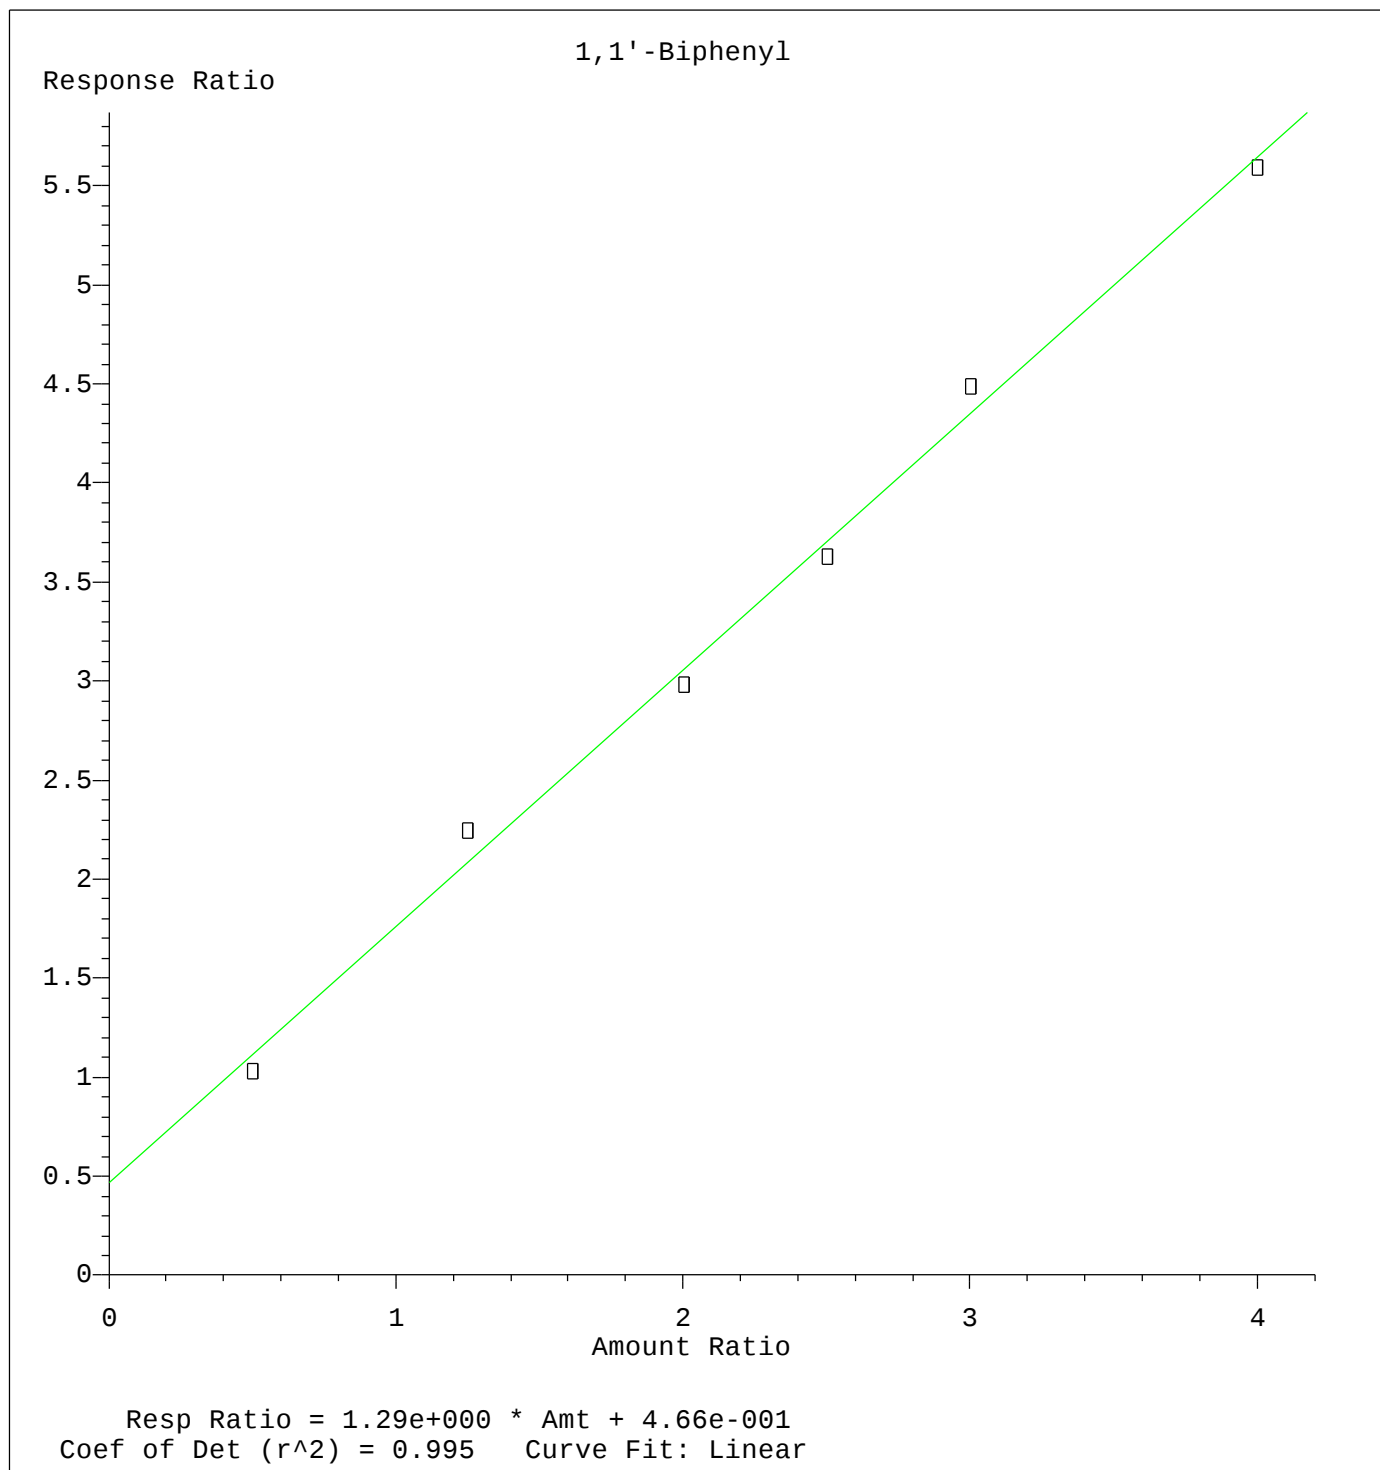

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016

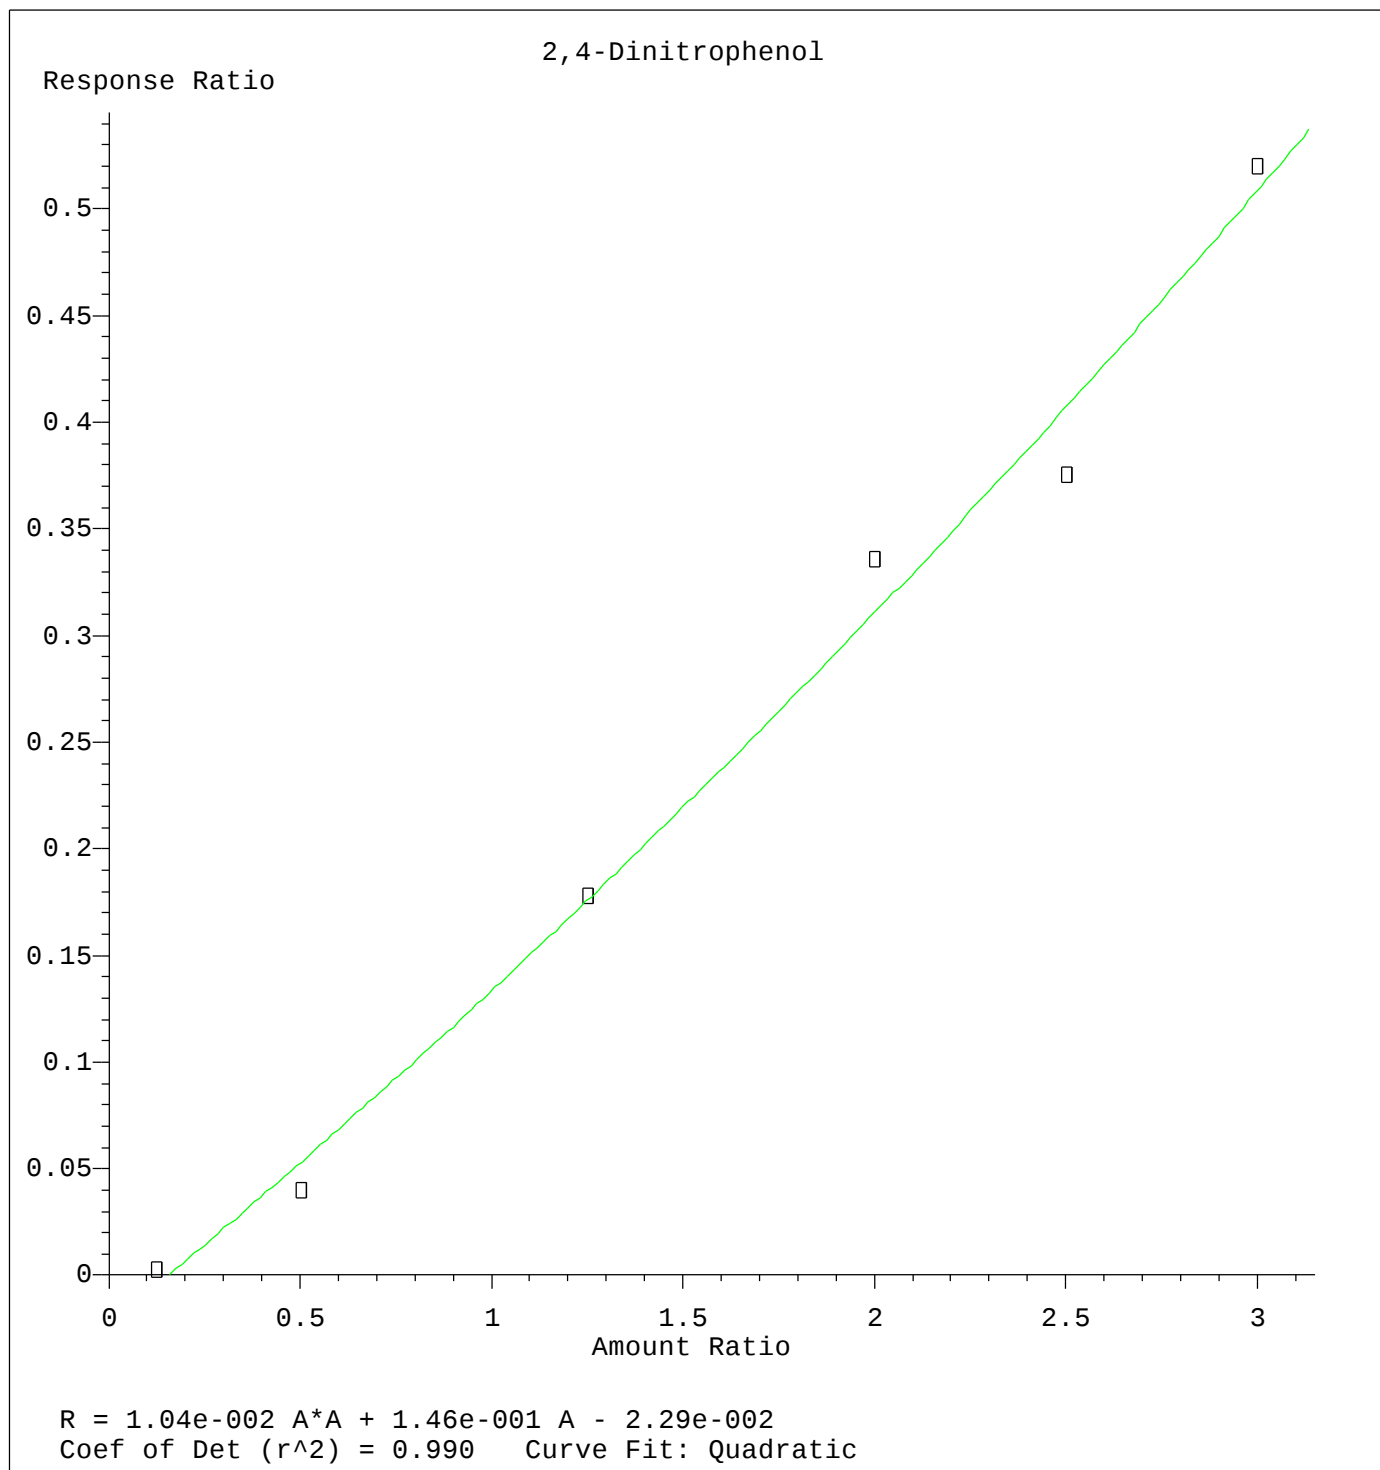


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016

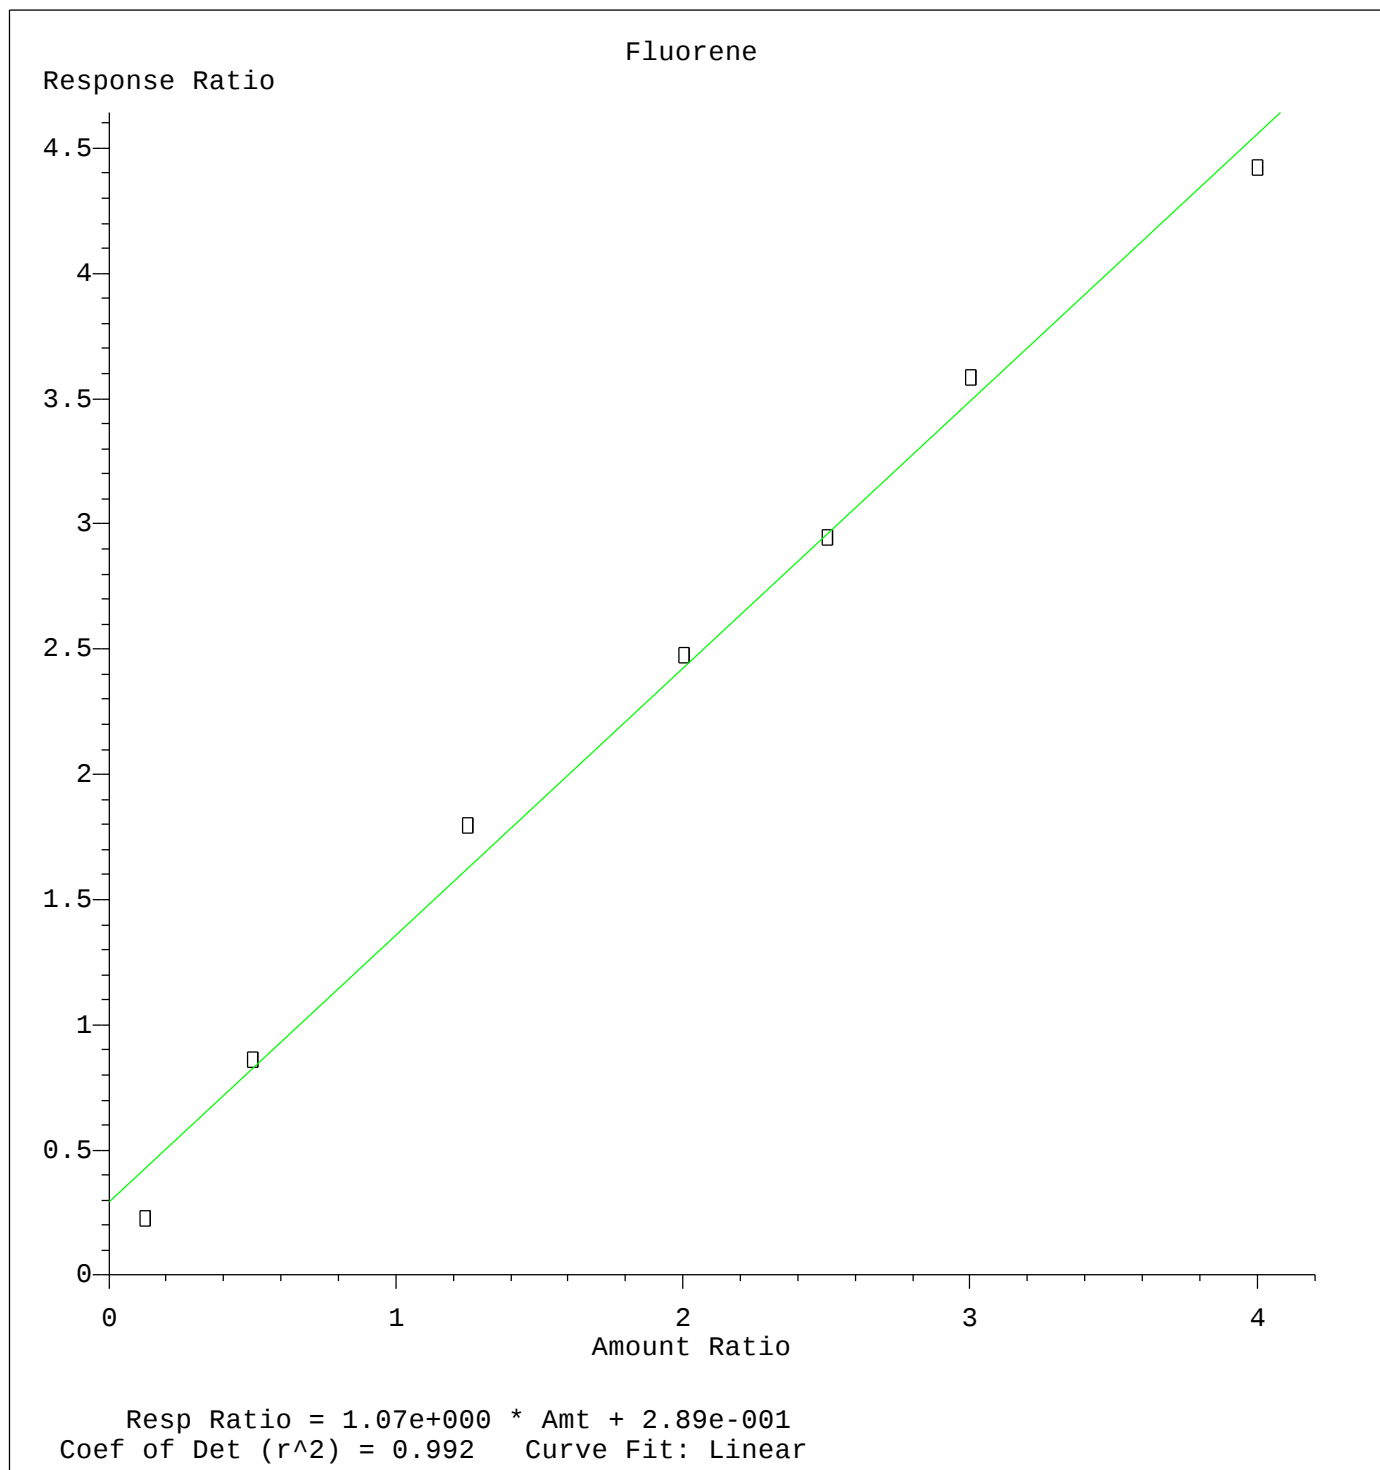

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016

4,6-Dinitro-2-methylphenol

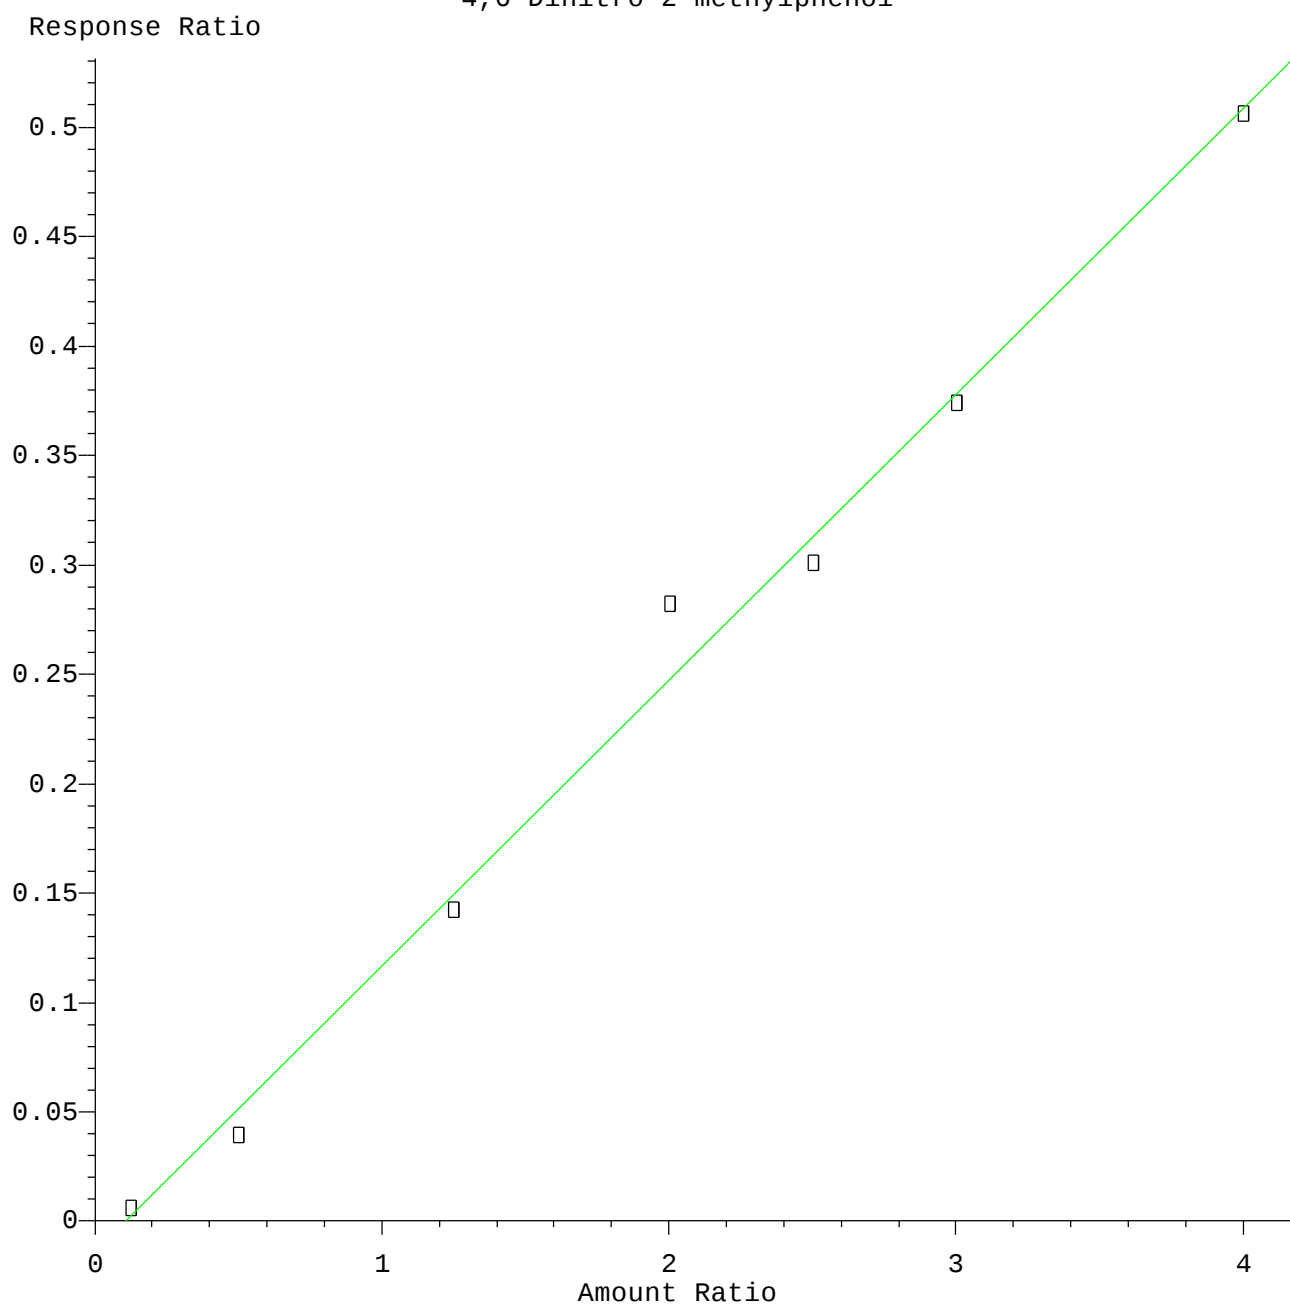

Resp Ratio = $1.31 \times 10^{-1} \times \text{Amt} - 1.41 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Calibration Table Last Updated: Tue Jun 07 18:51:55 2016