


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060716\
 Data File : BF087786.D
 Acq On : 7 Jun 2016 12:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 07 18:51:55 2016

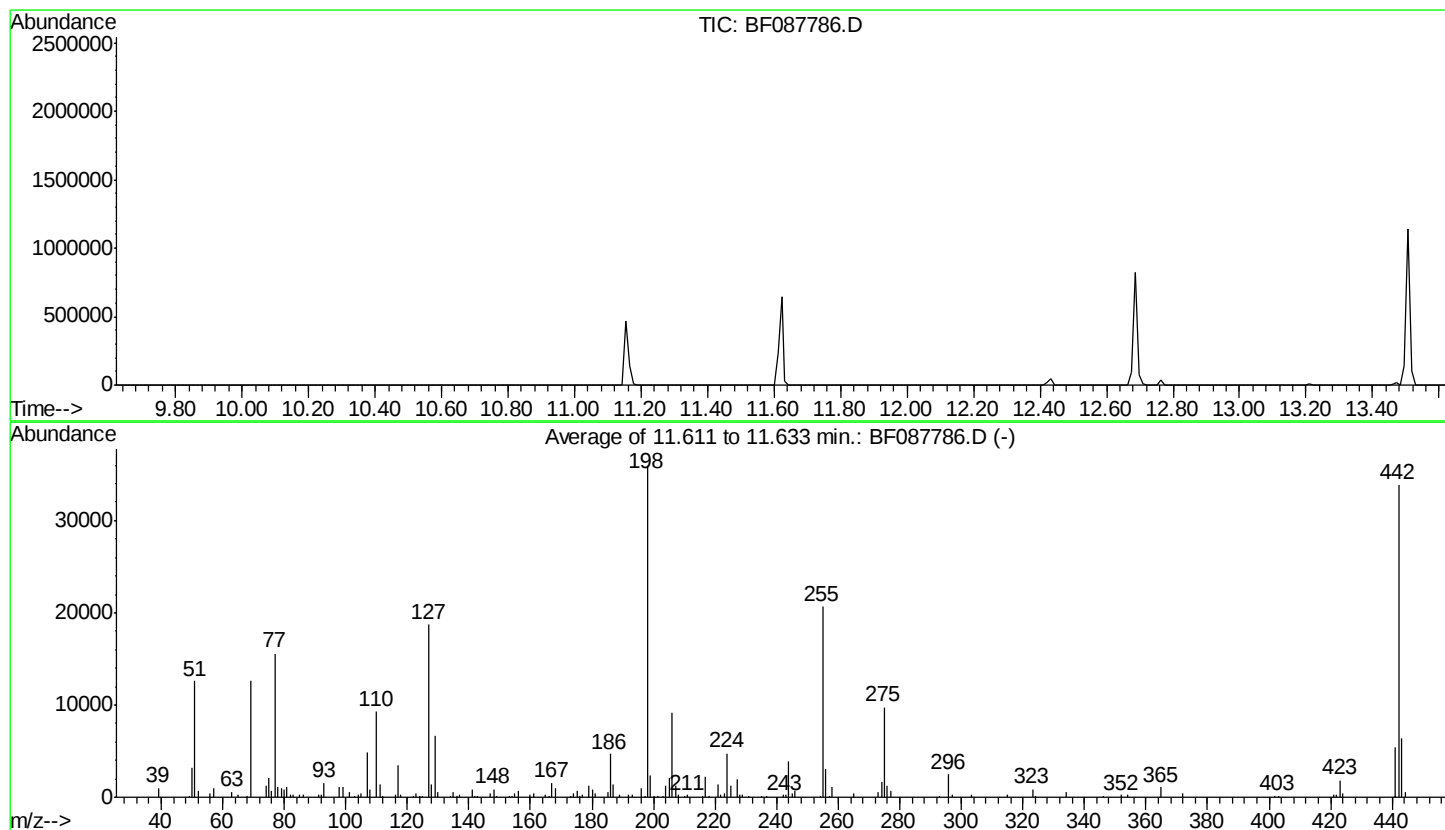

AutoFind: Scans 877, 878, 879; Background Corrected with Scan 874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	12584	PASS
68	69	0.00	2	0.9	117	PASS
69	198	0.00	100	35.3	12685	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	18693	PASS
197	198	0.00	2	0.6	209	PASS
198	198	100	100	100.0	35951	PASS
199	198	5	9	6.6	2364	PASS
275	198	10	60	27.2	9784	PASS
365	198	1	100	2.9	1052	PASS
441	442	0.01	24	15.8	5348	PASS
442	198	50	100	94.4	33923	PASS
443	442	15	24	18.7	6354	PASS