
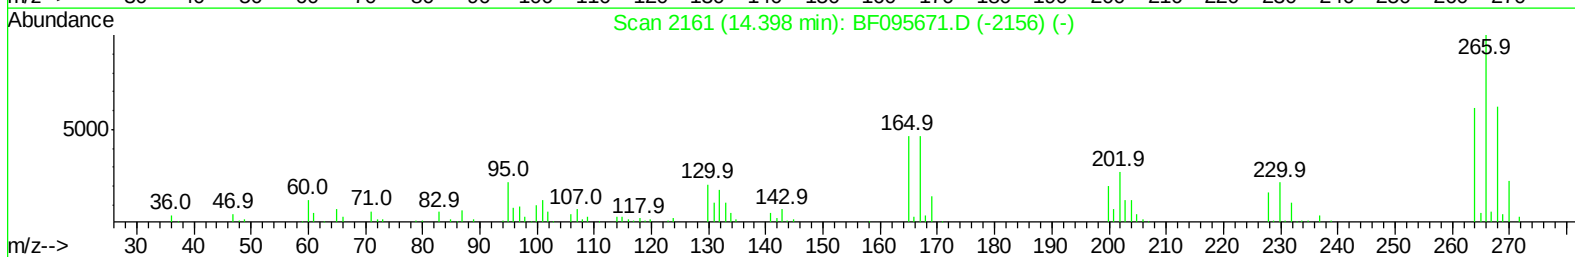
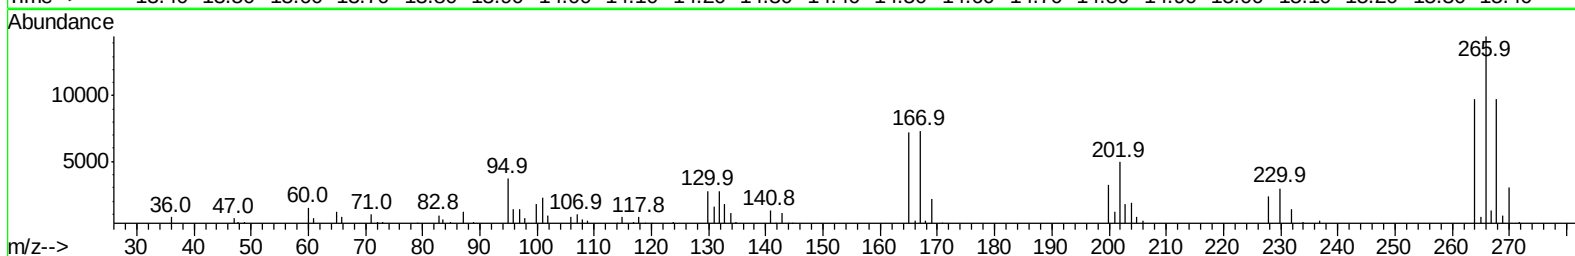


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060717\
Data File : BF095743.D
Acq On : 7 Jun 2017 13:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 15:01:40 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:19:45 2017
Response via : Initial Calibration

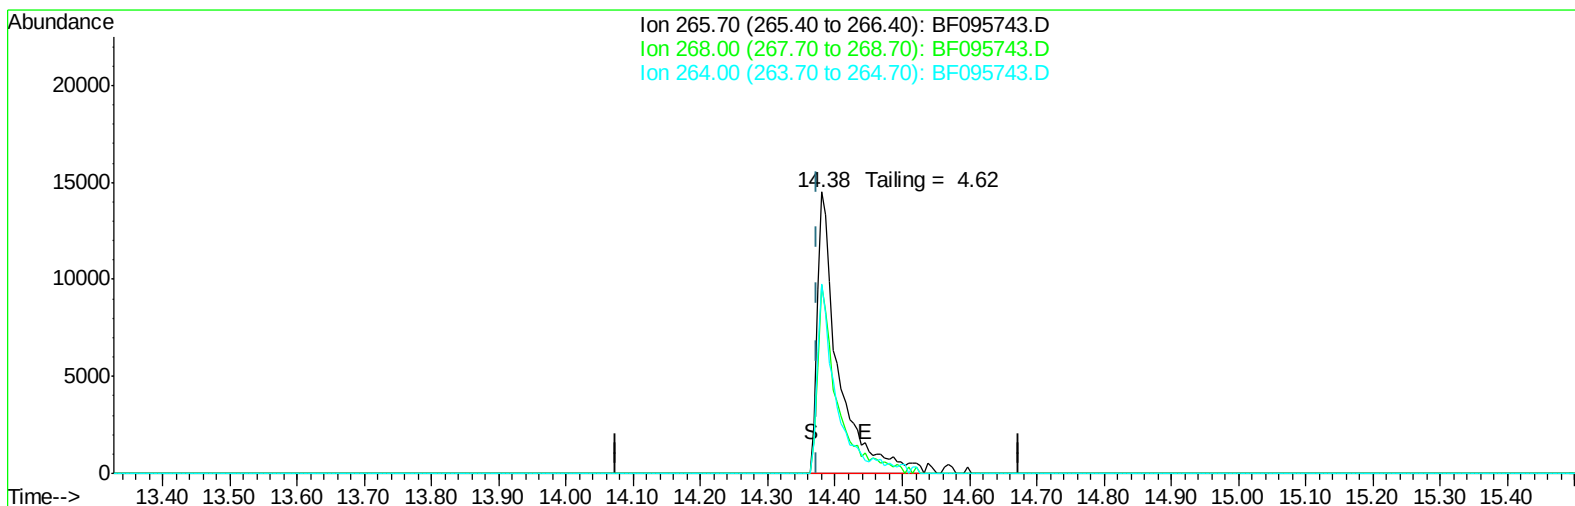

TIC: BF095743.D

(69) Pentachlorophenol (C)




14.380min (+0.006) 0.00ng

response 31196

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.90
264.00	64.60	67.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060717\
Data File : BF095743.D
Acq On : 7 Jun 2017 13:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 15:01:40 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:19:45 2017
Response via : Initial Calibration

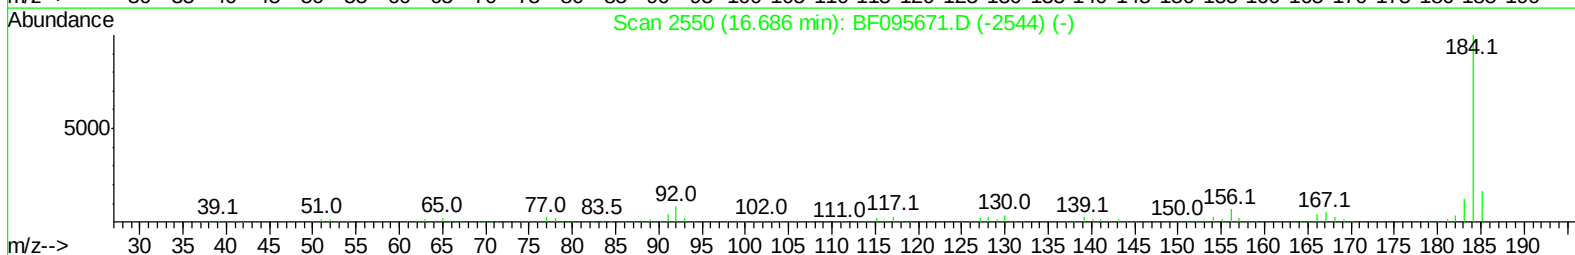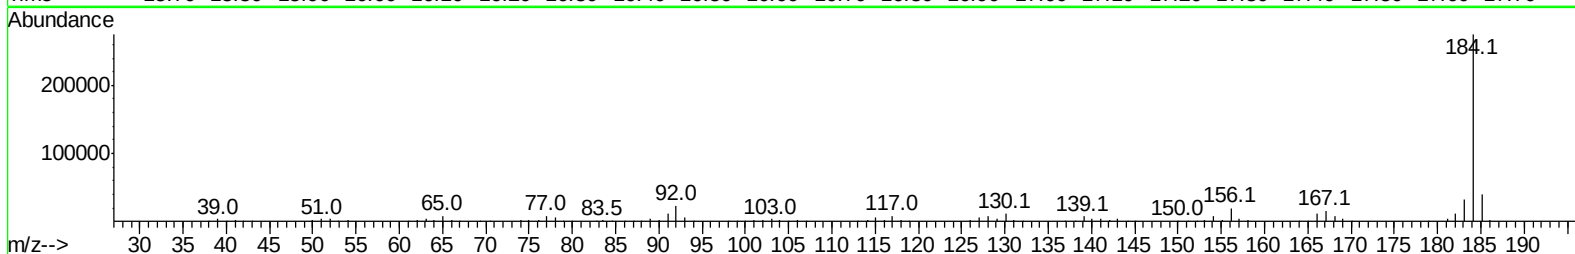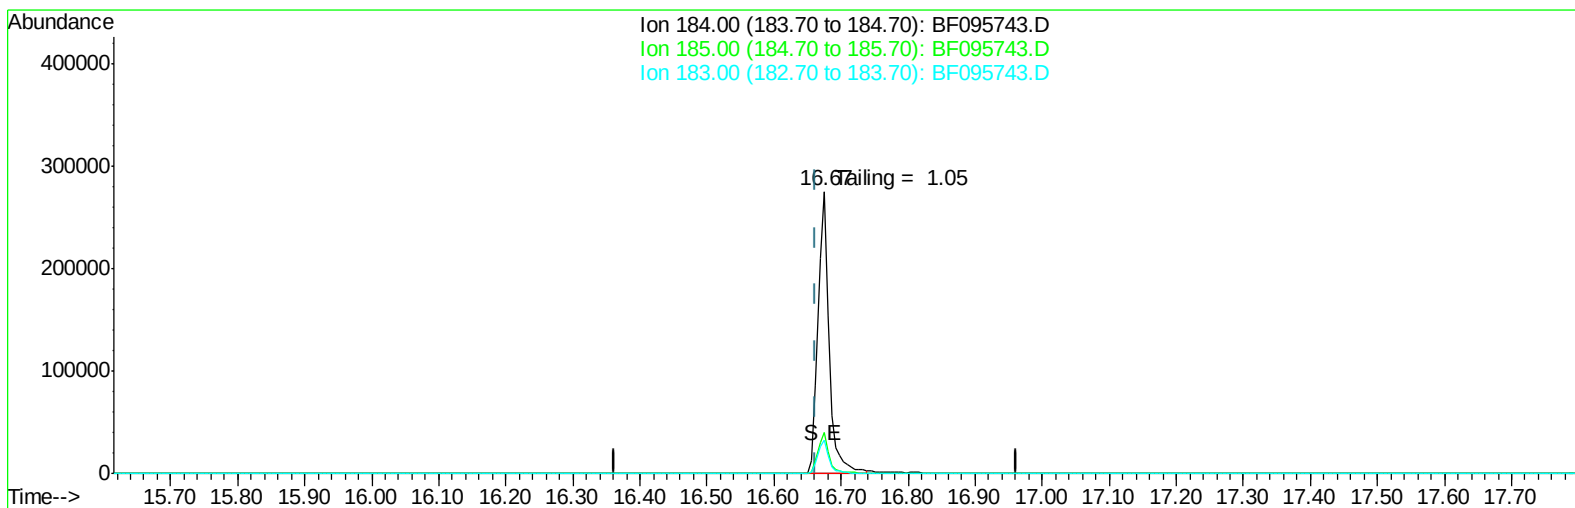

TIC: BF095743.D

(76) Benzidine

16.674min (+0.012) 0.00ng

response 313024

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.37#
183.00	12.20	11.86
0.00	0.00	0.00