
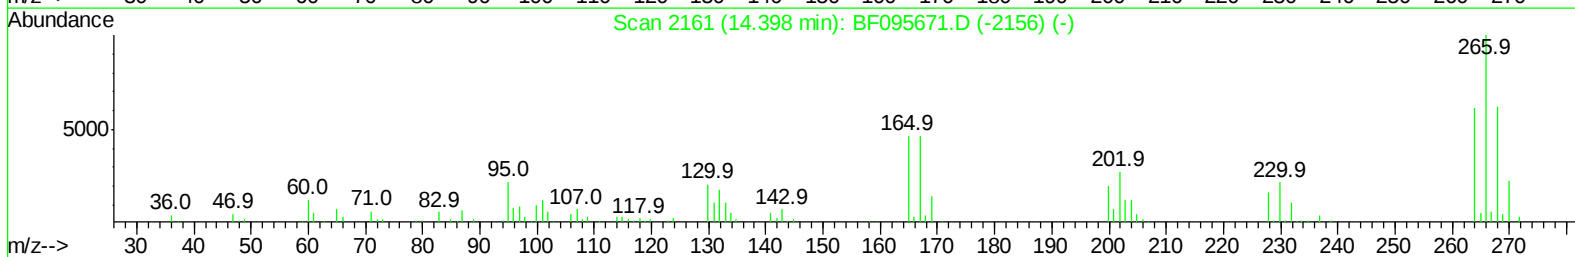
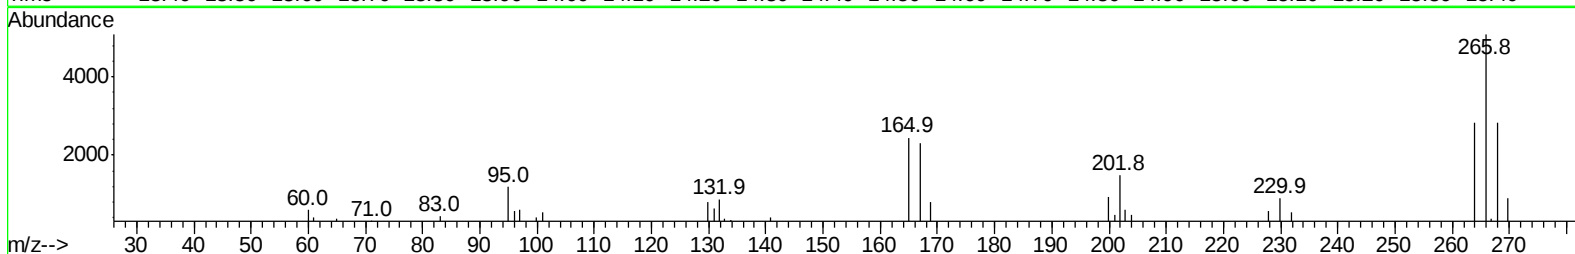


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060717\
Data File : BF095766.D
Acq On : 8 Jun 2017 2:43
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 15:05:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:19:45 2017
Response via : Initial Calibration

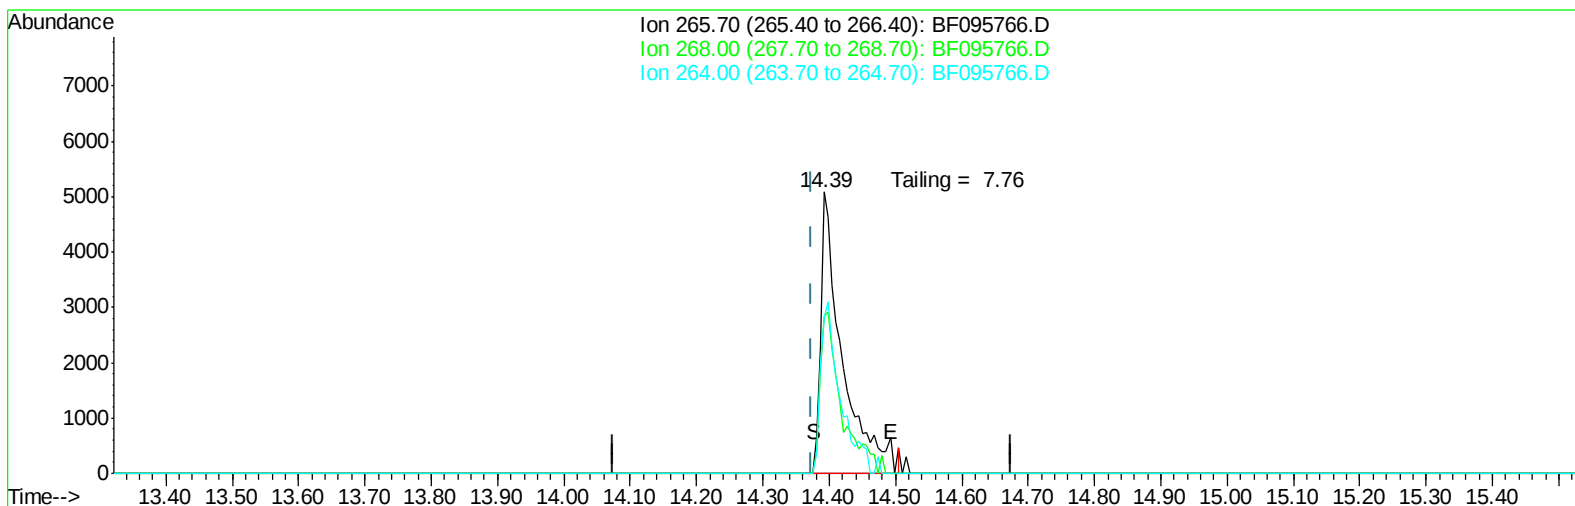

TIC: BF095766.D

(69) Pentachlorophenol (C)




14.392min (+0.018) 0.00ng

response 11711

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.87
264.00	64.60	55.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060717\
Data File : BF095766.D
Acq On : 8 Jun 2017 2:43
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 15:05:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:19:45 2017
Response via : Initial Calibration

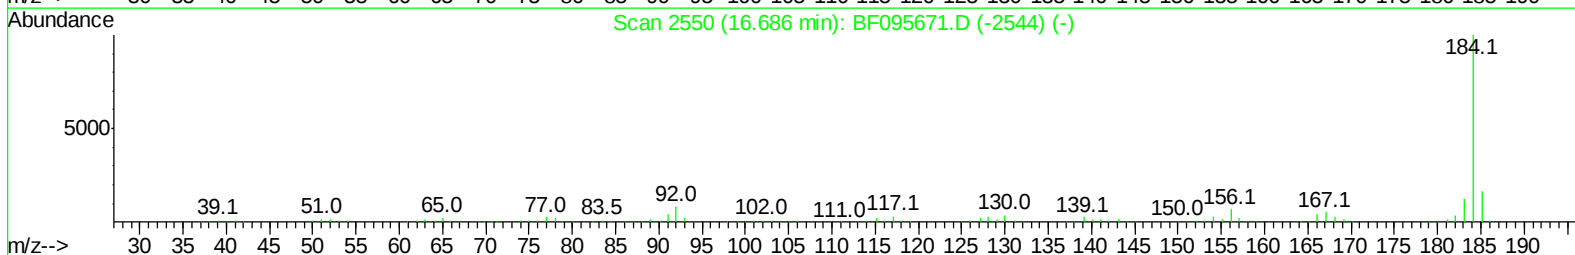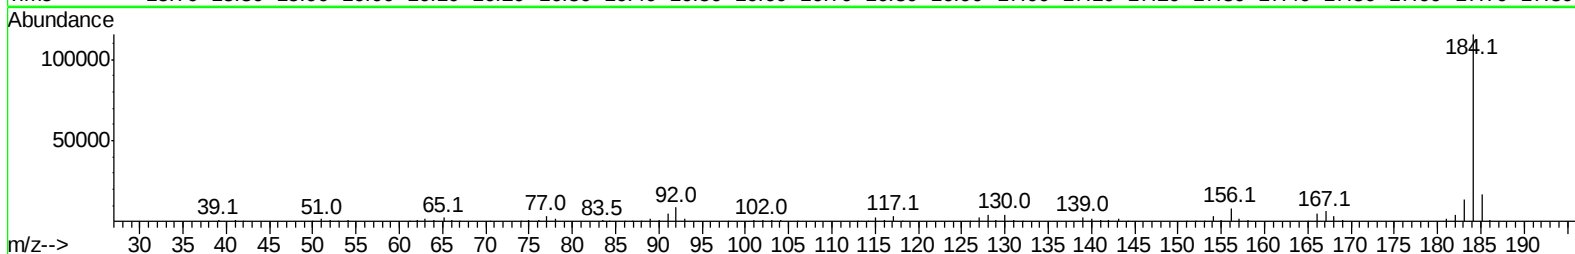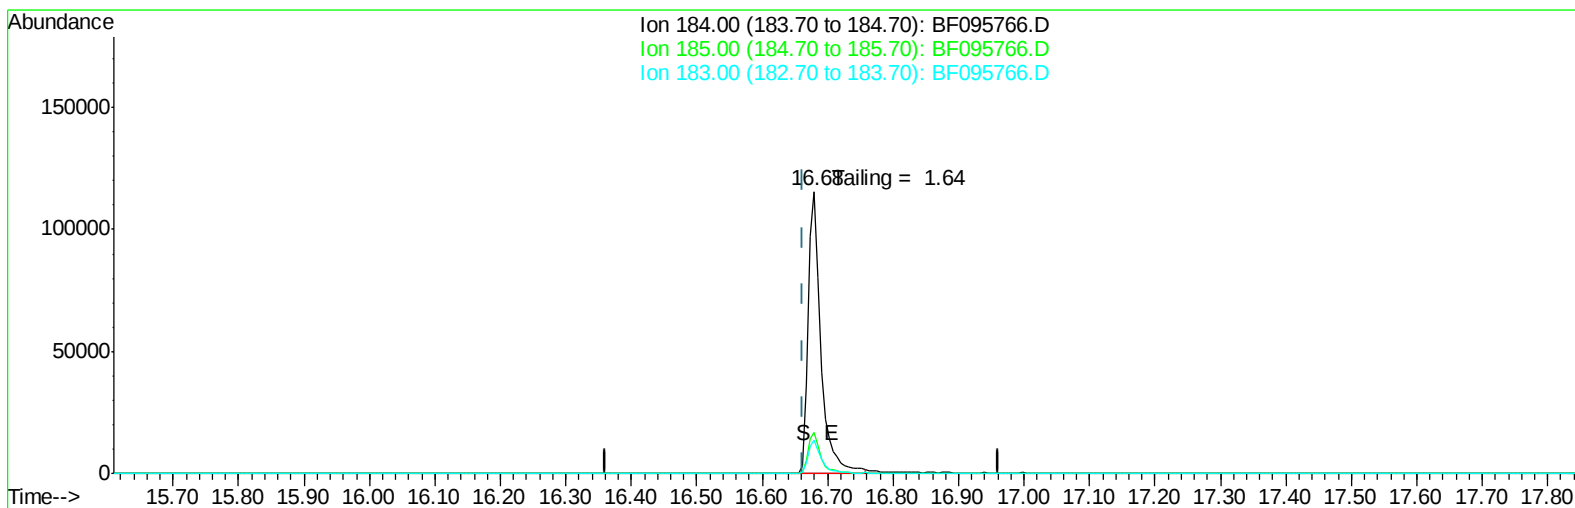

TIC: BF095766.D

(76) Benzidine

16.680min (+0.018) 0.00ng

response 159906

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.67#
183.00	12.20	11.78
0.00	0.00	0.00