


Data Path : Z:\HPCHEM1\BNA F\Data\BF060717\
 Data File : BF095743.D
 Acq On : 7 Jun 2017 13:33
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 08 11:19:45 2017

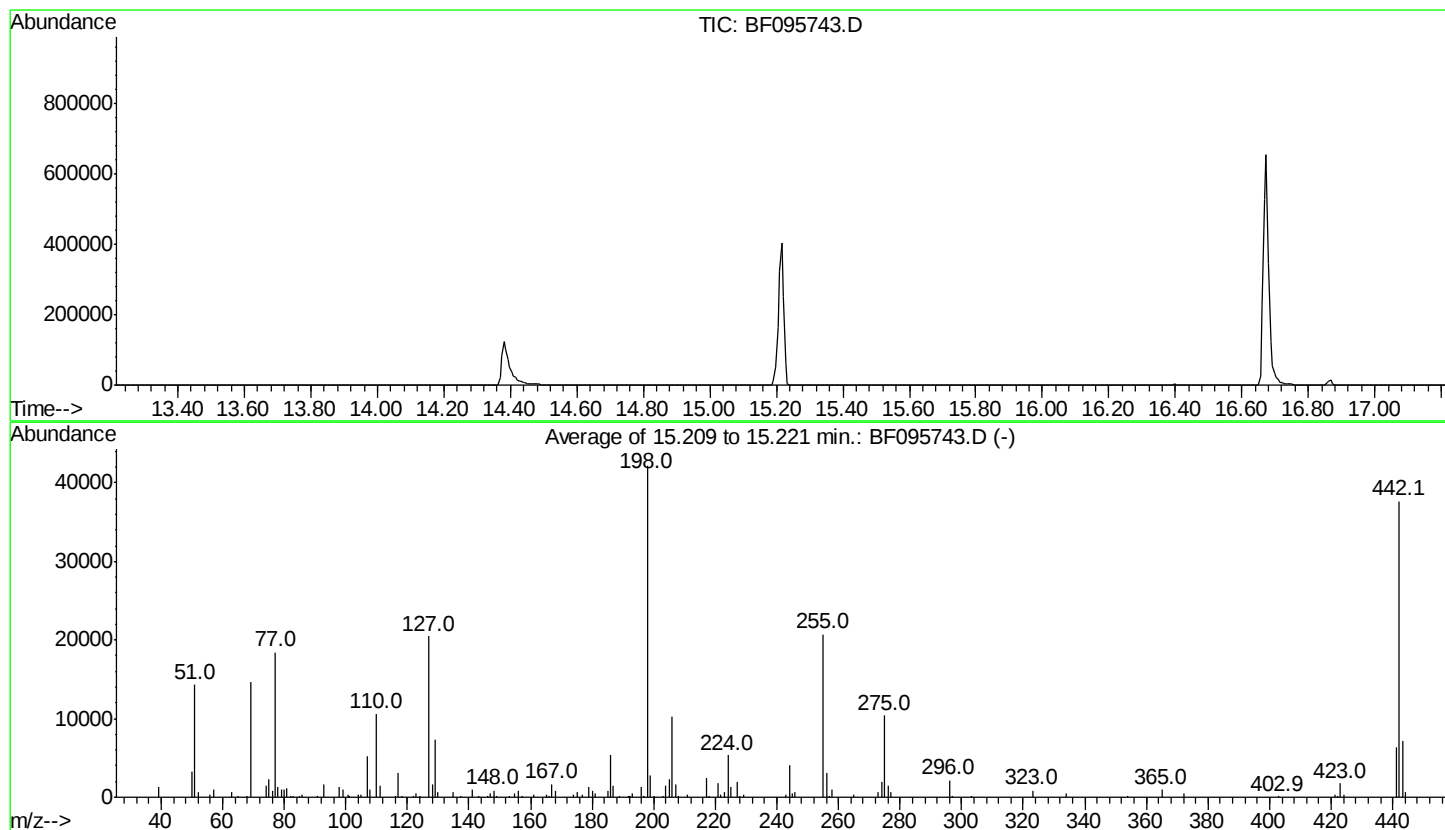

AutoFind: Scans 2316, 2317, 2318; Background Corrected with Scan 2309

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	14295	PASS
68	69	0.00	2	0.7	101	PASS
69	198	0.00	100	34.8	14659	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	20504	PASS
197	198	0.00	2	0.3	115	PASS
198	198	100	100	100.0	42181	PASS
199	198	5	9	6.8	2851	PASS
275	198	10	60	24.6	10377	PASS
365	198	1	100	2.1	906	PASS
441	442	0.01	24	17.0	6399	PASS
442	198	50	100	89.3	37680	PASS
443	442	15	24	18.9	7104	PASS