


Data Path : Z:\HPCHEM1\BNA F\Data\BF060717\
 Data File : BF095766.D
 Acq On : 8 Jun 2017 2:43
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 08 11:19:45 2017

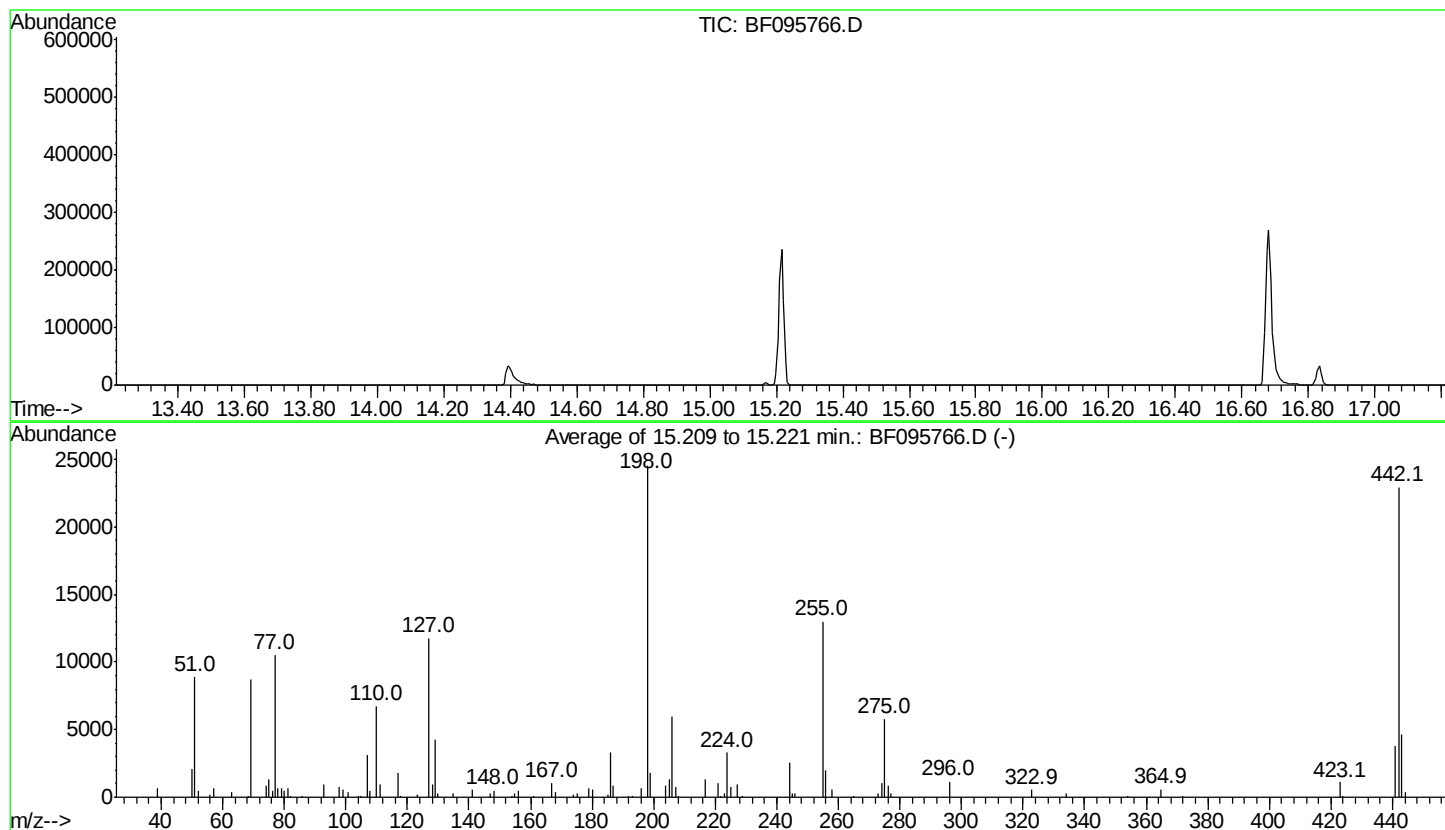

AutoFind: Scans 2316, 2317, 2318; Background Corrected with Scan 2310

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	8925	PASS
68	69	0.00	2	1.2	102	PASS
69	198	0.00	100	35.4	8672	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	11739	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24517	PASS
199	198	5	9	7.2	1758	PASS
275	198	10	60	23.6	5792	PASS
365	198	1	100	2.3	575	PASS
441	442	0.01	24	16.4	3763	PASS
442	198	50	100	93.5	22917	PASS
443	442	15	24	20.3	4643	PASS