


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060719\
 Data File : BF114889.D
 Acq On : 7 Jun 2019 9:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 04 16:57:15 2019

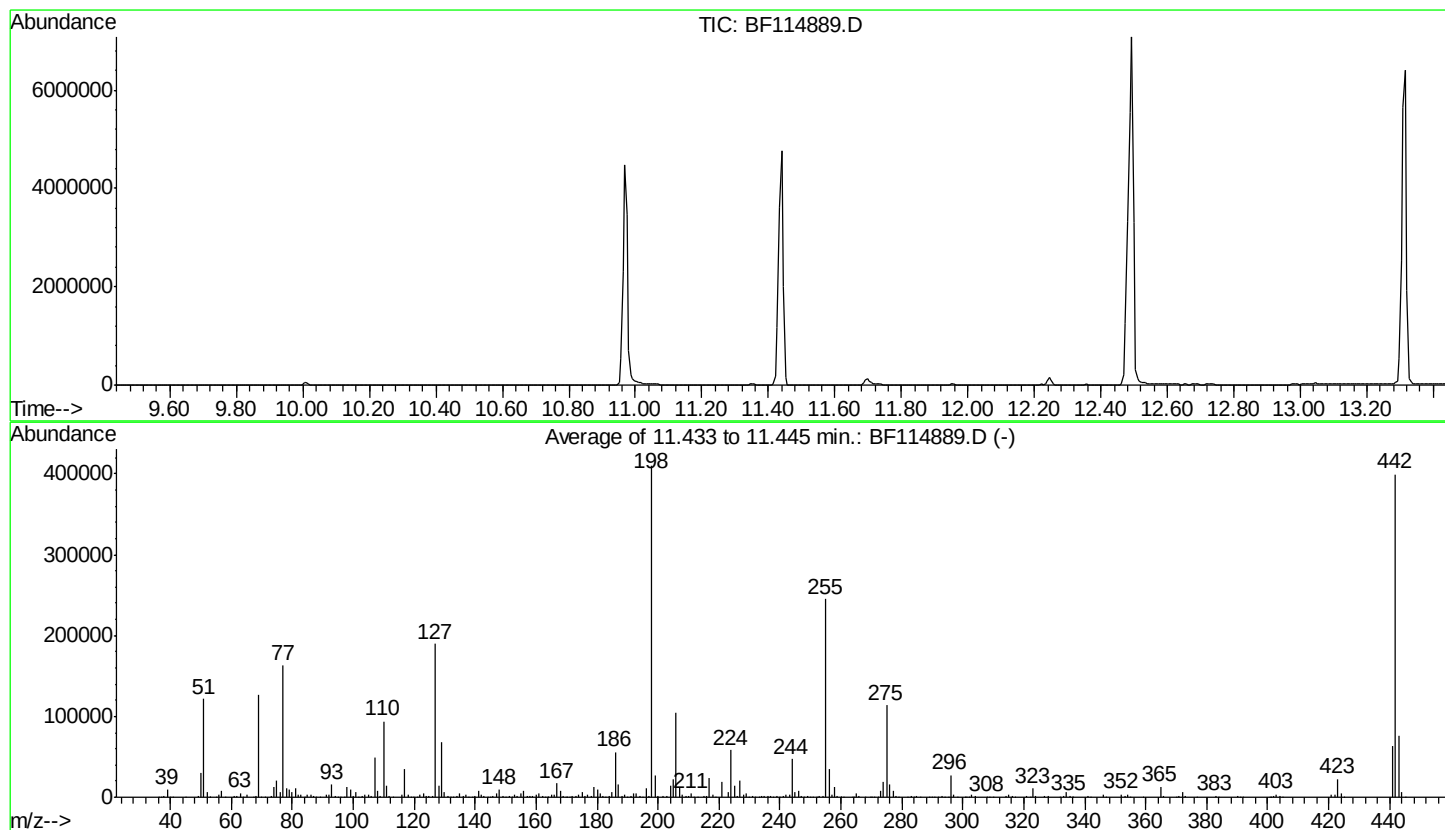

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	121650	PASS
68	69	0.00	2	1.7	2159	PASS
69	198	0.00	100	30.7	126012	PASS
70	69	0.00	2	0.7	826	PASS
127	198	10	80	46.2	189682	PASS
197	198	0.00	2	0.5	2036	PASS
198	198	100	100	100.0	410176	PASS
199	198	5	9	6.6	26929	PASS
275	198	10	60	27.6	113266	PASS
365	198	1	100	3.2	13309	PASS
441	198	0.01	100	15.4	63024	PASS
442	198	50	100	97.3	399296	PASS
443	442	15	24	19.2	76557	PASS