


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060719\
 Data File : BF114899.D
 Acq On : 7 Jun 2019 16:51
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 04 16:57:15 2019

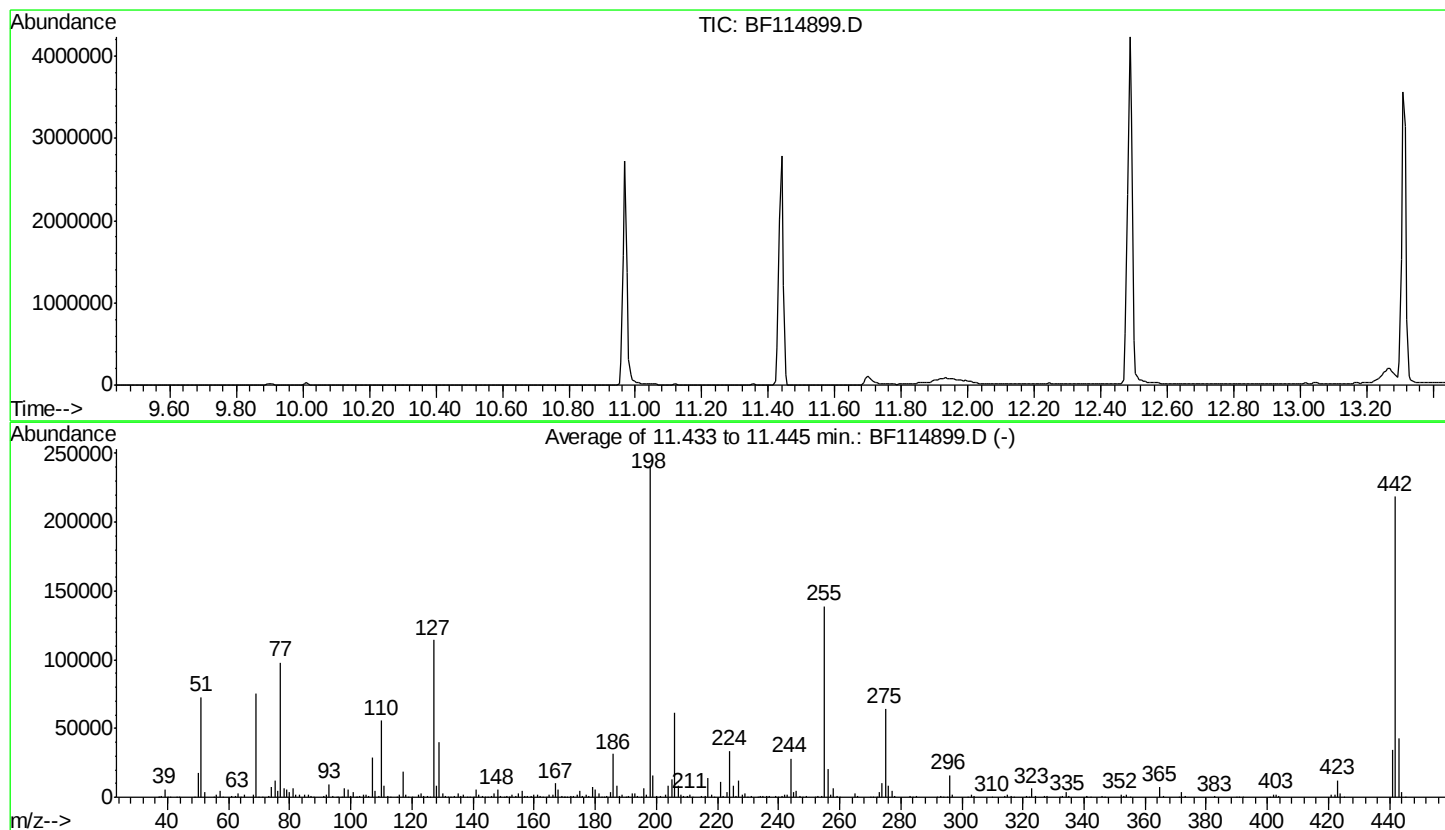

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	72669	PASS
68	69	0.00	2	2.0	1532	PASS
69	198	0.00	100	31.4	75634	PASS
70	69	0.00	2	0.6	441	PASS
127	198	10	80	47.4	114368	PASS
197	198	0.00	2	0.6	1502	PASS
198	198	100	100	100.0	241109	PASS
199	198	5	9	6.6	16002	PASS
275	198	10	60	26.8	64704	PASS
365	198	1	100	3.2	7669	PASS
441	198	0.01	100	14.3	34458	PASS
442	198	50	100	90.6	218530	PASS
443	442	15	24	19.6	42784	PASS