
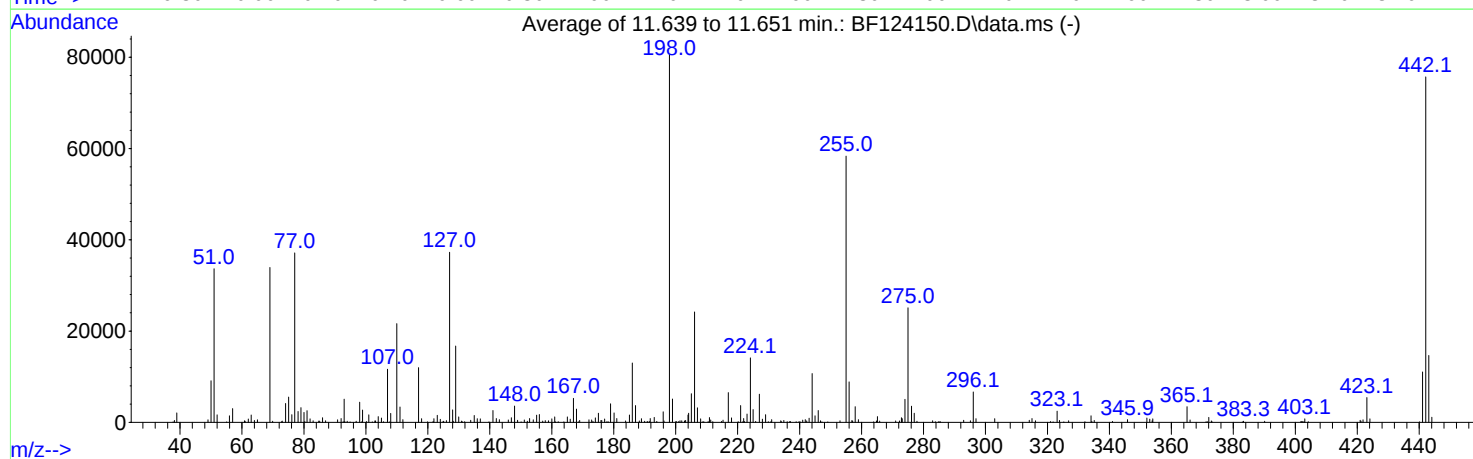


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060721\
 Data File : BF124150.D
 Acq On : 7 Jun 2021 10:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 07 13:32:21 2021

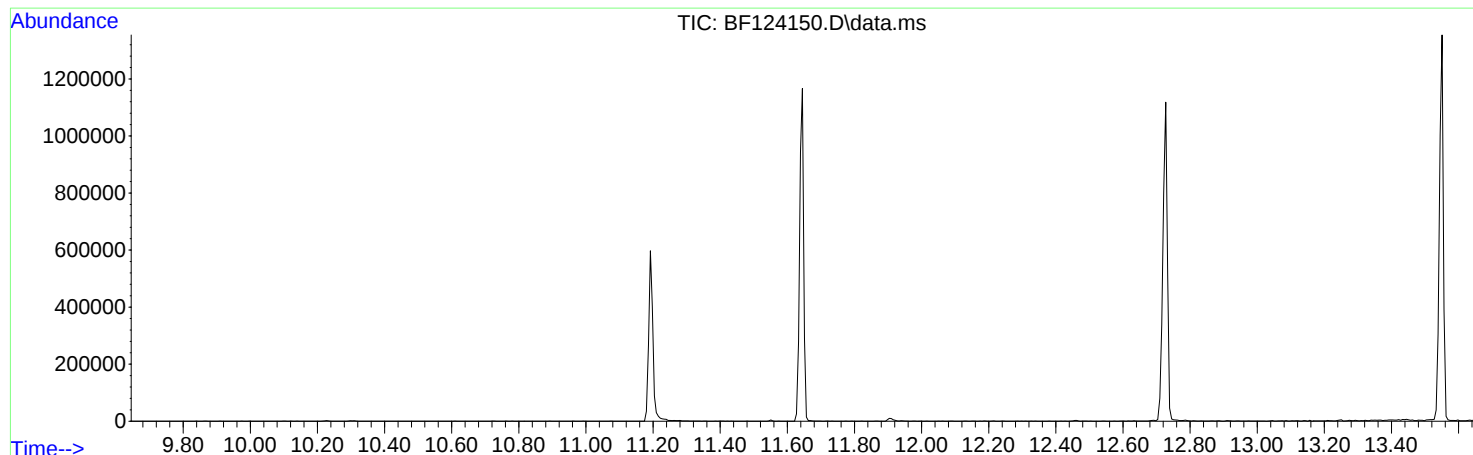




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	33657	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.1	33944	PASS
70	69	0.00	2	0.8	257	PASS
127	198	10	80	46.2	37273	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80608	PASS
199	198	5	9	6.4	5129	PASS
275	198	10	60	31.2	25122	PASS
365	198	1	100	4.2	3424	PASS
441	198	0.01	100	13.7	11062	PASS
442	442	50	100	100.0	75709	PASS
443	442	15	24	19.3	14648	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060721\
 Data File : BF124150.D
 Acq On : 7 Jun 2021 10:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 11:01:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 04 09:56:24 2021
 Response via : Initial Calibration

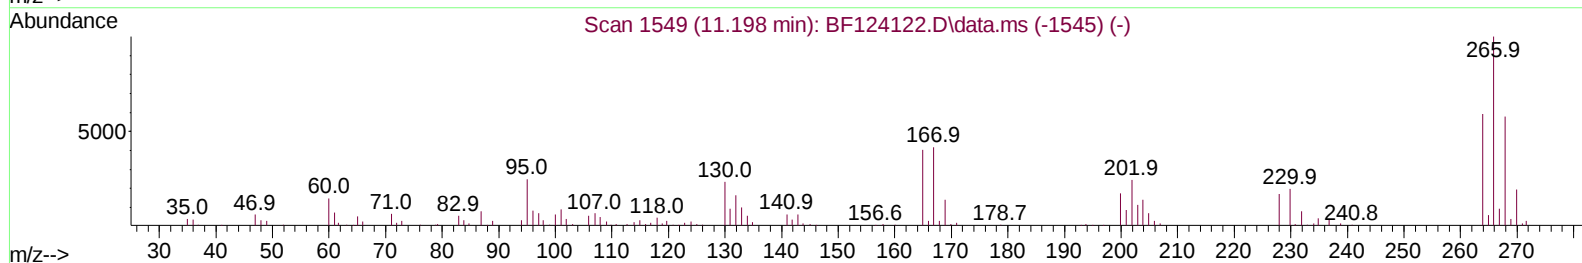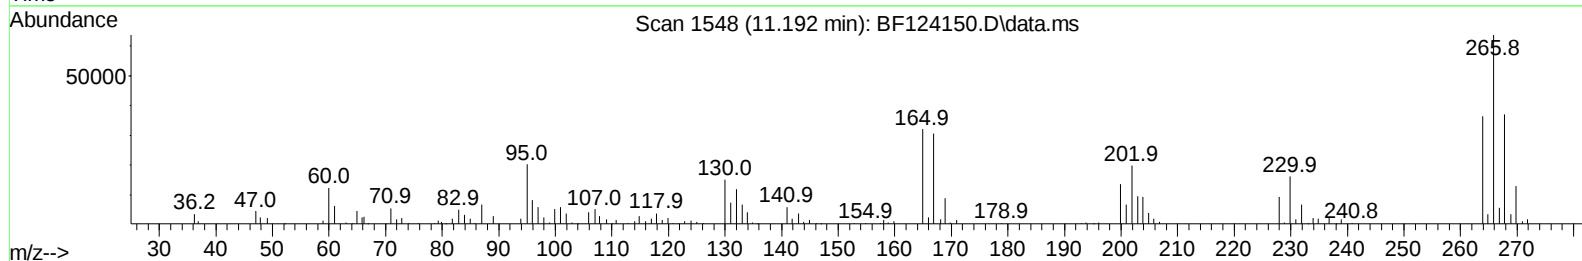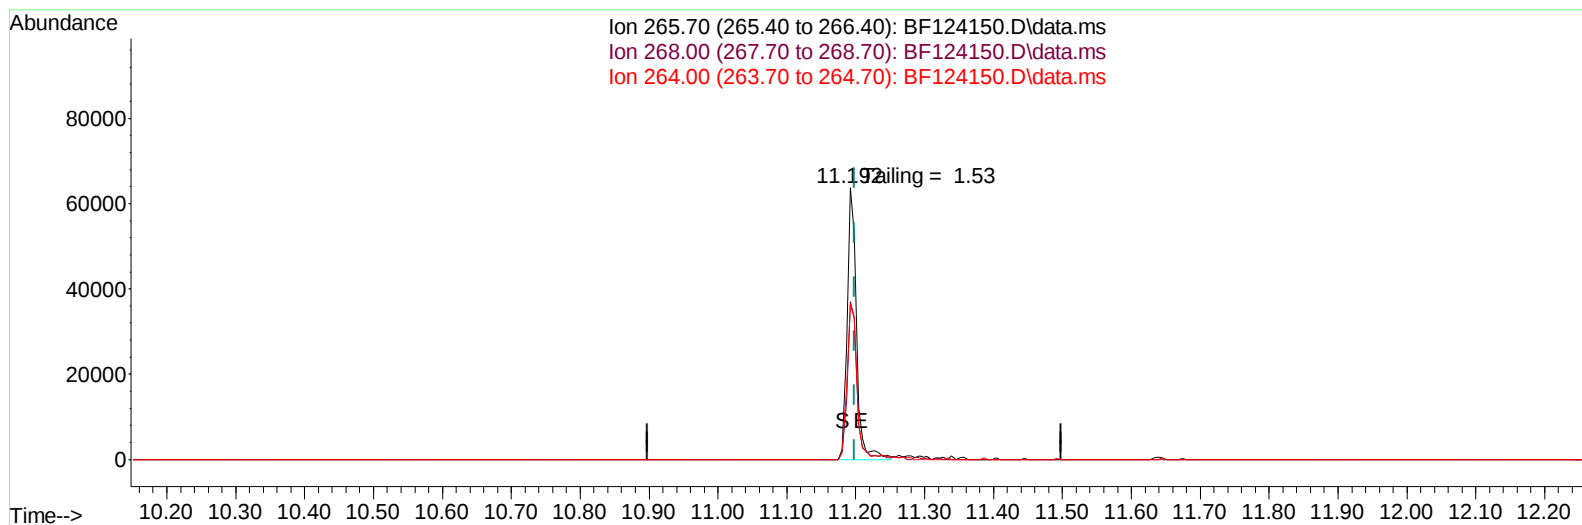

TIC: BF124150.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 15749.10 ng




response 60541

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.01
264.00	65.70	57.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060721\
 Data File : BF124150.D
 Acq On : 7 Jun 2021 10:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 11:01:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 04 09:56:24 2021
 Response via : Initial Calibration

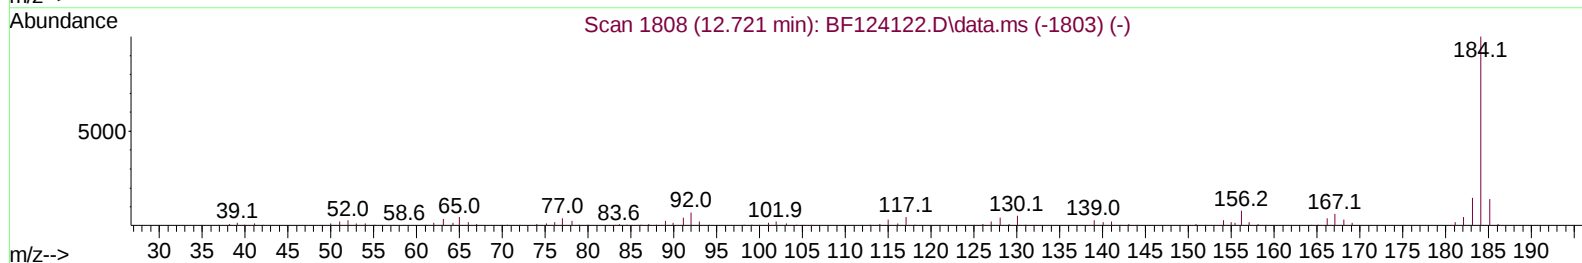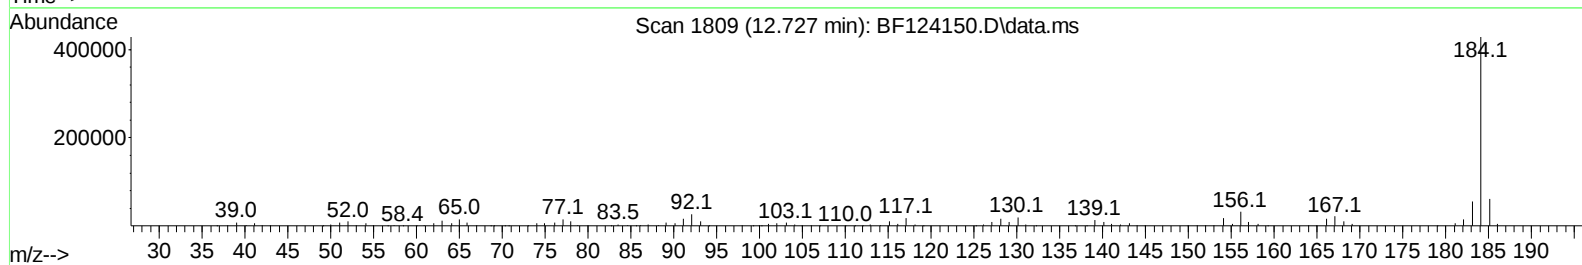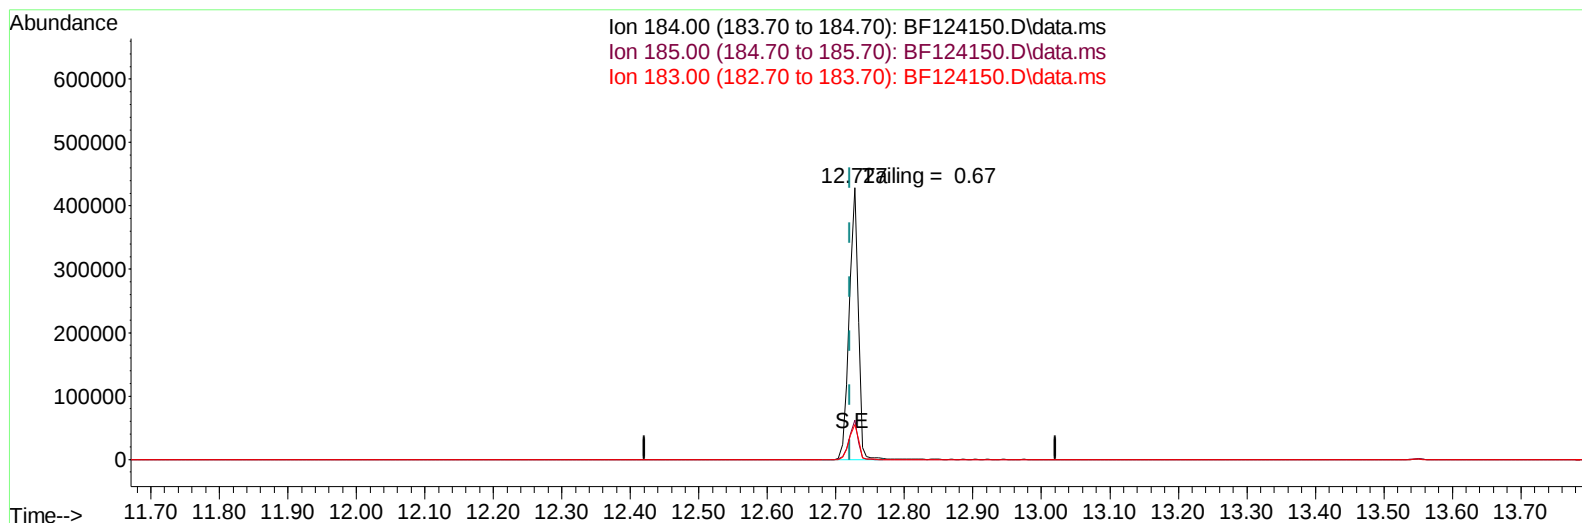

TIC: BF124150.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 391877

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.46
183.00	9.80	12.93#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2021	BNA_F	<u>BF124150.D</u>
Compound Name	Response	Retention Time
DDT	200095	13.551
DDD	2664	13.345
DDE	3007	11.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5671	205766	2.76