
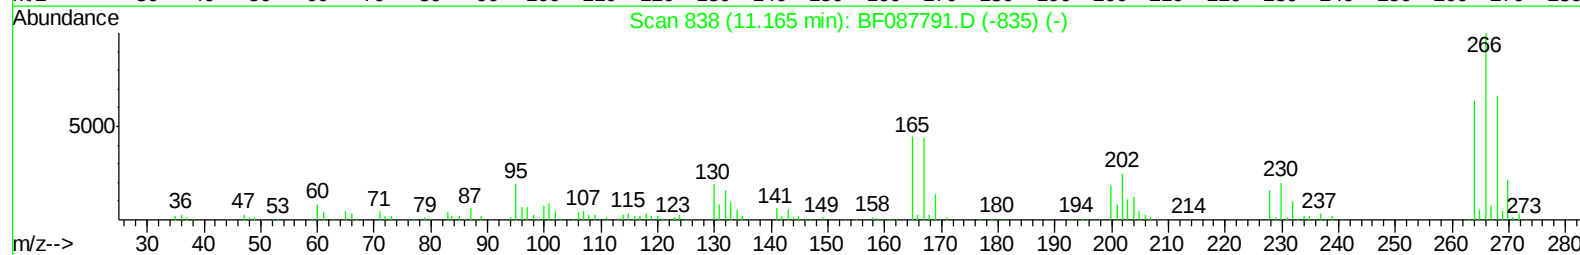
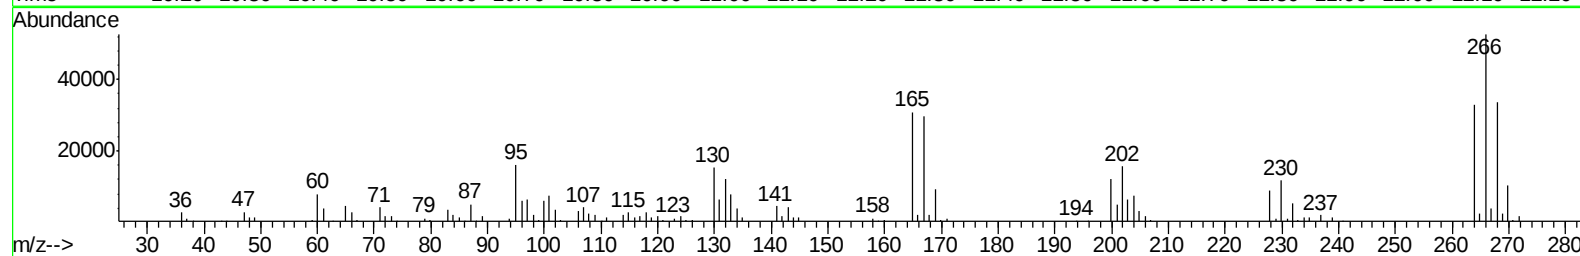


Data Path : Z:\HPCHEM1\BNA F\Data\BF060816\
Data File : BF087806.D
Acq On : 8 Jun 2016 13:22
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 13:46:21 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

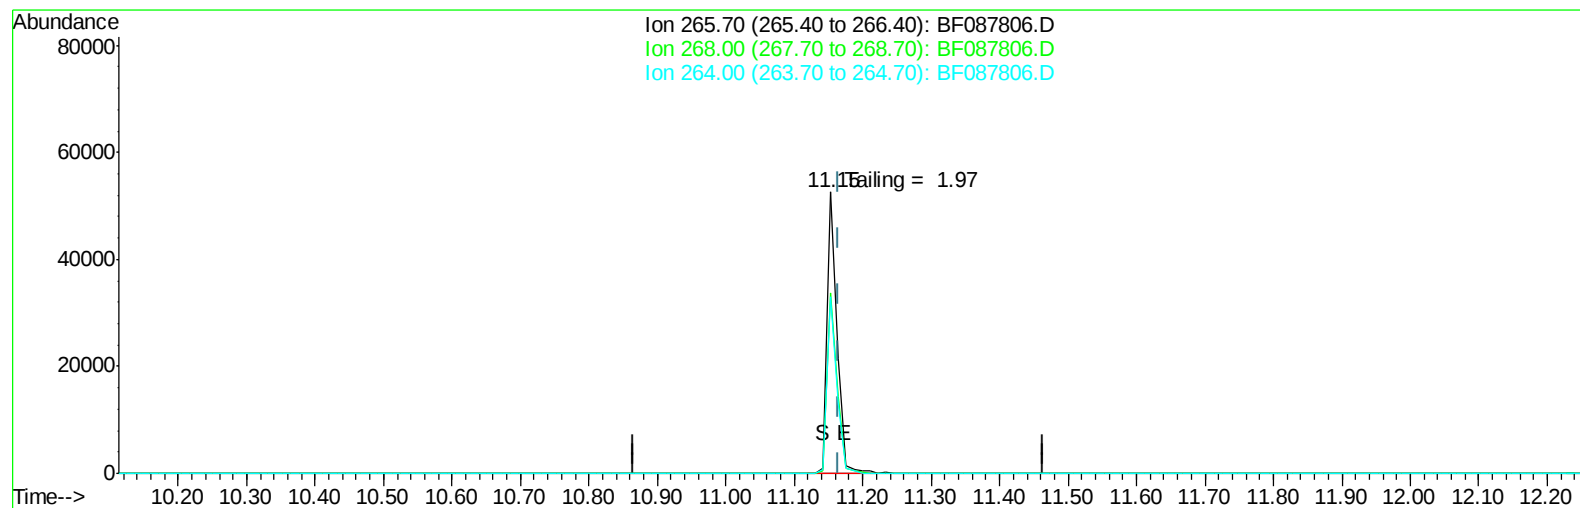

TIC: BF087806.D

(69) Pentachlorophenol (C)




11.153min (-0.012) 0.00ng

response 53886

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	64.23
264.00	62.00	62.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF060816\
Data File : BF087806.D
Acq On : 8 Jun 2016 13:22
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 13:46:21 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

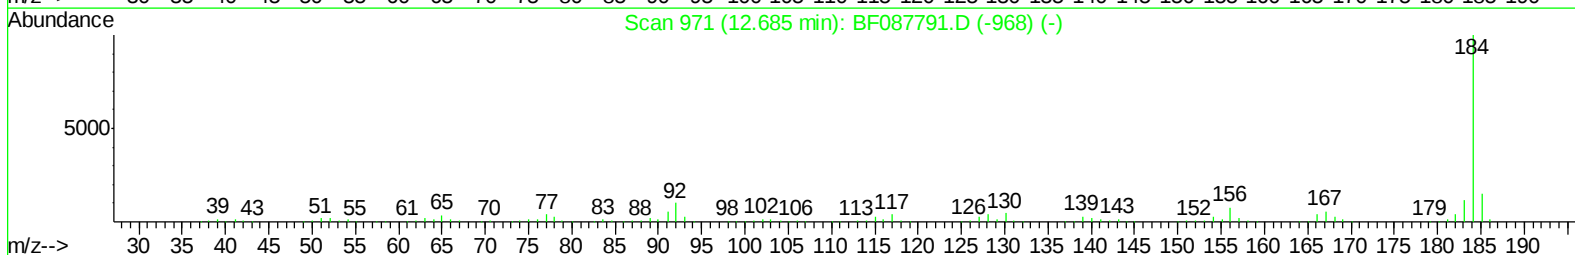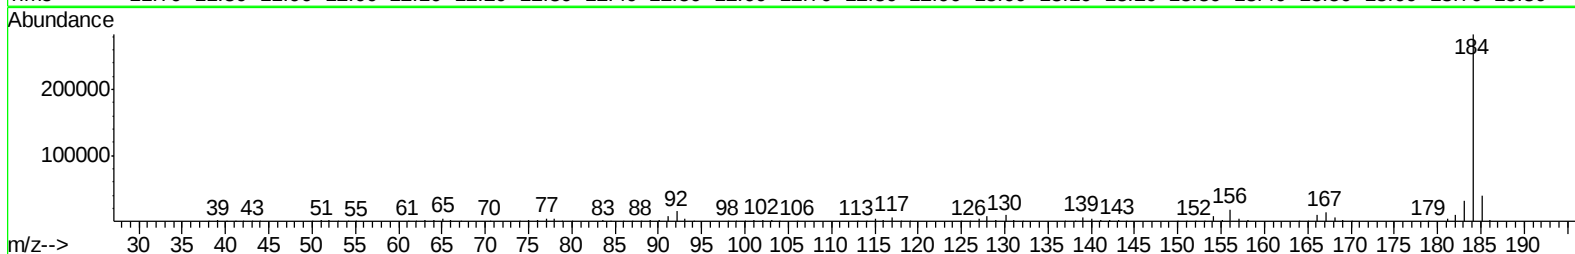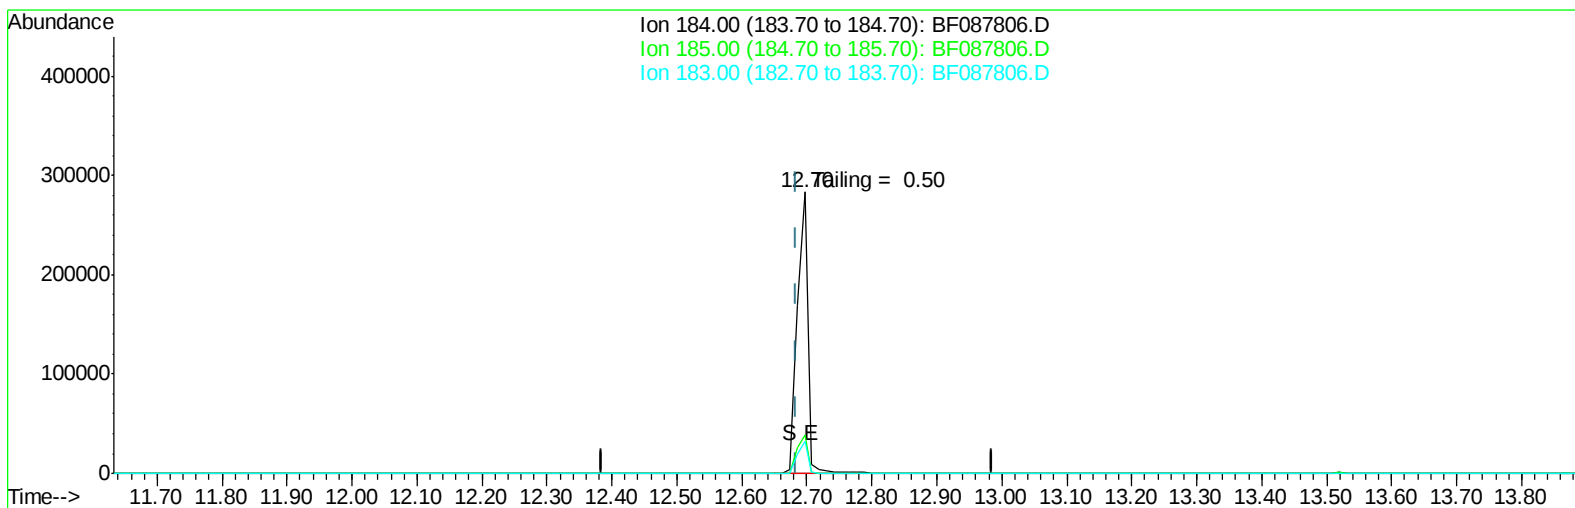

TIC: BF087806.D

(76) Benzidine




12.696min (+0.011) 0.00ng

response 329901

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.86
183.00	11.60	11.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF060816\
Data File : BF087831.D
Acq On : 9 Jun 2016 3:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 19:16:13 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

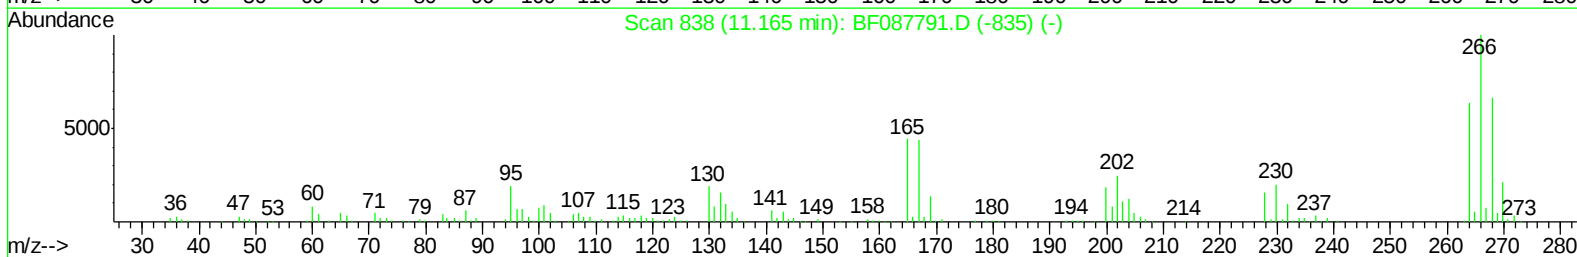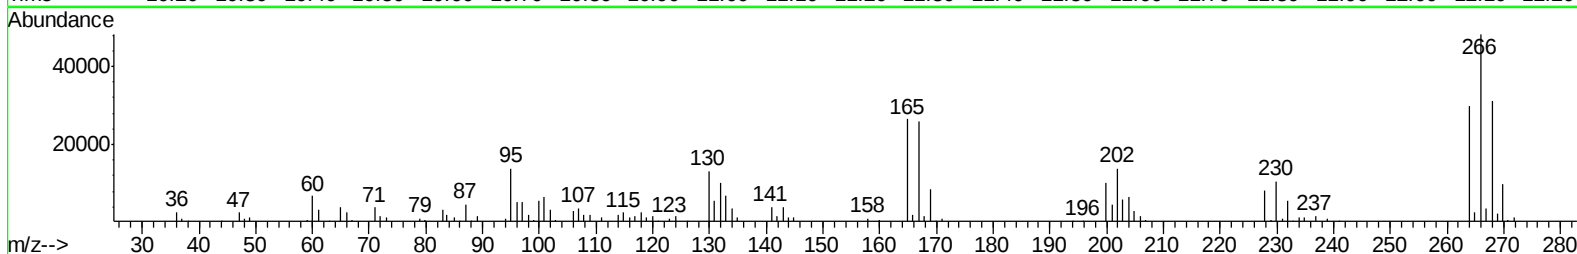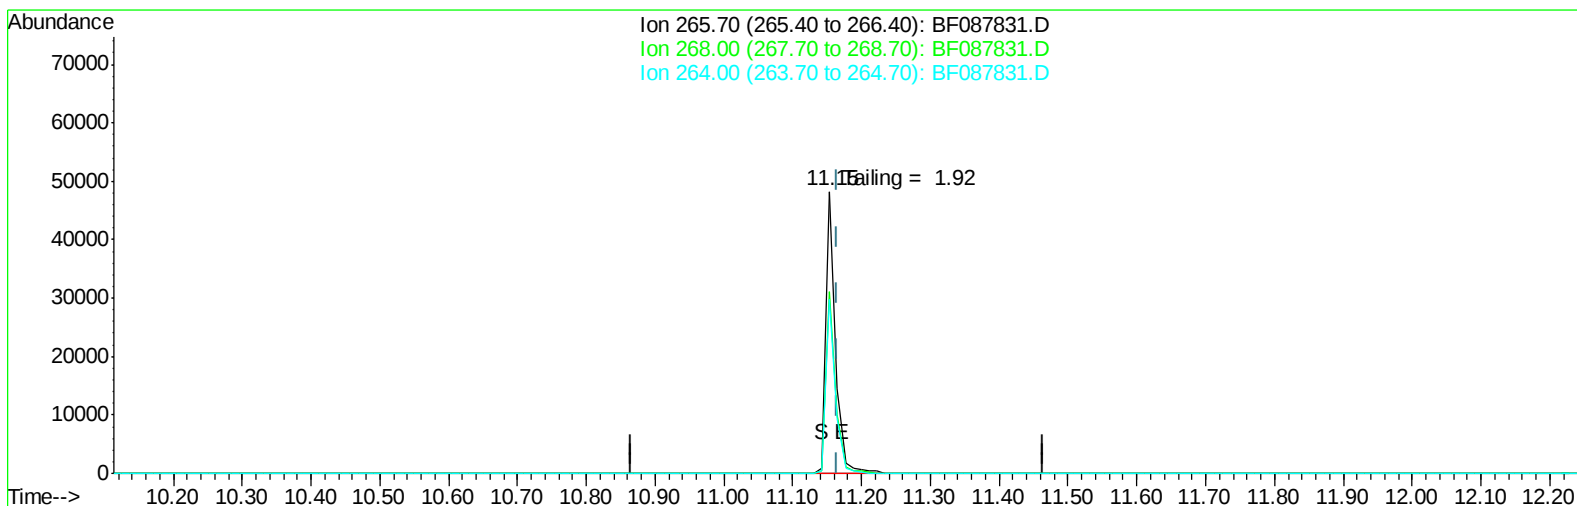

TIC: BF087831.D

(69) Pentachlorophenol (C)

11.154min (-0.011) 0.00ng

response 46173

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	64.37
264.00	62.00	61.86
0.00	0.00	0.00