


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060816\
 Data File : BF087806.D
 Acq On : 8 Jun 2016 13:22
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 07 18:51:55 2016

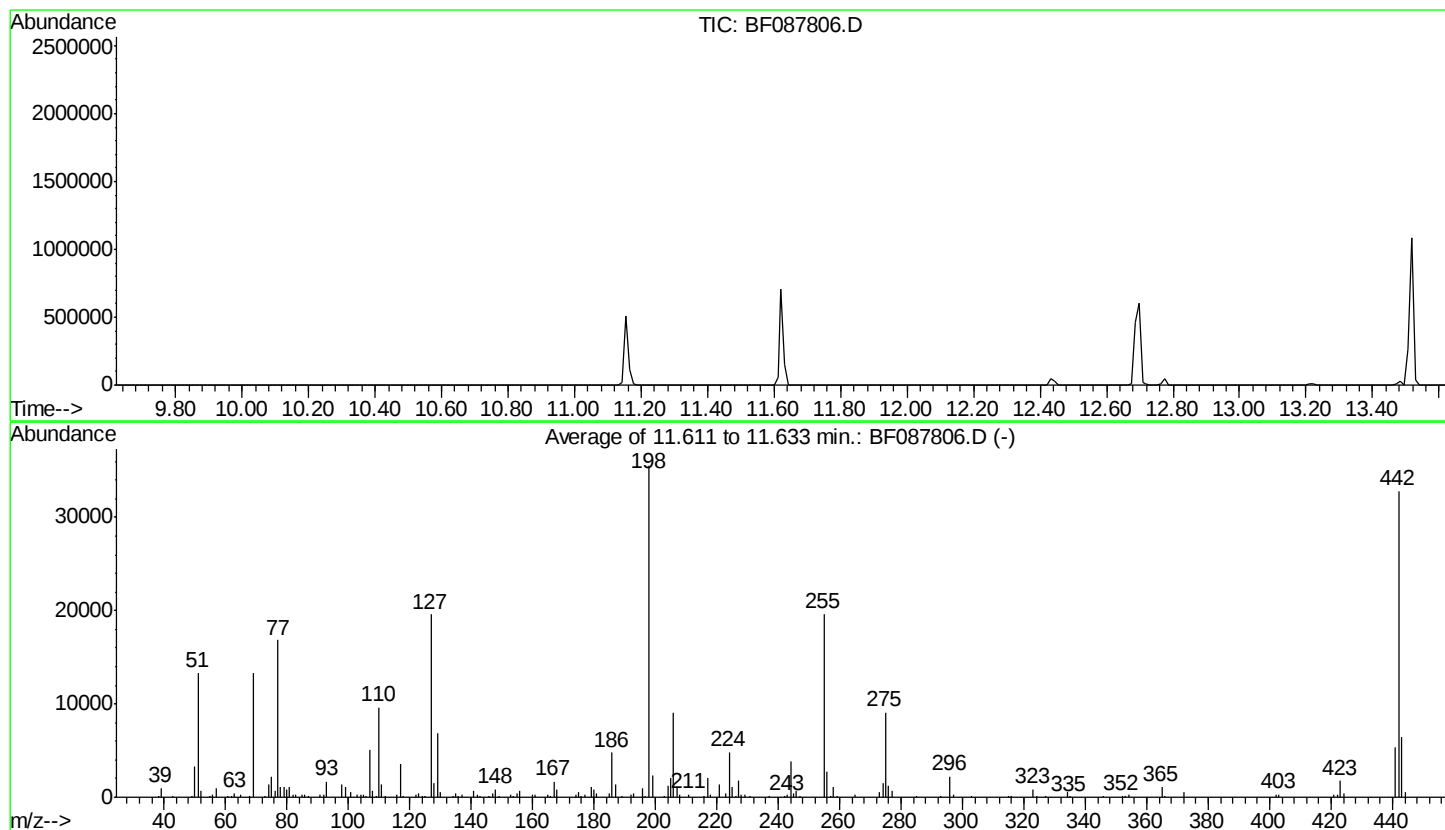

AutoFind: Scans 877, 878, 879; Background Corrected with Scan 874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	13331	PASS
68	69	0.00	2	1.4	192	PASS
69	198	0.00	100	37.6	13353	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.0	19572	PASS
197	198	0.00	2	0.4	157	PASS
198	198	100	100	100.0	35556	PASS
199	198	5	9	6.4	2274	PASS
275	198	10	60	25.6	9118	PASS
365	198	1	100	3.3	1159	PASS
441	442	0.01	24	16.4	5397	PASS
442	198	50	100	92.4	32867	PASS
443	442	15	24	19.7	6471	PASS