
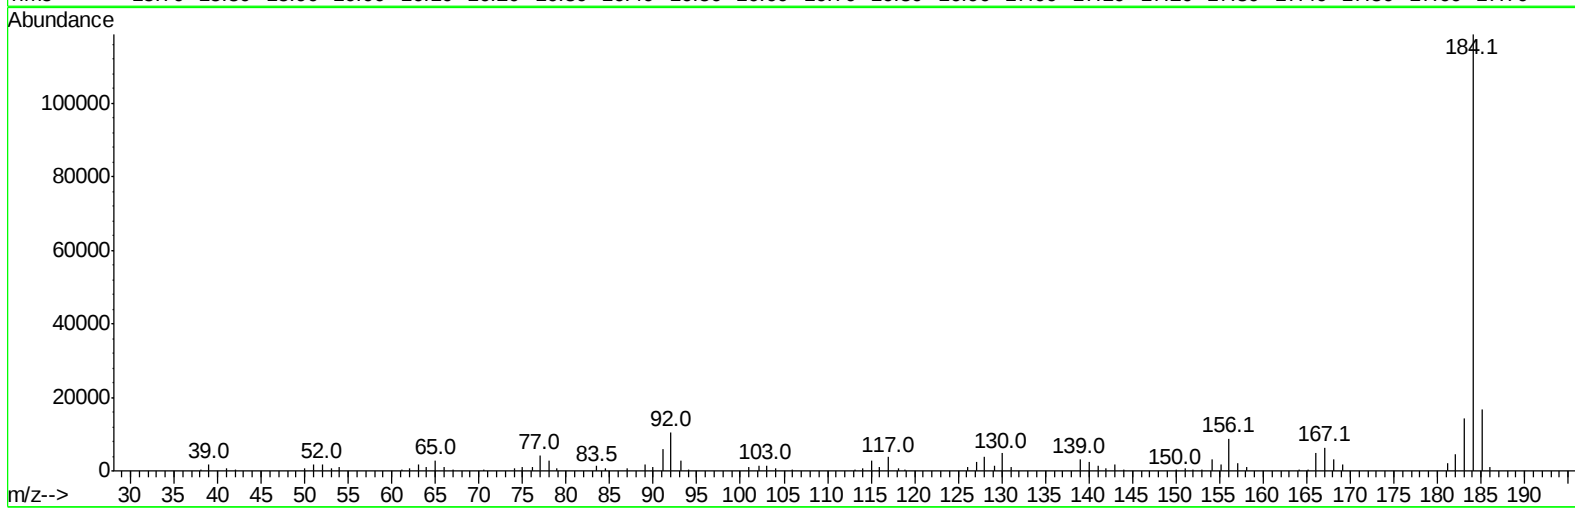


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060817\
Data File : BF095808.D
Acq On : 9 Jun 2017 5:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:54:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

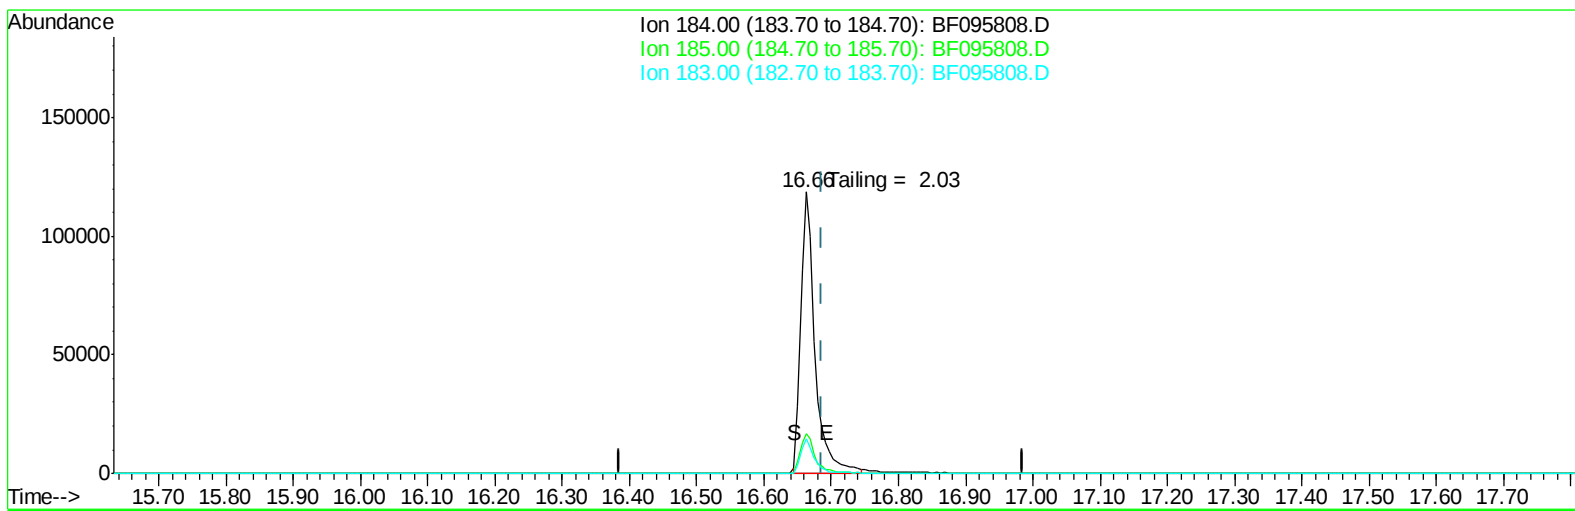

TIC: BF095808.D

(76) Benzidine



16.662min (-0.024) 0.00ng

response 175586

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.06#
183.00	12.20	12.16
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060817\
Data File : BF095808.D
Acq On : 9 Jun 2017 5:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:54:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

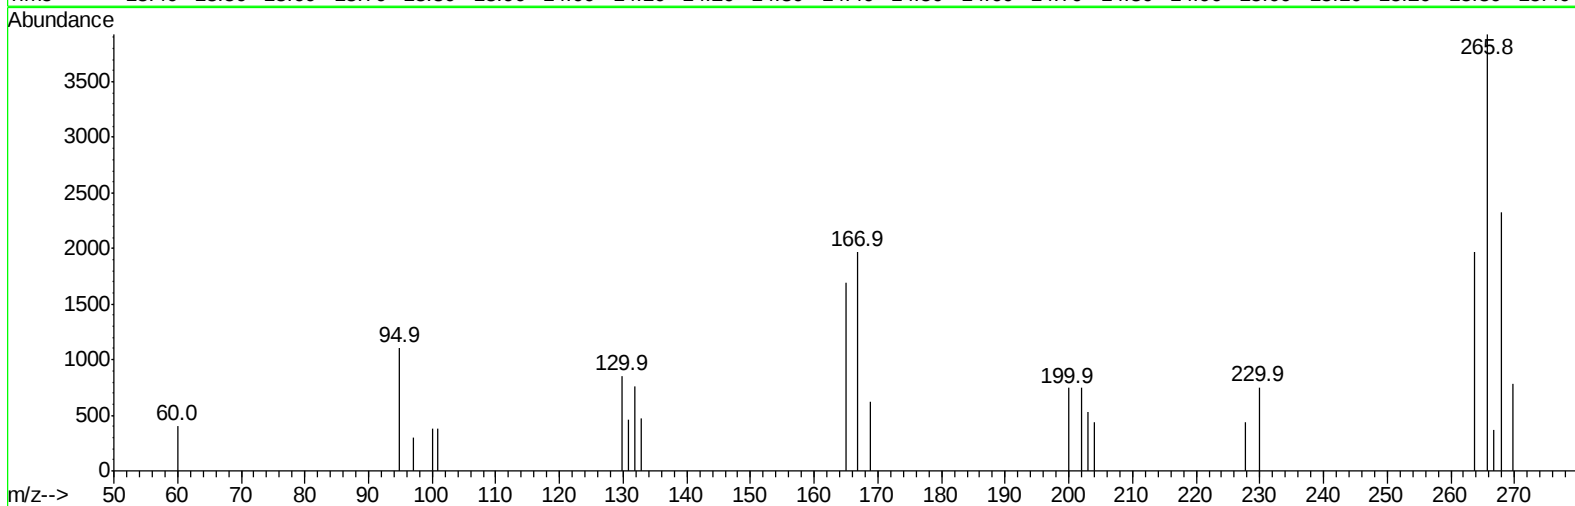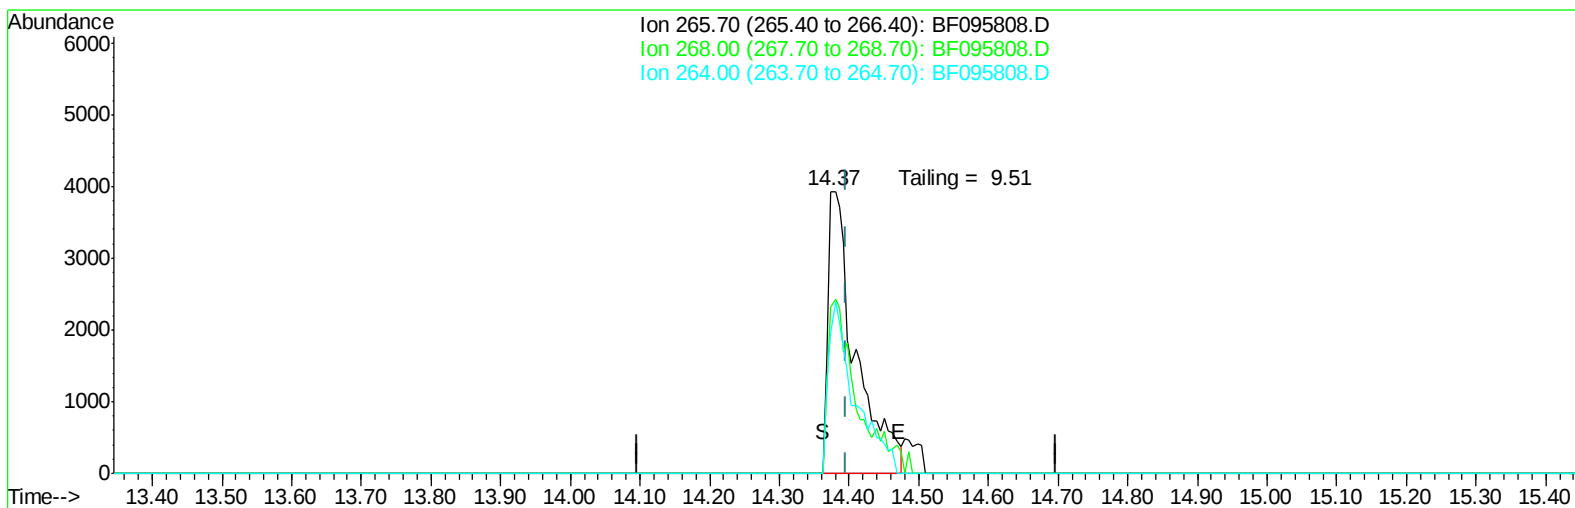

TIC: BF095808.D

(69) Pentachlorophenol (C)

14.374min (-0.023) 0.00ng

response 9670

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.27
264.00	64.60	50.03#
0.00	0.00	0.00