

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060817\
 Data File : BF095803.D
 Acq On : 9 Jun 2017 1:50
 Operator : SJ/MA
 Sample : I3470-03 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 POSTEX-45-20170602

Manual Integrations
 APPROVED

mohammad
 6/9/2017 12:09:31 PM

Quant Time: Jun 09 04:41:07 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:15:31 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	70638	20.00	ng	-0.03
21) Naphthalene-d8	9.40	136	282793	20.00	ng	-0.04
38) Acenaphthene-d10	12.22	164	118033	20.00	ng	-0.04
63) Phenanthrene-d10	14.61	188	186973	20.00	ng	-0.04
75) Chrysene-d12	18.33	240	141189	20.00	ng	-0.02
86) Perylene-d12	20.00	264	107458	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	229337	51.73	ng	-0.03
7) Phenol-d6	6.92	99	277325	52.26	ng	-0.04
23) Nitrobenzene-d5	8.28	82	159613	35.05	ng	-0.04
41) 2,4,6-Tribromophenol	13.52	330	47841	45.81	ng	-0.04
44) 2-Fluorobiphenyl	11.17	172	324158	38.22	ng	-0.04
78) Terphenyl-d14	16.99	244	216599	38.07	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	11.87	163	43607	4.87	ng	98
70) Phenanthrene	14.65	178	226820	21.02	ng	98
71) Anthracene	14.74	178	39225	3.48	ng	97
74) Fluoranthene	16.43	202	268975	25.19	ng	98
77) Pyrene	16.73	202	289554	27.49	ng	98
80) Benzo(a)anthracene	18.32	228	118829	14.48	ng	99
82) Chrysene	18.36	228	126988	15.48	ng	98
85) Indeno(1,2,3-cd)pyrene	21.17	276	38005	5.41	ng	95
87) Benzo(b)fluoranthene	19.60	252	103937m	15.45	ng	
88) Benzo(k)fluoranthene	19.63	252	31644m	4.92	ng	
89) Benzo(a)pyrene	19.94	252	69232	11.19	ng	98
90) Dibenzo(a,h)anthracene	21.17	278	10548	2.01	ng	# 80
91) Benzo(a,h,i)perylene	21.51	276	36395	6.80	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060817\
Data File : BF095803.D
Acq On : 9 Jun 2017 1:50
Operator : SJ/MA
Sample : I3470-03 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602

Manual Integrations
APPROVED

mohammad
6/9/2017 12:09:31 PM

Quant Time: Jun 09 04:41:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

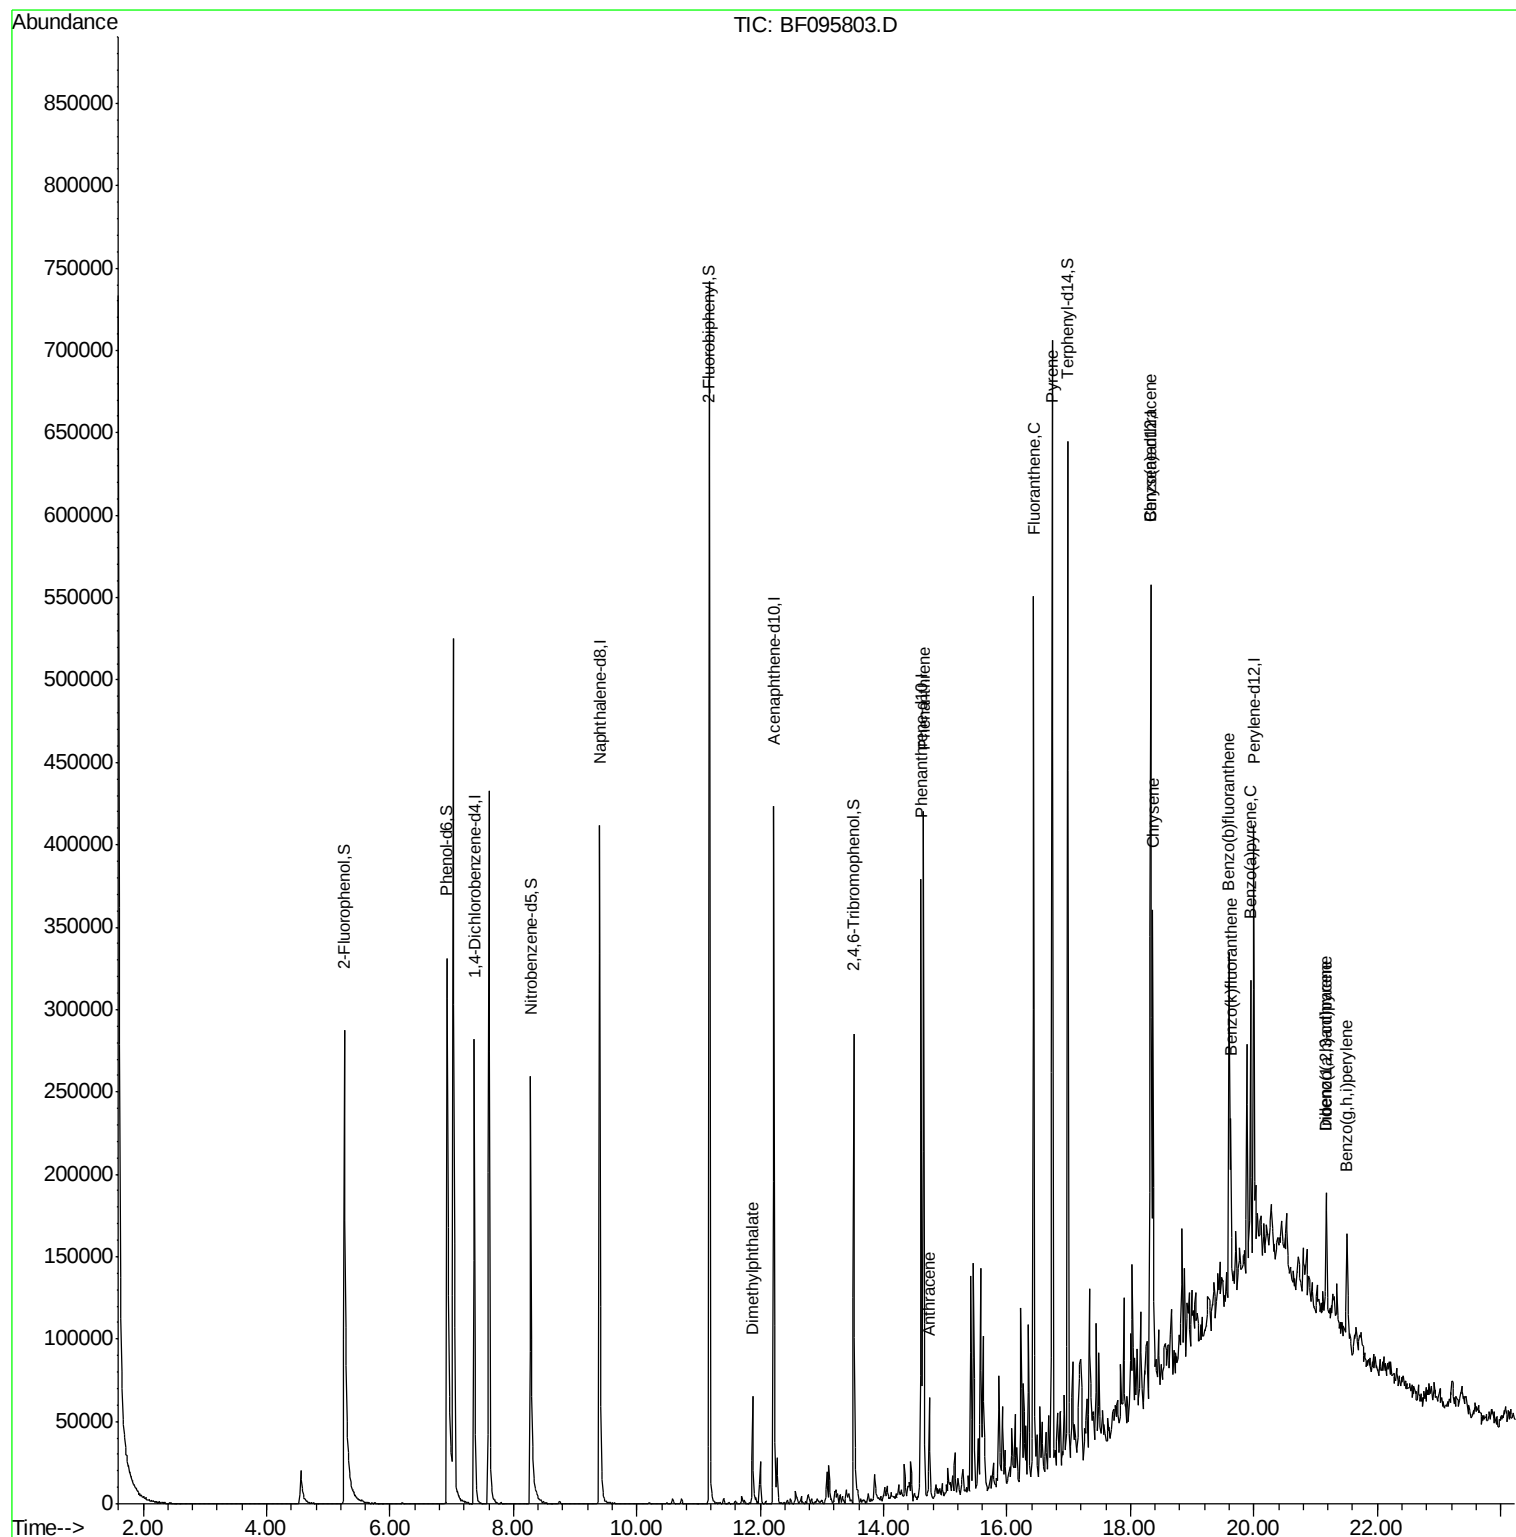



#1


1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.37 min Scan# 983
Delta R.T. -0.03 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602



Tot Ion	Ratio	Lower	Upper
152	100		
150	157.8	126.2	189.2
115	57.1	52.2	78.2

Manual Integrations
APPROVED

mohammad
6/9/2017 12:09:31 PM




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

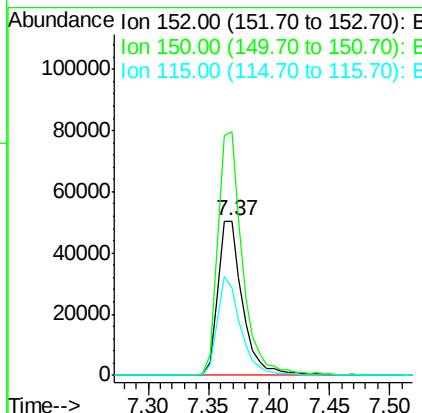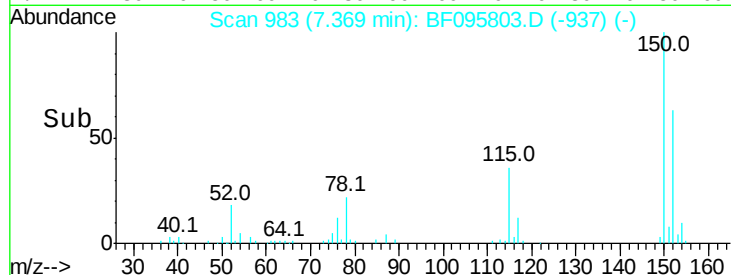



#5

2-Fluorophenol
Concen: 51.73 ng
RT: 5.26 min Scan# 624
Delta R.T. -0.03 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Lower	Upper
112	100		
64	51.1	46.0	69.0
63	25.4	23.4	35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

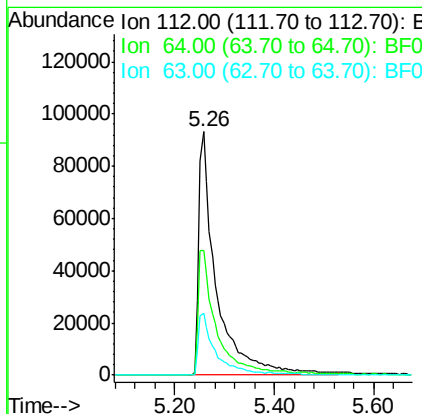



#7

Phenol-d6

Concen: 52.26 ng

RT: 6.92 min Scan# 907

Delta R.T. -0.04 min

Lab File: BF095803.D

Acq: 9 Jun 2017 1:50

Instrument :

BNA_F




ClientSampleId :

POSTEX-45-20170602

Tot Ion:	99	Resp:	277325
Ion Ratio	Lower	Upper	
99	100		
42	15.2	13.5	20.3
71	30.9	24.5	36.7

Manual Integrations
APPROVED

mohammad
6/9/2017 12:09:31 PM

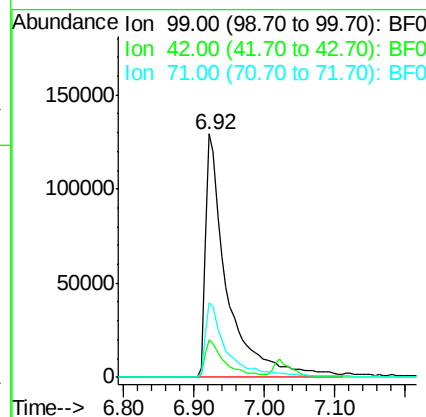

#21

Naphthalene-d8

Concen: 20.00 ng




RT: 9.40 min Scan# 1328

Delta R.T. -0.04 min

Lab File: BF095803.D

Acq: 9 Jun 2017 1:50

Tgt Ion:	136	Resp:	282793
Ion Ratio	Lower	Upper	
136	100		
137	10.8	8.5	12.7
54	6.3	4.9	7.3
68	5.2	4.1	6.1

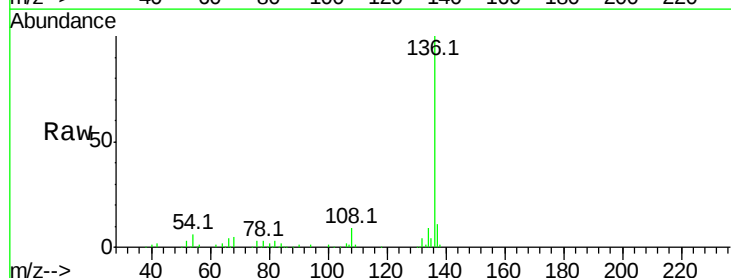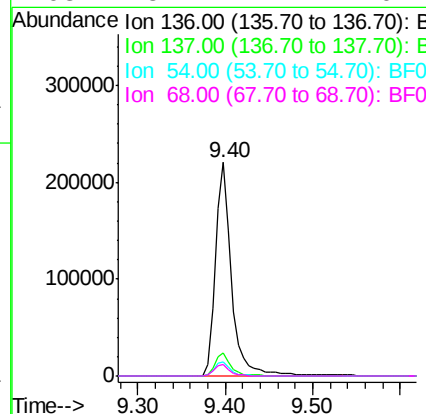




#23
 Nitrobenzene-d5
 Concen: 35.05 ng
 RT: 8.28 min Scan# 1138
 Delta R.T. -0.04 min
 Lab File: BF095803.D
 Acq: 9 Jun 2017 1:50

Instrument :
 BNA_F
 ClientSampleId :
 POSTEX-45-20170602




Tot Ion	Ratio	Lower	Upper
82	100		
128	48.8	34.0	51.0
54	46.3	42.2	63.2

Manual Integrations
 APPROVED

mohammad
 6/9/2017 12:09:31 PM

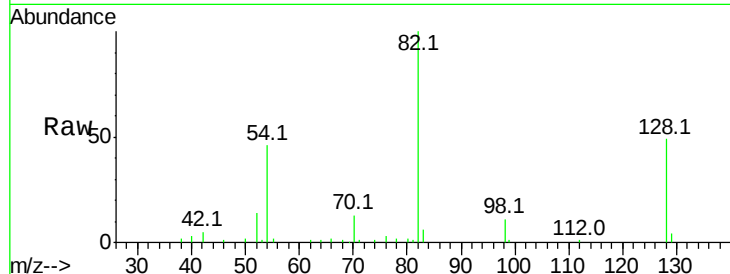




Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

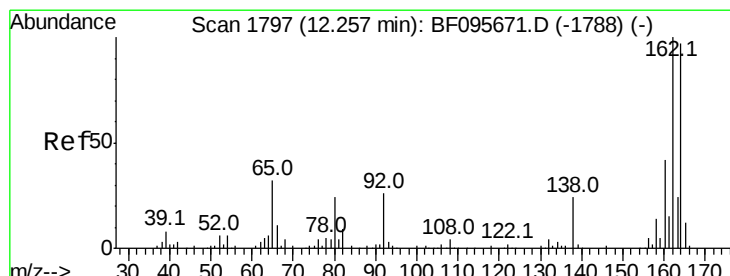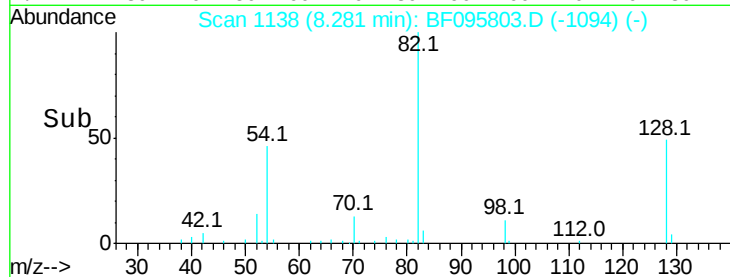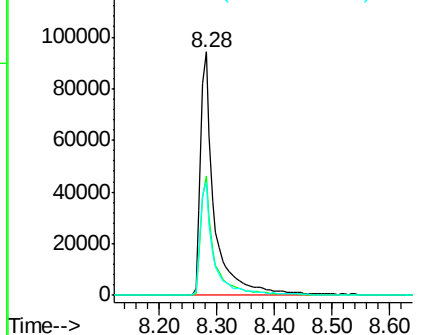

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.22 min Scan# 1808
 Delta R.T. -0.04 min
 Lab File: BF095803.D
 Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.8	82.6	123.8
160	43.8	36.2	54.2

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

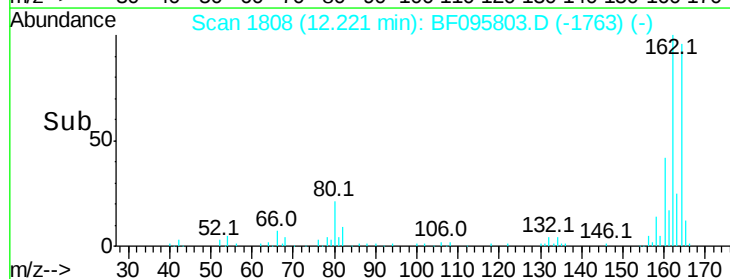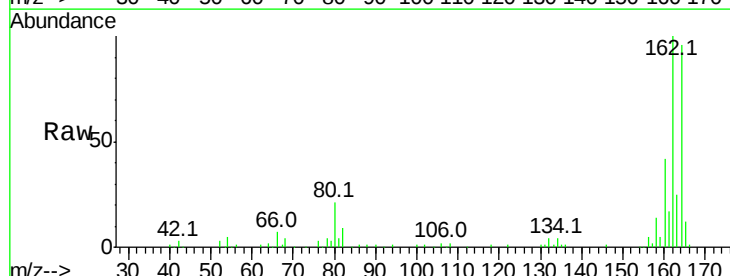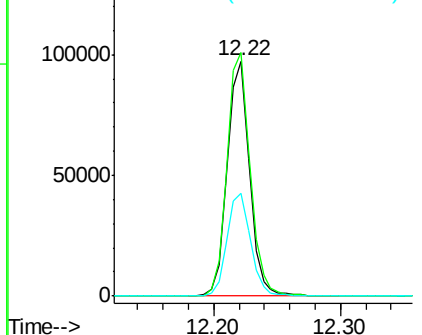




#41
 2,4,6-Tribromophenol
 Concen: 45.81 ng
 RT: 13.52 min Scan# 2028
 Delta R.T. -0.04 min
 Lab File: BF095803.D
 Acq: 9 Jun 2017 1:50

Instrument :
 BNA_F
 ClientSampleId :
 POSTEX-45-20170602



Tot Ion	Ratio	Lower	Upper
330	100		
332	97.5	76.6	115.0
141	38.4	31.4	47.2

Manual Integrations
 APPROVED

mohammad
 6/9/2017 12:09:31 PM




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


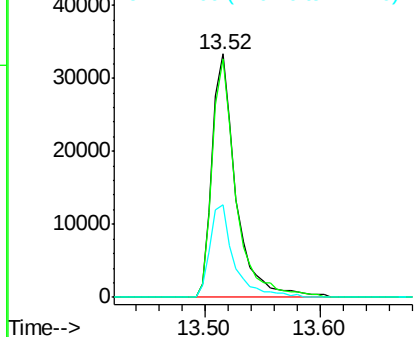


#44
 2-Fluorobiphenyl
 Concen: 38.22 ng
 RT: 11.17 min Scan# 1630
 Delta R.T. -0.04 min
 Lab File: BF095803.D
 Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	29.6	44.4
170	22.5	19.8	29.8

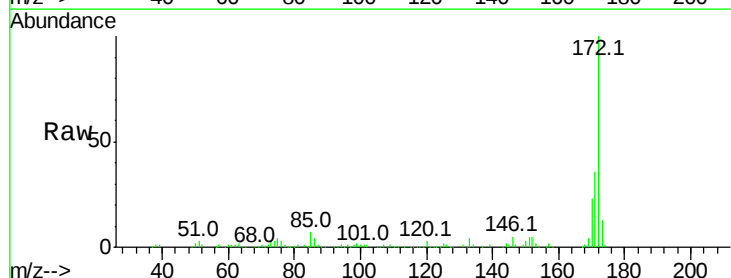

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

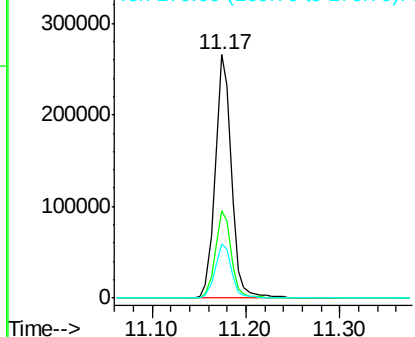




#49
Dimethylphthalate
Concen: 4.87 ng
RT: 11.87 min Scan# 1749
Delta R.T. -0.04 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.5	2.6	4.0
164	9.5	8.4	12.6

Manual Integrations
APPROVED

mohammad
6/9/2017 12:09:31 PM



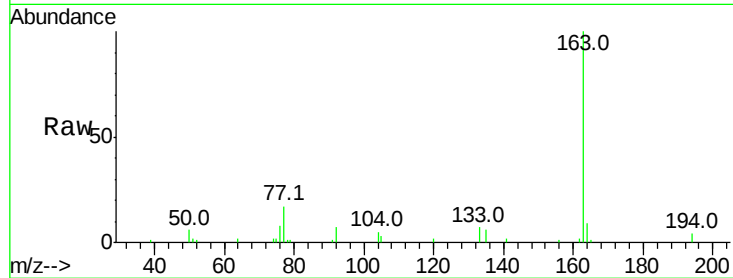


Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

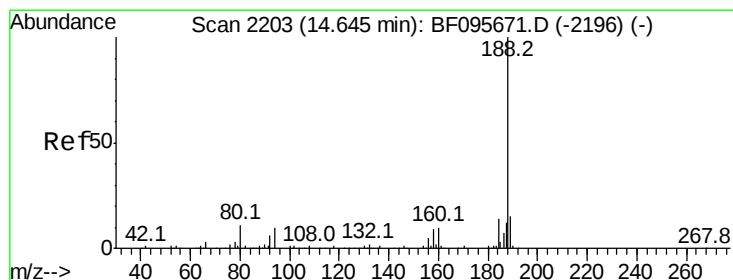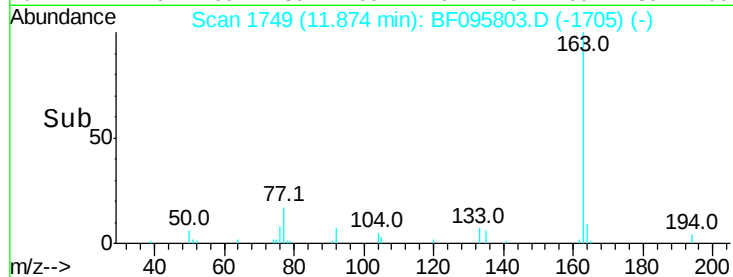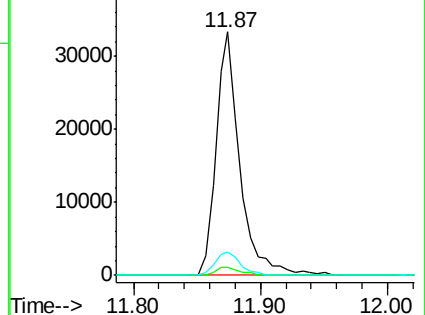

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.61 min Scan# 2214
Delta R.T. -0.04 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50




Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.3	9.4	14.2
80	11.6	10.2	15.2

Abundance

Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

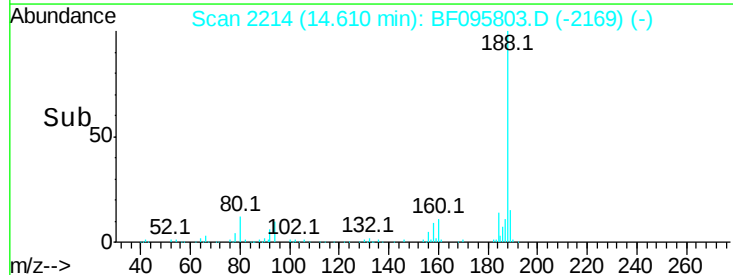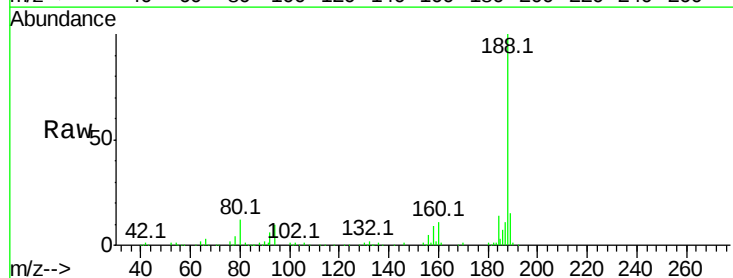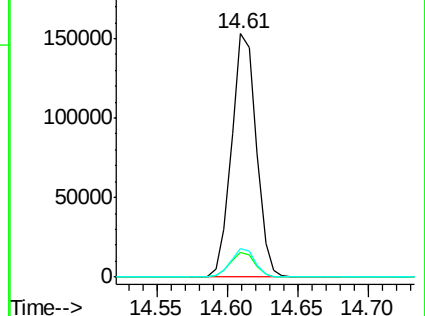







#70
Phenanthrene
Concen: 21.02 ng
RT: 14.65 min Scan# 2221
Delta R.T. -0.04 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602

Tot Ion	Ratio	Lower	Upper
178	100		
176	18.8	16.2	24.4
179	15.2	12.6	19.0




Manual Integrations
APPROVED


mohammad
6/9/2017 12:09:31 PM

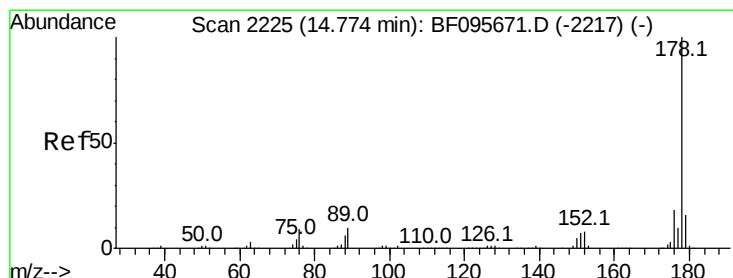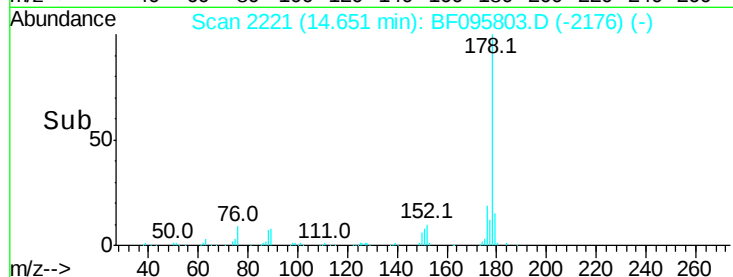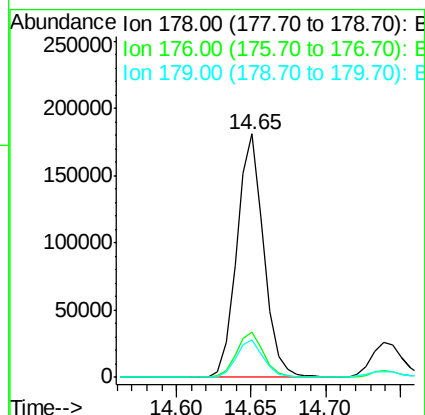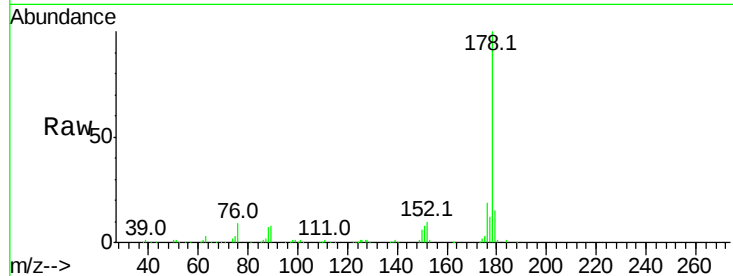

#71
Anthracene
Concen: 3.48 ng
RT: 14.74 min Scan# 2236
Delta R.T. -0.04 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Lower	Upper
178	100		
176	20.7	15.8	23.8
179	17.9	12.7	19.1

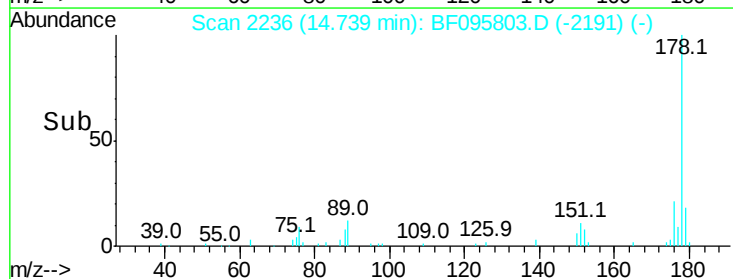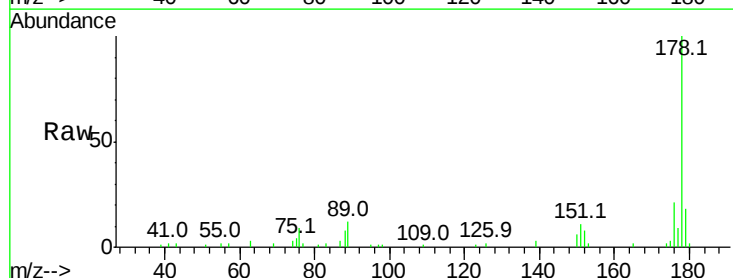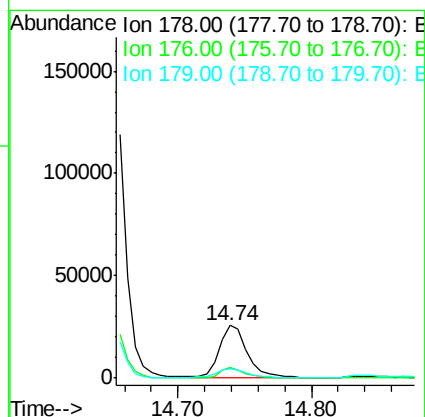

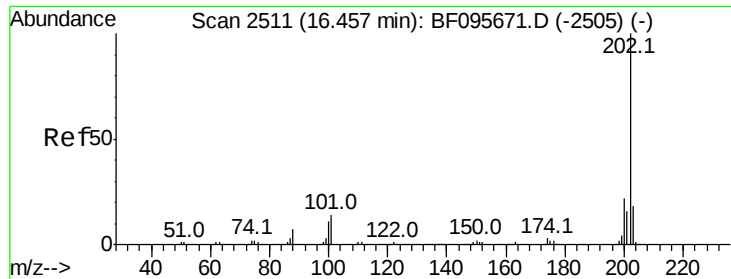

#74

Fluoranthene

Concen: 25.19 ng

RT: 16.43 min Scan# 2524

Delta R.T. -0.02 min

Lab File: BF095803.D

Acq: 9 Jun 2017 1:50

Instrument :

BNA_F


ClientSampleId :

POSTEX-45-20170602




Tot Ion	Ratio	Resp	Lower	Upper
202	100	268975		
101	11.6	0.0	33.2	
203	18.2	0.0	38.1	

Manual Integrations
APPROVED

mohammad
6/9/2017 12:09:31 PM



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

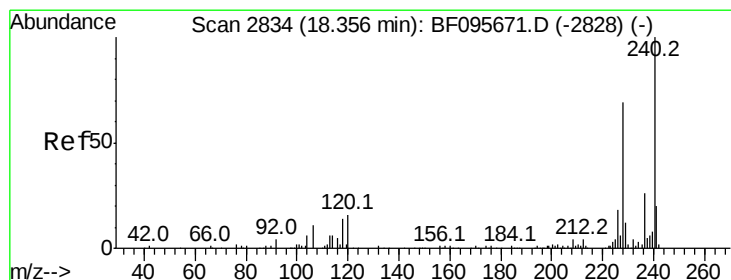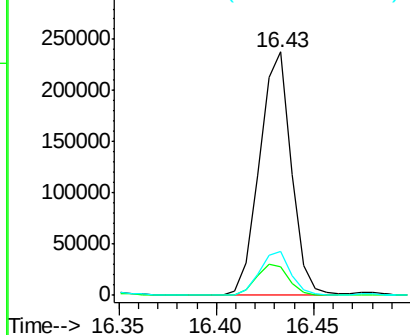

#75

Chrysene-d12

Concen: 20.00 ng


RT: 18.33 min Scan# 2847

Delta R.T. -0.02 min



Lab File: BF095803.D


Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Resp	Lower	Upper
240	100	141189		
120	14.2	5.8	8.8#	
236	25.4	20.5	30.7	

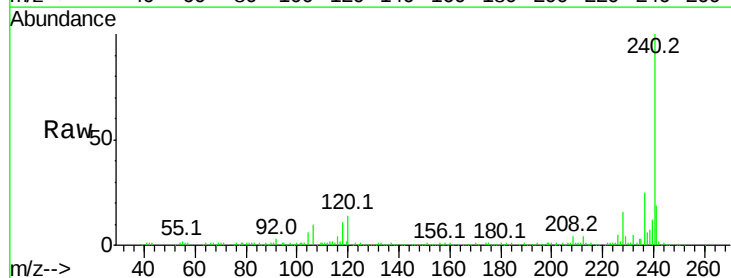

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

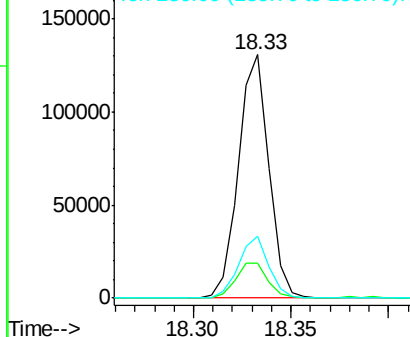

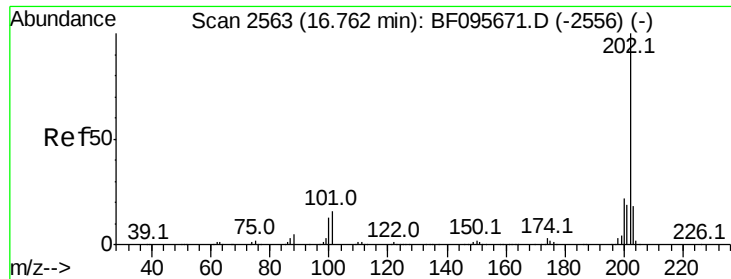





#77
Pvrene
Concen: 27.49 ng
RT: 16.73 min Scan# 2575
Delta R.T. -0.03 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602

Tot Ion	Ratio	Resp Lower	Upper
202	100		
200	21.6	17.6	26.4
203	19.9	14.4	21.6




Manual Integrations
APPROVED


mohammad
6/9/2017 12:09:31 PM

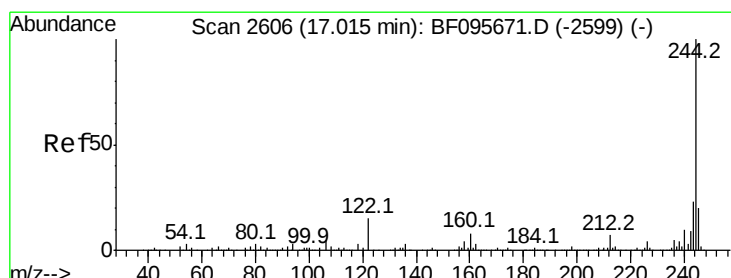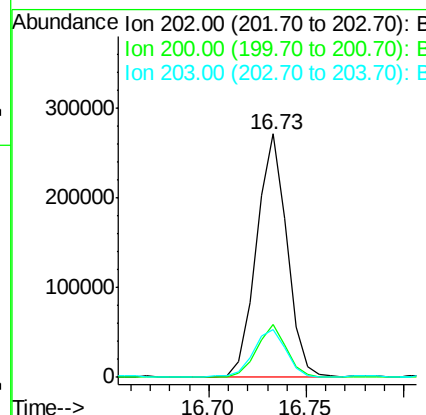

#78
Terphenyl-d14
Concen: 38.07 ng
RT: 16.99 min Scan# 2618
Delta R.T. -0.03 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Resp Lower	Upper
244	100		
212	6.6	6.0	9.0
122	13.5	10.3	15.5

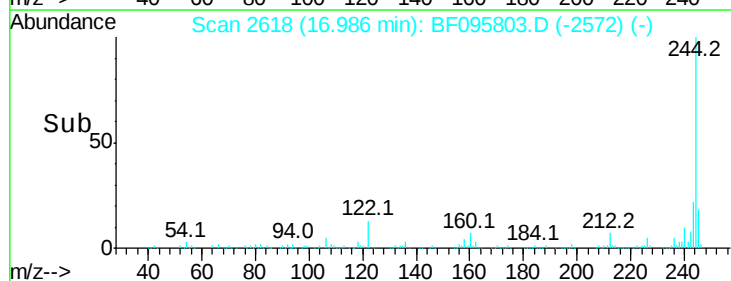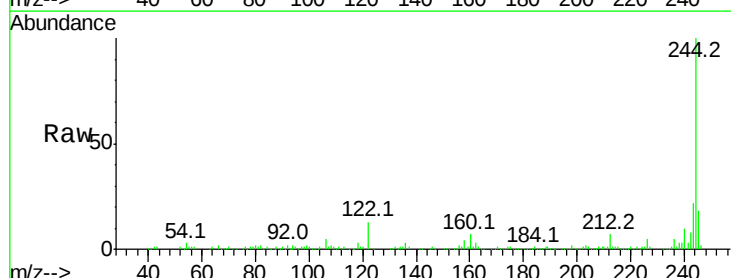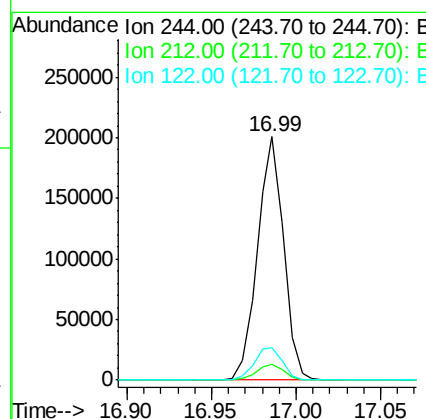

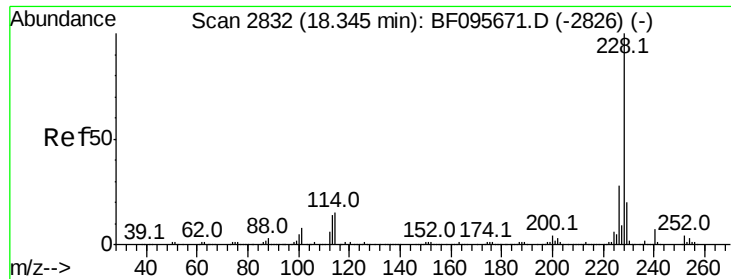





#80
Benzo(a)anthracene
Concen: 14.48 ng
RT: 18.32 min Scan# 2845
Delta R.T. -0.02 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602

Tot Ion	Ratio	Resp	Lower	Upper
228	100	118829		
226	28.8		22.6	33.8
229	21.2		16.3	24.5




Manual Integrations
APPROVED


mohammad
6/9/2017 12:09:31 PM

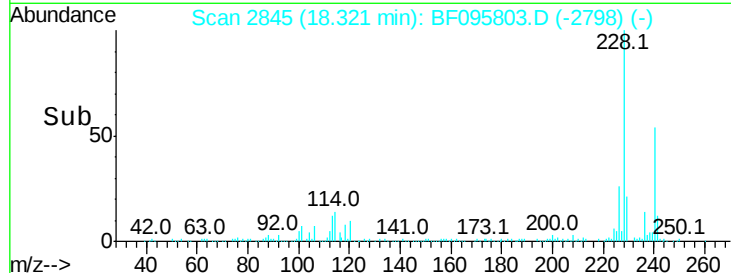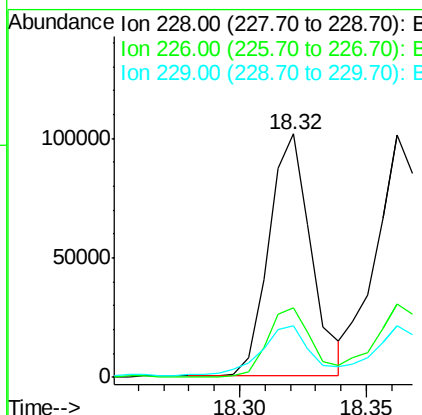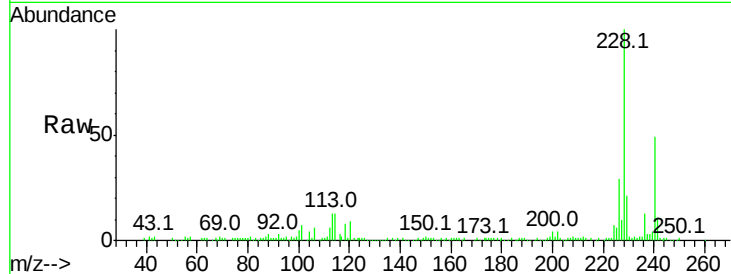

#82
Chrysene
Concen: 15.48 ng
RT: 18.36 min Scan# 2852
Delta R.T. -0.03 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	126988		
226	30.1		24.9	37.3
229	21.1		15.8	23.6

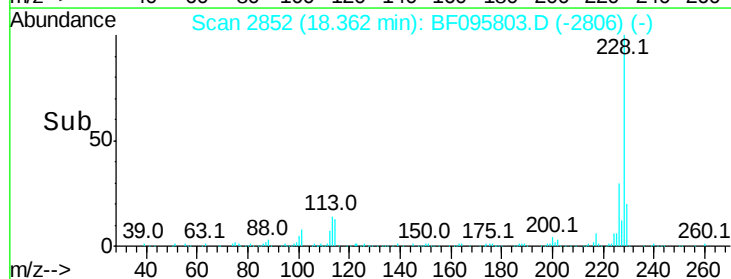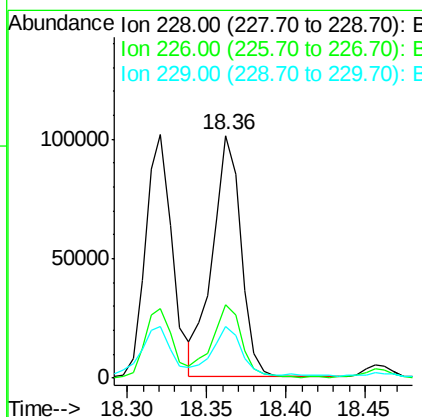

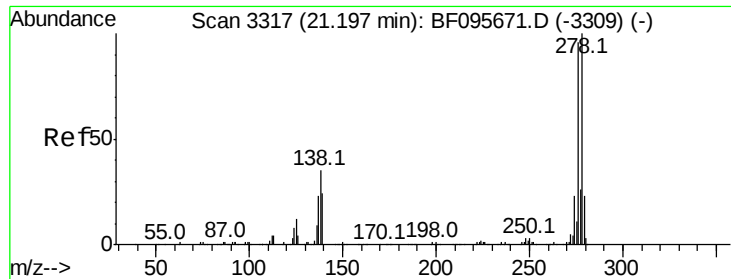


#85
Indeno(1,2,3-cd)pyrene
Concen: 5.41 ng
RT: 21.17 min Scan# 3330
Delta R.T. -0.02 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602




Tot Ion	Ratio	Lower	Upper
276	100		
138	30.4	27.8	41.6
277	25.0	20.2	30.4

Manual Integrations
APPROVED

mohammad
6/9/2017 12:09:31 PM




Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

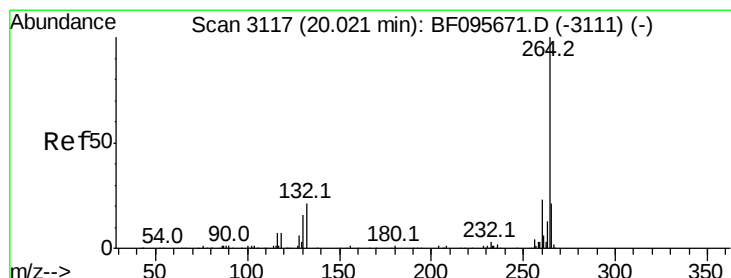
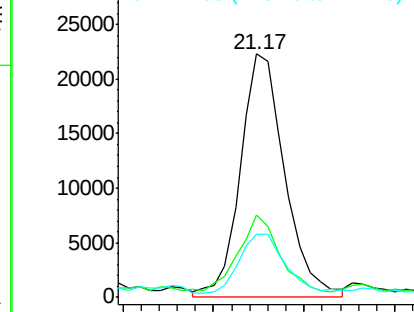



#86
Perylene-d12
Concen: 20.00 ng
RT: 20.00 min Scan# 3130
Delta R.T. -0.02 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.5	29.3
265	21.5	17.2	25.8

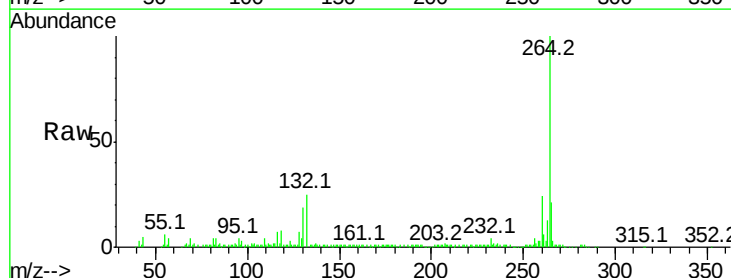

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

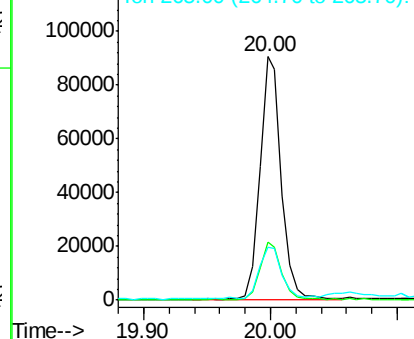

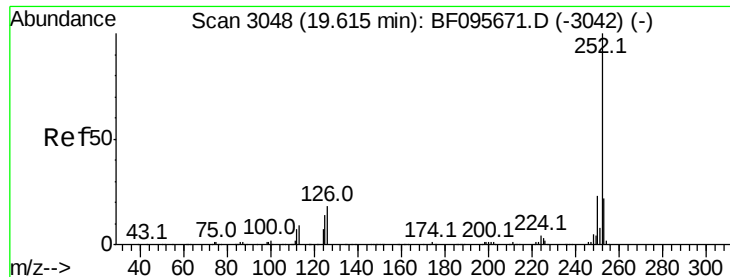

#87

Benzo(b)fluoranthene

Concen: 15.45 ng m

RT: 19.60 min Scan# 3062

Delta R.T. -0.02 min

Lab File: BF095803.D

Acq: 9 Jun 2017 1:50

Instrument :

BNA_F





ClientSampleId :

POSTEX-45-20170602

Tot Ion:	252	Resp:	103937
Ion Ratio	Lower	Upper	
252	100		
253	21.7	18.1	27.1
125	17.1	9.8	14.8#

Manual Integrations
APPROVED

mohammad
6/9/2017 12:09:31 PM

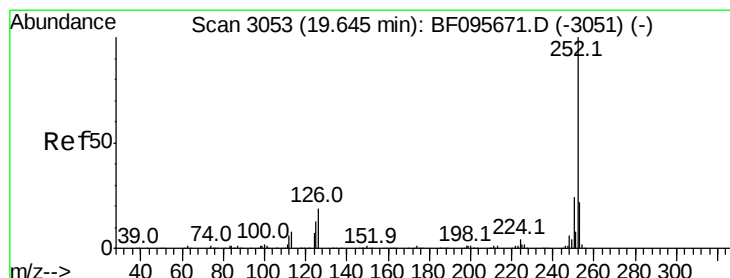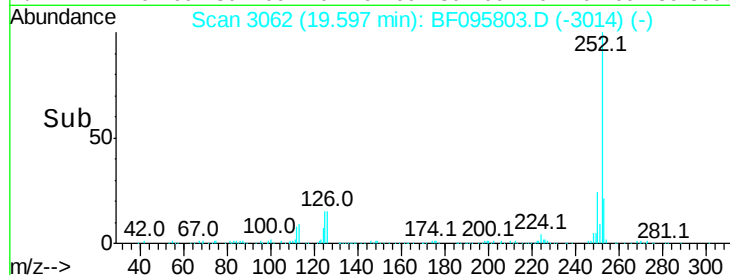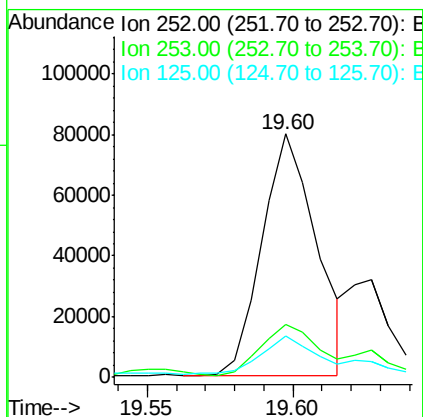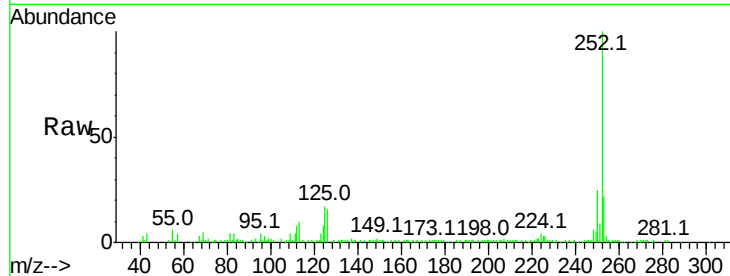

#88

Benzo(k)fluoranthene

Concen: 4.92 ng m




RT: 19.63 min Scan# 3067


Delta R.T. -0.02 min

Lab File: BF095803.D

Acq: 9 Jun 2017 1:50

Tgt Ion:	252	Resp:	31644
Ion Ratio	Lower	Upper	
252	100		
253	27.5	18.4	27.6
125	15.8	13.1	19.7

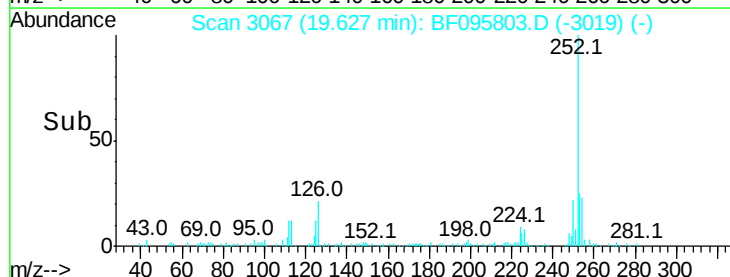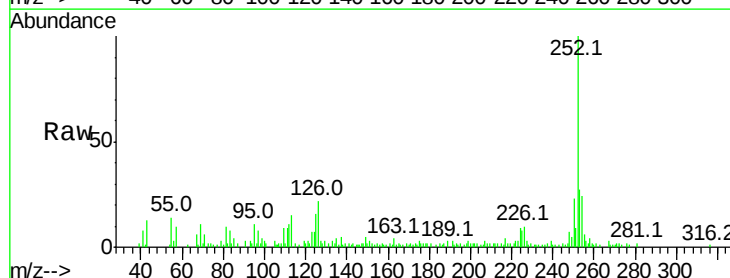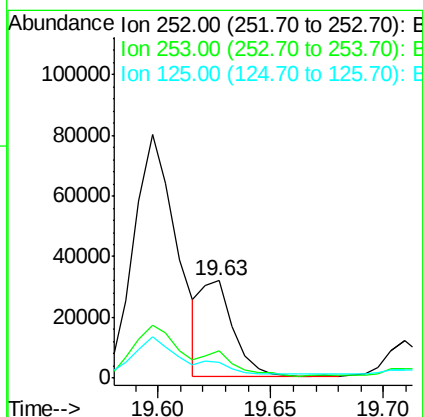

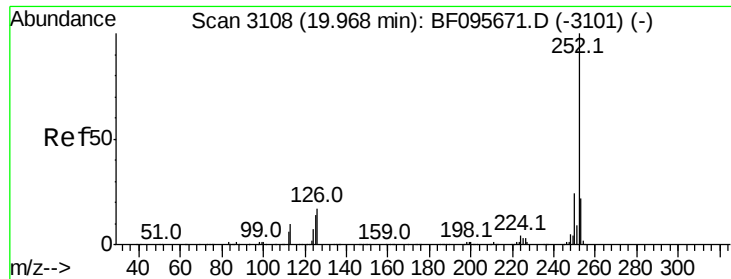





#89
Benzo(a)pyrene
Concen: 11.19 ng
RT: 19.94 min Scan# 3121
Delta R.T. -0.02 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Instrument :
BNA_F
ClientSampleId :
POSTEX-45-20170602

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.5	26.3
125	15.8	11.0	16.4




Manual Integrations
APPROVED


mohammad
6/9/2017 12:09:31 PM

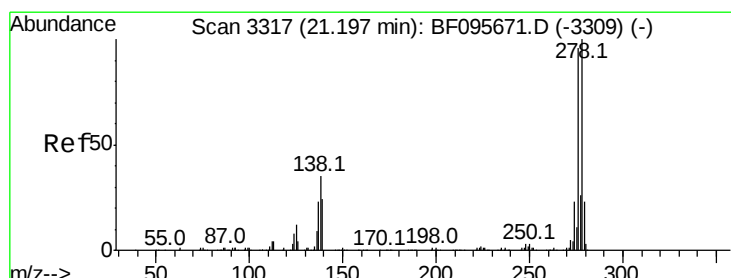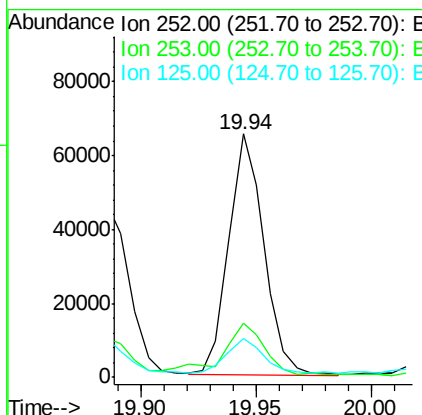

#90
Dibenzo(a,h)anthracene
Concen: 2.01 ng
RT: 21.17 min Scan# 3330
Delta R.T. -0.02 min
Lab File: BF095803.D
Acq: 9 Jun 2017 1:50

Tgt Ion	Ratio	Lower	Upper
278	100		
139	38.4	16.6	24.8#
279	25.9	19.3	28.9

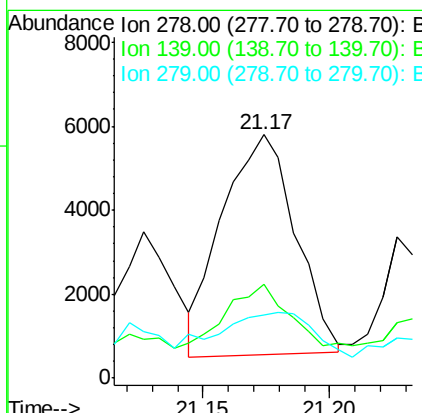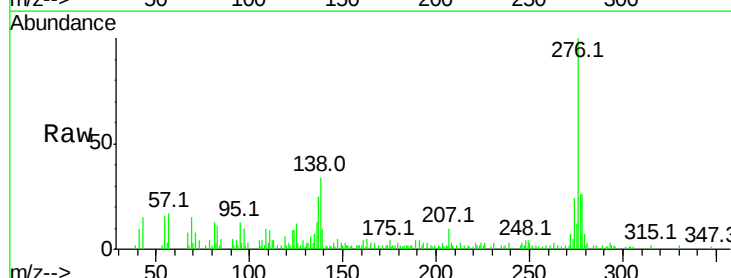

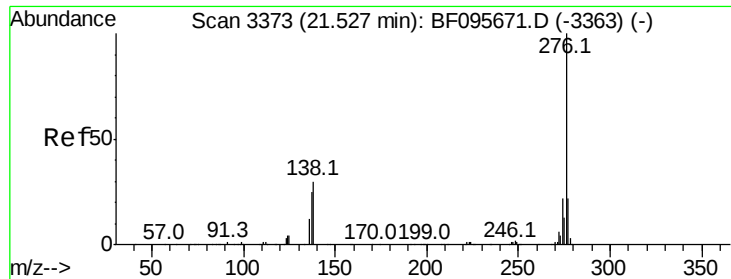

#91
 Benzo(a,h,i)perylene
 Concen: 6.80 ng
 RT: 21.51 min Scan# 3387
 Delta R.T. -0.02 min
 Lab File: BF095803.D
 Acq: 9 Jun 2017 1:50

Instrument :
 BNA_F
 ClientSampleId :
 POSTEX-45-20170602

Tot Ion	Ratio	Resp Lower	Upper
276	100		
277	29.0	18.6	28.0#
138	34.1	25.4	38.0

Manual Integrations
 APPROVED

mohammad
 6/9/2017 12:09:31 PM

