


Data Path : Z:\HPCHEM1\BNA F\Data\BF060817\
 Data File : BF095774.D
 Acq On : 8 Jun 2017 10:09
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

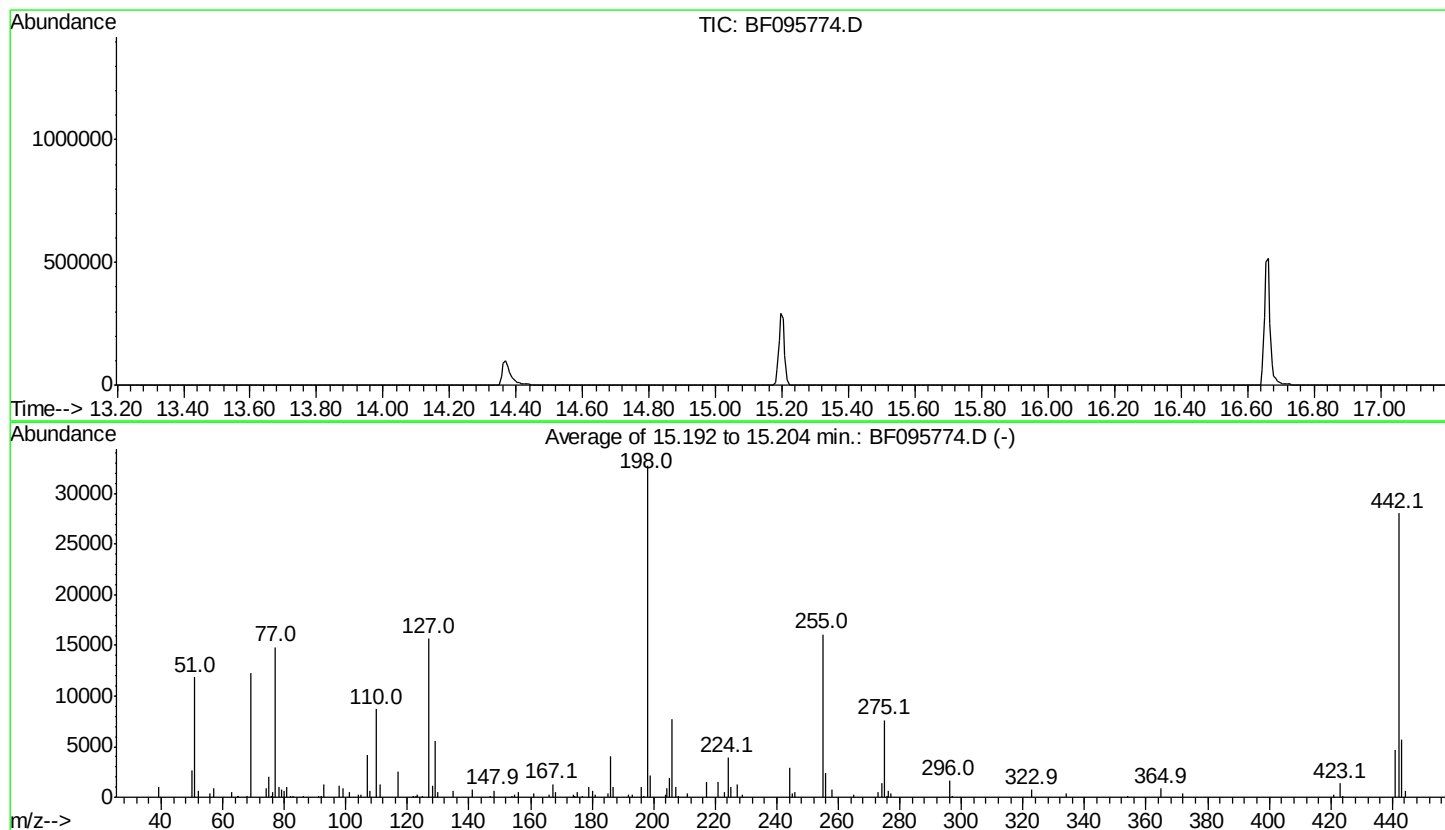

AutoFind: Scans 2313, 2314, 2315; Background Corrected with Scan 2307

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	11855	PASS
68	69	0.00	2	0.8	102	PASS
69	198	0.00	100	37.3	12229	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	15683	PASS
197	198	0.00	2	0.4	146	PASS
198	198	100	100	100.0	32776	PASS
199	198	5	9	6.7	2189	PASS
275	198	10	60	23.3	7650	PASS
365	198	1	100	2.5	832	PASS
441	442	0.01	24	16.8	4705	PASS
442	198	50	100	85.6	28056	PASS
443	442	15	24	20.5	5758	PASS