
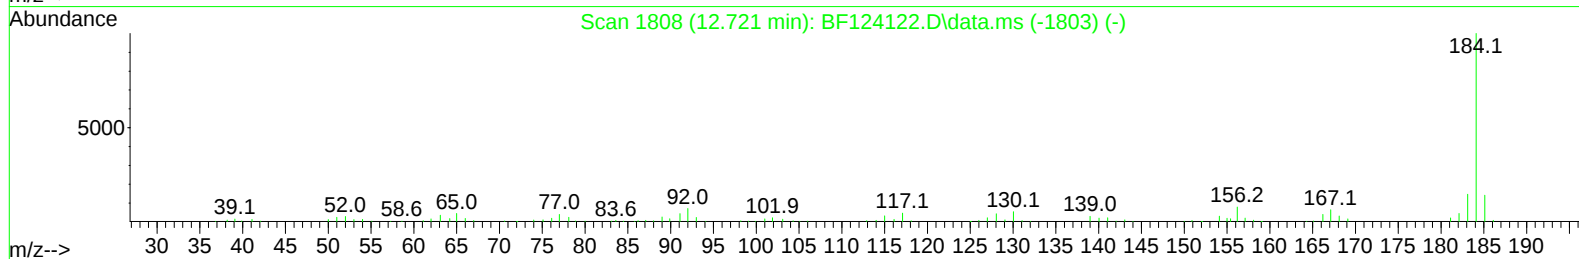
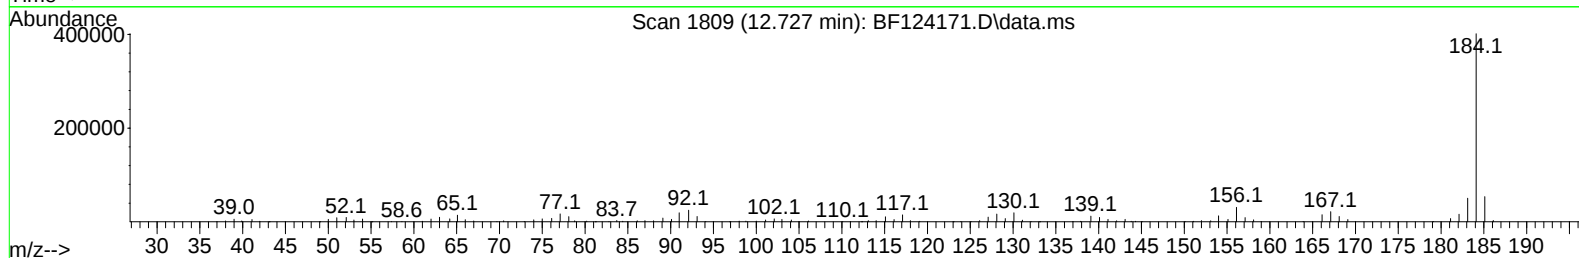


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
 Data File : BF124171.D
 Acq On : 8 Jun 2021 8:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 11:25:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 07 13:32:21 2021
 Response via : Initial Calibration

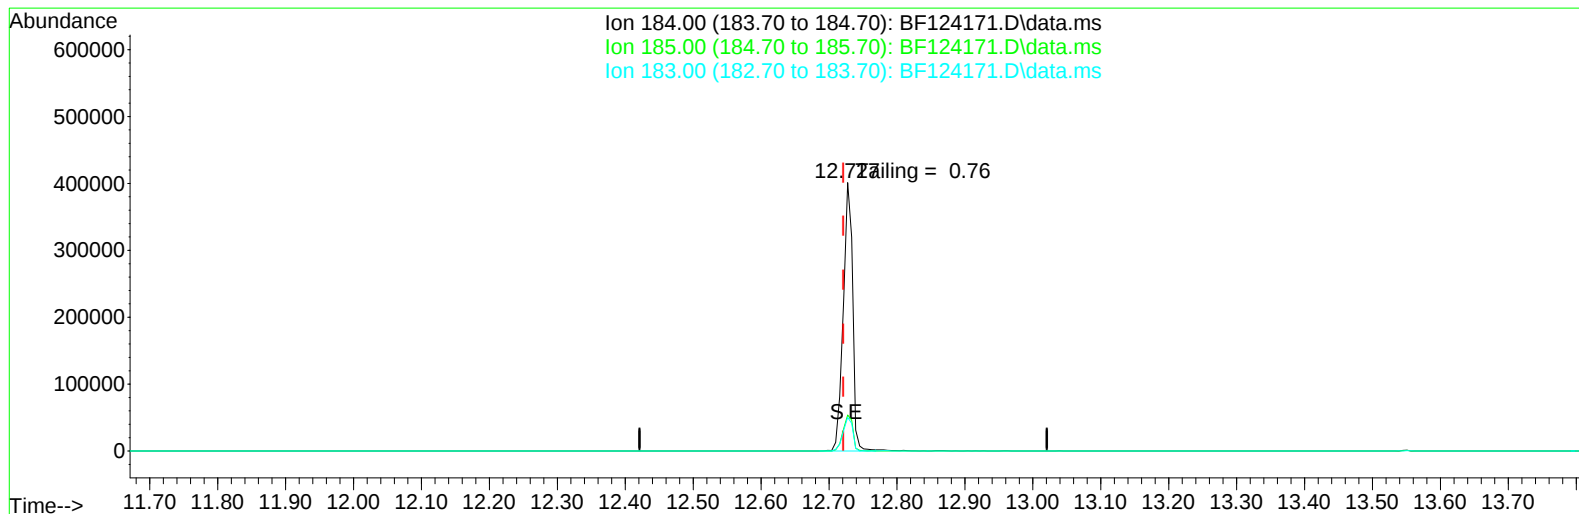

TIC: BF124171.D\data.ms

(77) Benzidine




12.727min (+ 0.006) 0.00 ng

response 387464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.41
183.00	9.80	12.56#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124171.D
Acq On : 8 Jun 2021 8:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 11:25:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 07 13:32:21 2021
Response via : Initial Calibration

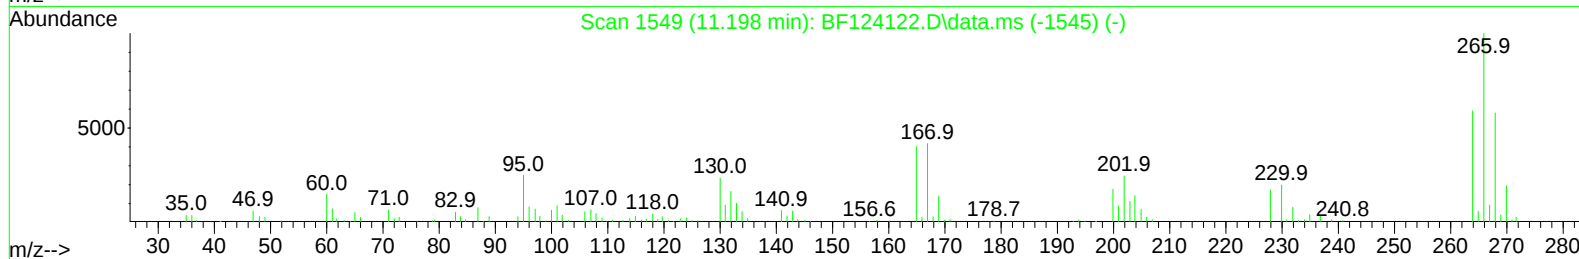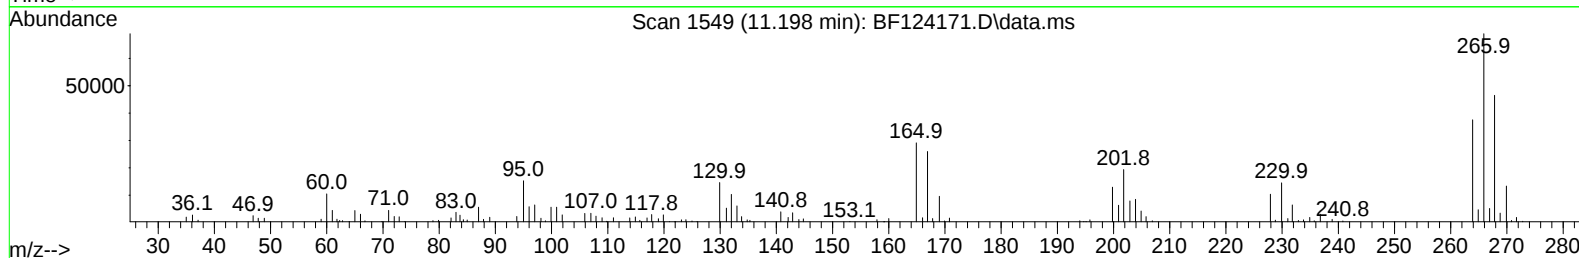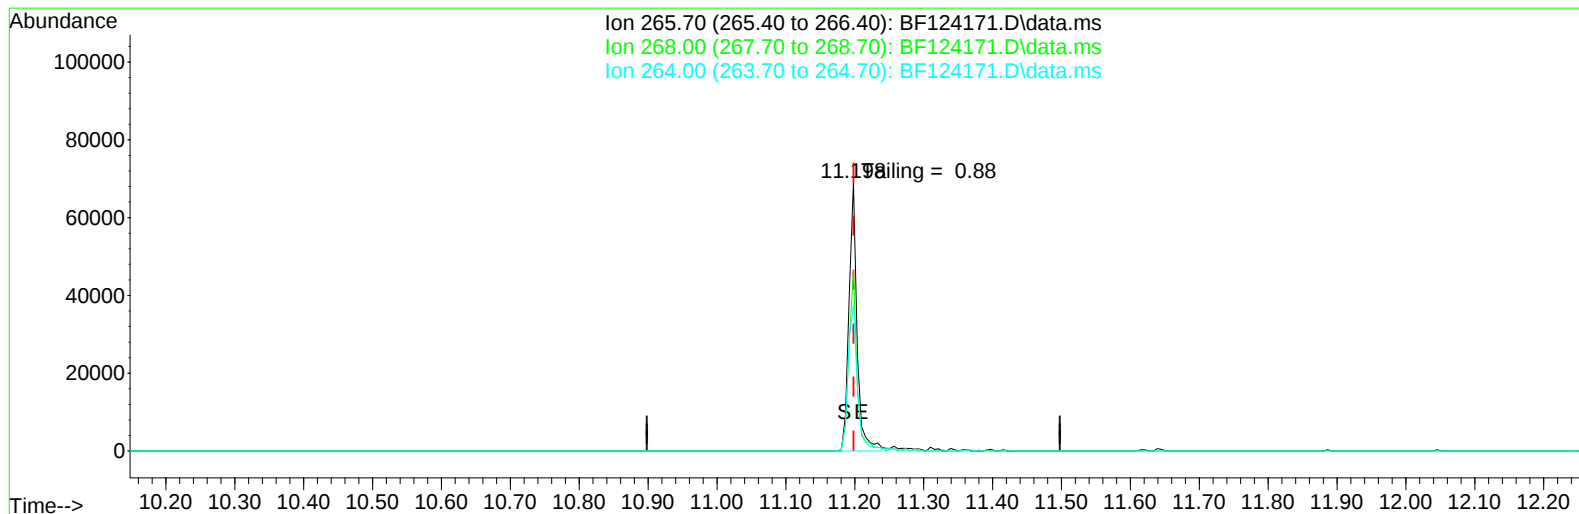

TIC: BF124171.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 12425.32 ng

response 57053

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	67.40
264.00	65.70	54.42
0.00	0.00	0.00