

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
 Data File : BF124197.D
 Acq On : 9 Jun 2021 00:34
 Operator : JU/CG
 Sample : M2589-19RE 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 18-B12(2-4)RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.446	398	401	407	rBB	26298	27189	10.33%	0.739%
2	5.069	503	507	511	rBV	233728	224568	85.28%	6.106%
3	5.504	578	581	588	rBB	39417	43104	16.37%	1.172%
4	6.510	749	752	766	rBB	105066	116131	44.10%	3.158%
5	6.693	780	783	788	rBB3	5771	7016	2.66%	0.191%
6	6.863	808	812	817	rBB	304234	223137	84.74%	6.067%
7	7.422	903	907	911	rVV	156884	119657	45.44%	3.253%
8	7.457	911	913	918	rVB2	11131	8785	3.34%	0.239%
9	8.145	1025	1030	1033	rBV	289279	241374	91.67%	6.563%
10	8.569	1099	1102	1104	rBV2	7657	7128	2.71%	0.194%
11	8.734	1128	1130	1135	rBV	15378	12317	4.68%	0.335%
12	8.857	1148	1151	1155	rVB	7453	8437	3.20%	0.229%
13	8.957	1166	1168	1171	rBV	5648	5423	2.06%	0.147%
14	9.092	1189	1191	1195	rBV2	3844	4820	1.83%	0.131%
15	9.169	1200	1204	1206	rVB	6819	6299	2.39%	0.171%
16	9.222	1209	1213	1216	rBV	261716	219711	83.44%	5.974%
17	9.298	1223	1226	1233	rVB	19056	21980	8.35%	0.598%
18	9.416	1243	1246	1251	rBV	3515	4898	1.86%	0.133%
19	9.486	1254	1258	1262	rBV3	5634	7297	2.77%	0.198%
20	9.563	1267	1271	1273	rBV2	9554	9628	3.66%	0.262%
21	9.622	1277	1281	1283	rBV3	12805	12583	4.78%	0.342%
22	9.681	1288	1291	1294	rBV3	5636	5126	1.95%	0.139%
23	9.763	1303	1305	1307	rBV2	5517	4117	1.56%	0.112%
24	9.828	1310	1316	1320	rBV	18297	22146	8.41%	0.602%
25	9.904	1325	1329	1332	rVV	302710	244410	92.82%	6.645%
26	9.934	1332	1334	1338	rVB3	11340	9800	3.72%	0.266%
27	10.004	1343	1346	1348	rBV3	3892	4575	1.74%	0.124%
28	10.110	1358	1364	1367	rVB4	10720	17584	6.68%	0.478%
29	10.145	1367	1370	1375	rBV4	8501	13474	5.12%	0.366%
30	10.245	1385	1387	1390	rBV2	6081	4522	1.72%	0.123%
31	10.328	1393	1401	1405	rBV4	21574	22954	8.72%	0.624%
32	10.451	1416	1422	1425	rBV3	10496	15442	5.86%	0.420%
33	10.510	1428	1432	1433	rVV2	3357	4663	1.77%	0.127%
34	10.557	1436	1440	1444	rVV3	12035	19688	7.48%	0.535%
35	10.610	1444	1449	1451	rVB2	5293	7546	2.87%	0.205%
36	10.675	1457	1460	1461	rBV3	5921	7010	2.66%	0.191%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
 Data File : BF124197.D
 Acq On : 9 Jun 2021 00:34
 Operator : JU/CG
 Sample : M2589-19RE 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 18-B12(2-4)RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	10.692	1461	1463	1467	rVV5	12179	10441	3.97%	0.284%
38	10.769	1473	1476	1479	rBV4	3721	4392	1.67%	0.119%
39	10.804	1479	1482	1483	rBV	22415	18502	7.03%	0.503%
40	10.992	1511	1514	1517	rBV2	18646	17447	6.63%	0.474%

41	11.028	1519	1520	1523	rVB2	7152	4476	1.70%	0.122%
42	11.192	1546	1548	1550	rBV3	4807	4321	1.64%	0.117%
43	11.251	1553	1558	1560	rVV2	21336	20557	7.81%	0.559%
44	11.280	1560	1563	1568	rVB4	16941	19702	7.48%	0.536%
45	11.392	1578	1582	1584	rBV	320681	263318	100.00%	7.160%

46	11.416	1584	1586	1588	rVV	92415	72786	27.64%	1.979%
47	11.445	1588	1591	1592	rVV2	7926	7572	2.88%	0.206%
48	11.469	1592	1595	1597	rVB	22314	16862	6.40%	0.458%
49	11.498	1597	1600	1603	rBV4	8536	7983	3.03%	0.217%
50	11.569	1609	1612	1614	rVB3	5204	5932	2.25%	0.161%

51	11.622	1619	1621	1624	rVV3	10642	11582	4.40%	0.315%
52	11.680	1628	1631	1634	rVB5	16363	17761	6.75%	0.483%
53	11.716	1634	1637	1641	rBV6	5640	9081	3.45%	0.247%
54	11.780	1645	1648	1650	rBV3	8088	8338	3.17%	0.227%
55	11.804	1650	1652	1654	rBV3	5324	5023	1.91%	0.137%

56	11.845	1657	1659	1661	rVV3	5163	5064	1.92%	0.138%
57	11.892	1664	1667	1669	rVV4	18378	14785	5.61%	0.402%
58	11.922	1670	1672	1675	rVV2	24227	20631	7.84%	0.561%
59	11.963	1677	1679	1680	rVV2	5748	4573	1.74%	0.124%
60	12.004	1683	1686	1688	rVV3	22842	22403	8.51%	0.609%

61	12.028	1688	1690	1694	rVB5	15618	12402	4.71%	0.337%
62	12.086	1697	1700	1704	rBV6	21314	20478	7.78%	0.557%
63	12.186	1714	1717	1720	rBV4	8463	11657	4.43%	0.317%
64	12.216	1720	1722	1724	rBV3	8311	8571	3.25%	0.233%
65	12.322	1736	1740	1741	rBV4	11984	11539	4.38%	0.314%

66	12.339	1741	1743	1744	rVV2	9217	6541	2.48%	0.178%
67	12.369	1746	1748	1751	rVV4	11958	12428	4.72%	0.338%
68	12.392	1751	1752	1754	rVV2	10013	7832	2.97%	0.213%
69	12.445	1758	1761	1763	rBV3	20344	23797	9.04%	0.647%
70	12.480	1763	1767	1769	rVV5	19499	20598	7.82%	0.560%

71	12.604	1785	1788	1792	rVB	119330	114386	43.44%	3.110%
72	12.639	1792	1794	1796	rBV3	18682	17651	6.70%	0.480%
73	12.710	1803	1806	1808	rBV4	12205	16541	6.28%	0.450%
74	12.786	1817	1819	1822	rBV4	8375	9330	3.54%	0.254%
75	12.833	1822	1827	1833	rBV	101221	133705	50.78%	3.635%

76	12.933	1841	1844	1845	rBV3	11094	13941	5.29%	0.379%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124197.D
Acq On : 9 Jun 2021 00:34
Operator : JU/CG
Sample : M2589-19RE 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B12(2-4)RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	12.975	1848	1851	1854	rVB	304579	257203	97.68%	6.993%
78	13.163	1880	1883	1886	rVB5	28568	35259	13.39%	0.959%
79	13.210	1886	1891	1892	rBV5	22886	34396	13.06%	0.935%
80	13.227	1892	1894	1897	rVV4	21944	18214	6.92%	0.495%
81	13.457	1931	1933	1936	rVB3	39982	33883	12.87%	0.921%
82	13.645	1963	1965	1967	rBV3	23298	21941	8.33%	0.597%
83	14.010	2025	2027	2028	rBV	44137	28729	10.91%	0.781%
84	14.039	2028	2032	2034	rVV2	249898	250365	95.08%	6.807%
85	14.063	2034	2036	2039	rVB	44246	36331	13.80%	0.988%
86	15.521	2281	2284	2290	rVB2	129878	192076	72.94%	5.222%



Sum of corrected areas: 3677865

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124197.D
Acq On : 9 Jun 2021 00:34
Operator : JU/CG
Sample : M2589-19RE 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B12(2-4)RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

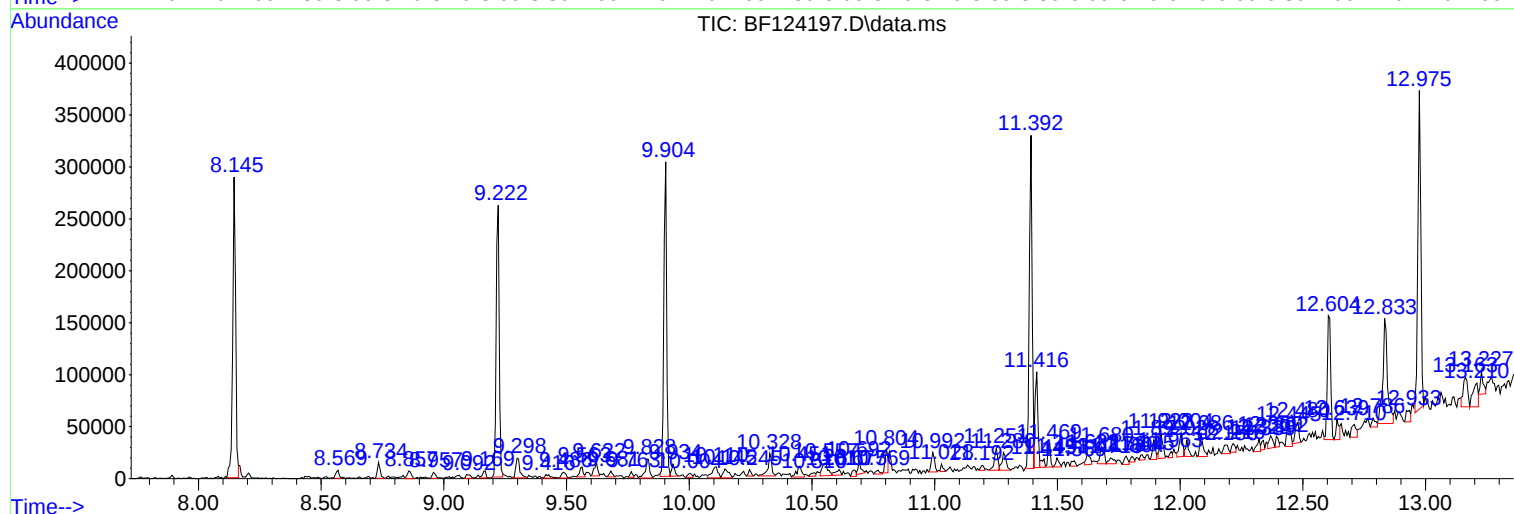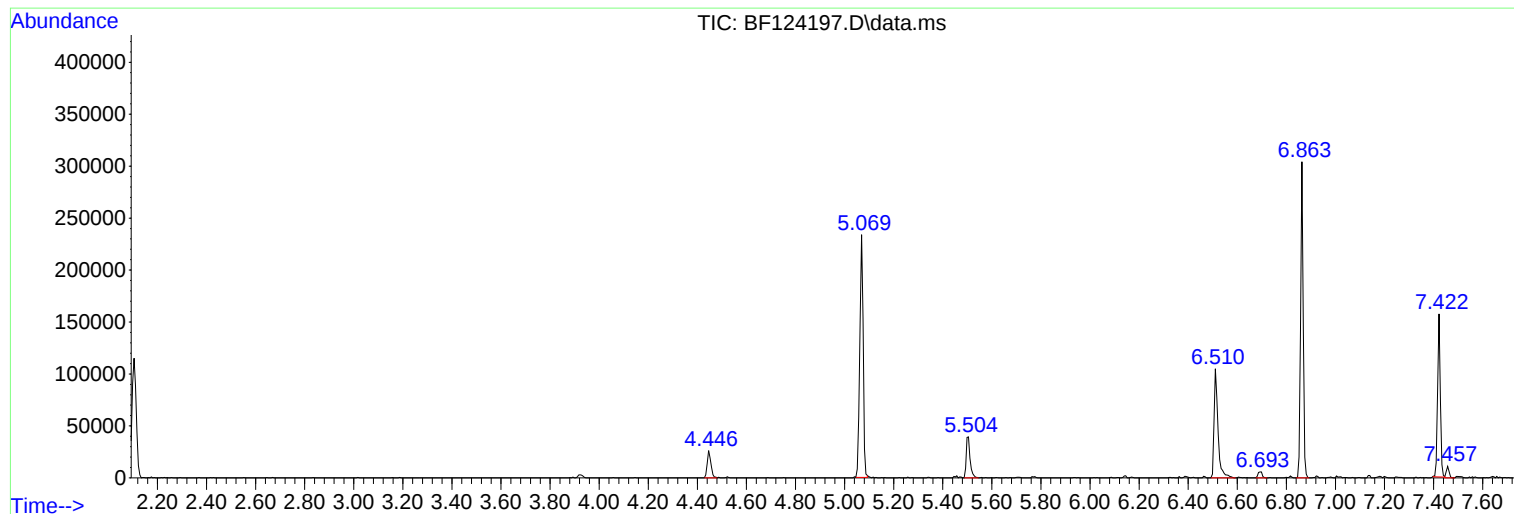

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124197.D
Acq On : 9 Jun 2021 00:34
Operator : JU/CG
Sample : M2589-19RE 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B12(2-4)RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124197.D
Acq On : 9 Jun 2021 00:34
Operator : JU/CG
Sample : M2589-19RE 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B12(2-4)RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------