

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
 Data File : BF124200.D
 Acq On : 9 Jun 2021 2:12
 Operator : JU/CG
 Sample : M2589-07 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 18-B9(0-2)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.445	398	401	405	rBB2	12680	13082	5.87%	0.813%
2	5.063	503	506	512	rBB	24996	24518	11.01%	1.524%
3	5.498	577	580	584	rBV2	13444	13877	6.23%	0.863%
4	6.516	750	753	760	rBB	21397	23746	10.66%	1.476%
5	6.863	809	812	815	rBV	227489	172957	77.66%	10.751%
6	7.422	904	907	911	rBV	26174	21244	9.54%	1.321%
7	8.145	1027	1030	1038	rVB	247207	192728	86.54%	11.980%
8	9.222	1210	1213	1220	rVB	39506	35061	15.74%	2.179%
9	9.904	1325	1329	1332	rBV	270791	205938	92.47%	12.801%
10	10.698	1461	1464	1467	rVB2	3590	4052	1.82%	0.252%
11	11.392	1578	1582	1585	rBV	270317	222710	100.00%	13.844%
12	11.416	1585	1586	1592	rVB4	10177	6355	2.85%	0.395%
13	11.527	1603	1605	1609	rBV	2055	3124	1.40%	0.194%
14	11.604	1614	1618	1620	rBV	3332	4202	1.89%	0.261%
15	11.686	1628	1632	1634	rBV	4086	4758	2.14%	0.296%
16	11.757	1641	1644	1647	rBV	2338	3345	1.50%	0.208%
17	11.898	1663	1668	1670	rBV3	2781	4142	1.86%	0.257%
18	11.957	1677	1678	1682	rBV3	3837	3123	1.40%	0.194%
19	12.004	1684	1686	1688	rBV2	3782	3478	1.56%	0.216%
20	12.033	1688	1691	1695	rVB3	3797	5052	2.27%	0.314%
21	12.139	1705	1709	1714	rVB5	5181	7923	3.56%	0.492%
22	12.257	1725	1729	1731	rVB4	4449	5478	2.46%	0.341%
23	12.333	1740	1742	1747	rVB3	14825	15948	7.16%	0.991%
24	12.368	1747	1748	1749	rBV	6956	3072	1.38%	0.191%
25	12.451	1759	1762	1763	rBV2	4575	3462	1.55%	0.215%
26	12.604	1786	1788	1792	rBV	25574	21879	9.82%	1.360%
27	12.645	1792	1795	1799	rVV5	7105	7820	3.51%	0.486%
28	12.839	1822	1828	1833	rBV	24868	35098	15.76%	2.182%
29	12.927	1841	1843	1845	rBV3	5914	4302	1.93%	0.267%
30	12.974	1848	1851	1854	rVB	76333	62839	28.22%	3.906%
31	13.010	1854	1857	1858	rBV2	5098	5675	2.55%	0.353%
32	13.057	1863	1865	1867	rBV2	4209	4295	1.93%	0.267%
33	13.098	1871	1872	1873	rBV	10543	5798	2.60%	0.360%
34	13.115	1873	1875	1878	rVB4	14860	12926	5.80%	0.803%
35	13.157	1880	1882	1885	rBV4	8542	6643	2.98%	0.413%
36	13.357	1914	1916	1917	rBV2	6976	4343	1.95%	0.270%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124200.D
Acq On : 9 Jun 2021 2:12
Operator : JU/CG
Sample : M2589-07 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B9(0-2)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	13.586	1953	1955	1957	rBV3	11487	10718	4.81%	0.666%
38	14.039	2028	2032	2035	rBV	232320	222463	99.89%	13.828%
39	14.168	2052	2054	2055	rVB2	16115	7468	3.35%	0.464%
40	15.527	2281	2285	2292	rVB	148875	193096	86.70%	12.003%


Sum of corrected areas: 1608738

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124200.D
Acq On : 9 Jun 2021 2:12
Operator : JU/CG
Sample : M2589-07 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B9(0-2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

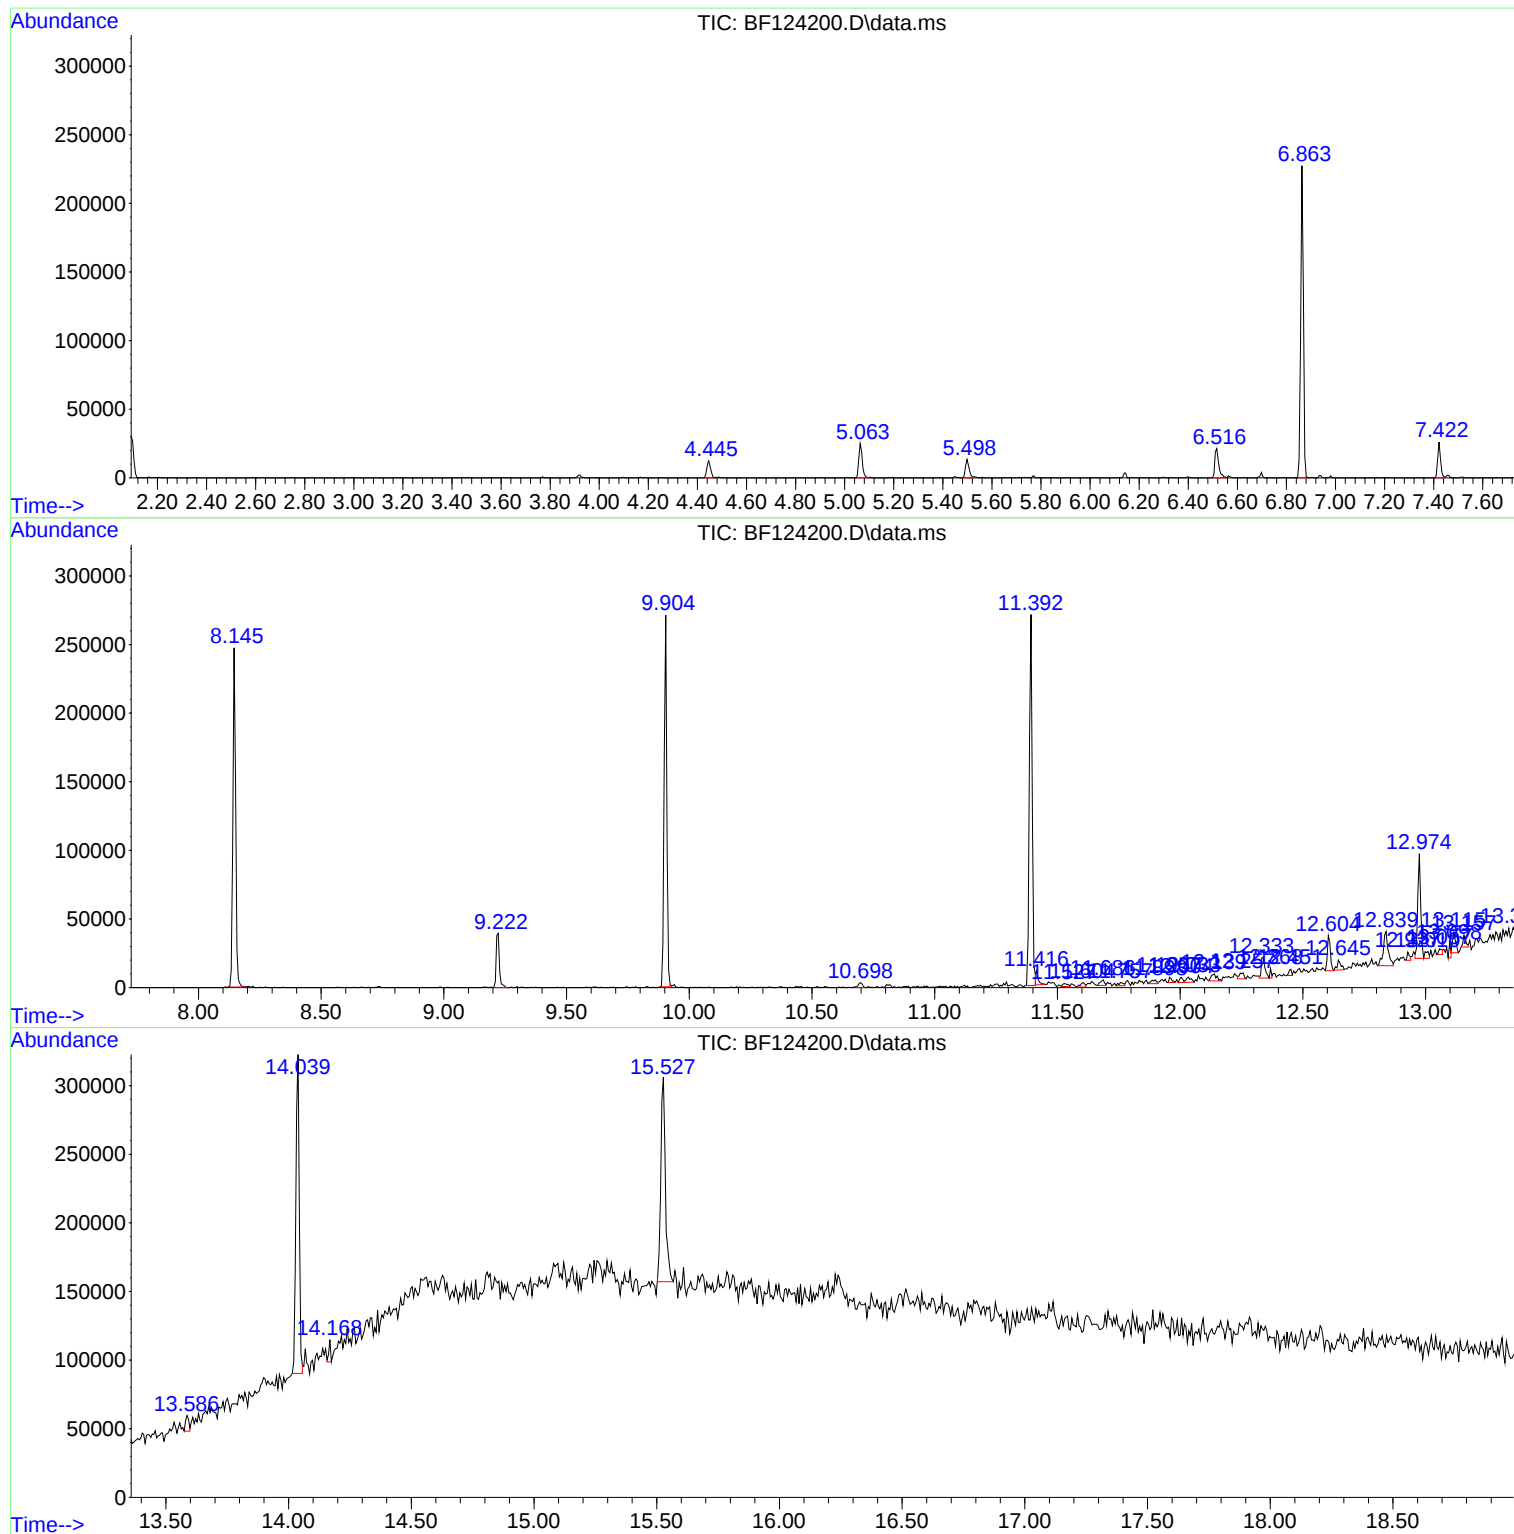

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124200.D
Acq On : 9 Jun 2021 2:12
Operator : JU/CG
Sample : M2589-07 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B9(0-2)









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.063 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.063	2.84 ng	24518	1,4-Dichlorobenzene-d4	6.863

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	43		
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	9		
3	Propylamine	59	C3H9N	000107-10-8	7		
4	Acetone	58	C3H6O	000067-64-1	7		
5	Guanidine	59	CH5N3	000113-00-8	7		

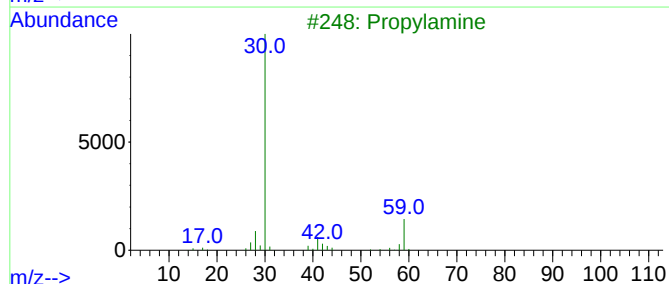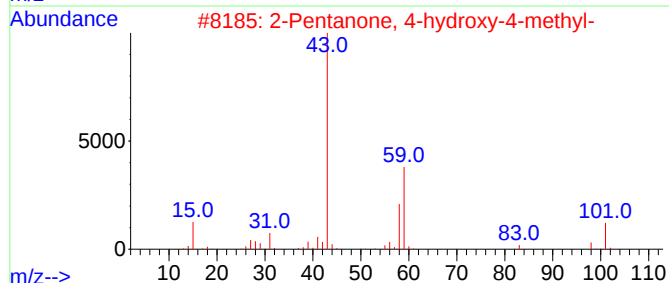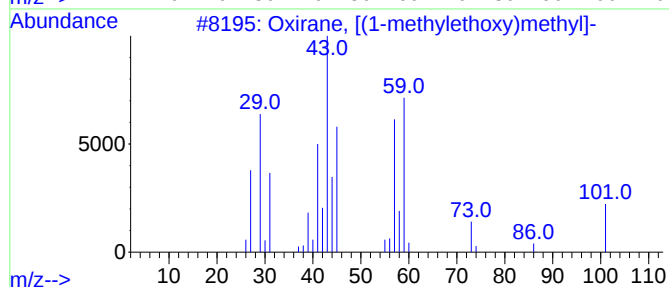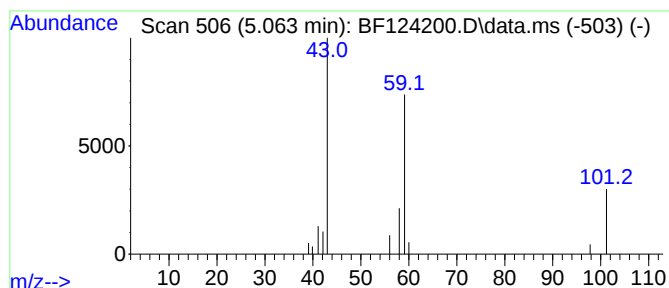

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124200.D
Acq On : 9 Jun 2021 2:12
Operator : JU/CG
Sample : M2589-07 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
18-B9(0-2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.063	5.063	2.8	ng	24518	1	6.863	172957	20.0