


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
 Data File : BF124171.D
 Acq On : 8 Jun 2021 8:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 07 13:32:21 2021

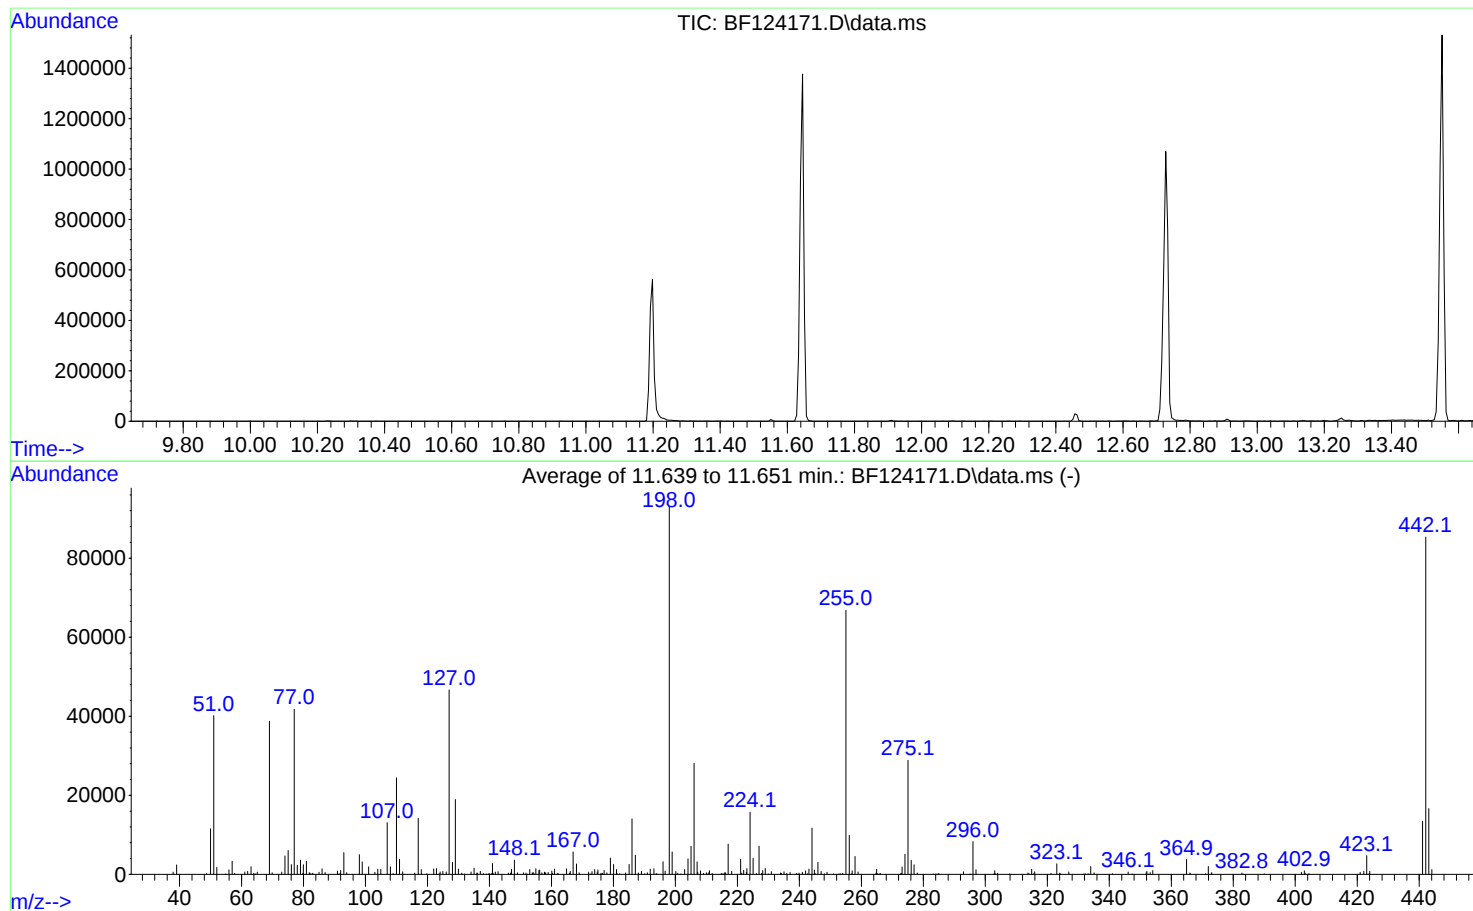




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	40166	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.6	38726	PASS
70	69	0.00	2	1.1	425	PASS
127	198	10	80	50.1	46663	PASS
197	198	0.00	2	0.9	796	PASS
198	198	100	100	100.0	93069	PASS
199	198	5	9	6.1	5680	PASS
275	198	10	60	31.0	28856	PASS
365	198	1	100	4.1	3773	PASS
441	198	0.01	100	14.5	13454	PASS
442	442	50	100	100.0	85344	PASS
443	442	15	24	19.5	16649	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060821\
Data File : BF124171.D
Acq On : 8 Jun 2021 8:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 08 11:25:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 07 13:32:21 2021
Response via : Initial Calibration

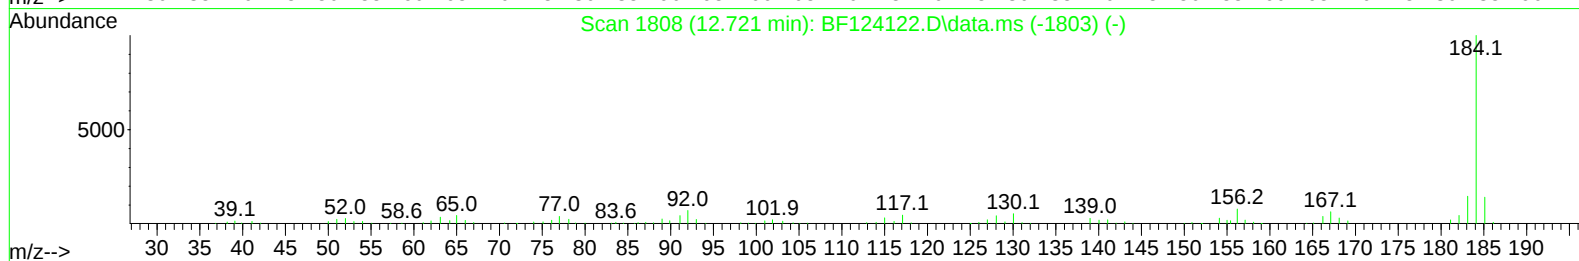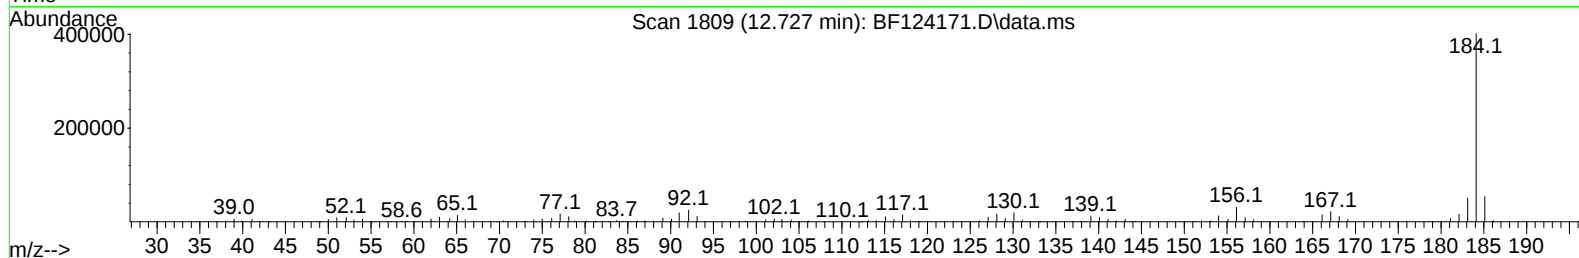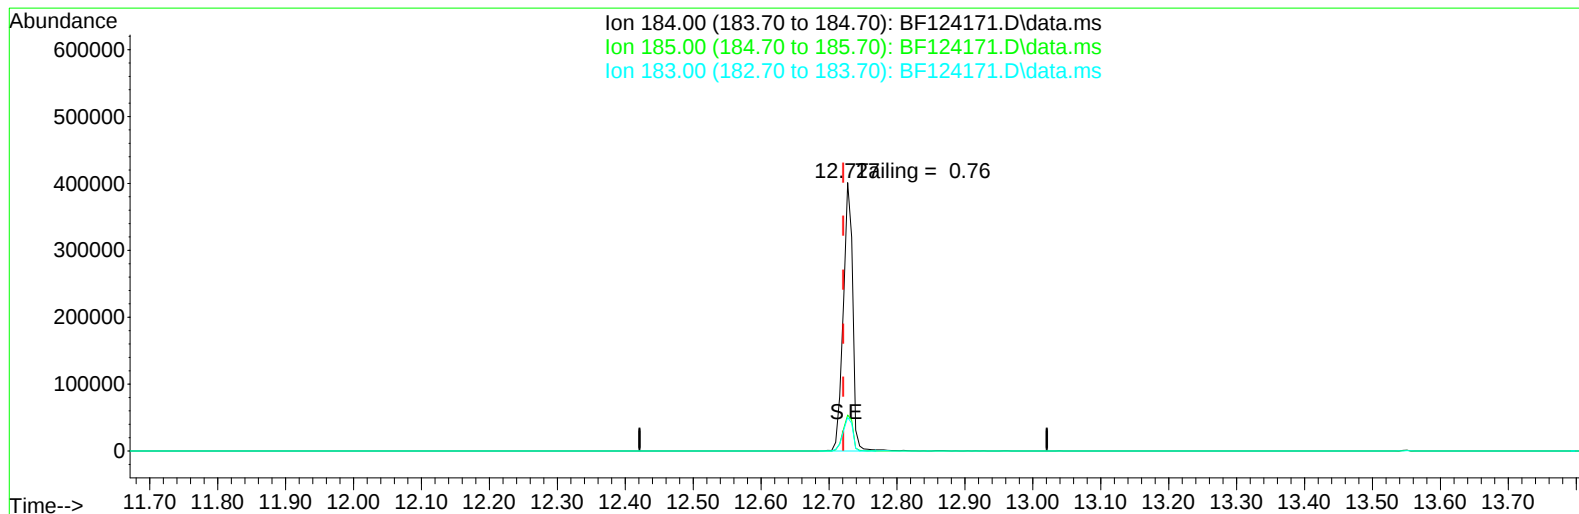

TIC: BF124171.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 387464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.41
183.00	9.80	12.56#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2021	BNA_F	<u>BF124171.D</u>
Compound Name	Response	Retention Time
DDT	229116	13.55
DDD	2302	13.25
DDE	1434	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3736	232852	1.60

Instrument :
BNA_F
ClientSampleId :
DFTPP