


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF060821\  
 Data File : BF124183.D  
 Acq On : 8 Jun 2021 16:45  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF060321.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jun 07 13:32:21 2021

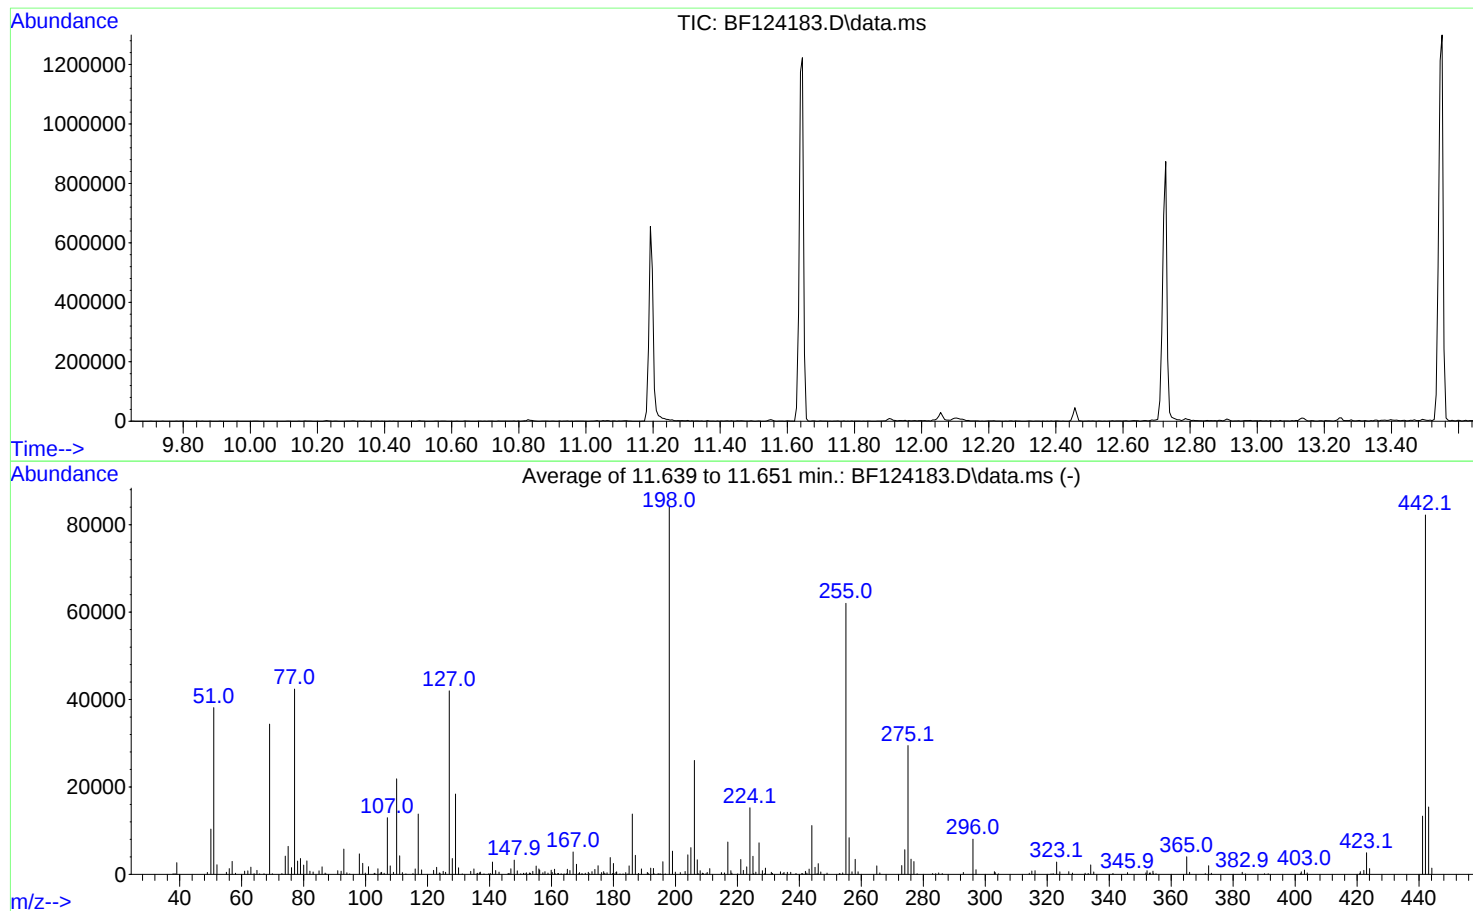




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 45.3         | 38140      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 40.8         | 34379      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 139        | PASS                |
| 127            | 198             | 10              | 80              | 49.9         | 41990      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.1          | 114        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 84163      | PASS                |
| 199            | 198             | 5               | 9               | 6.3          | 5317       | PASS                |
| 275            | 198             | 10              | 60              | 35.0         | 29478      | PASS                |
| 365            | 198             | 1               | 100             | 4.8          | 4016       | PASS                |
| 441            | 198             | 0.01            | 100             | 15.8         | 13310      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 82237      | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 15413      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF060821\  
Data File : BF124183.D  
Acq On : 8 Jun 2021 16:45  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 08 17:17:00 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF060321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 07 13:32:21 2021  
Response via : Initial Calibration

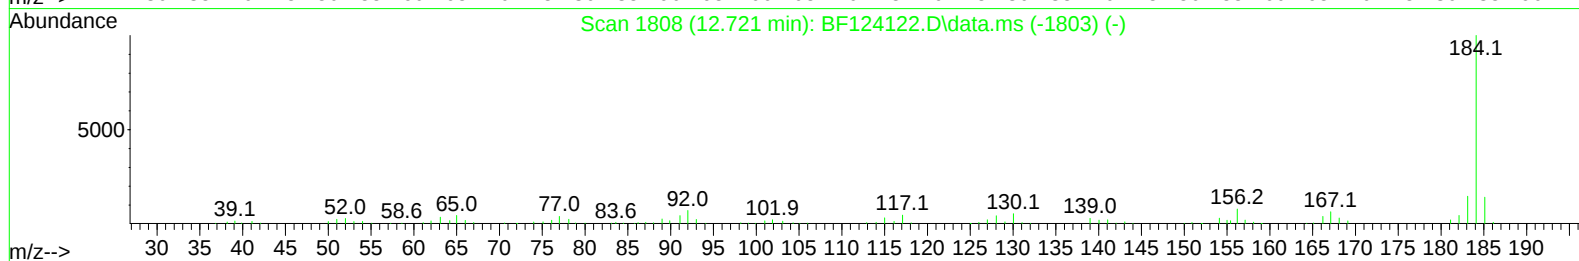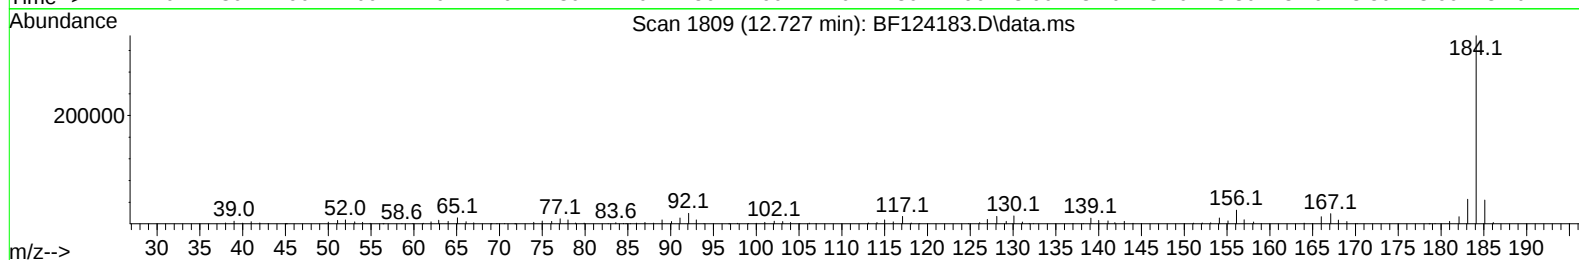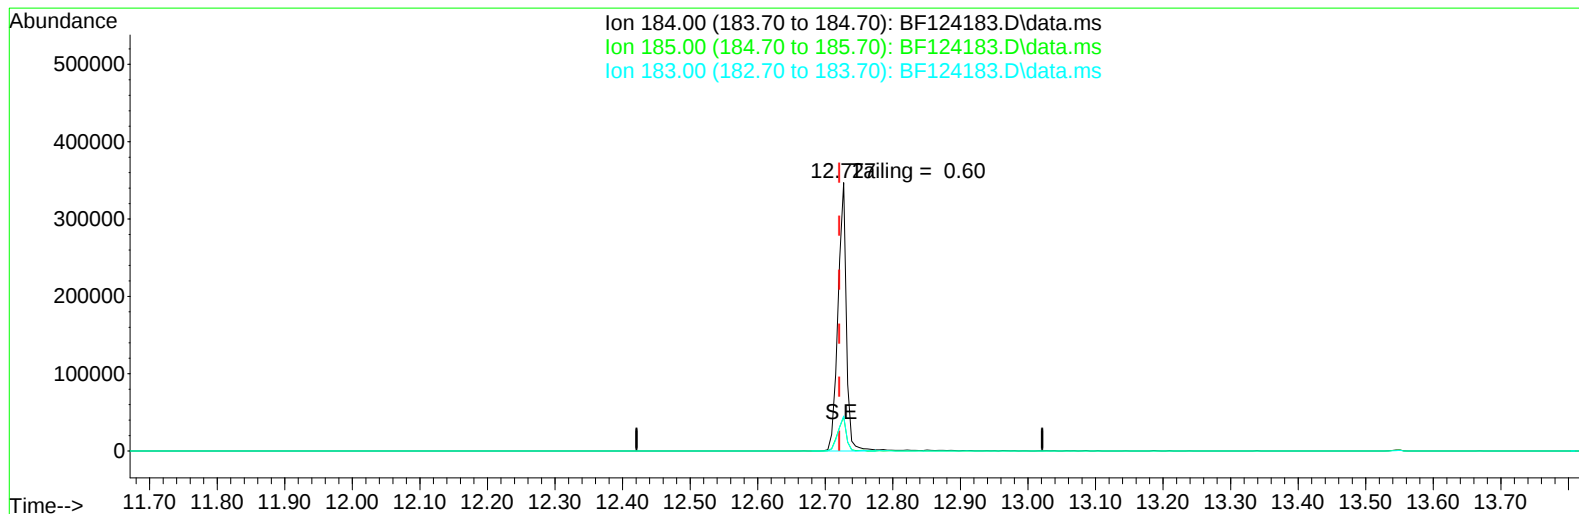

TIC: BF124183.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng




response 298250

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 12.69  |
| 183.00 | 9.80   | 13.07# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF060821\  
Data File : BF124183.D  
Acq On : 8 Jun 2021 16:45  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 08 17:17:00 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF060321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 07 13:32:21 2021  
Response via : Initial Calibration

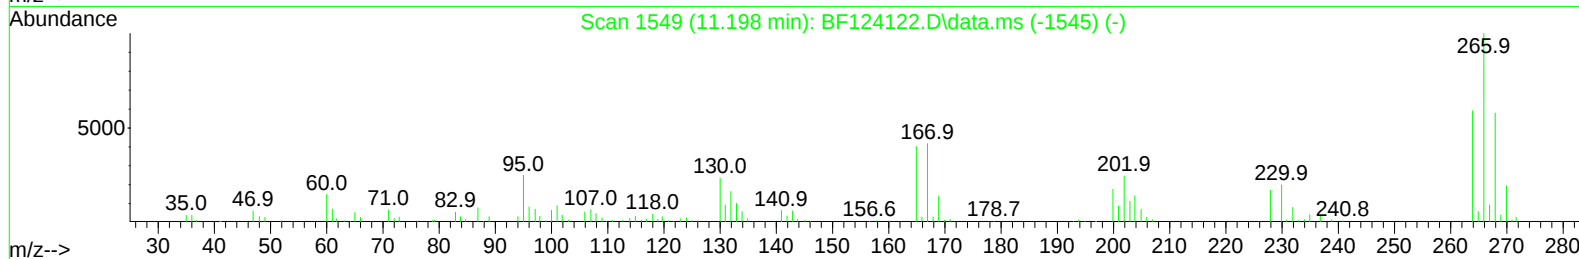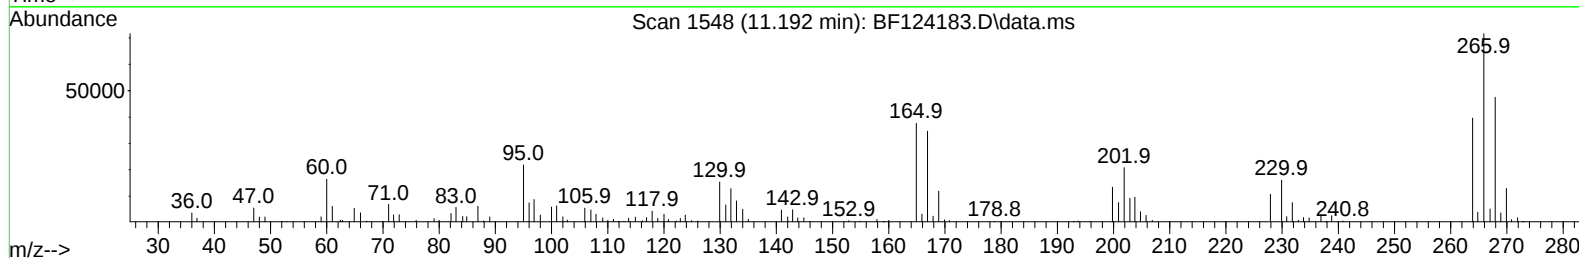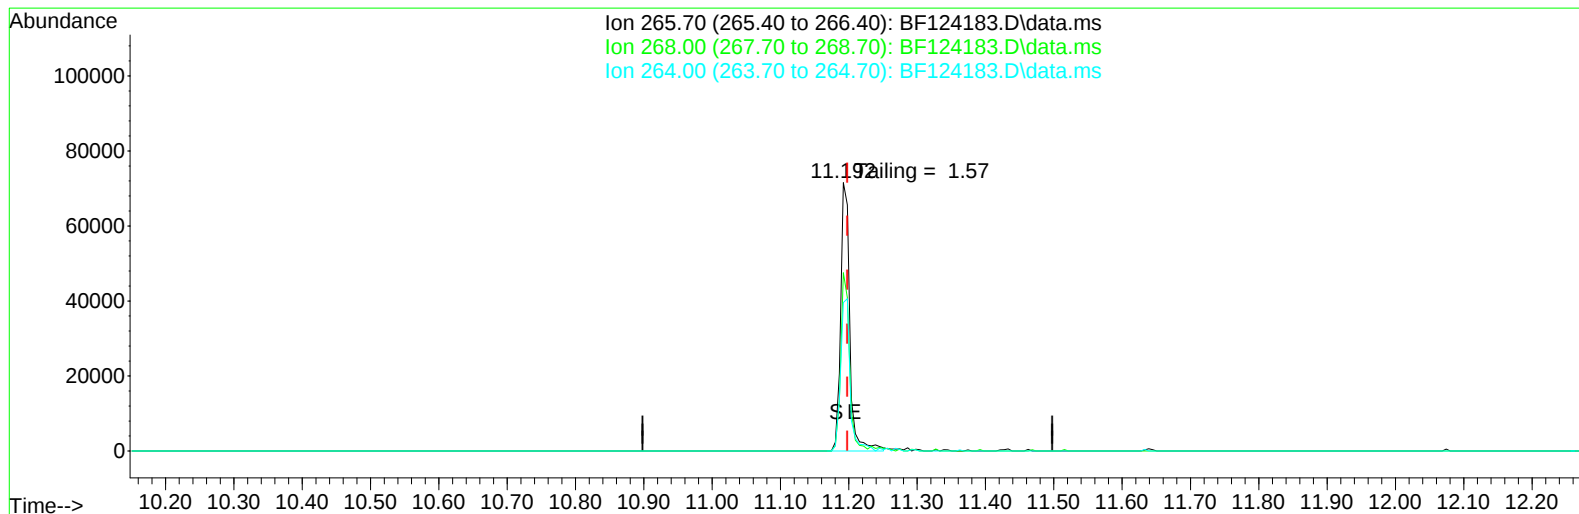

TIC: BF124183.D\data.ms

**(70) Pentachlorophenol (C)**

**11.192min (-0.006) 31997.47 ng**

**response 67633**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 66.39  |
| 264.00 | 65.70  | 55.36  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/8/2021      | BNA_F            | <u>BF124183.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 215860           | 13.55              |
| DDD           | 2782             | 13.55              |
| DDE           | 929              | 12.91              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3711          | 219571           | 1.69               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP