


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060822\
 Data File : BF128728.D
 Acq On : 08 Jun 2022 10:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 08 14:28:39 2022

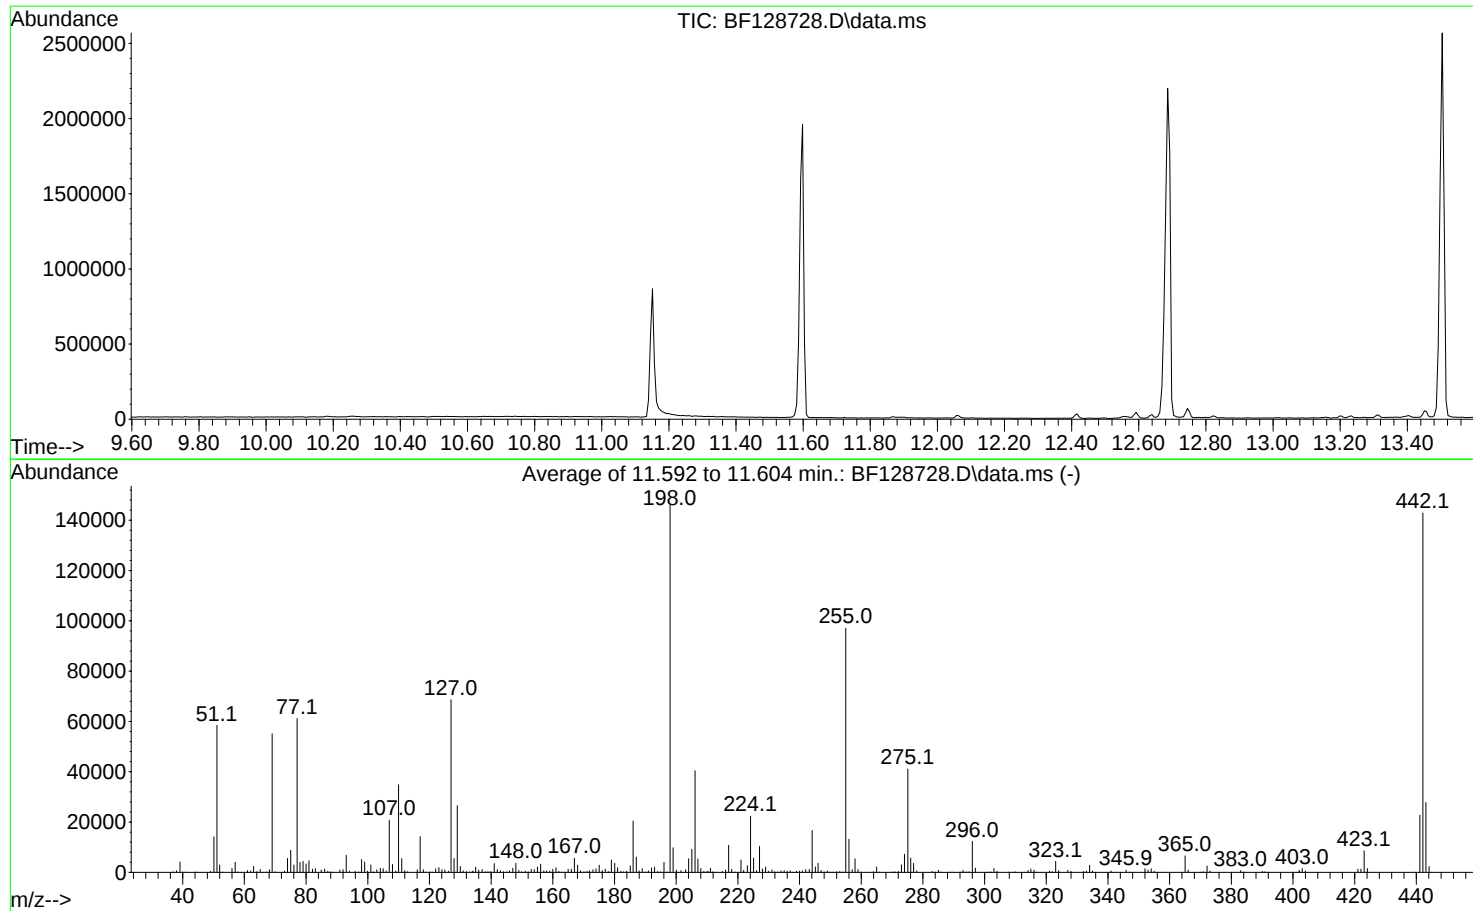




AutoFind: Scans 1582, 1583, 1584; Background Corrected with Scan 1575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	58452	PASS
68	69	0.00	2	1.8	1003	PASS
69	198	0.00	100	37.7	55120	PASS
70	69	0.00	2	0.4	235	PASS
127	198	10	80	46.9	68624	PASS
197	198	0.00	2	0.1	179	PASS
198	198	100	100	100.0	146248	PASS
199	198	5	9	6.7	9779	PASS
275	198	10	60	28.1	41091	PASS
365	198	1	100	4.5	6535	PASS
441	198	0.01	100	15.5	22714	PASS
442	442	50	100	100.0	142901	PASS
443	442	15	24	19.5	27813	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060822\
Data File : BF128728.D
Acq On : 08 Jun 2022 10:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 08 18:40:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 08 14:28:39 2022
Response via : Initial Calibration

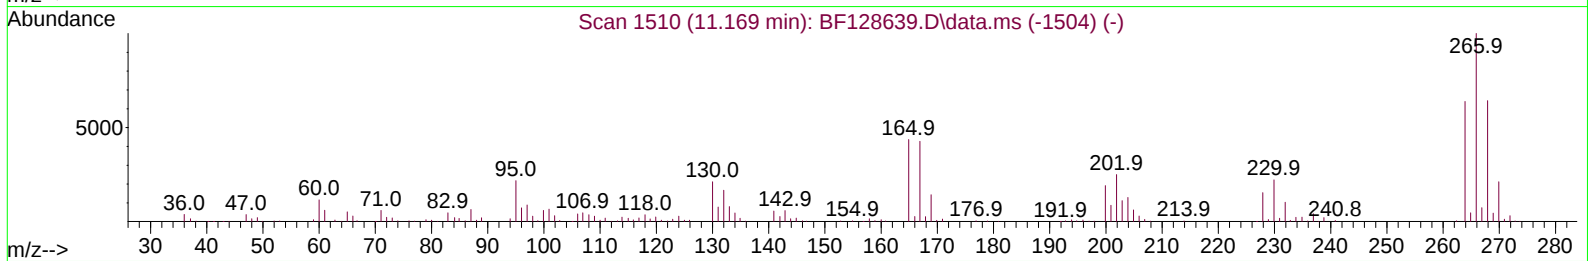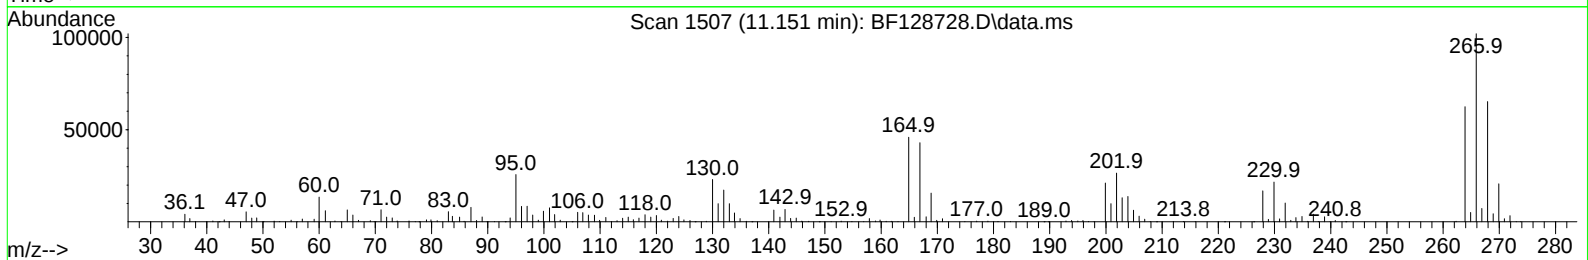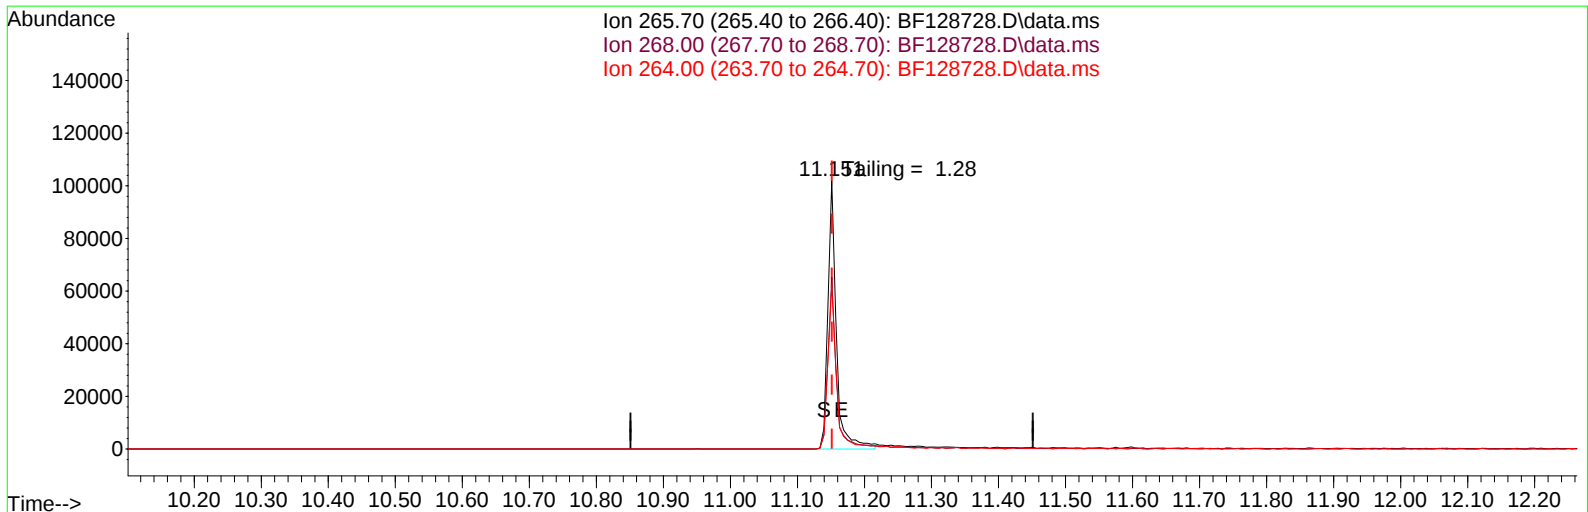

TIC: BF128728.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.000) 19218.58 ng




response 93744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.97
264.00	61.80	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060822\
Data File : BF128728.D
Acq On : 08 Jun 2022 10:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 08 18:40:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 08 14:28:39 2022
Response via : Initial Calibration

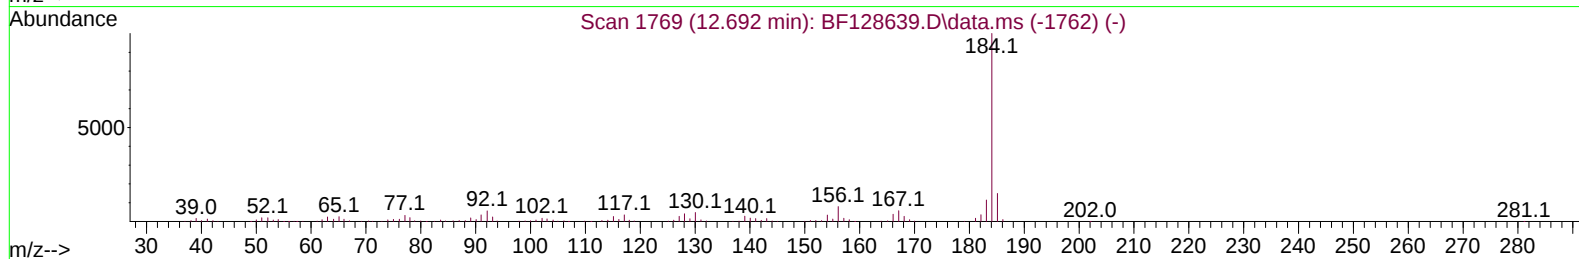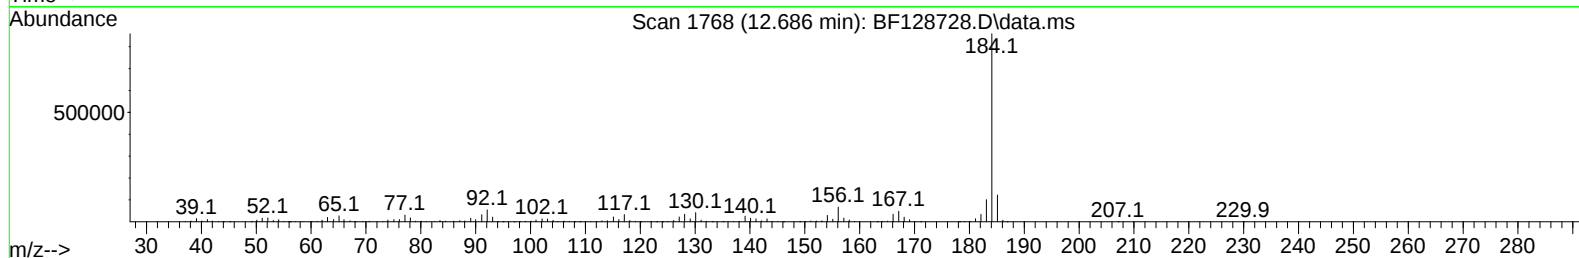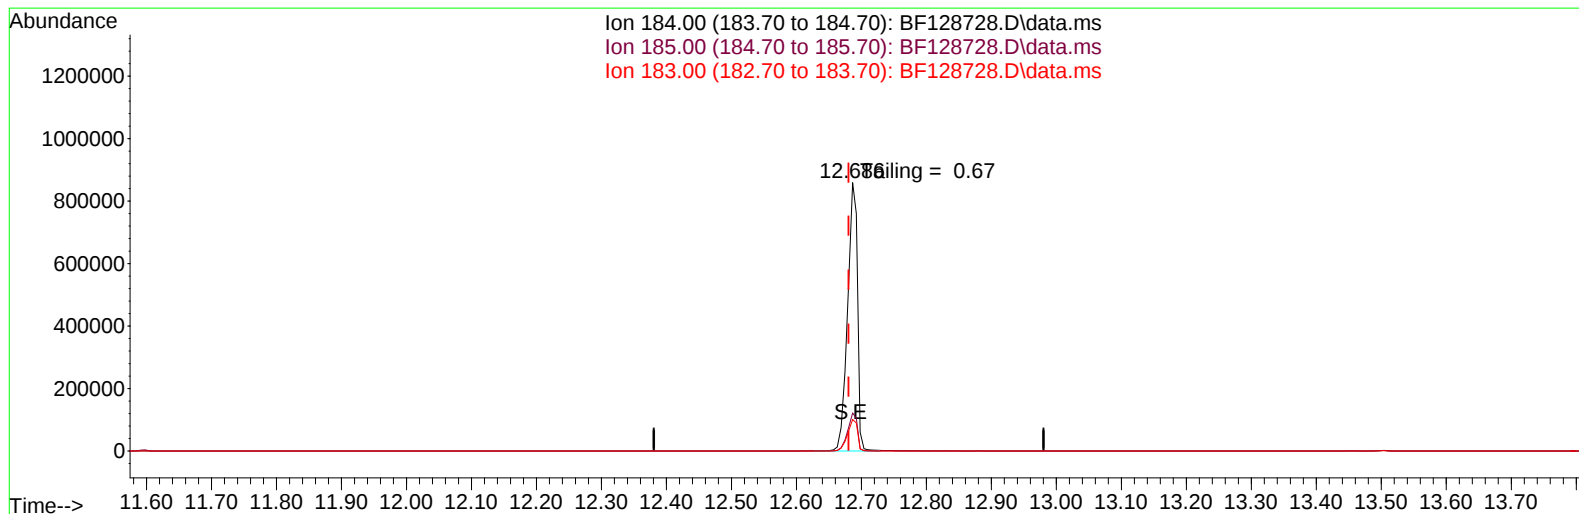

TIC: BF128728.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response 922014

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.20
183.00	11.60	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2022	BNA_F	<u>BF128728.D</u>
Compound Name	Response	Retention Time
DDT	415178	13.5
DDD	2605	13.2
DDE	475	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3080	418258	0.74

Instrument :
BNA_F
ClientSampleId :
DFTPP