

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060915\
 Data File : BF079852.D
 Acq On : 10 Jun 2015 1:03
 Operator : TP/IZ
 Sample : G2572-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-149-6815

Quant Time: Jun 10 02:27:04 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 09 15:11:40 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	46617	20.00	ng	0.00
21) Naphthalene-d8	8.71	136	185707	20.00	ng	0.00
38) Acenaphthene-d10	10.48	164	92582	20.00	ng	0.00
63) Phenanthrene-d10	11.99	188	194059	20.00	ng	-0.01
75) Chrysene-d12	14.95	240	193261	20.00	ng	-0.11
86) Perylene-d12	16.86	264	176999	20.00	ng	-0.16
System Monitoring Compounds						
5) 2-Fluorophenol	6.03	112	171891	60.77	ng	0.00
7) Phenol-d6	7.02	99	128362	35.07	ng	0.00
23) Nitrobenzene-d5	7.98	82	273868	85.19	ng	0.00
41) 2,4,6-Tribromophenol	11.28	330	120178	149.99	ng	0.00
44) 2-Fluorobiphenyl	9.78	172	665457	101.09	ng	0.00
78) Terphenyl-d14	13.68	244	830835	96.92	ng	-0.06
Target Compounds						
56) 2,4-Dinitrotoluene	10.48	165	12001	12.48	ng	Qvalue # 32

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060915\
Data File : BF079852.D
Acq On : 10 Jun 2015 1:03
Operator : TP/IZ
Sample : G2572-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-149-6815

Quant Time: Jun 10 02:27:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 09 15:11:40 2015
Response via : Initial Calibration

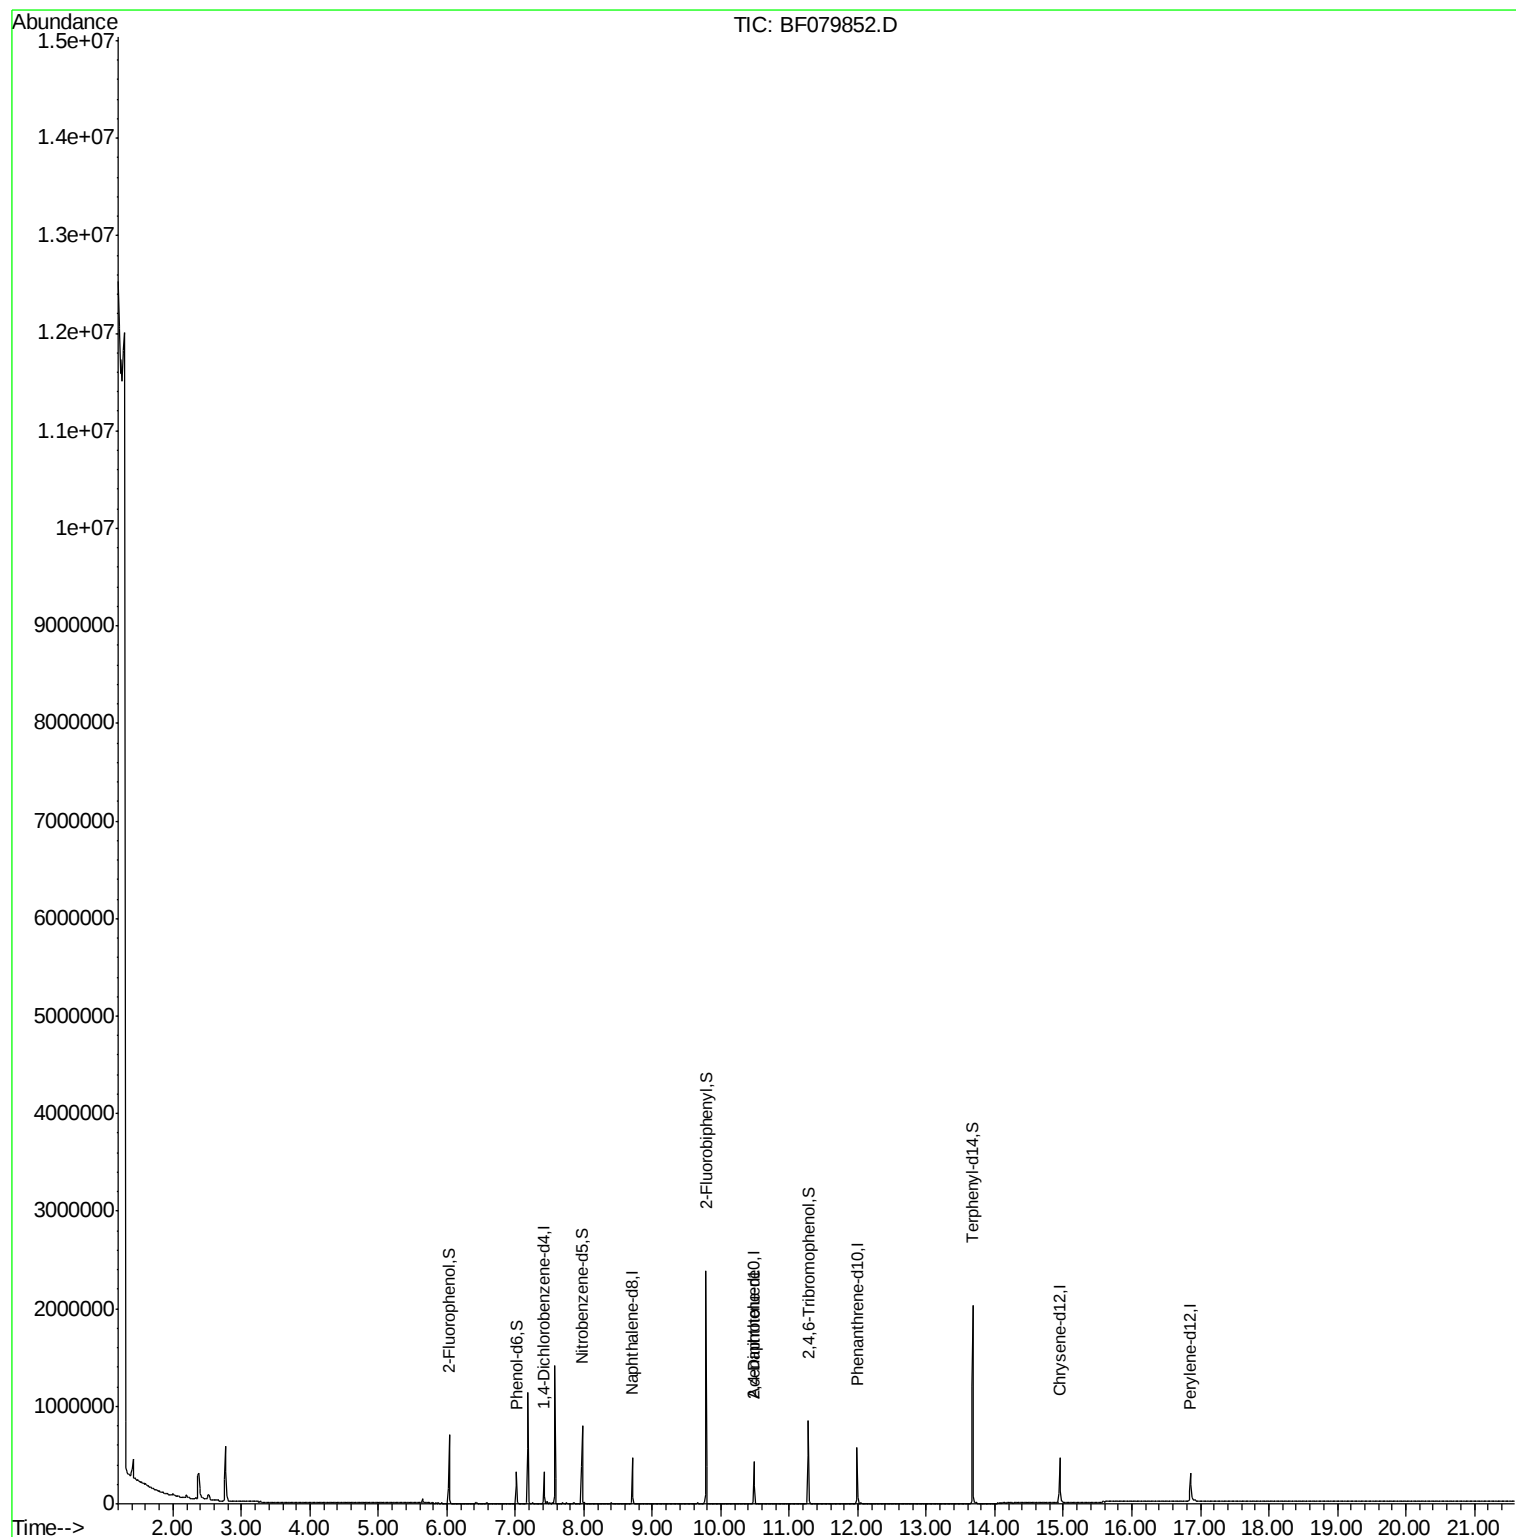



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.42 min Scan# 545

Delta R.T. 0.00 min

Lab File: BF079852.D

Acq: 10 Jun 2015 1:03

Instrument :

BNA_F

ClientSampleId :

DCW-WW-149-6815


Tgt Ion:152 Resp: 46617

Ion Ratio Lower Upper

152 100

150 160.1 131.4 197.2




115 60.5 56.5 84.7



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

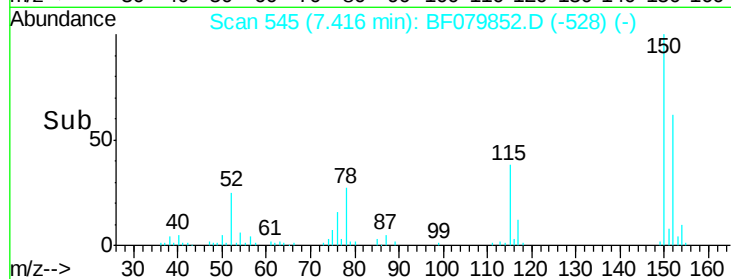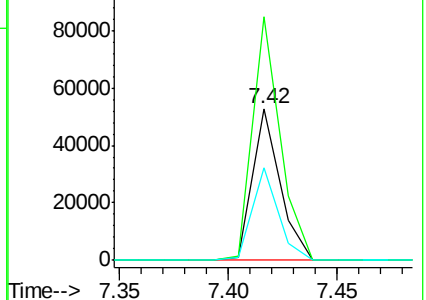

#5

2-Fluorophenol

Concen: 60.77 ng

RT: 6.03 min Scan# 424

Delta R.T. 0.00 min

Lab File: BF079852.D

Acq: 10 Jun 2015 1:03


Tgt Ion:112 Resp: 171891

Ion Ratio Lower Upper

112 100

64 58.3 44.2 66.4



63 30.0 22.8 34.2




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

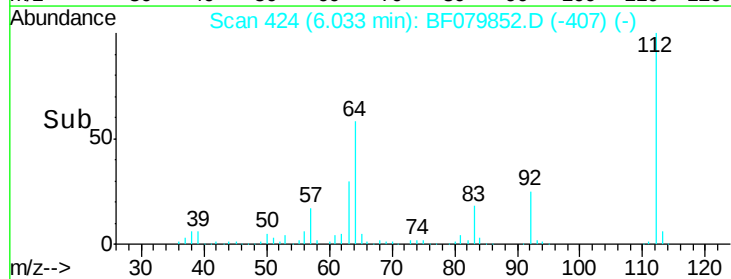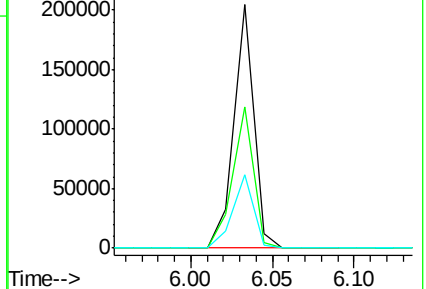

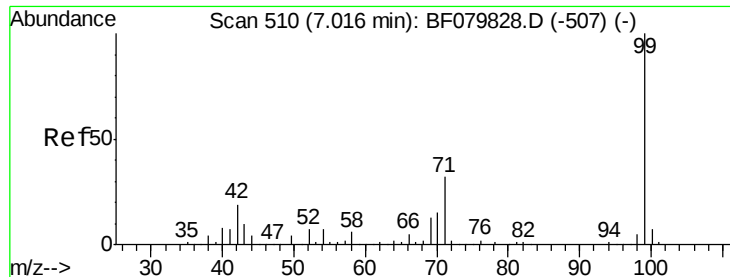

#7

Phenol-d6

Concen: 35.07 ng

RT: 7.02 min Scan# 510

Delta R.T. 0.00 min

Lab File: BF079852.D

Acq: 10 Jun 2015 1:03

Instrument :

BNA_F

ClientSampleId :

DCW-WW-149-6815


Tgt Ion: 99 Resp: 128362

Ion Ratio Lower Upper

99 100

42 14.7 13.7 20.5




71 28.0 25.1 37.7

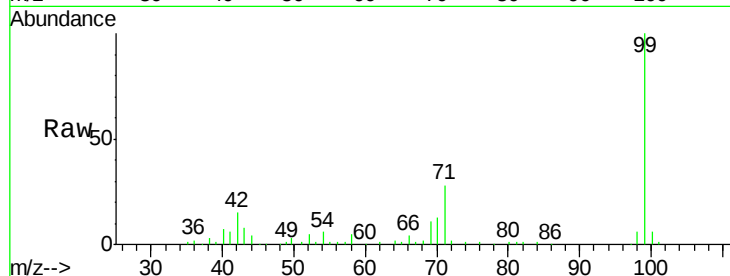

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

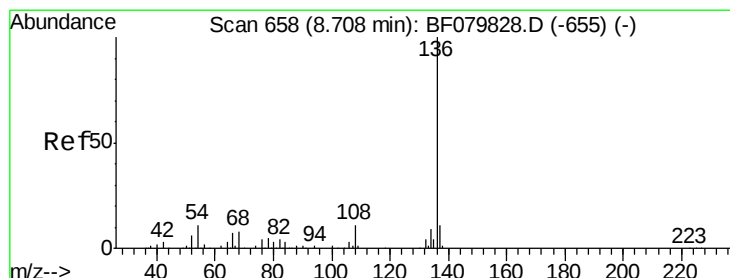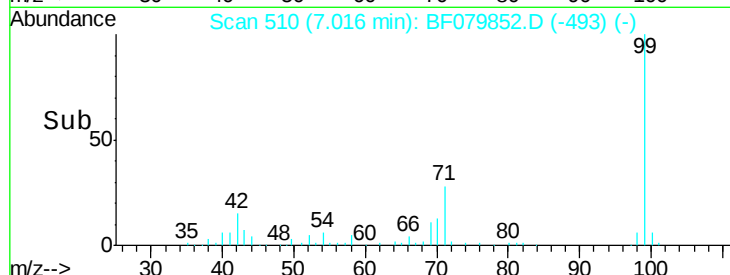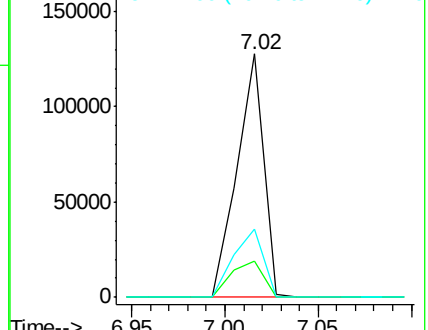

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.71 min Scan# 658

Delta R.T. 0.00 min

Lab File: BF079852.D

Acq: 10 Jun 2015 1:03

Tgt Ion: 136 Resp: 185707


Ion Ratio Lower Upper

136 100

137 11.0 9.3 13.9

54 9.5 8.1 12.1

68 6.9 4.8 7.2


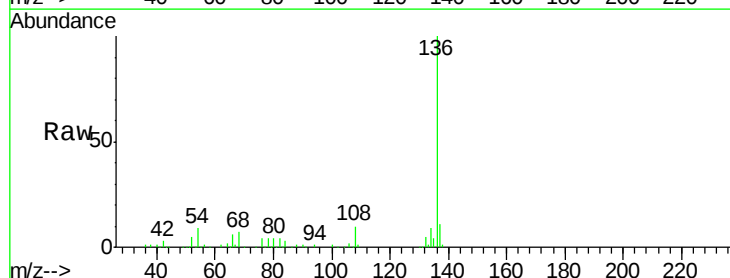


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

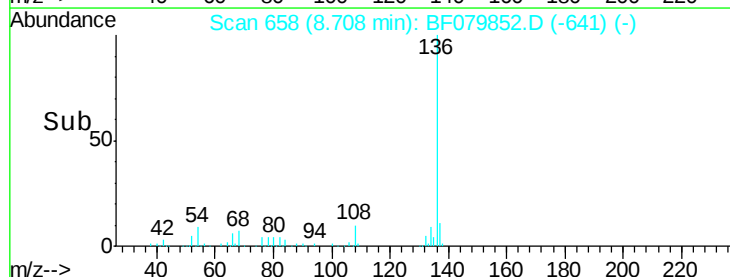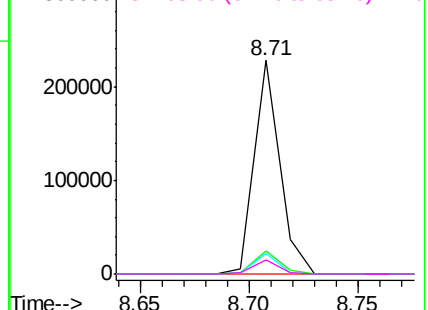







#23
 Nitrobenzene-d5
 Concen: 85.19 ng
 RT: 7.98 min Scan# 594
 Delta R.T. 0.00 min
 Lab File: BF079852.D
 Acq: 10 Jun 2015 1:03

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-149-6815

Tgt Ion	Ratio	Lower	Upper
82	100		
128	49.1	35.2	52.8
54	46.4	39.2	58.8

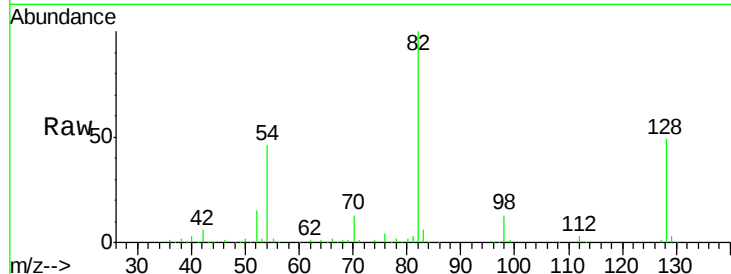


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

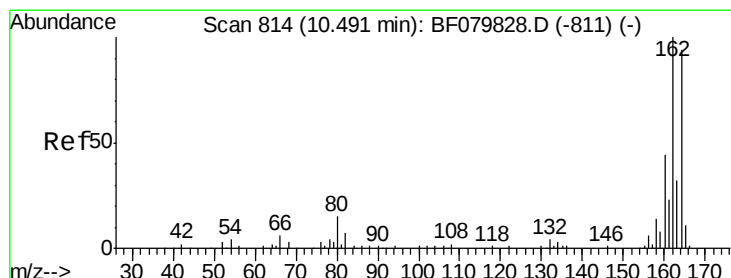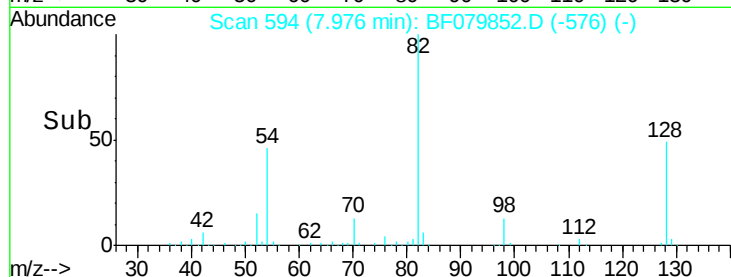
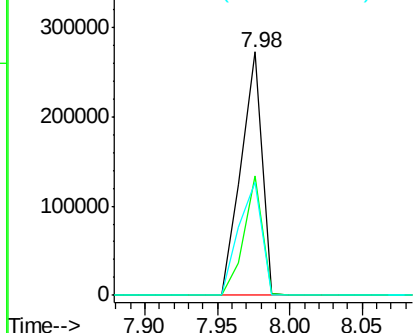



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.48 min Scan# 813
 Delta R.T. 0.00 min
 Lab File: BF079852.D
 Acq: 10 Jun 2015 1:03

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.8	89.8	134.8
160	44.8	39.6	59.4



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

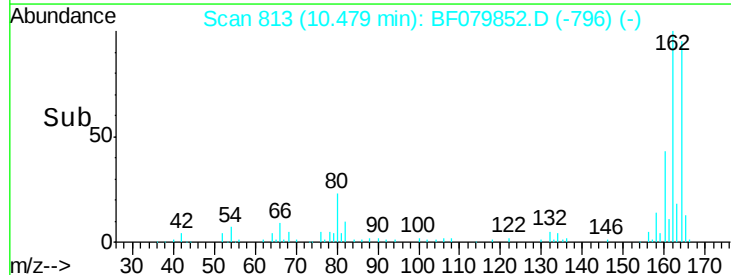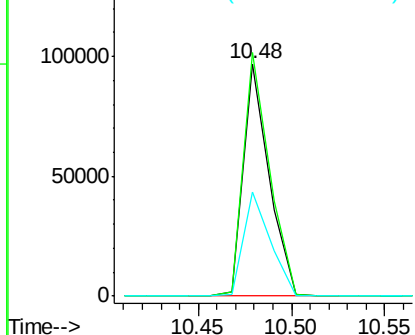


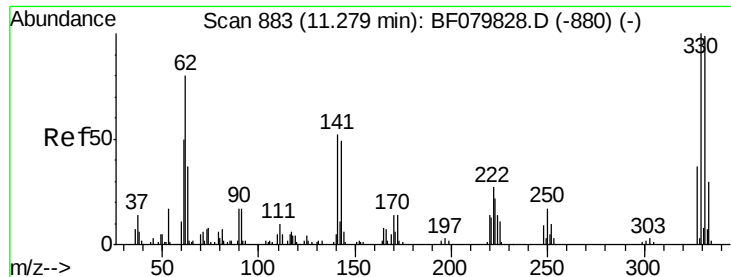




#41
 2,4,6-Tribromophenol
 Concen: 149.99 ng
 RT: 11.28 min Scan# 883
 Delta R.T. 0.00 min
 Lab File: BF079852.D
 Acq: 10 Jun 2015 1:03

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-149-6815

Tgt Ion:330 Resp: 120178
 Ion Ratio Lower Upper
 330 100
 332 94.4 76.8 115.2
 141 32.4 29.1 43.7

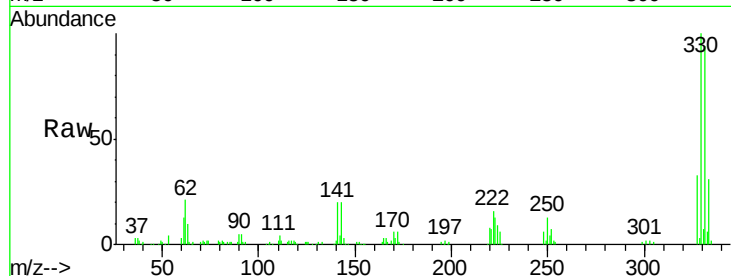


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

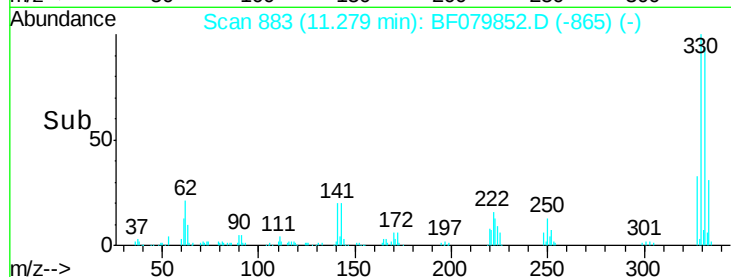
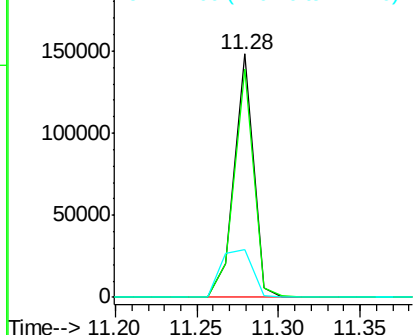



#44
 2-Fluorobiphenyl
 Concen: 101.09 ng
 RT: 9.78 min Scan# 752
 Delta R.T. 0.00 min
 Lab File: BF079852.D
 Acq: 10 Jun 2015 1:03

Tgt Ion:172 Resp: 665457
 Ion Ratio Lower Upper
 172 100
 171 36.2 28.5 42.7
 170 24.6 18.8 28.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



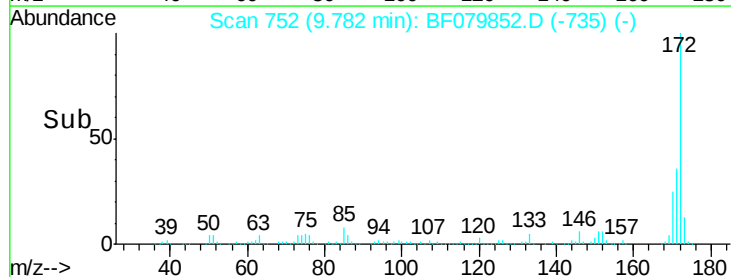
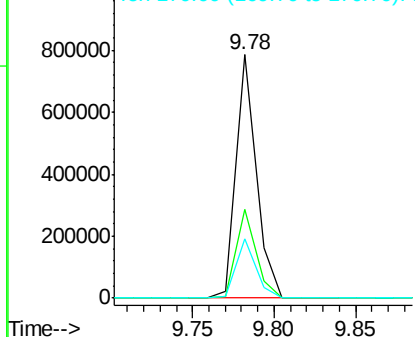


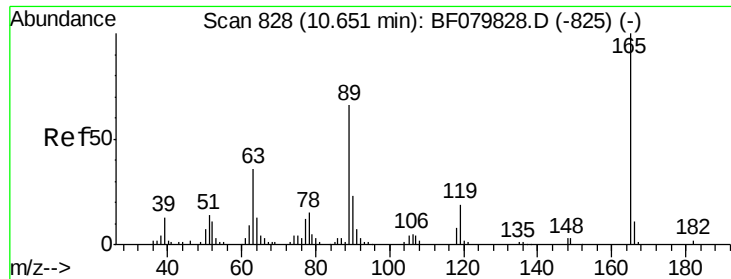

#56
 2,4-Dinitrotoluene
 Concen: 12.48 ng
 RT: 10.48 min Scan# 813
 Delta R.T. -0.17 min
 Lab File: BF079852.D
 Acq: 10 Jun 2015 1:03




Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-149-6815


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	24.4	36.6#
89	0.0	45.3	67.9#
182	0.0	2.0	3.0#

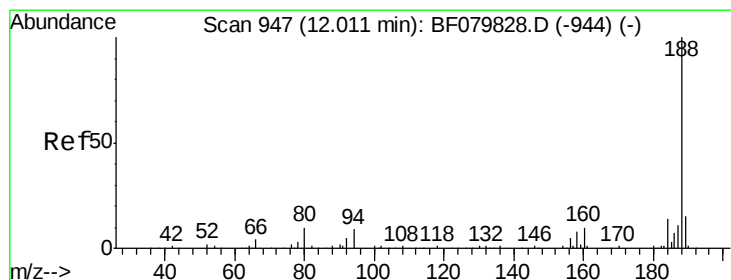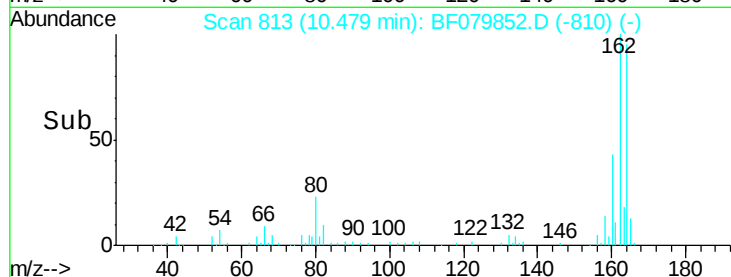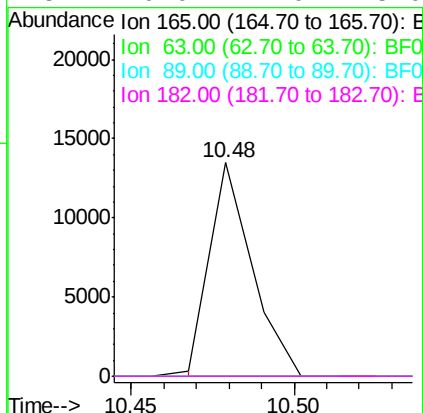

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.99 min Scan# 945
 Delta R.T. -0.01 min
 Lab File: BF079852.D
 Acq: 10 Jun 2015 1:03

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.5	7.4	11.0
80	10.7	8.0	12.0

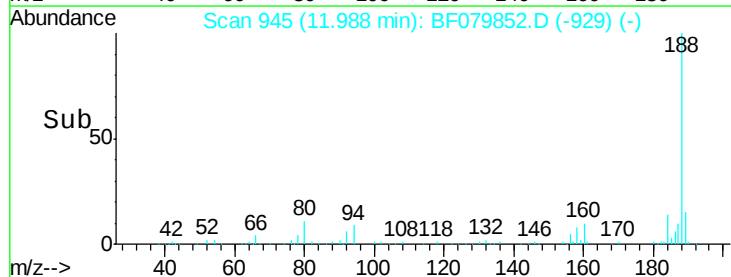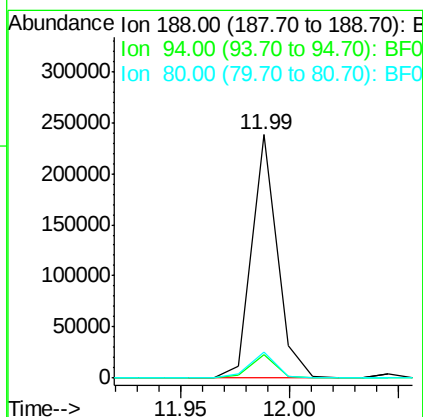

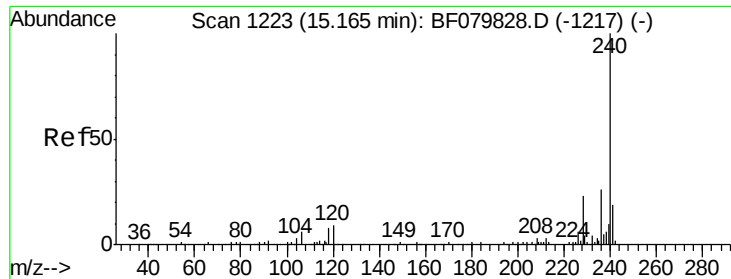

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.95 min Scan# 1204

Delta R.T. -0.11 min

Lab File: BF079852.D

Acq: 10 Jun 2015 1:03

Instrument :

BNA_F

ClientSampleId :

DCW-WW-149-6815


Tgt Ion:240 Resp: 193261

Ion Ratio Lower Upper

240 100

120 10.9 6.6 9.8#




236 25.0 20.2 30.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

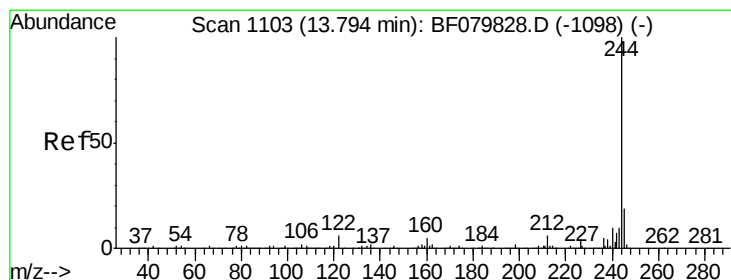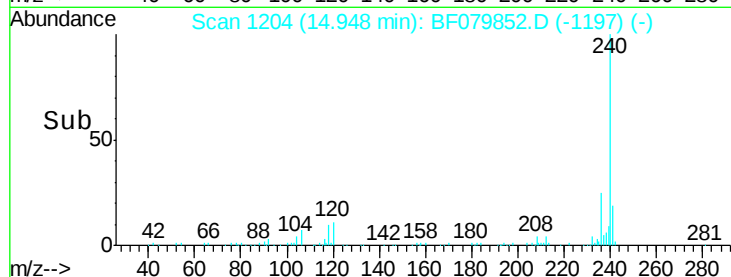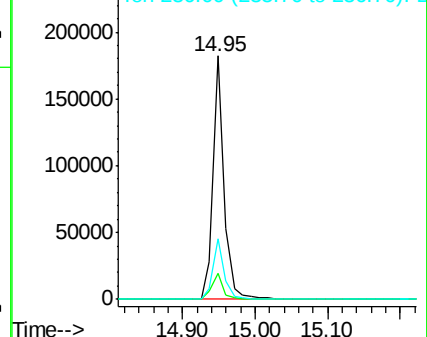

#78

Terphenyl-d14

Concen: 96.92 ng

RT: 13.68 min Scan# 1093

Delta R.T. -0.06 min

Lab File: BF079852.D

Acq: 10 Jun 2015 1:03


Tgt Ion:244 Resp: 830835

Ion Ratio Lower Upper

244 100

212 6.5 5.6 8.4



122 7.2 8.2 12.2#



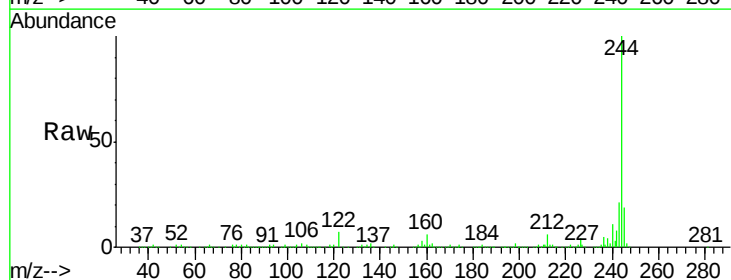


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

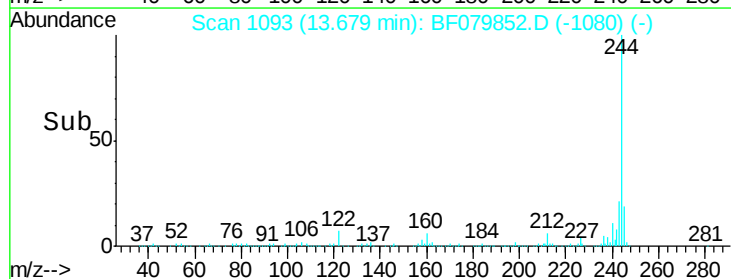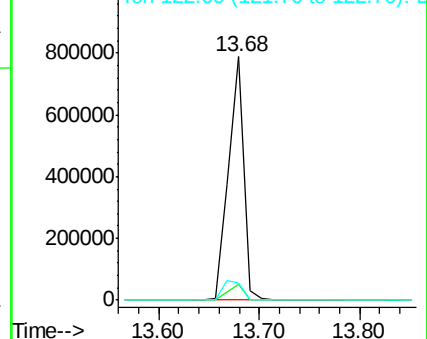

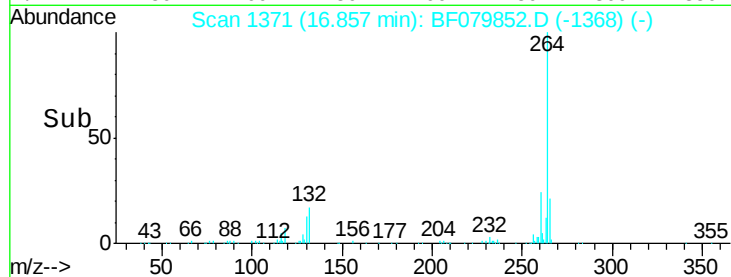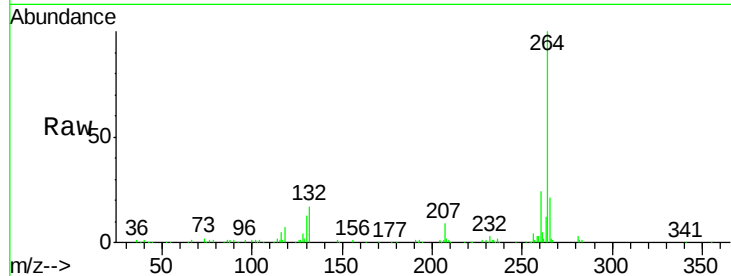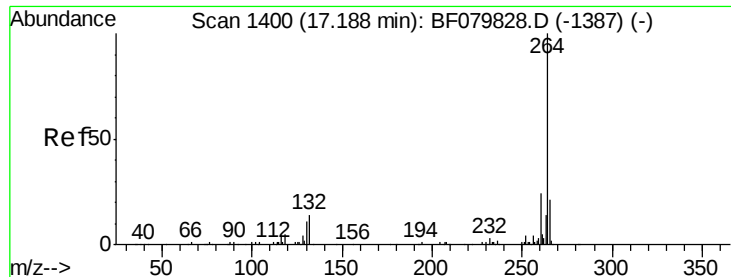

#86

Perylene-d12

Concen: 20.00 ng

RT: 16.86 min Scan# 1371

Delta R.T. -0.16 min

Lab File: BF079852.D

Acq: 10 Jun 2015 1:03

Instrument :

BNA_F

ClientSampleId :

DCW-WW-149-6815

Tgt Ion: 264 Resp: 176999

Ion Ratio Lower Upper

264 100

260 23.5 19.5 29.3

265 21.4 18.0 27.0

