



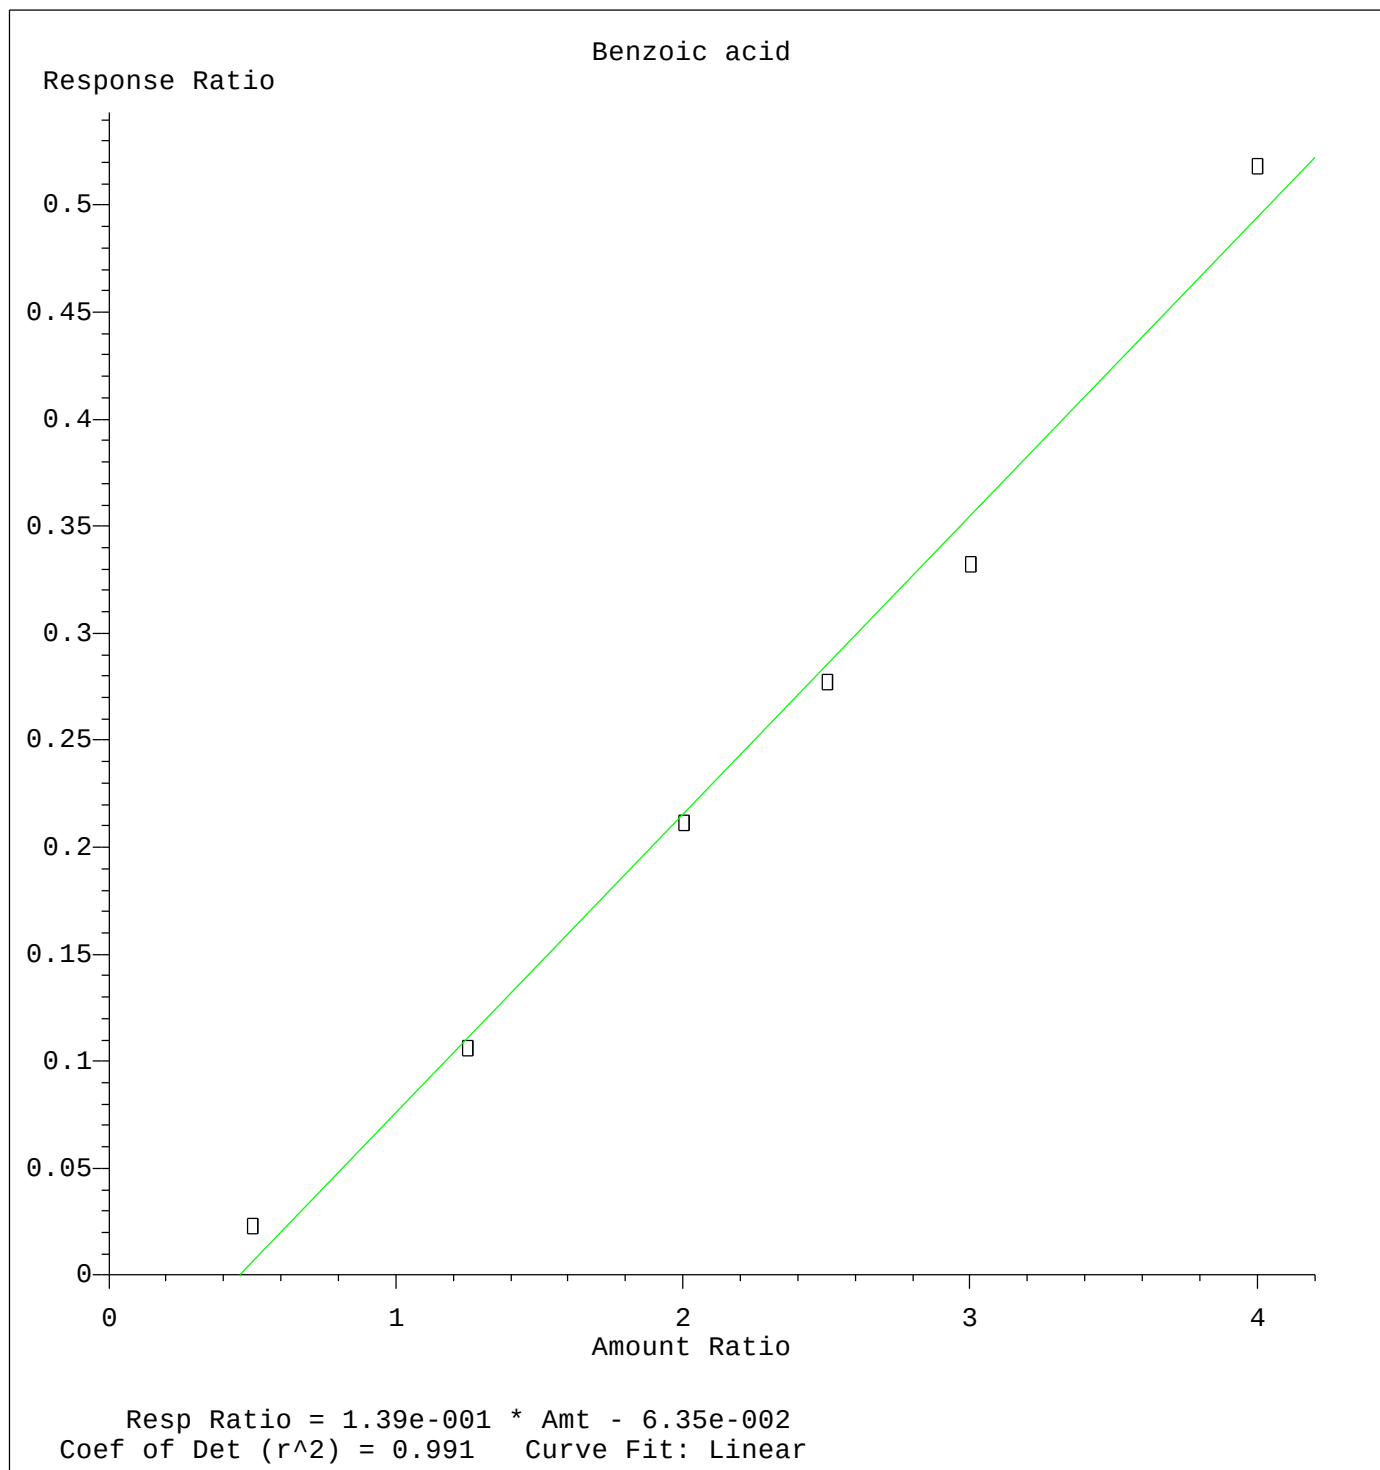


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Calibration Table Last Updated: Tue Jun 09 15:11:40 2015

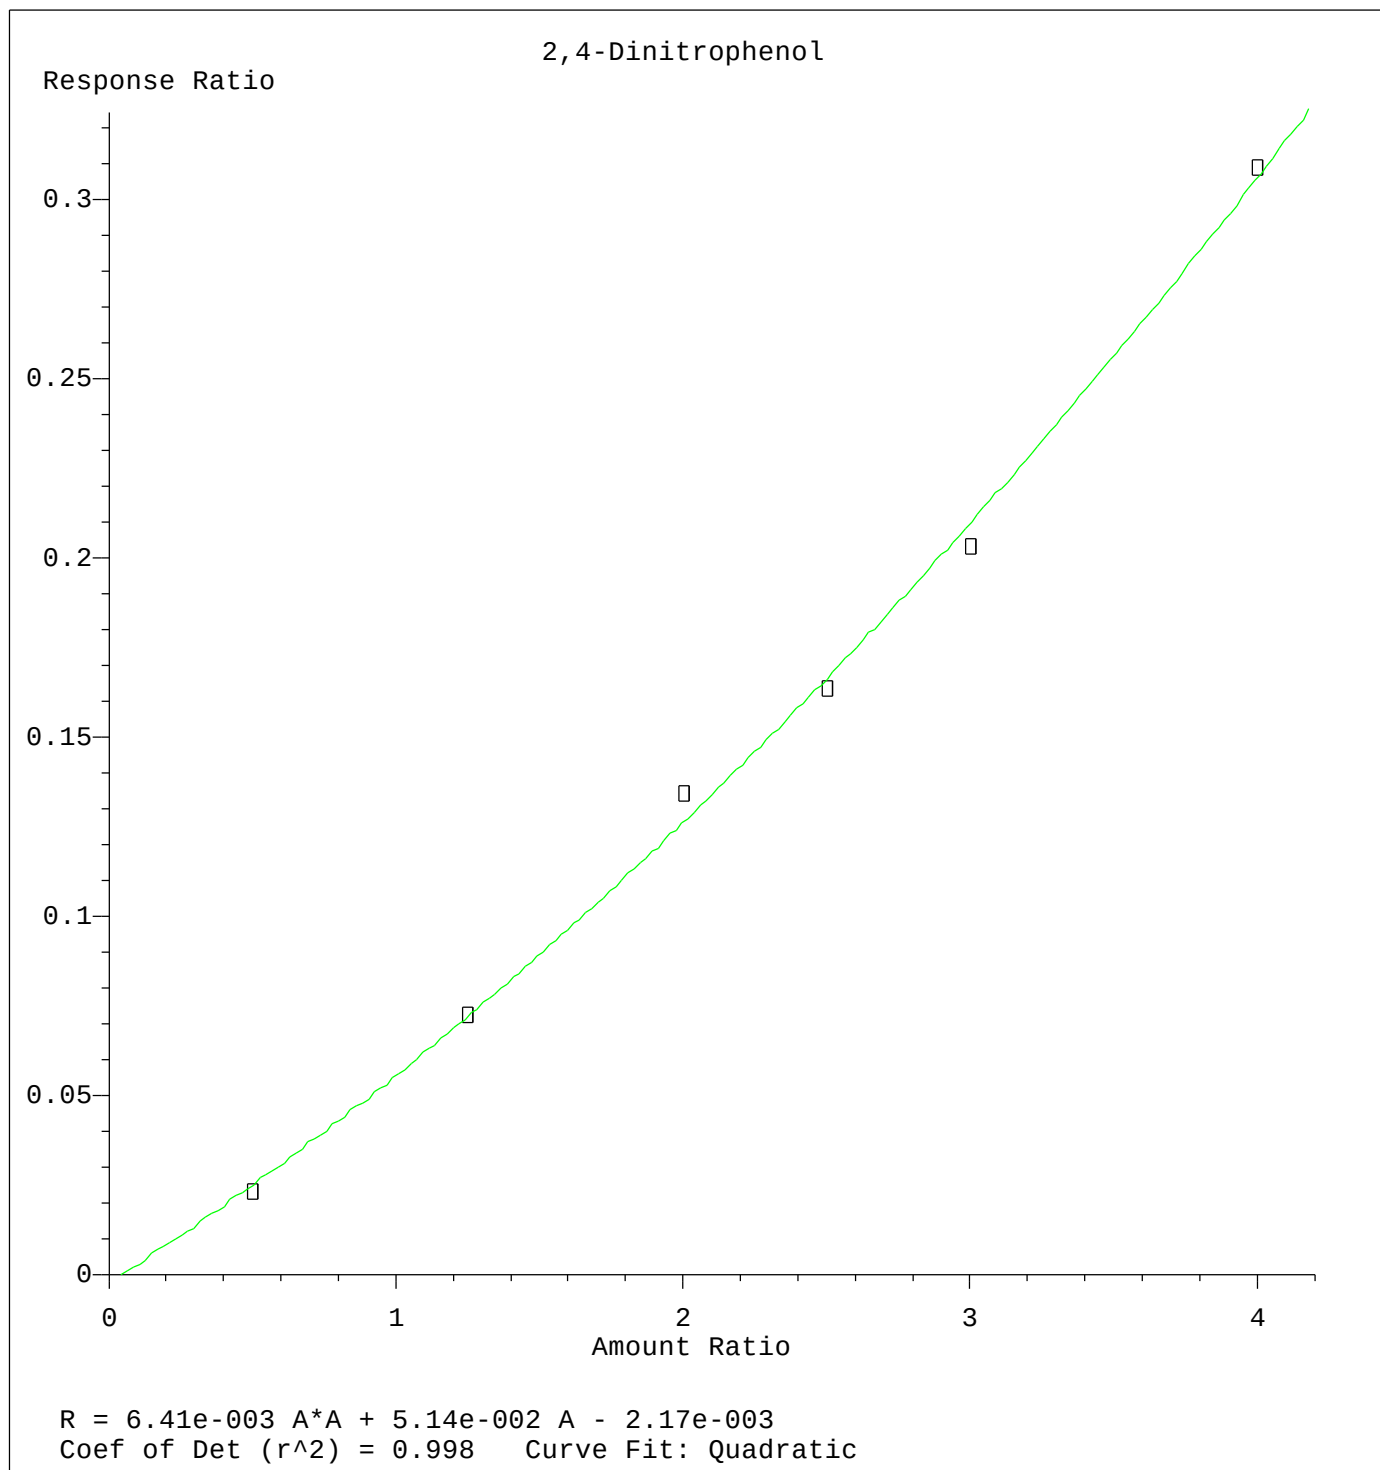

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Calibration Table Last Updated: Tue Jun 09 15:11:40 2015

2,4-Dinitrotoluene


Response Ratio

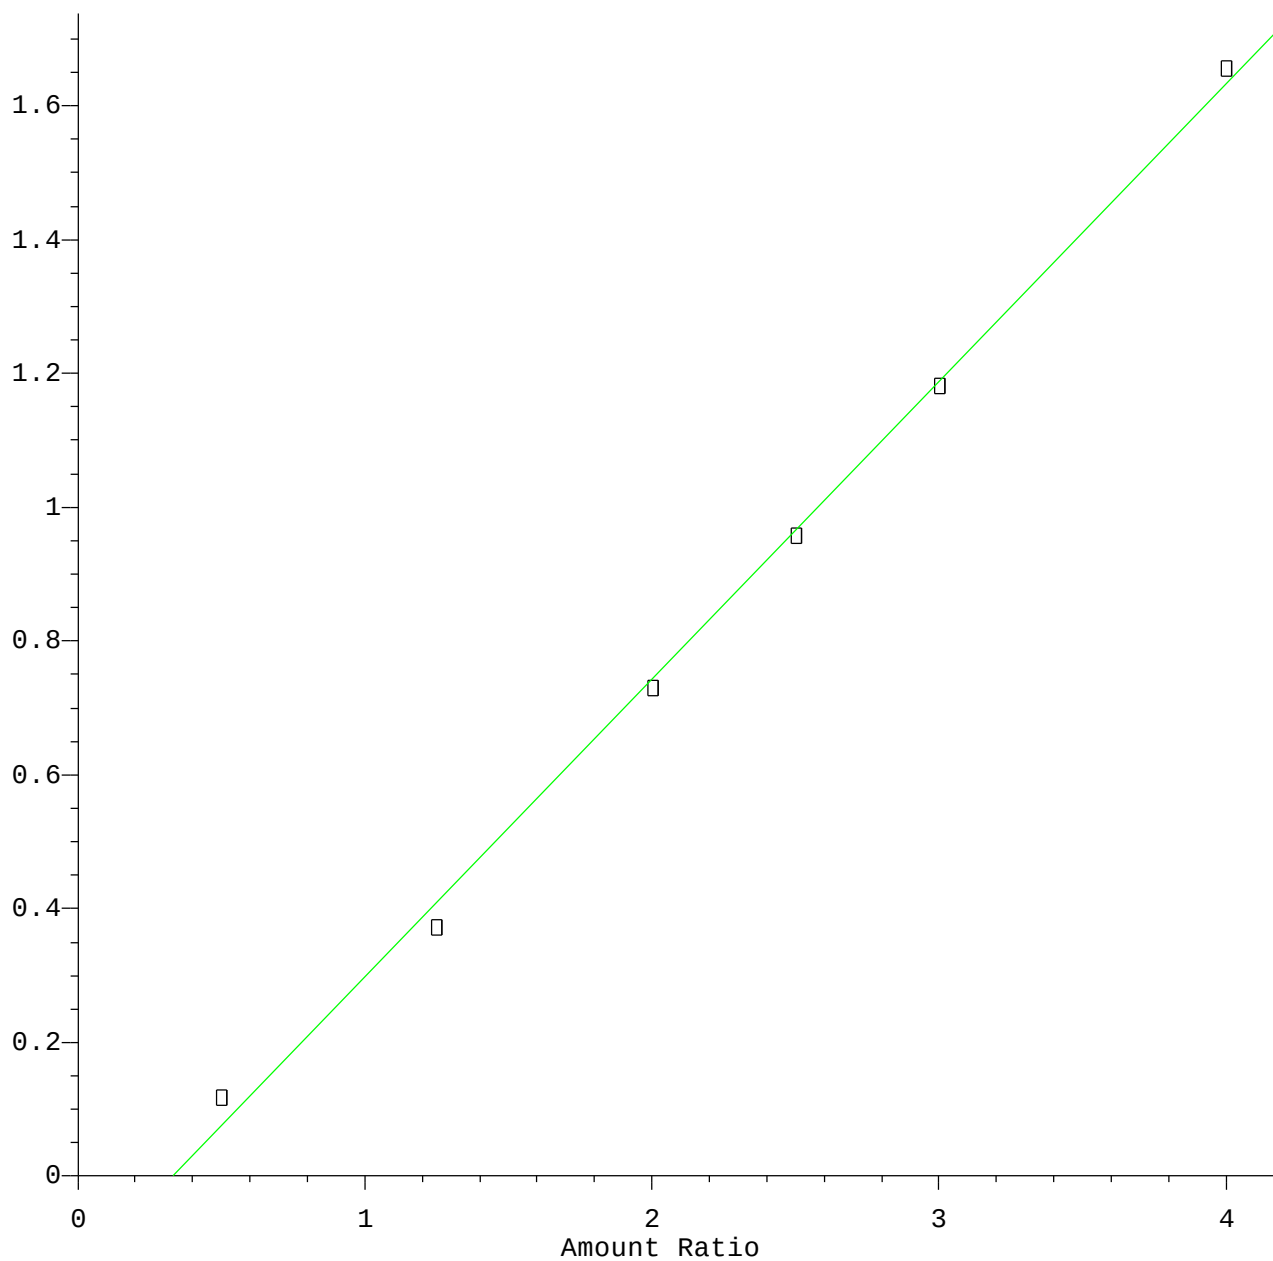

Resp Ratio = $4.45 \times 10^{-1} \times \text{Amt} - 1.48 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Calibration Table Last Updated: Tue Jun 09 15:11:40 2015

4,6-Dinitro-2-methylphenol

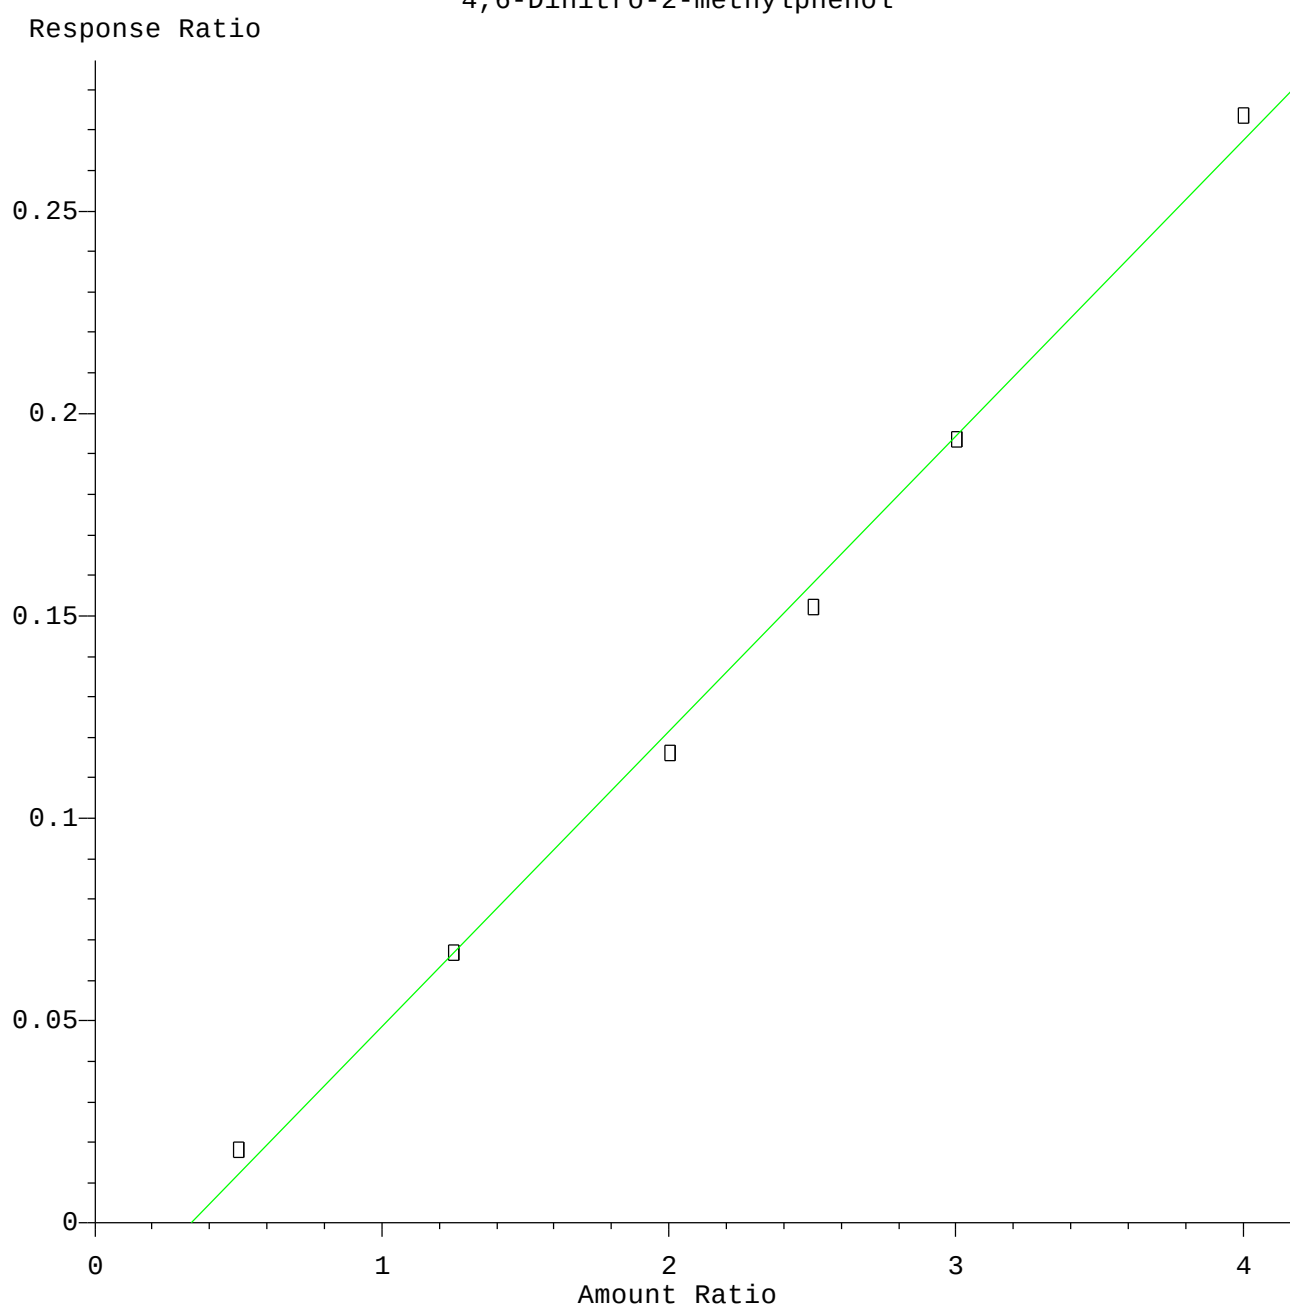

Resp Ratio = 7.28×10^{-2} * Amt - 2.42×10^{-2}
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Calibration Table Last Updated: Tue Jun 09 15:11:40 2015

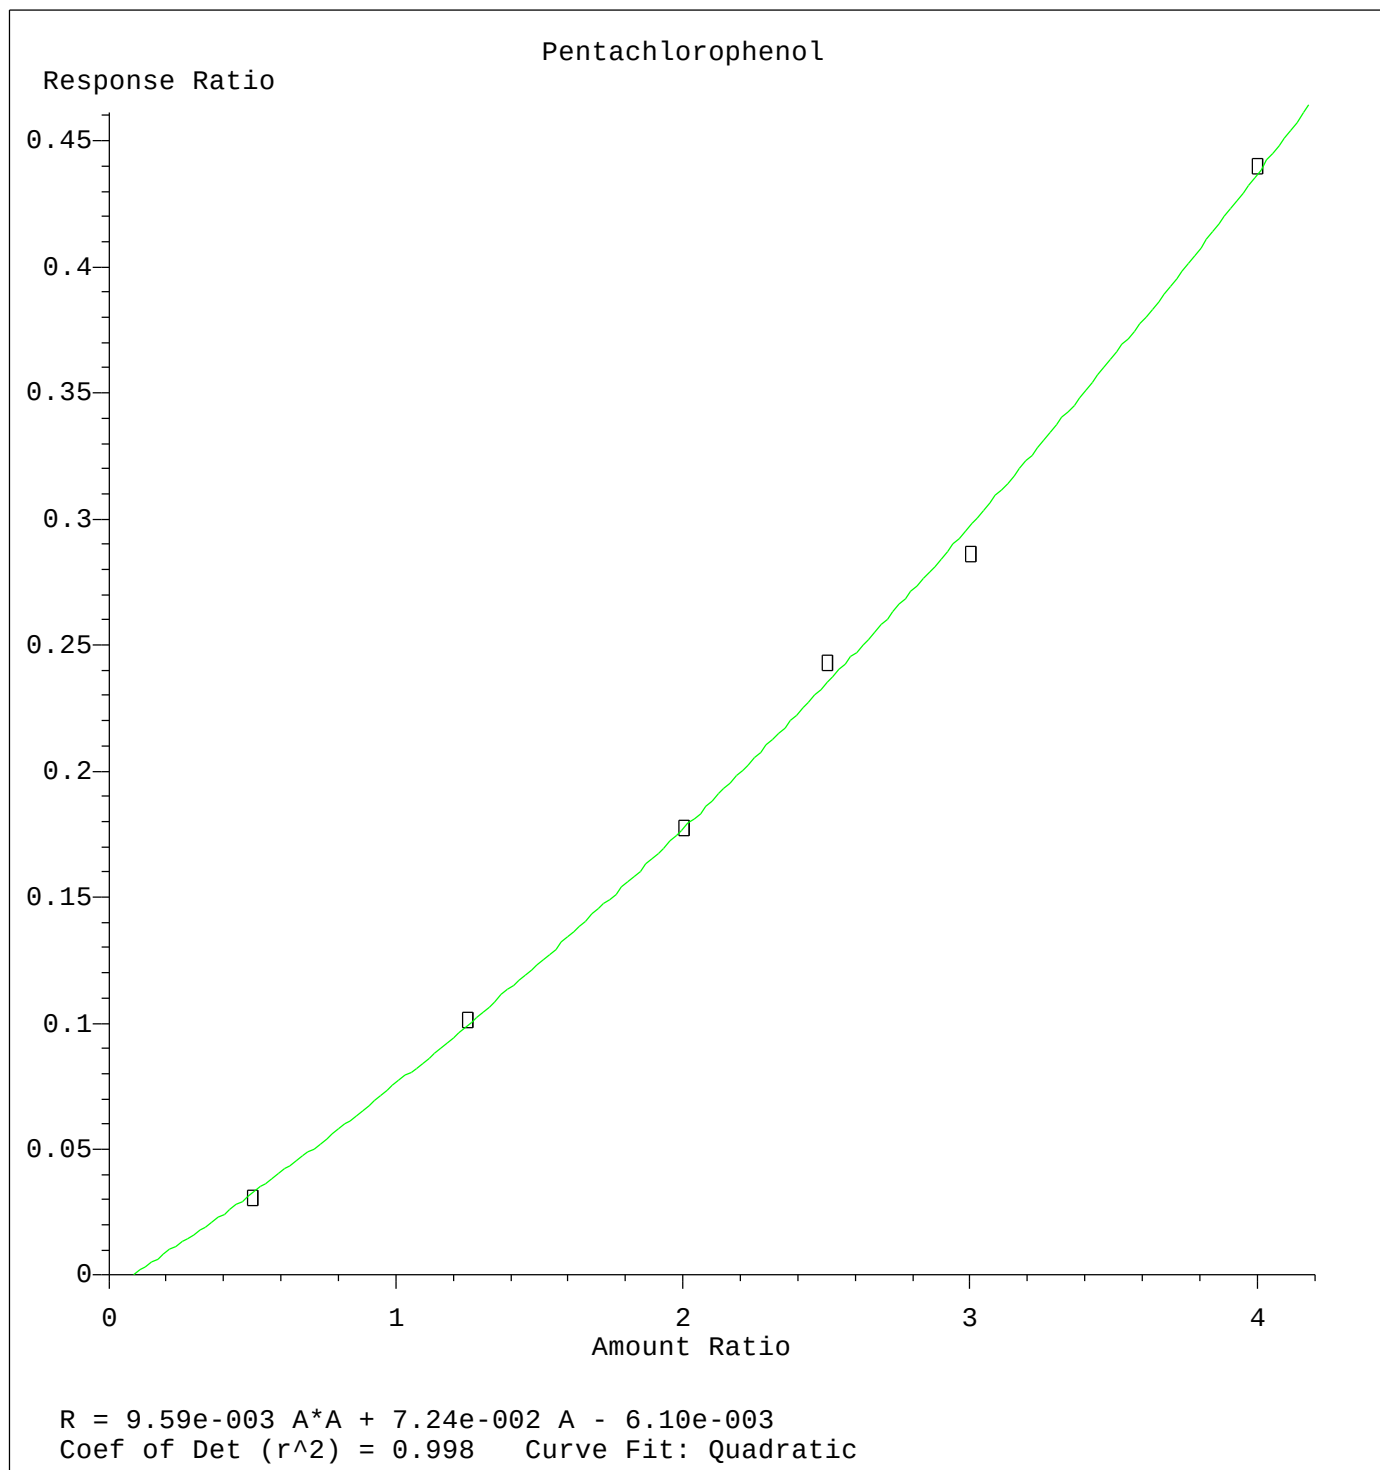

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Calibration Table Last Updated: Tue Jun 09 15:11:40 2015

2,4-Dinitrotoluene

Response Ratio

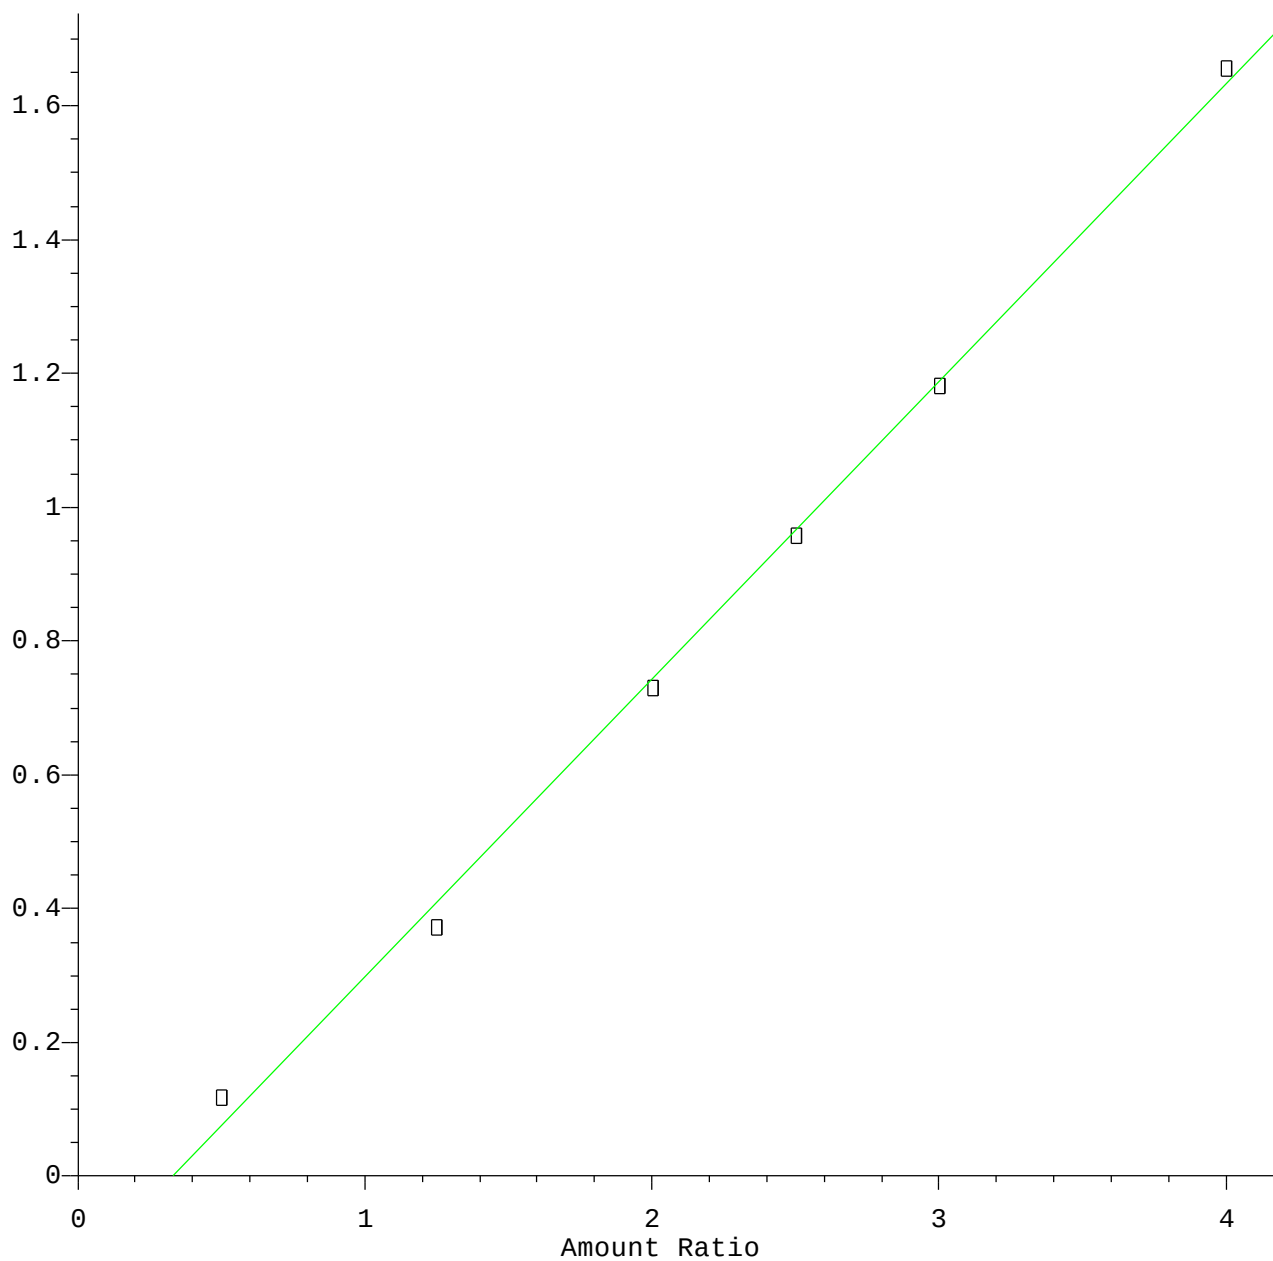

Resp Ratio = $4.45 \times 10^{-1} \times \text{Amt} - 1.48 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Calibration Table Last Updated: Tue Jun 09 15:11:40 2015