


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060915\
 Data File : BF079824.D
 Acq On : 9 Jun 2015 10:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 15:11:40 2015

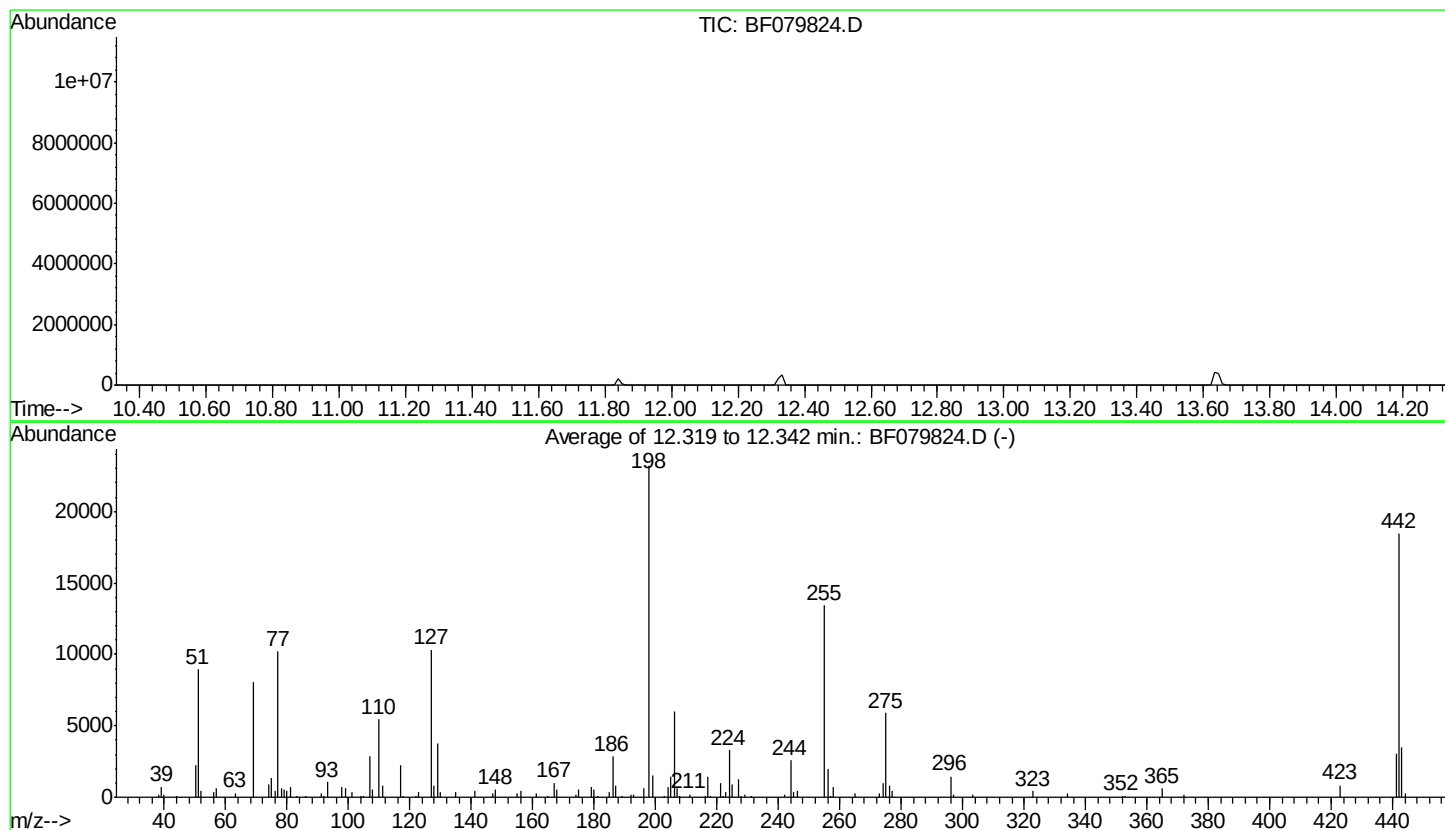

AutoFind: Scans 974, 975, 976; Background Corrected with Scan 971

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	8944	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	8101	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.6	10345	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23200	PASS
199	198	5	9	6.5	1513	PASS
275	198	10	60	25.3	5880	PASS
365	198	1	100	2.5	589	PASS
441	442	0.01	24	16.6	3068	PASS
442	198	50	100	79.5	18438	PASS
443	442	15	24	19.1	3528	PASS