

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060916\
 Data File : BF087849.D
 Acq On : 9 Jun 2016 13:38
 Operator : UM/SJ
 Sample : H3477-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 1300-03-SE-06072016

Quant Time: Jun 09 15:36:39 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 18:51:55 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	124956	20.00	ng	-0.02
21) Naphthalene-d8	8.10	136	484224	20.00	ng	-0.02
38) Acenaphthene-d10	9.85	164	232695	20.00	ng	-0.03
63) Phenanthrene-d10	11.32	188	414671	20.00	ng	-0.03
75) Chrysene-d12	13.95	240	316264	20.00	ng	-0.03
86) Perylene-d12	15.36	264	243214	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	652481	89.27	ng	-0.01
7) Phenol-d6	6.46	99	911548	102.90	ng	-0.02
23) Nitrobenzene-d5	7.38	82	505571	60.97	ng	-0.03
41) 2,4,6-Tribromophenol	10.64	330	216060	87.94	ng	-0.03
44) 2-Fluorobiphenyl	9.18	172	944768	62.30	ng	-0.03
78) Terphenyl-d14	12.91	244	809376	58.24	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	9.58	163	137584	8.16	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060916\
Data File : BF087849.D
Acq On : 9 Jun 2016 13:38
Operator : UM/SJ
Sample : H3477-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1300-03-SE-06072016

Quant Time: Jun 09 15:36:39 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

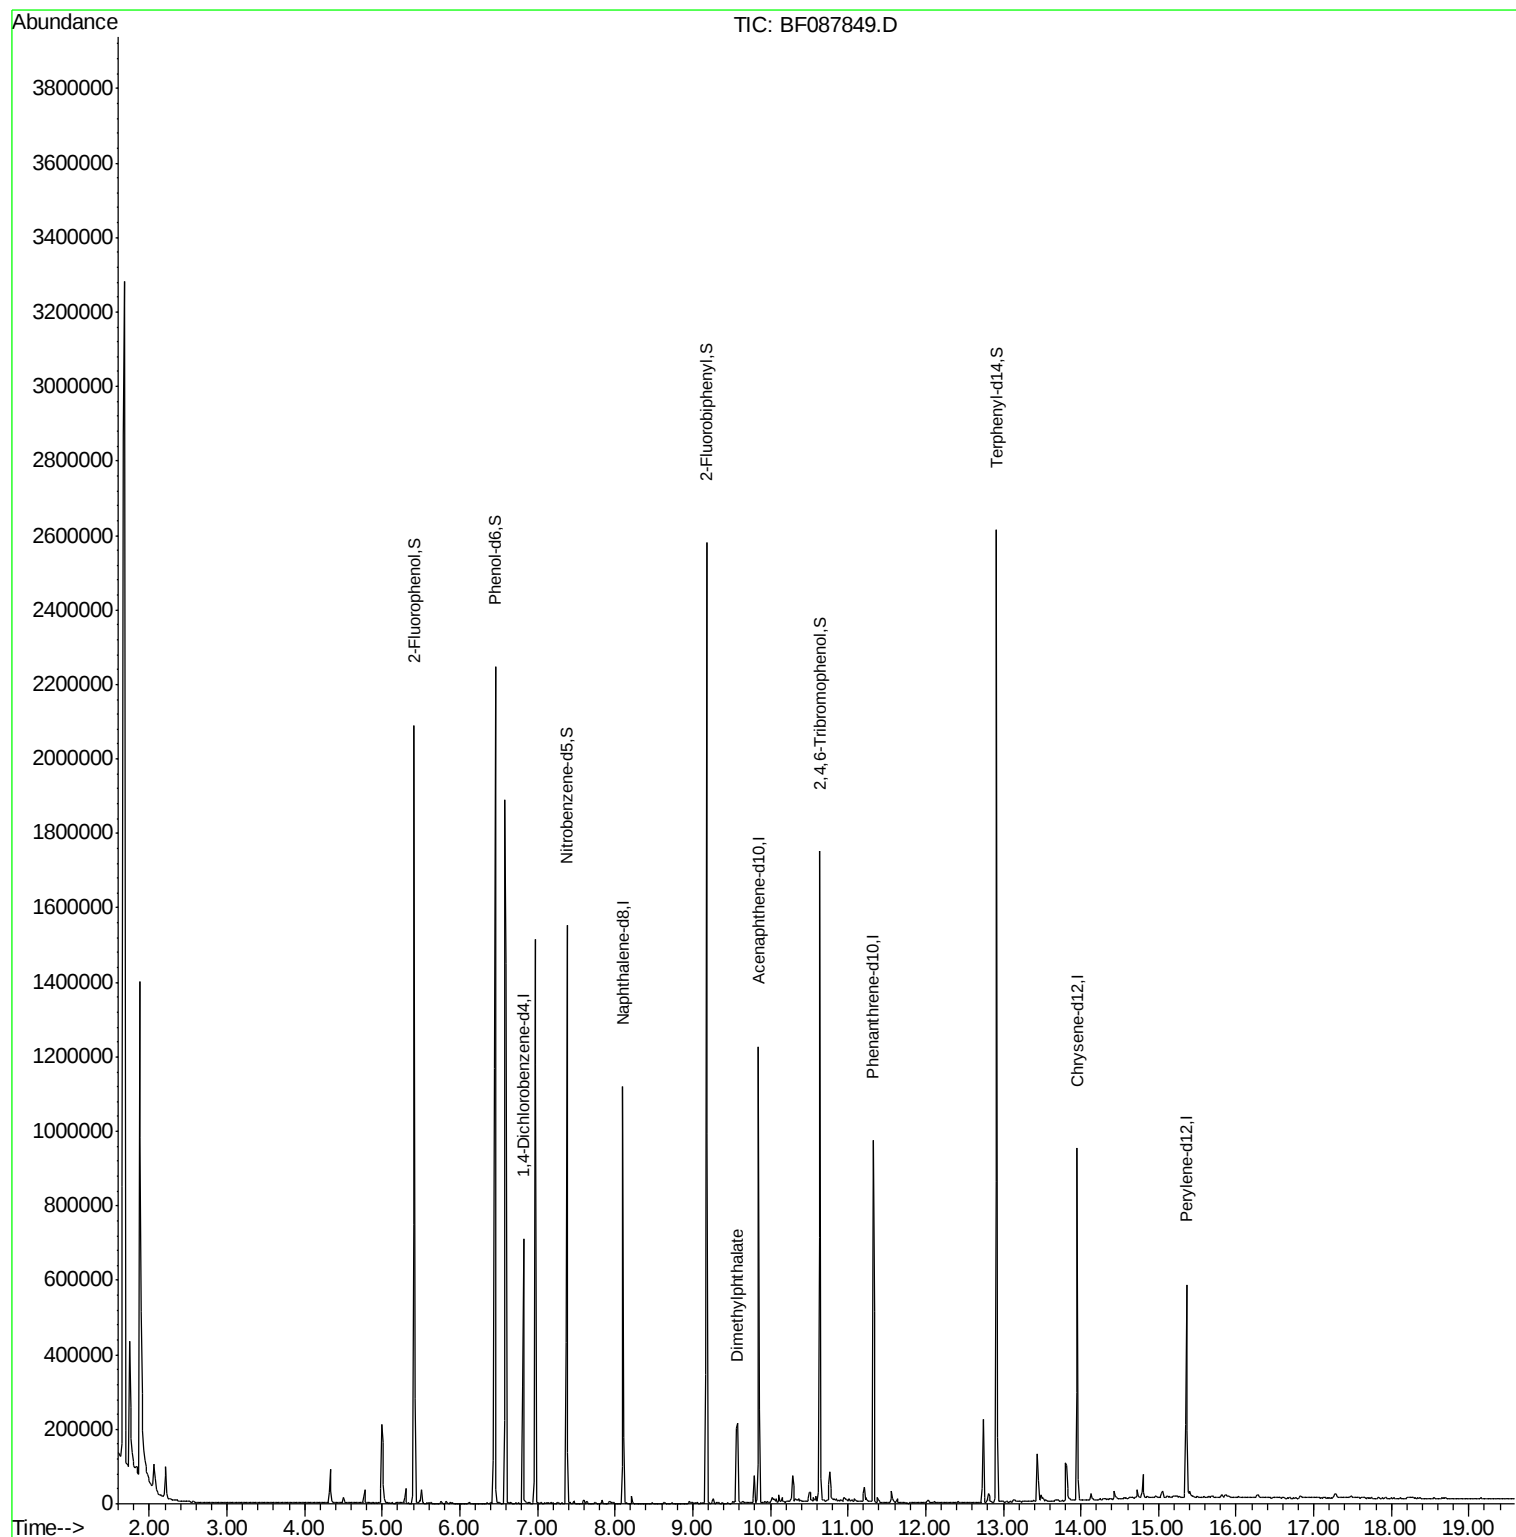

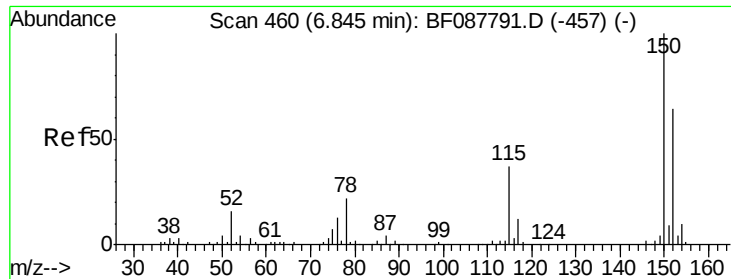

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.82 min Scan# 458

Delta R.T. -0.02 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38

Instrument :

BNA_F

ClientSampleId :

1300-03-SE-06072016


Tot Ion:152 Resp: 124956

Ion Ratio Lower Upper

152 100

150 153.4 123.8 185.6




115 52.6 39.6 59.4

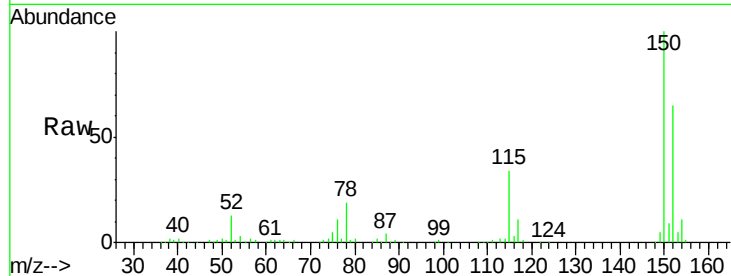

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

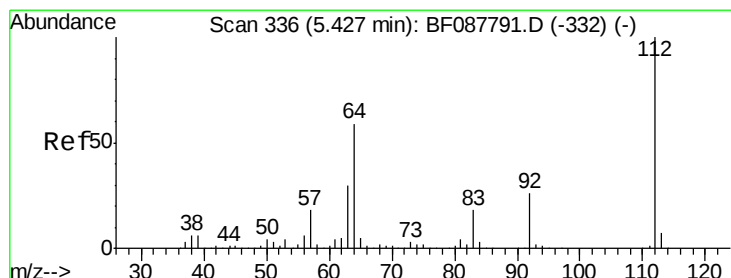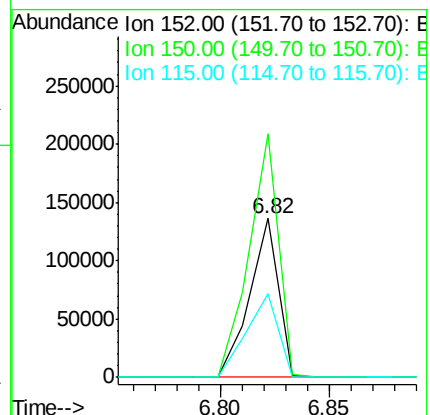

#5

2-Fluorophenol

Concen: 89.27 ng

RT: 5.42 min Scan# 335

Delta R.T. -0.01 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38


Tgt Ion:112 Resp: 652481

Ion Ratio Lower Upper

112 100

64 57.4 42.2 63.2



63 29.6 21.8 32.8

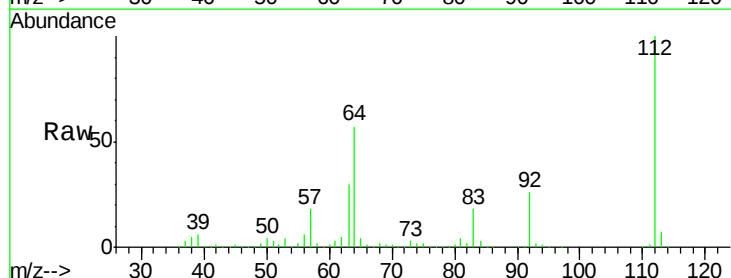


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

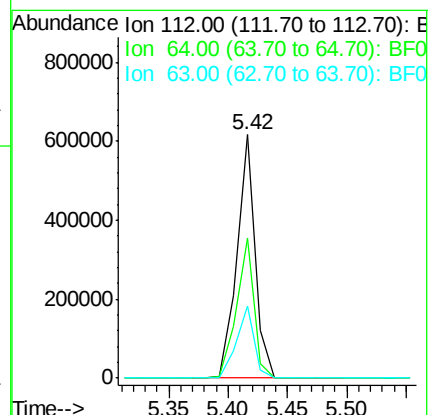

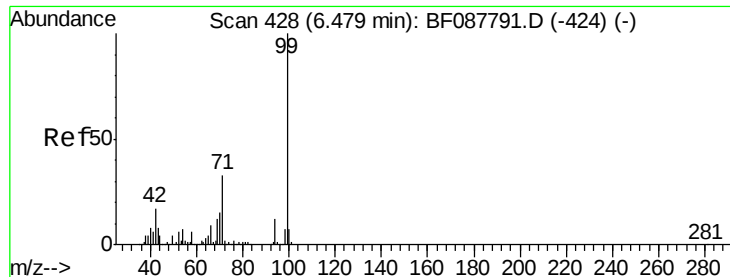

#7

Phenol-d6

Concen: 102.90 ng

RT: 6.46 min Scan# 426

Delta R.T. -0.02 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38

Instrument :

BNA_F

ClientSampleId :

1300-03-SE-06072016


Tot Ion: 99 Resp: 911548

Ion Ratio Lower Upper

99 100

42 16.5 12.2 18.2




71 33.0 23.4 35.0

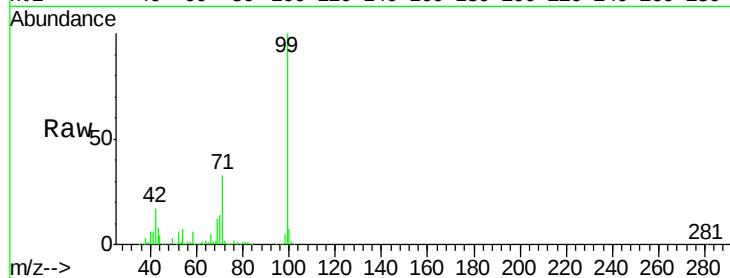

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

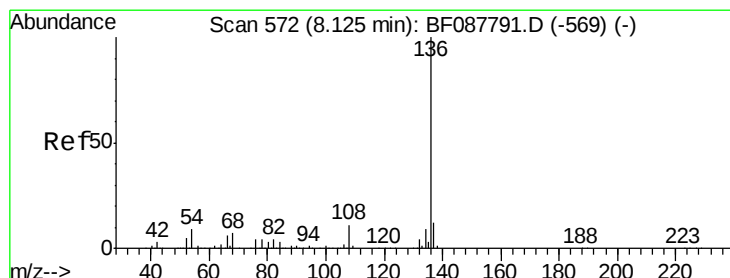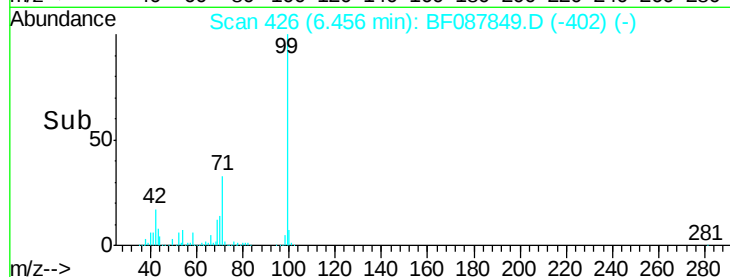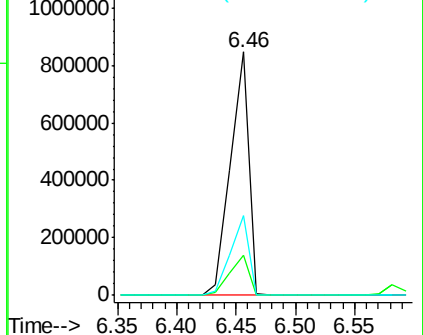

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.10 min Scan# 570

Delta R.T. -0.02 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38

Tgt Ion: 136 Resp: 484224


Ion Ratio Lower Upper

136 100

137 11.4 9.1 13.7

54 8.0 6.6 10.0

68 6.5 5.1 7.7


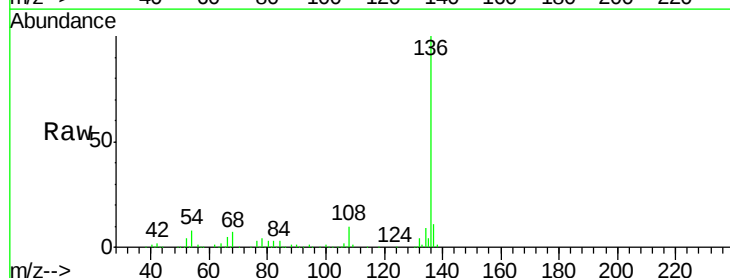



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

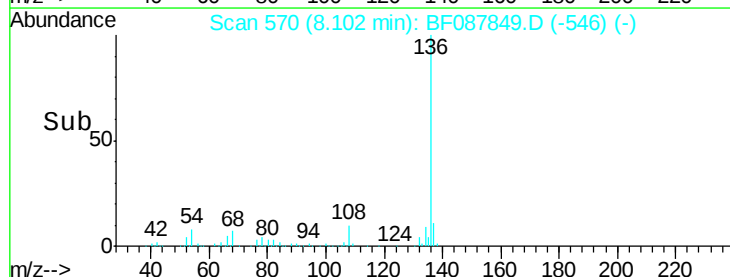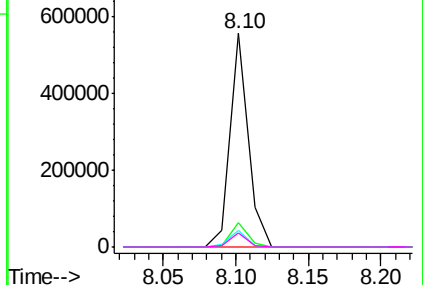



#23

Nitrobenzene-d5

Concen: 60.97 ng

RT: 7.38 min Scan# 507

Delta R.T. -0.03 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38

Instrument :

BNA_F

ClientSampleId :

1300-03-SE-06072016


Tot Ion: 82 Resp: 505571

Ion Ratio Lower Upper

82 100

128 46.3 35.9 53.9




54 49.4 40.9 61.3

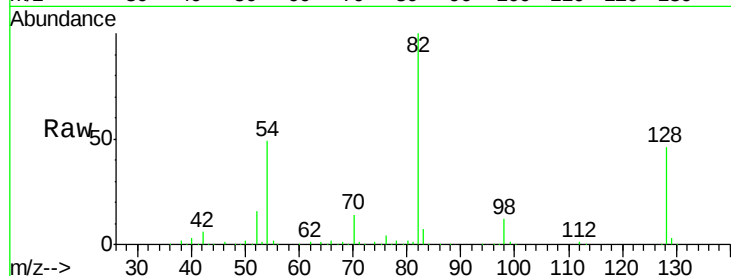

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

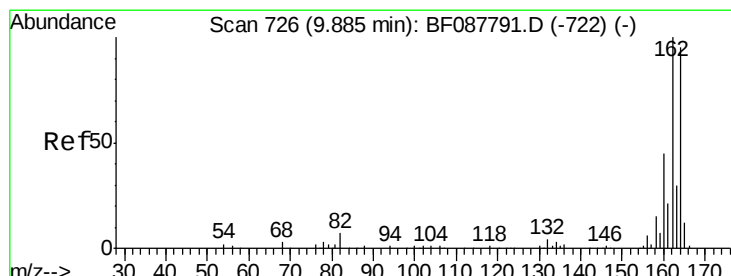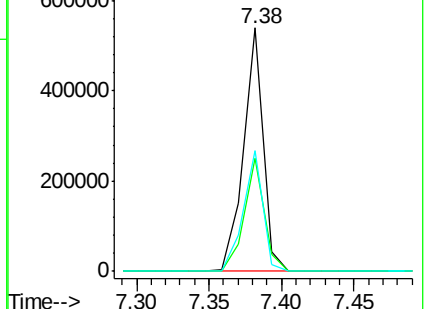

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.85 min Scan# 723

Delta R.T. -0.03 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38


Tgt Ion:164 Resp: 232695

Ion Ratio Lower Upper

164 100

162 102.2 85.4 128.2



160 45.6 39.5 59.3

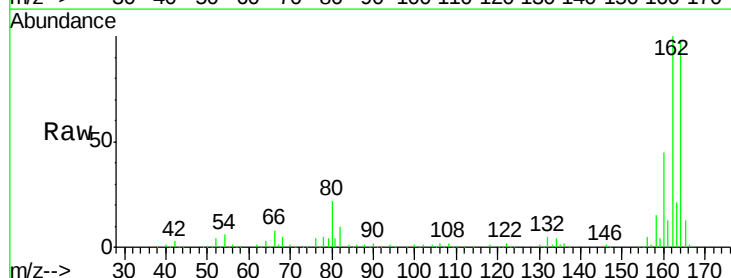


Abundance Ion 164.00 (163.70 to 164.70): BF0

Ion 162.00 (161.70 to 162.70): BF0

Ion 160.00 (159.70 to 160.70): BF0

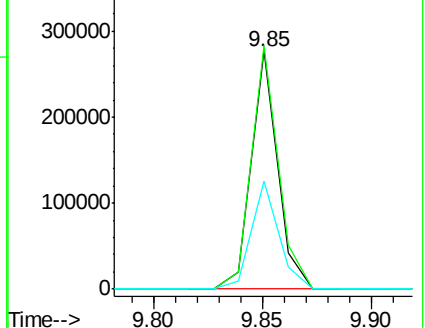







#41
 2,4,6-Tribromophenol
 Concen: 87.94 ng
 RT: 10.64 min Scan# 792
 Delta R.T. -0.03 min
 Lab File: BF087849.D
 Acq: 9 Jun 2016 13:38

Instrument :
 BNA_F
 ClientSampleId :
 1300-03-SE-06072016

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	0.0	0.0#
141	38.7	0.0	0.0#

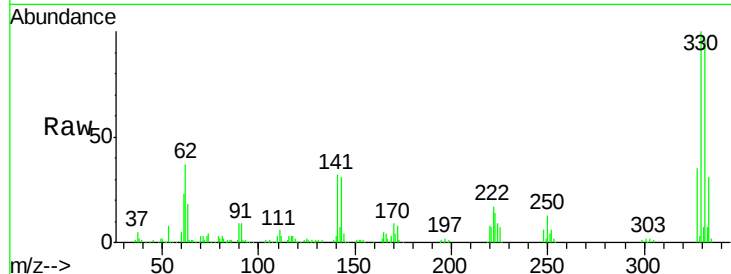


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

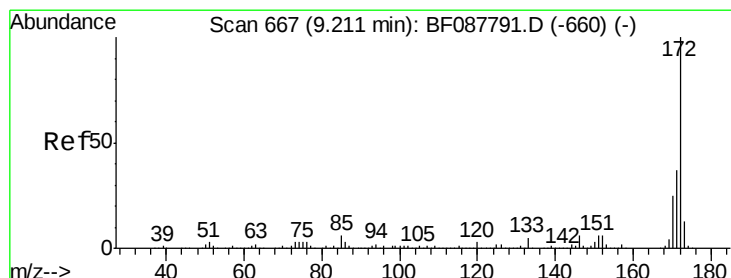
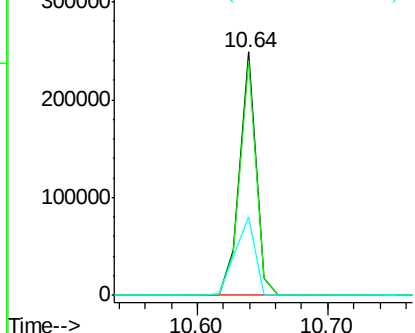



#44
 2-Fluorobiphenyl
 Concen: 62.30 ng
 RT: 9.18 min Scan# 664
 Delta R.T. -0.03 min
 Lab File: BF087849.D
 Acq: 9 Jun 2016 13:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	28.6	43.0
170	24.5	19.2	28.8

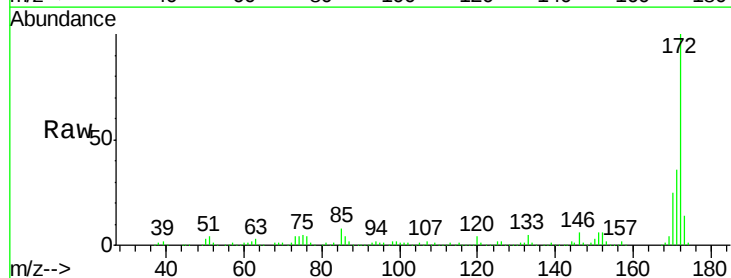

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

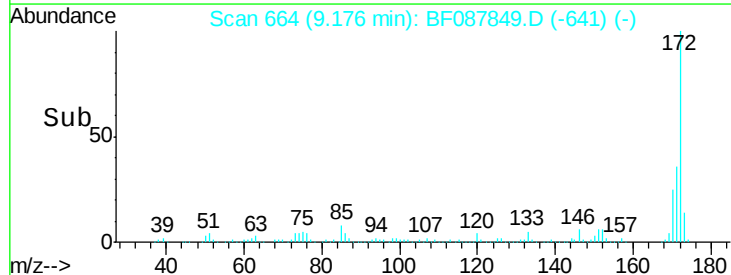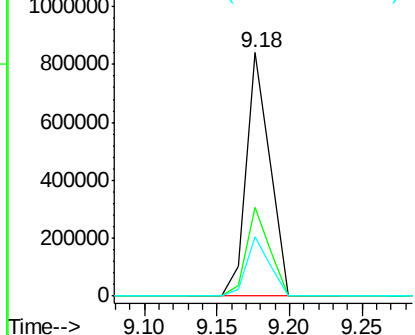







#49
Dimethylphthalate
Concen: 8.16 ng
RT: 9.58 min Scan# 699
Delta R.T. -0.03 min
Lab File: BF087849.D
Acq: 9 Jun 2016 13:38

Instrument :
BNA_F
ClientSampleId :
1300-03-SE-06072016

Tot Ion:163 Resp: 137584
Ion Ratio Lower Upper
163 100
194 3.9 2.8 4.2
164 9.2 8.3 12.5

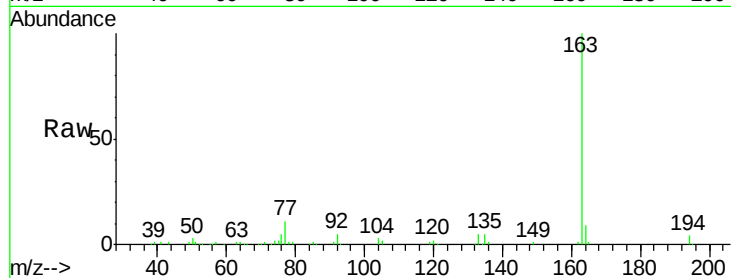


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

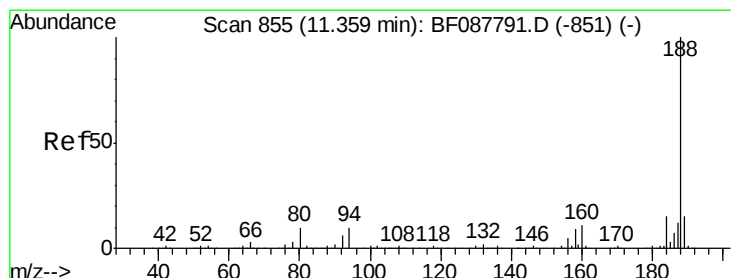
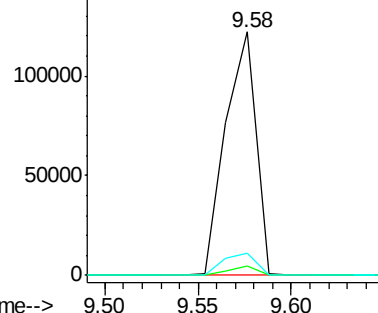



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.32 min Scan# 852
Delta R.T. -0.03 min
Lab File: BF087849.D
Acq: 9 Jun 2016 13:38

Tgt Ion:188 Resp: 414671
Ion Ratio Lower Upper
188 100
94 13.4 9.0 13.6
80 14.8 10.0 15.0

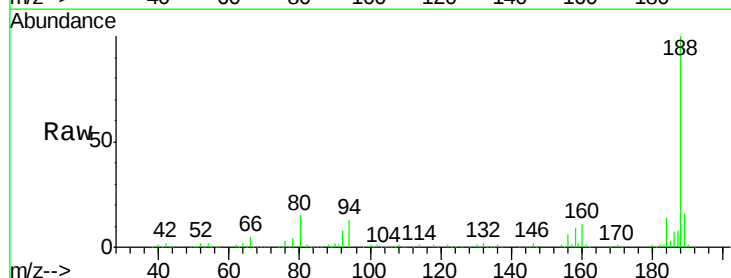

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

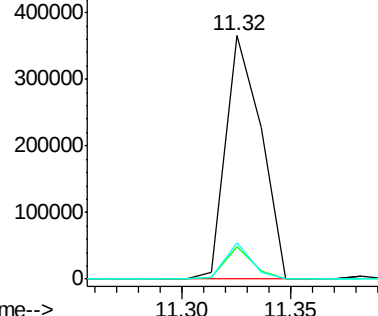

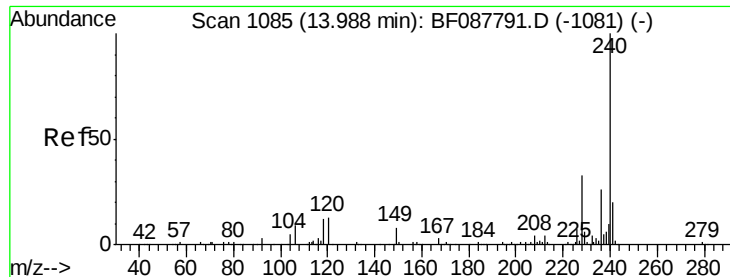

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.95 min Scan# 1082

Delta R.T. -0.03 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38

Instrument :

BNA_F

ClientSampleId :

1300-03-SE-06072016


Tot Ion:240 Resp: 316264

Ion Ratio Lower Upper

240 100

120 11.6 6.8 10.2#




236 26.2 20.2 30.2

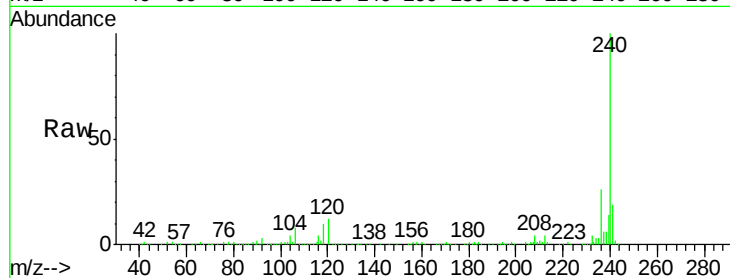

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

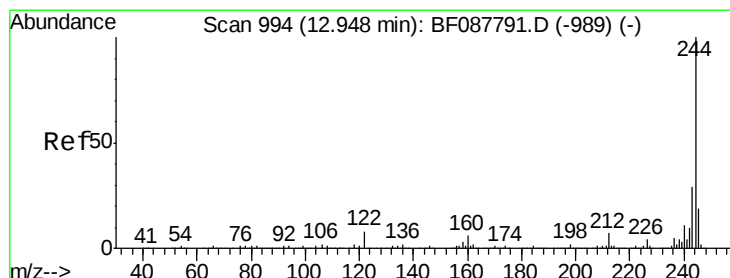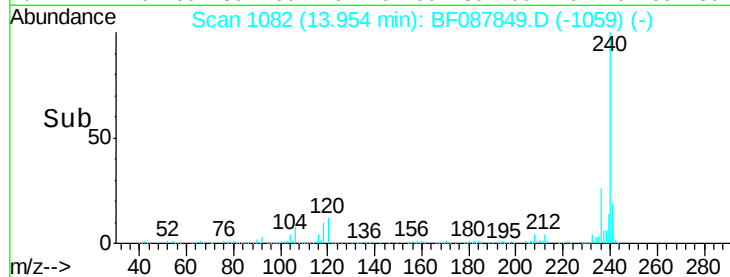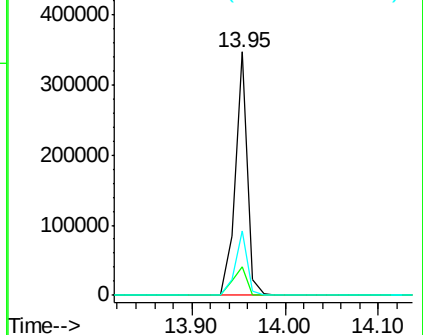

#78

Terphenyl-d14

Concen: 58.24 ng

RT: 12.91 min Scan# 991

Delta R.T. -0.03 min

Lab File: BF087849.D

Acq: 9 Jun 2016 13:38


Tgt Ion:244 Resp: 809376

Ion Ratio Lower Upper

244 100

212 7.5 6.0 9.0



122 13.2 11.2 16.8

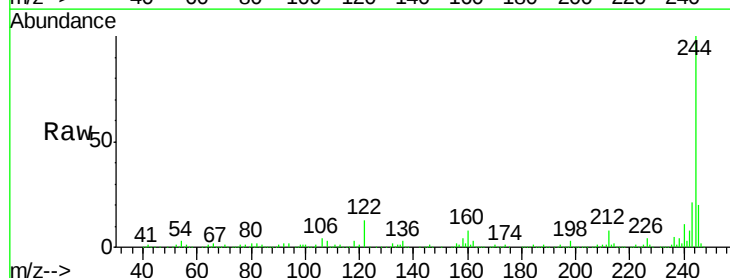


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

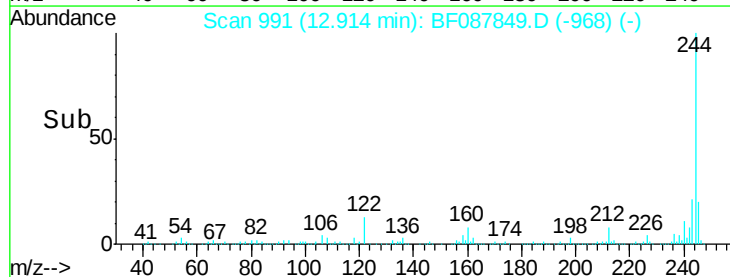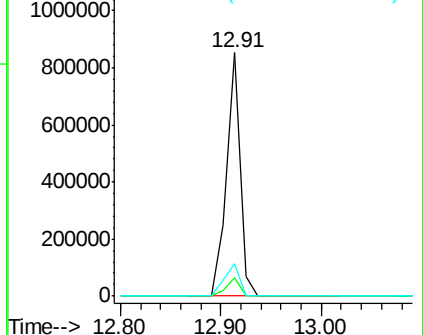

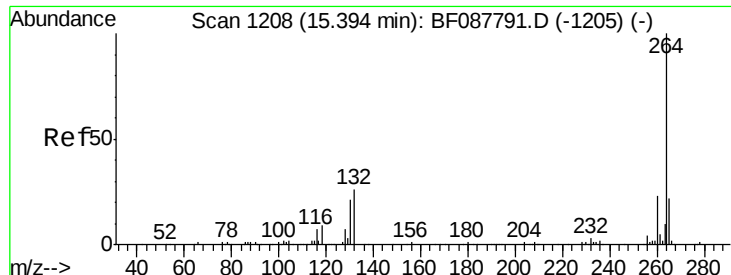


#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.36 min Scan# 1205
Delta R.T. -0.03 min
Lab File: BF087849.D
Acq: 9 Jun 2016 13:38

Instrument :
BNA_F
ClientSampleId :
1300-03-SE-06072016

Tot Ion: 264 Resp: 243214

Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	21.8	16.9	25.3

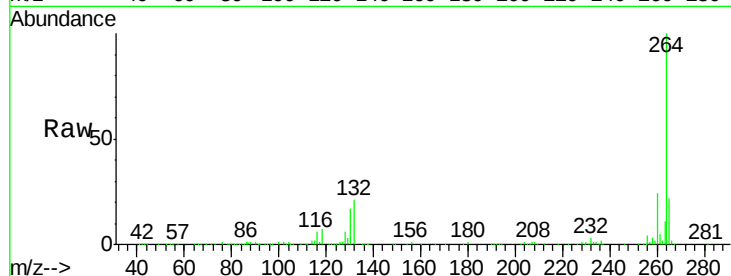

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

