

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060916\
 Data File : BF087855.D
 Acq On : 9 Jun 2016 16:31
 Operator : UM/SJ
 Sample : H3399-13 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SS-32

Quant Time: Jun 09 17:18:20 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 18:51:55 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	123218	20.00	ng	-0.02
21) Naphthalene-d8	8.10	136	448633	20.00	ng	-0.02
38) Acenaphthene-d10	9.85	164	200082	20.00	ng	-0.03
63) Phenanthrene-d10	11.32	188	302001	20.00	ng	-0.03
75) Chrysene-d12	13.95	240	233625	20.00	ng	-0.03
86) Perylene-d12	15.37	264	233485	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	532769	73.92	ng	-0.01
7) Phenol-d6	6.46	99	702455	80.42	ng	-0.02
23) Nitrobenzene-d5	7.38	82	372875	48.53	ng	-0.03
41) 2,4,6-Tribromophenol	10.64	330	137765	65.21	ng	-0.03
44) 2-Fluorobiphenyl	9.18	172	609674	45.28	ng	-0.03
78) Terphenyl-d14	12.91	244	440685	42.92	ng	-0.03
Target Compounds						Qvalue
31) Naphthalene	8.12	128	46398	2.09	ng	99
49) Dimethylphthalate	9.58	163	68312	4.71	ng	98
51) Acenaphthene	9.88	154	35592	2.77	ng	98
70) Phenanthrene	11.36	178	358945	22.65	ng	97
71) Anthracene	11.40	178	101385	6.34	ng	97
72) Carbazole	11.55	167	38751	2.59	ng	99
73) Di-n-butylphthalate	11.90	149	74501	3.93	ng	99
74) Fluoranthene	12.54	202	433109	25.90	ng	98
77) Pyrene	12.77	202	394654	22.76	ng	99
79) Butylbenzylphthalate	13.42	149	2214773	288.96	ng	97
80) Benzo(a)anthracene	13.94	228	197798	14.86	ng	98
82) Chrysene	13.99	228	153748	12.28	ng	96
83) Bis(2-ethylhexyl)phthalate	13.95	149	482048	51.66	ng	# 58
84) Di-n-octyl phthalate	14.56	149	857763	56.58	ng	# 100
85) Indeno(1,2,3-cd)pyrene	16.72	276	78384	6.74	ng	# 100
87) Benzo(b)fluoranthene	14.97	252	230418m	14.16	ng	
88) Benzo(k)fluoranthene	14.98	252	52920m	4.31	ng	
89) Benzo(a)pyrene	15.30	252	144556	10.98	ng	97
91) Benzo(a,h,i)perylene	17.13	276	73007	5.80	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060916\
Data File : BF087855.D
Acq On : 9 Jun 2016 16:31
Operator : UM/SJ
Sample : H3399-13 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS-32

Quant Time: Jun 09 17:18:20 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

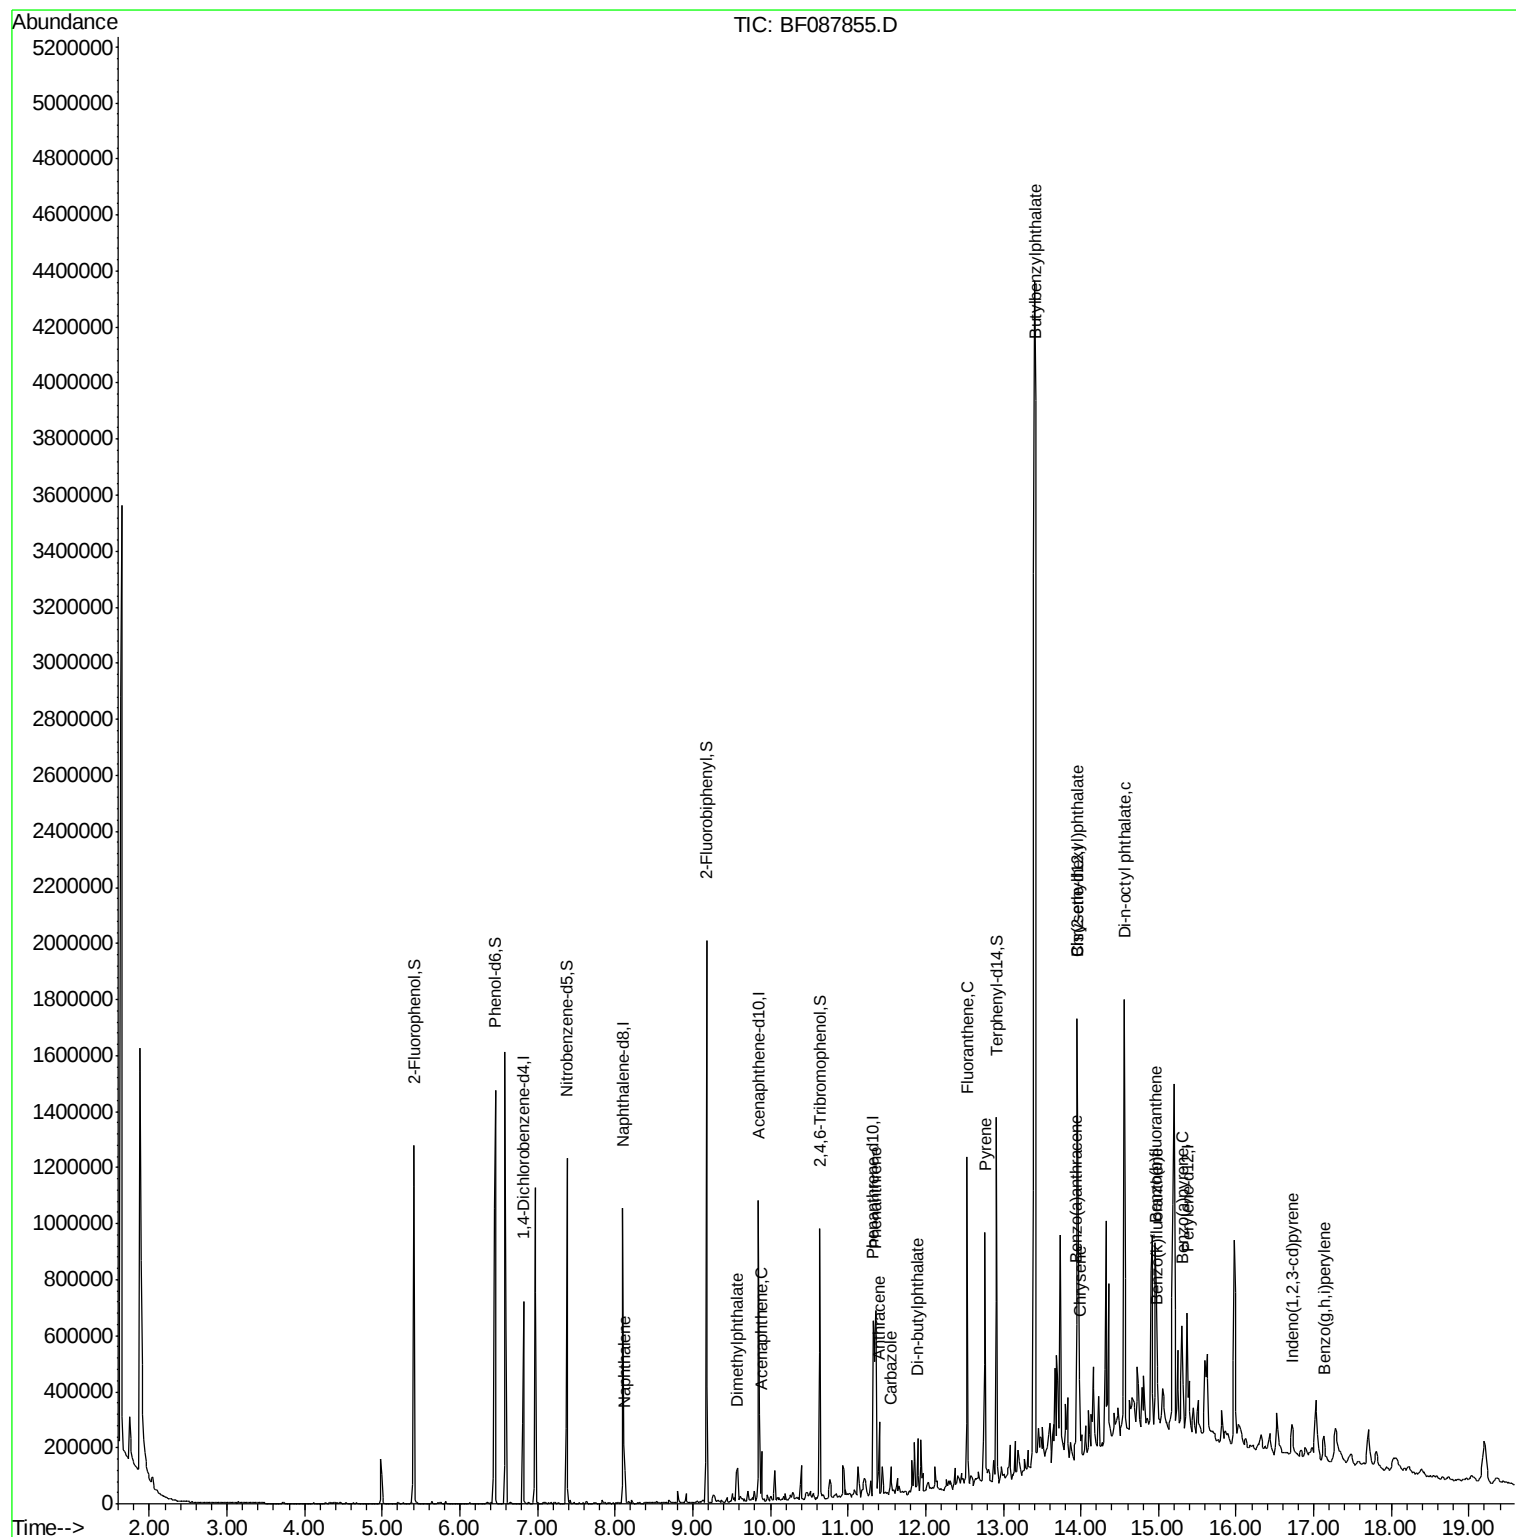




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.82 min Scan# 458
Delta R.T. -0.02 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Instrument :
BNA_F
ClientSampleId :
SS-32

Tot Ion:152 Resp: 123218
Ion Ratio Lower Upper
152 100
150 152.7 123.8 185.6
115 53.8 39.6 59.4

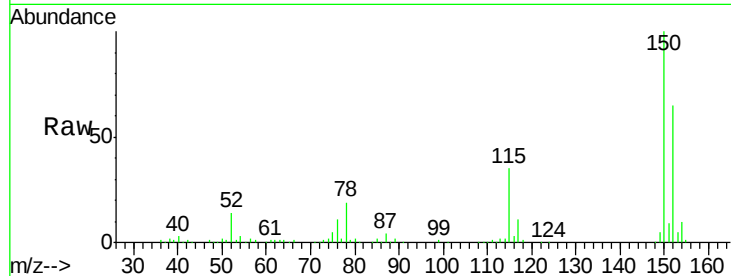


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

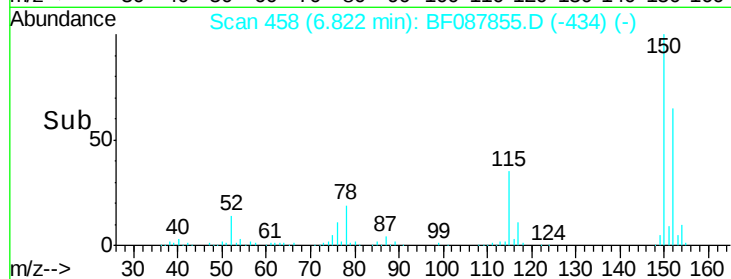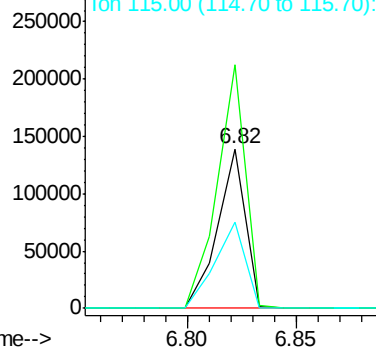



#5


2-Fluorophenol
Concen: 73.92 ng
RT: 5.42 min Scan# 335
Delta R.T. -0.01 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Tgt Ion:112 Resp: 532769
Ion Ratio Lower Upper
112 100
64 45.7 42.2 63.2
63 23.8 21.8 32.8



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

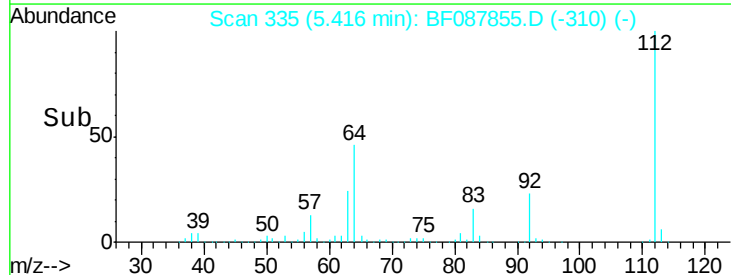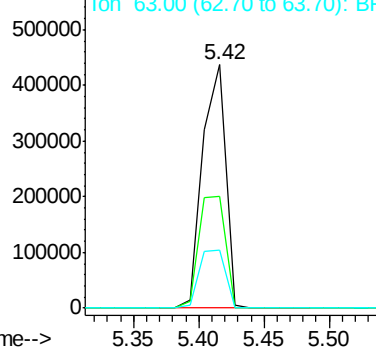

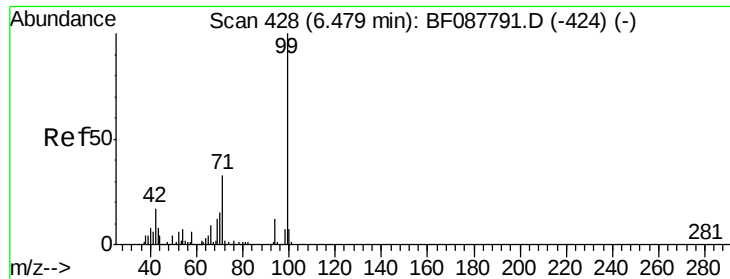

#7

Phenol-d6

Concen: 80.42 ng

RT: 6.46 min Scan# 426

Delta R.T. -0.02 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampleId :

SS-32


Tot Ion: 99 Resp: 702455

Ion Ratio Lower Upper

99 100

42 13.2 12.2 18.2

71 29.4 23.4 35.0

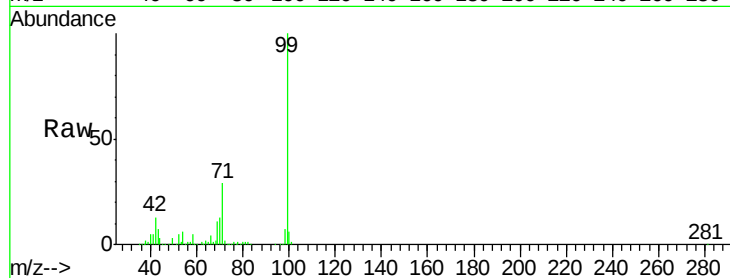

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0



6.46

400000

200000

0

Time-->

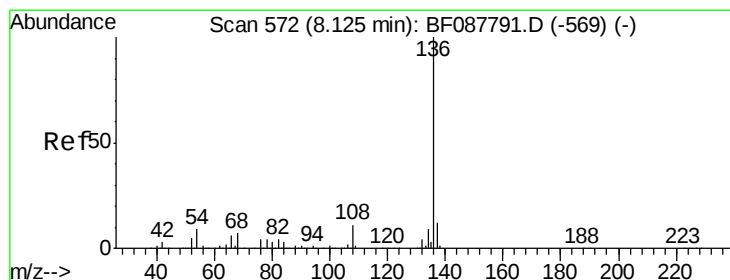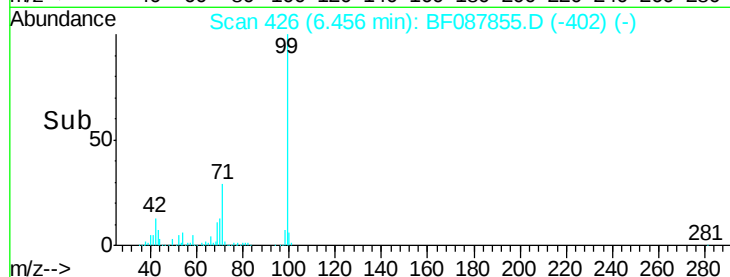

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.10 min Scan# 570

Delta R.T. -0.02 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Tgt Ion: 136 Resp: 448633


Ion Ratio Lower Upper

136 100

137 11.5 9.1 13.7

54 8.6 6.6 10.0

68 6.7 5.1 7.7

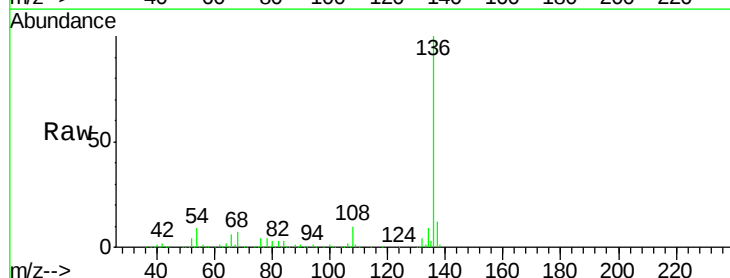

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0


8.10


400000

200000

0

Time-->

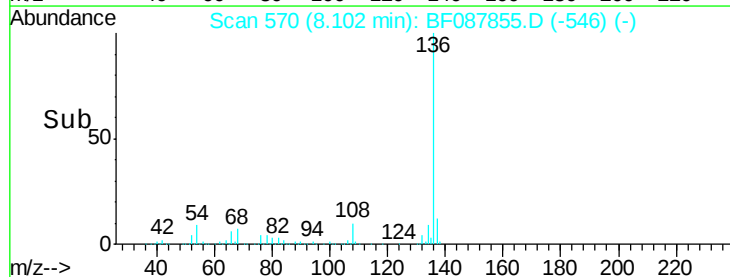

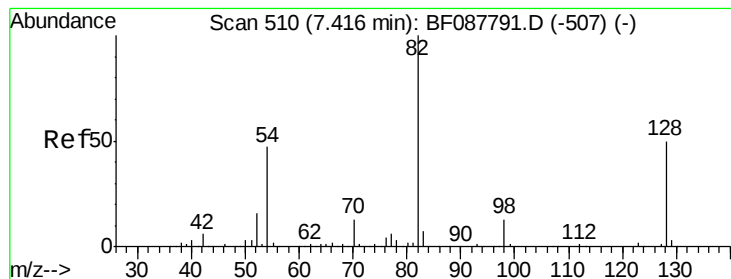

#23

Nitrobenzene-d5

Concen: 48.53 ng

RT: 7.38 min Scan# 507

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampleId :

SS-32


Tot Ion: 82 Resp: 372875

Ion Ratio Lower Upper

82 100

128 45.8 35.9 53.9




54 48.7 40.9 61.3



Abundance Ion 82.00 (81.70 to 82.70): BF087791.D (-507) (-)

Ion 128.00 (127.70 to 128.70): BF087791.D (-507) (-)

Ion 54.00 (53.70 to 54.70): BF087791.D (-507) (-)

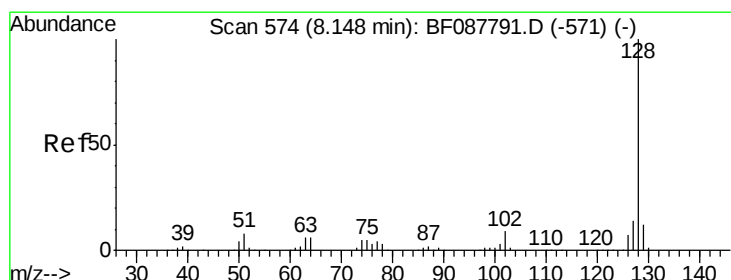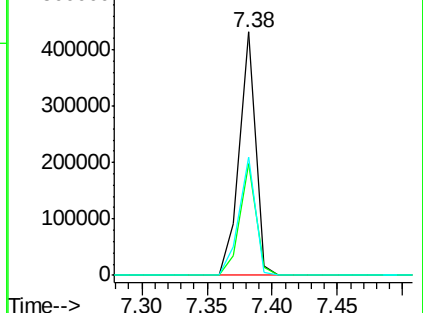

#31

Naphthalene

Concen: 2.09 ng

RT: 8.12 min Scan# 572

Delta R.T. -0.02 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31


Tgt Ion: 128 Resp: 46398

Ion Ratio Lower Upper

128 100

129 11.4 9.4 14.2



127 12.9 10.9 16.3




Abundance Ion 128.00 (127.70 to 128.70): BF087791.D (-571) (-)

Ion 129.00 (128.70 to 129.70): BF087791.D (-571) (-)

Ion 127.00 (126.70 to 127.70): BF087791.D (-571) (-)

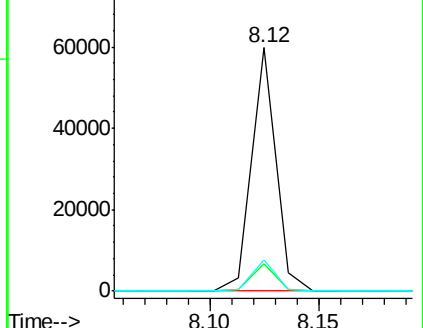


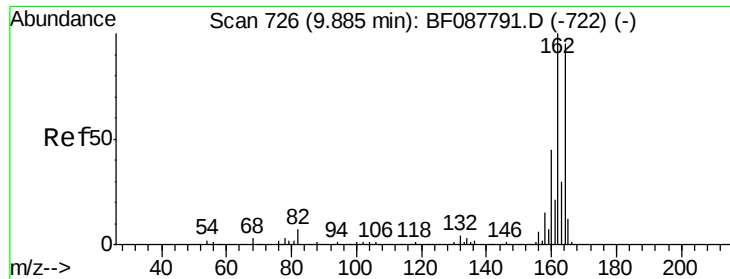




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.85 min Scan# 723
Delta R.T. -0.03 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Instrument :
BNA_F
ClientSampleId :
SS-32

Tot Ion:164 Resp: 200082
Ion Ratio Lower Upper
164 100
162 103.0 85.4 128.2
160 46.7 39.5 59.3

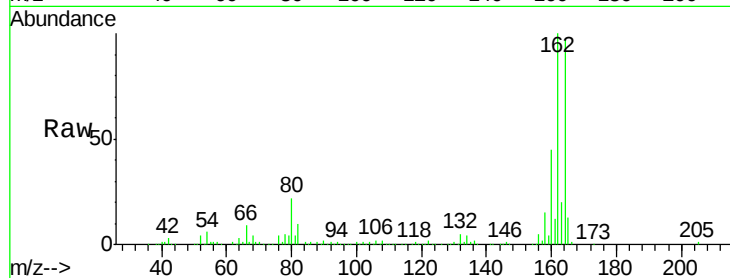


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

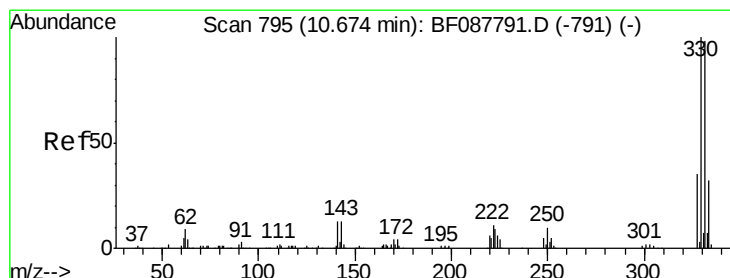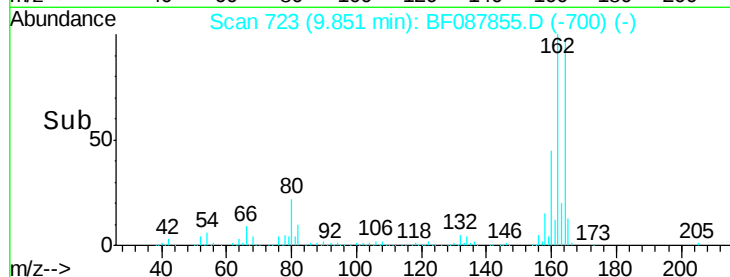
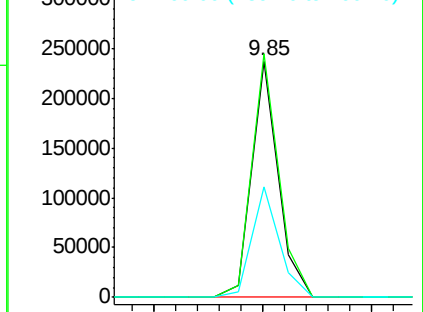



#41
2,4,6-Tribromophenol
Concen: 65.21 ng
RT: 10.64 min Scan# 792
Delta R.T. -0.03 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Tgt Ion:330 Resp: 137765
Ion Ratio Lower Upper
330 100
332 96.5 0.0 0.0#
141 33.4 0.0 0.0#

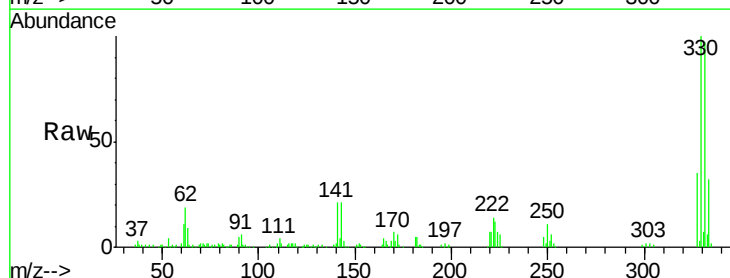

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

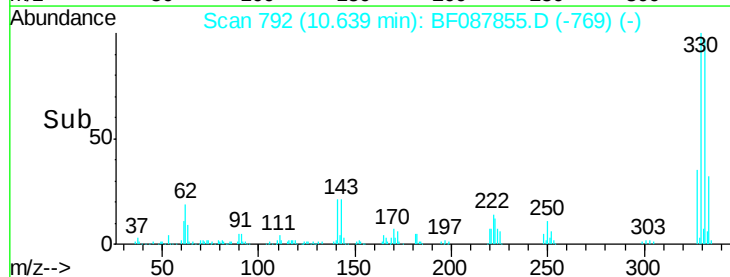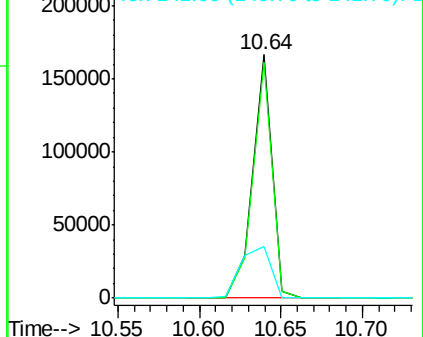







#44
2-Fluorobiphenyl
Concen: 45.28 ng
RT: 9.18 min Scan# 664
Delta R.T. -0.03 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Instrument :
BNA_F
ClientSampleId :
SS-32

Tot Ion:172 Resp: 609674
Ion Ratio Lower Upper
172 100
171 35.7 28.6 43.0
170 23.9 19.2 28.8




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


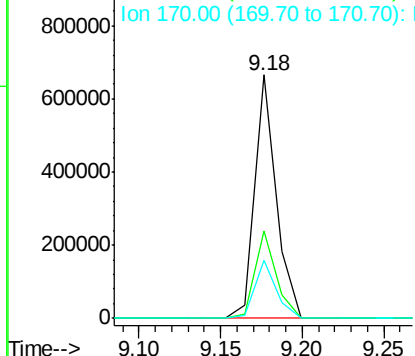



#49
Dimethylphthalate
Concen: 4.71 ng
RT: 9.58 min Scan# 699
Delta R.T. -0.03 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Tgt Ion:163 Resp: 68312
Ion Ratio Lower Upper
163 100
194 3.8 2.8 4.2
164 9.5 8.3 12.5



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

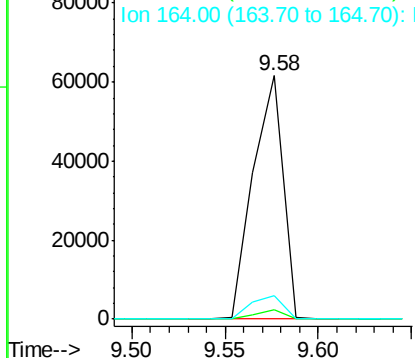

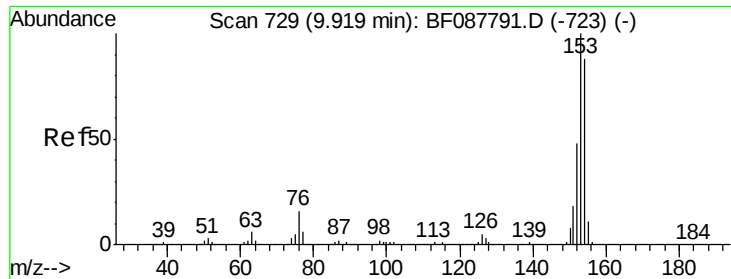

#51

Acenaphthene

Concen: 2.77 ng

RT: 9.88 min Scan# 726

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampleId :

SS-32


Tot Ion:154 Resp: 35592

Ion Ratio Lower Upper

154 100

153 113.8 89.5 134.3




152 54.6 42.7 64.1

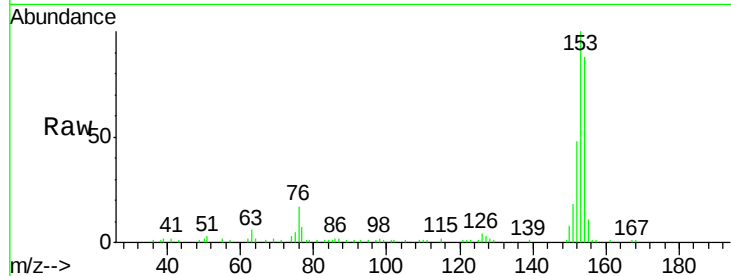

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

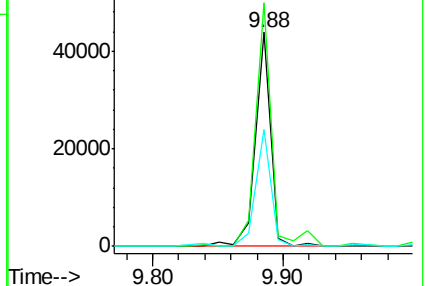

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.32 min Scan# 852

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31


Tgt Ion:188 Resp: 302001

Ion Ratio Lower Upper

188 100

94 14.1 9.0 13.6#



80 15.2 10.0 15.0#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

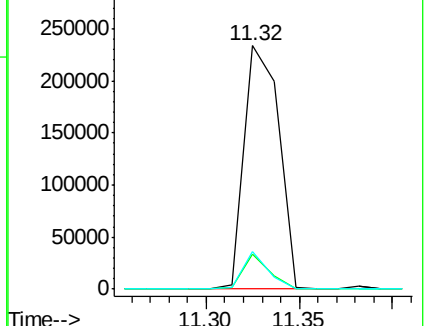

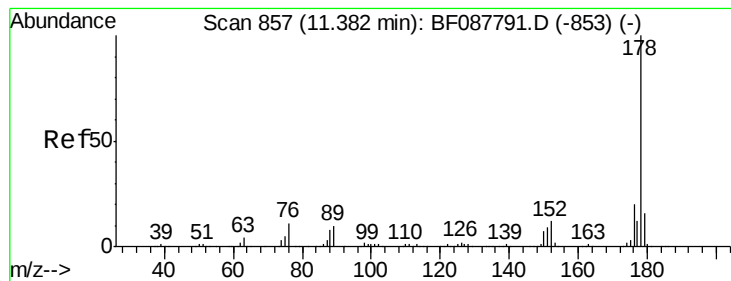

#70

Phenanthrene

Concen: 22.65 ng

RT: 11.36 min Scan# 855

Delta R.T. -0.02 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampleId :

SS-32


Tot Ion:178 Resp: 358945

Ion Ratio Lower Upper

178 100

176 18.6 15.8 23.6




179 15.0 13.0 19.4



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

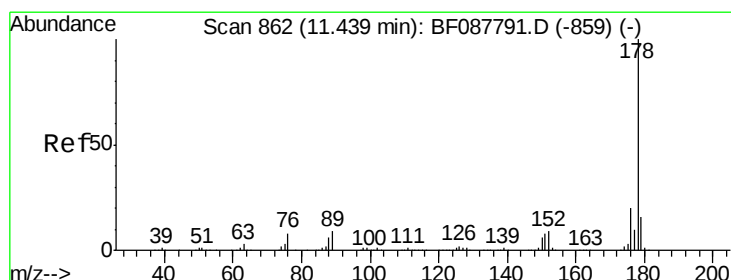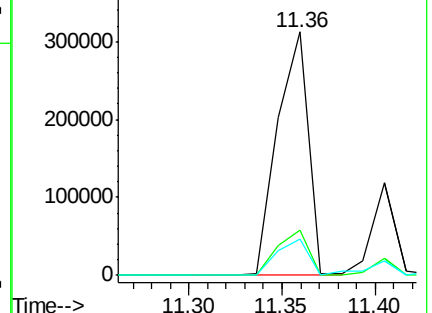

#71

Anthracene

Concen: 6.34 ng

RT: 11.40 min Scan# 859

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31


Tgt Ion:178 Resp: 101385

Ion Ratio Lower Upper

178 100

176 18.0 15.6 23.4



179 15.2 12.8 19.2

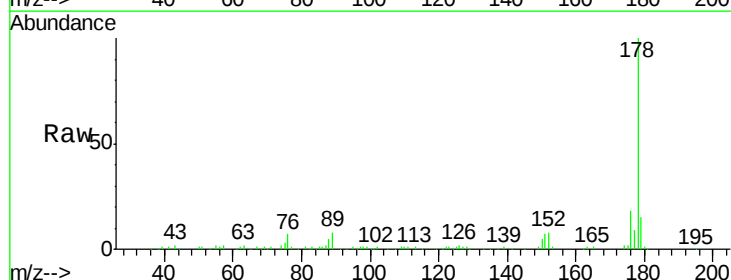


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

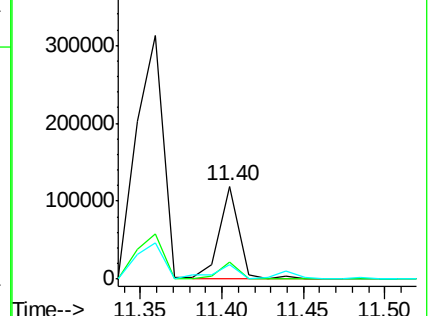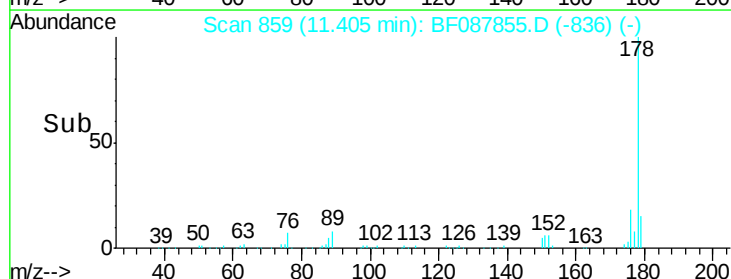







#72
 Carbazole
 Concen: 2.59 ng
 RT: 11.55 min Scan# 872
 Delta R.T. -0.03 min
 Lab File: BF087855.D
 Acq: 9 Jun 2016 16:31

Instrument :
 BNA_F
 ClientSampleId :
 SS-32

Tot Ion:167 Resp: 38751
 Ion Ratio Lower Upper
 167 100
 166 21.9 17.8 26.6
 139 14.8 11.2 16.8




Abundance Ion 167.00 (166.70 to 167.70): E
 Ion 166.00 (165.70 to 166.70): E
 Ion 139.00 (138.70 to 139.70): E


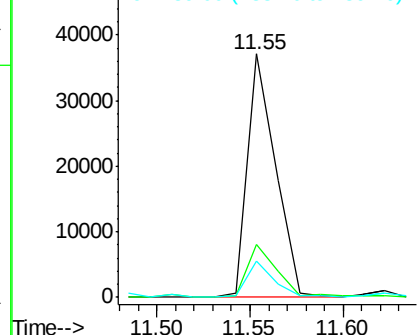



#73
 Di-n-butylphthalate
 Concen: 3.93 ng
 RT: 11.90 min Scan# 902
 Delta R.T. -0.03 min
 Lab File: BF087855.D
 Acq: 9 Jun 2016 16:31

Tgt Ion:149 Resp: 74501
 Ion Ratio Lower Upper
 149 100
 150 9.5 7.8 11.6
 104 4.5 4.0 6.0



Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 104.00 (103.70 to 104.70): E

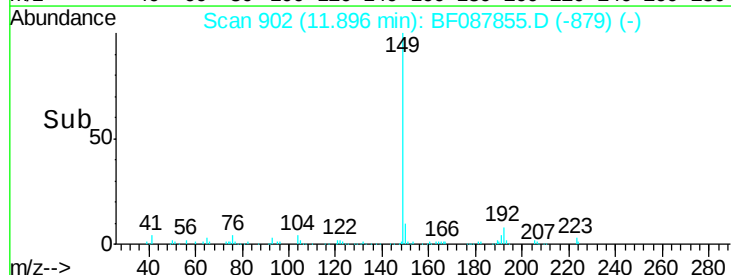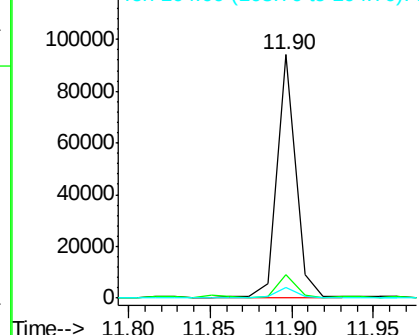

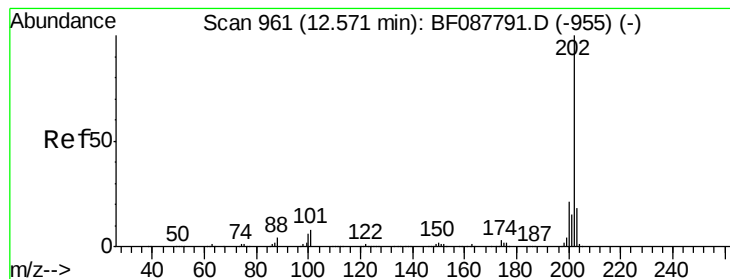

#74

Fluoranthene

Concen: 25.90 ng

RT: 12.54 min Scan# 958

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampleId :

SS-32


Tot Ion:202 Resp: 433109

Ion Ratio Lower Upper

202 100

101 12.0 0.0 33.1




203 17.6 0.0 38.1

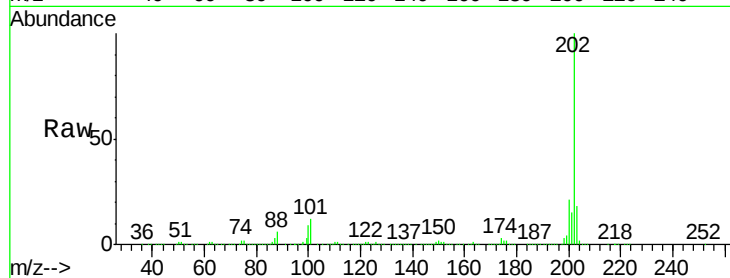

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

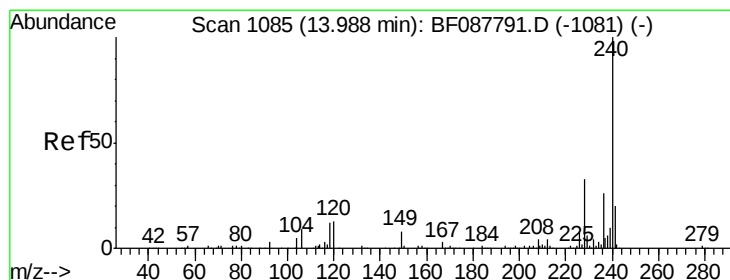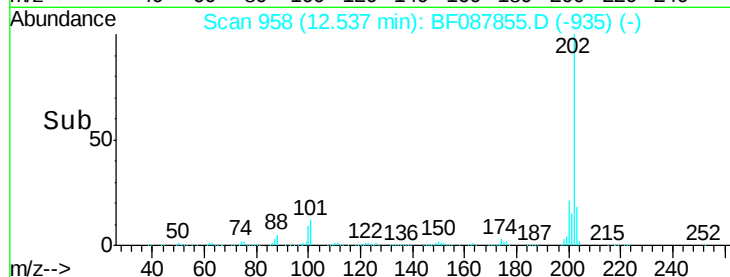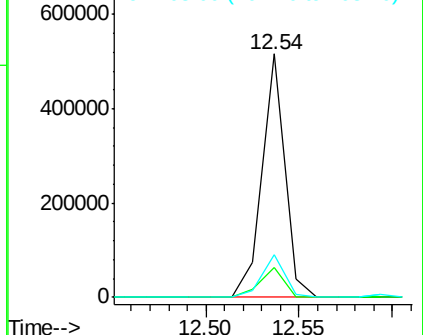

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.95 min Scan# 1082

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31


Tgt Ion:240 Resp: 233625

Ion Ratio Lower Upper

240 100

120 16.9 6.8 10.2#



236 25.2 20.2 30.2

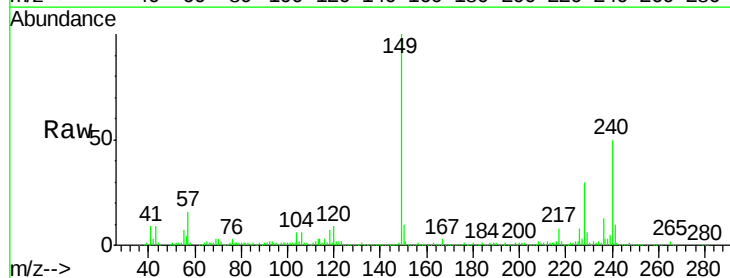


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

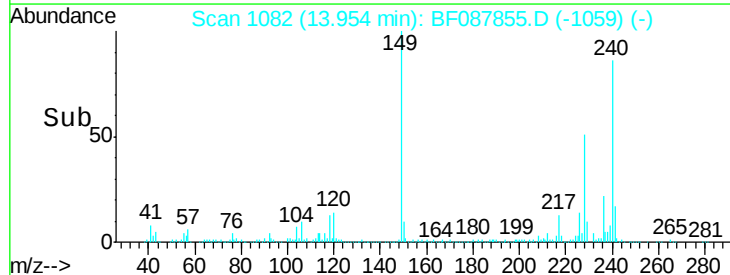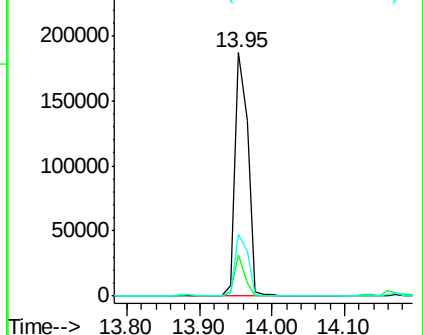

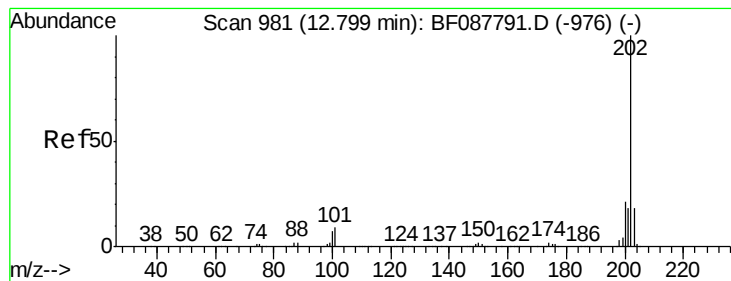

#77

Pvrene

Concen: 22.76 ng

RT: 12.77 min Scan# 978

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampled :

SS-32


Tot Ion:202 Resp: 394654

Ion Ratio Lower Upper

202 100

200 21.2 17.4 26.2




203 17.8 14.5 21.7



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

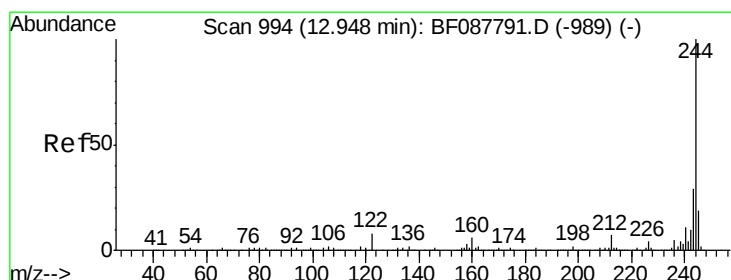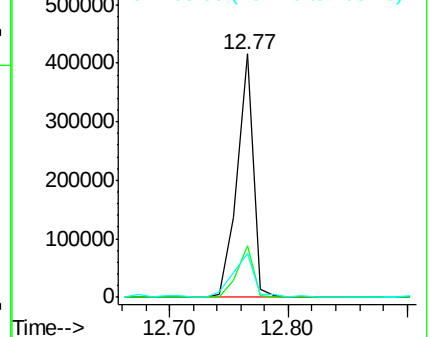

#78

Terphenyl-d14

Concen: 42.92 ng

RT: 12.91 min Scan# 991

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31


Tgt Ion:244 Resp: 440685

Ion Ratio Lower Upper

244 100

212 6.6 6.0 9.0



122 9.6 11.2 16.8#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

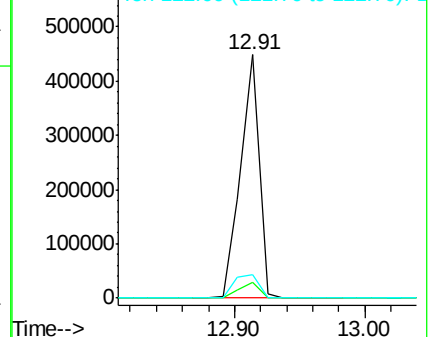

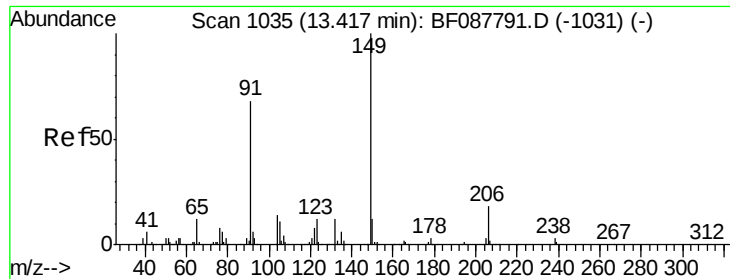

#79

Butylbenzylphthalate

Concen: 288.96 ng

RT: 13.42 min Scan# 1035

Delta R.T. -0.00 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampleId :

SS-32


Tot Ion:149 Resp: 2214773

Ion Ratio Lower Upper

149 100

91 62.9 48.0 72.0




206 21.1 16.0 24.0

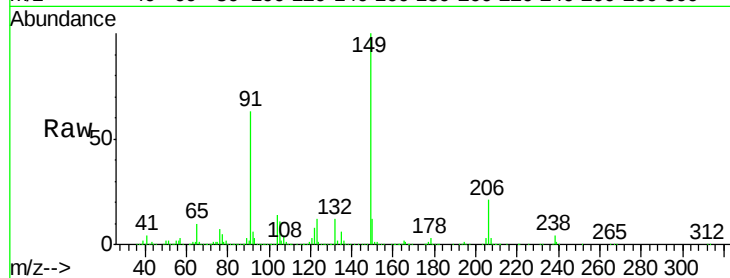

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BF0

Ion 206.00 (205.70 to 206.70): E

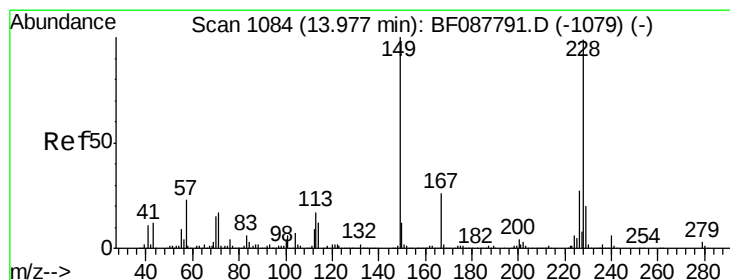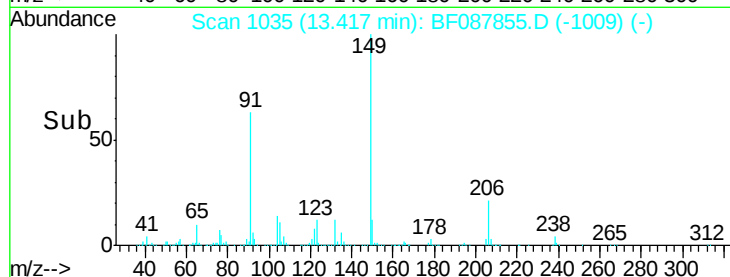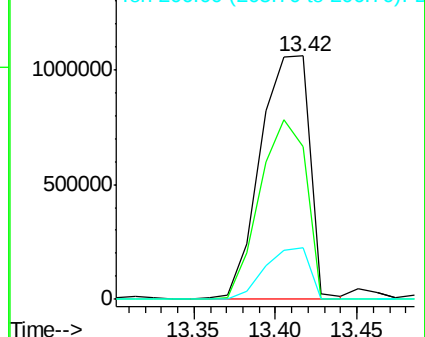

#80

Benzo(a)anthracene

Concen: 14.86 ng

RT: 13.94 min Scan# 1081

Delta R.T. -0.03 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31


Tgt Ion:228 Resp: 197798

Ion Ratio Lower Upper

228 100

226 28.3 22.3 33.5



229 21.2 16.0 24.0

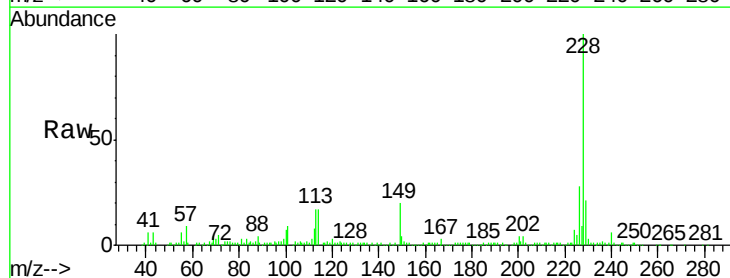


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

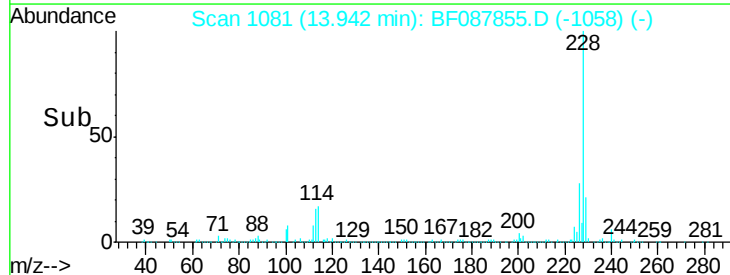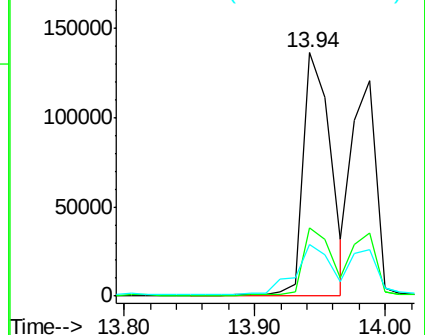



#82

Chrysene

Concen: 12.28 ng

RT: 13.99 min Scan# 1085

Delta R.T. -0.02 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31

Instrument :

BNA_F

ClientSampleId :

SS-32


Tot Ion:228 Resp: 153748

Ion Ratio Lower Upper

228 100

226 29.5 25.4 38.2




229 21.7 16.3 24.5



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

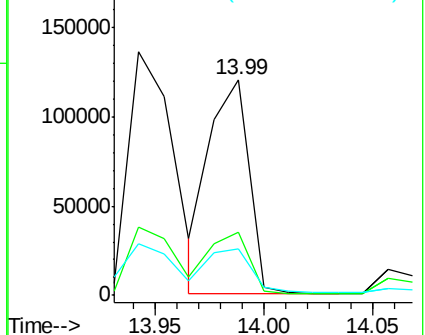

#83

Bis(2-ethylhexyl)phthalate

Concen: 51.66 ng

RT: 13.95 min Scan# 1082

Delta R.T. -0.02 min

Lab File: BF087855.D

Acq: 9 Jun 2016 16:31


Tgt Ion:149 Resp: 482048

Ion Ratio Lower Upper

149 100

167 2.6 20.5 30.7#



279 0.3 2.0 3.0#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

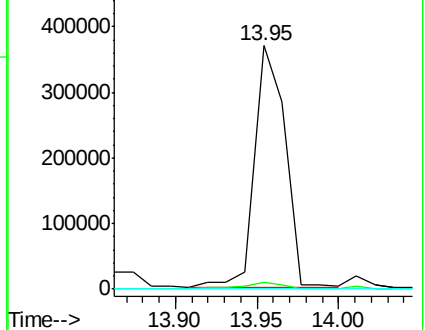







#84
Di-n-octyl phthalate
Concen: 56.58 ng
RT: 14.56 min Scan# 1135
Delta R.T. -0.02 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Instrument :
BNA_F
ClientSampled :
SS-32

Tot Ion	Ratio	Lower	Upper
149	100		
167	2.2	0.0	0.0#
43	9.1	0.0	0.0#

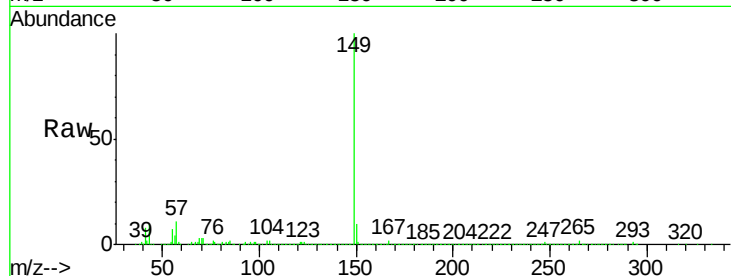


Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 43.00 (42.70 to 43.70): BF0


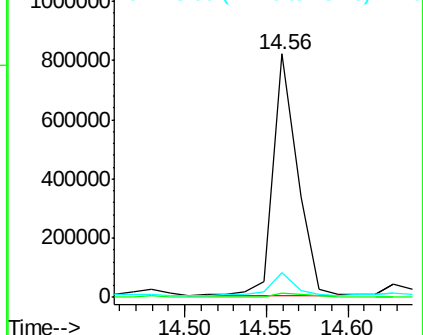



#85
Indeno(1,2,3-cd)pyrene
Concen: 6.74 ng
RT: 16.72 min Scan# 1324
Delta R.T. -0.07 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Tgt Ion	Ratio	Lower	Upper
276	100		
138	28.0	0.0	0.0#
277	30.3	0.0	0.0#



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E




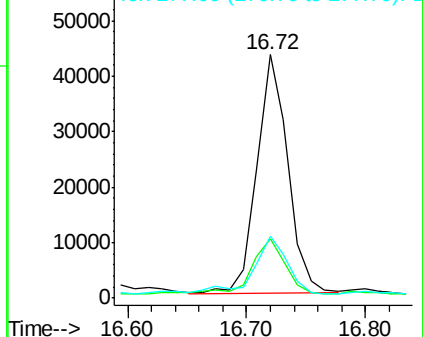


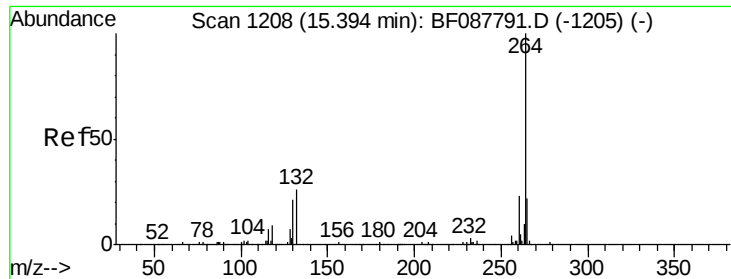

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.37 min Scan# 1206
Delta R.T. -0.02 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31




Instrument :
BNA_F
ClientSampleId :
SS-32


Tot Ion:264 Resp: 233485
Ion Ratio Lower Upper
264 100
260 23.6 19.2 28.8
265 22.1 16.9 25.3

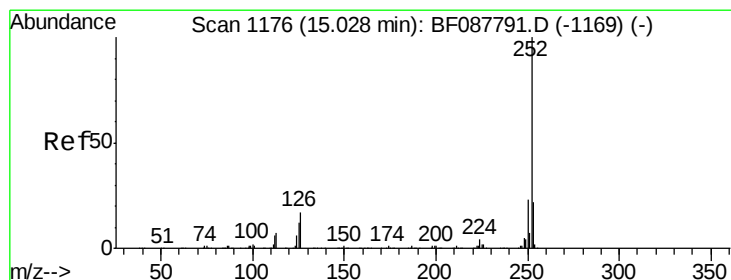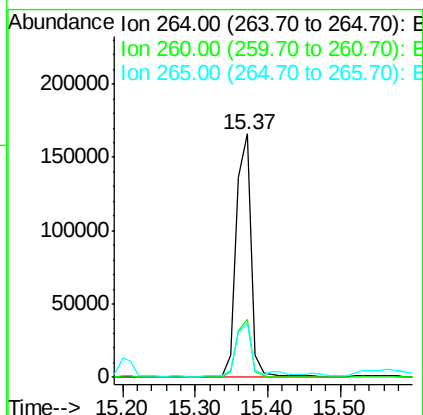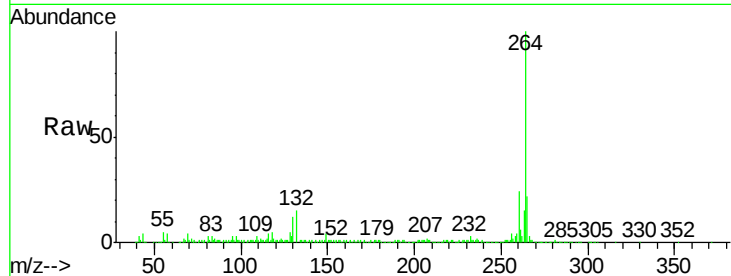

#87
Benzo(b)fluoranthene
Concen: 14.16 ng m
RT: 14.97 min Scan# 1171
Delta R.T. -0.02 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Tgt Ion:252 Resp: 230418
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.2
125 14.3 7.1 10.7#

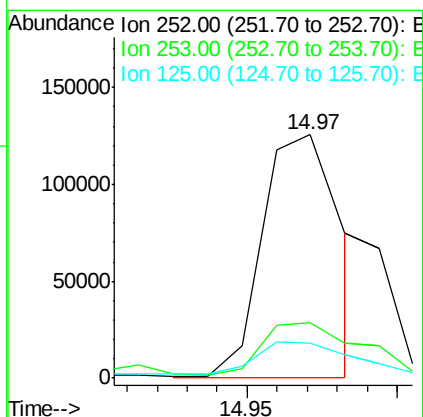


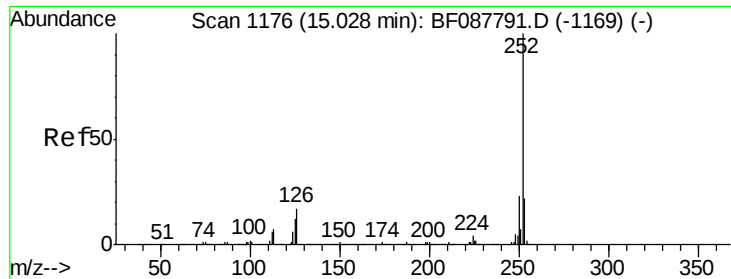




#88
Benzo(k)fluoranthene
Concen: 4.31 ng m
RT: 14.98 min Scan# 1172
Delta R.T. -0.05 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Instrument :
BNA_F
ClientSampleId :
SS-32

Tot Ion:252 Resp: 52920
Ion Ratio Lower Upper
252 100
253 24.1 18.0 27.0
125 16.1 11.2 16.8

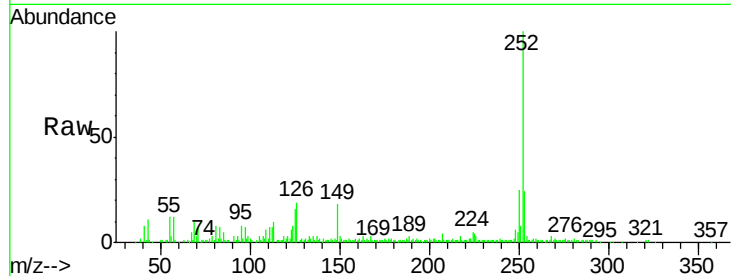


Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E


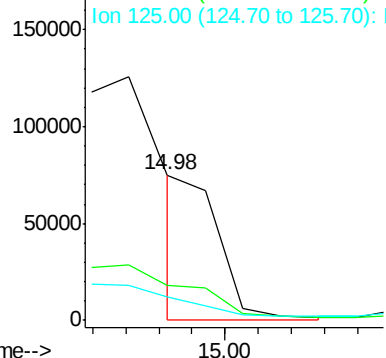



#89
Benzo(a)pyrene
Concen: 10.98 ng
RT: 15.30 min Scan# 1200
Delta R.T. -0.05 min
Lab File: BF087855.D
Acq: 9 Jun 2016 16:31

Tgt Ion:252 Resp: 144556
Ion Ratio Lower Upper
252 100
253 24.1 17.9 26.9
125 16.8 12.5 18.7



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

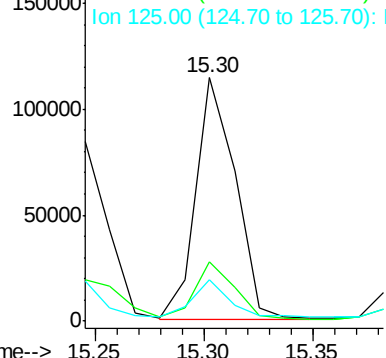

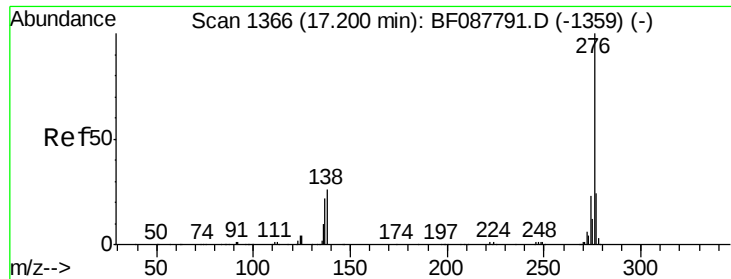

#91
 Benzo(a,h,i)perylene
 Concen: 5.80 ng
 RT: 17.13 min Scan# 1360
 Delta R.T. -0.07 min
 Lab File: BF087855.D
 Acq: 9 Jun 2016 16:31

Instrument :
 BNA_F
 ClientSampleId :
 SS-32

Tot Ion	Ratio	Lower	Upper
276	100		
277	24.6	18.9	28.3
138	23.7	21.4	32.2

