


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060917\
 Data File : BF095812.D
 Acq On : 9 Jun 2017 10:04
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

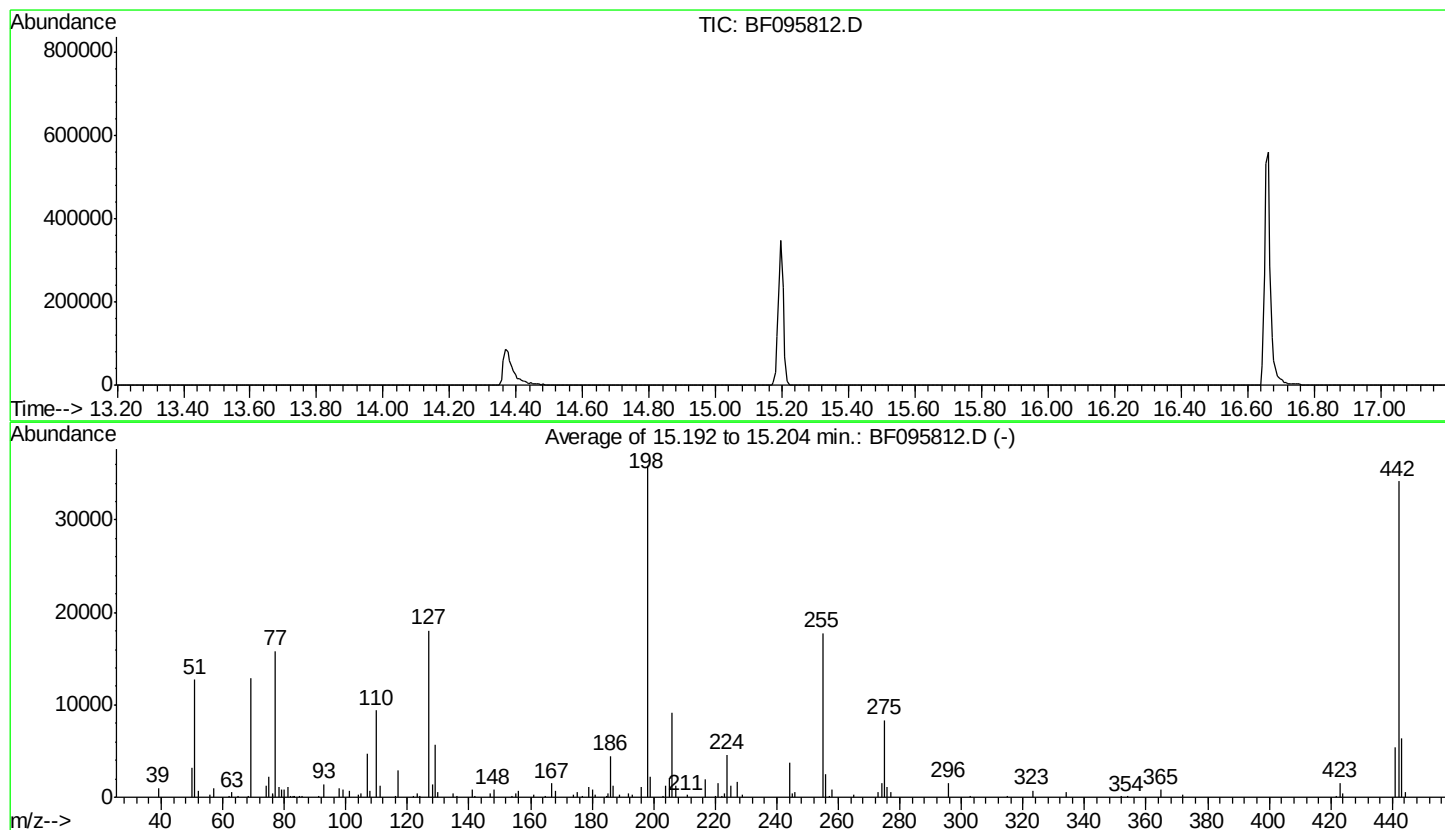

AutoFind: Scans 2313, 2314, 2315; Background Corrected with Scan 2306

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	12729	PASS
68	69	0.00	2	0.8	106	PASS
69	198	0.00	100	36.0	12920	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	18042	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35888	PASS
199	198	5	9	6.3	2264	PASS
275	198	10	60	23.2	8330	PASS
365	198	1	100	2.3	821	PASS
441	442	0.01	24	15.6	5347	PASS
442	198	50	100	95.2	34170	PASS
443	442	15	24	18.7	6381	PASS