
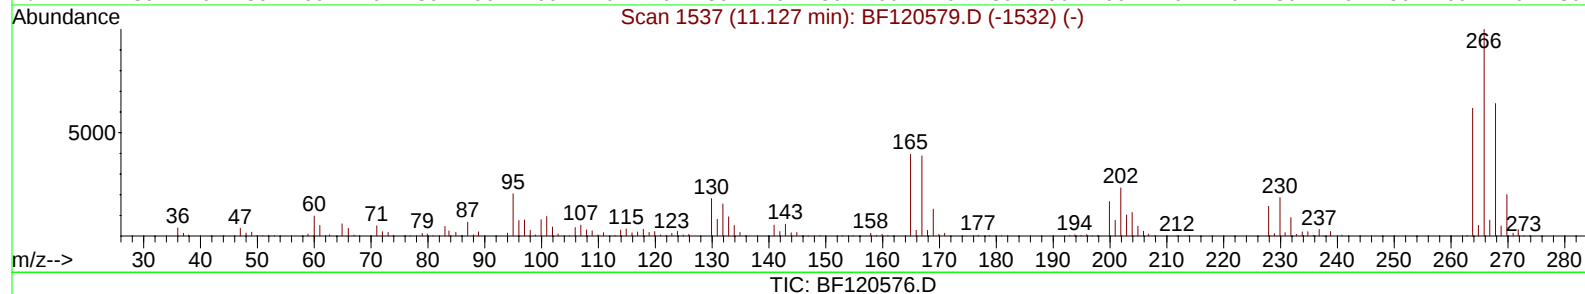
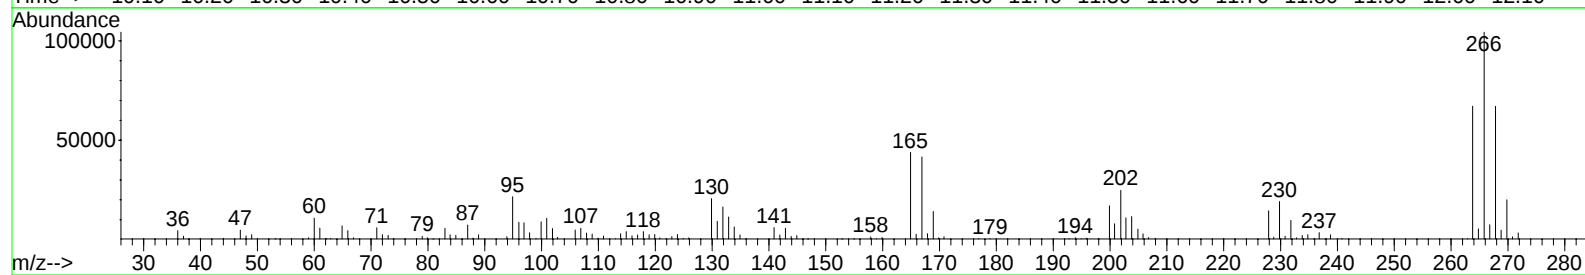


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060920\  
Data File : BF120576.D  
Acq On : 9 Jun 2020 11:49  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 18:42:44 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF060920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 09 18:08:31 2020  
Response via : Initial Calibration

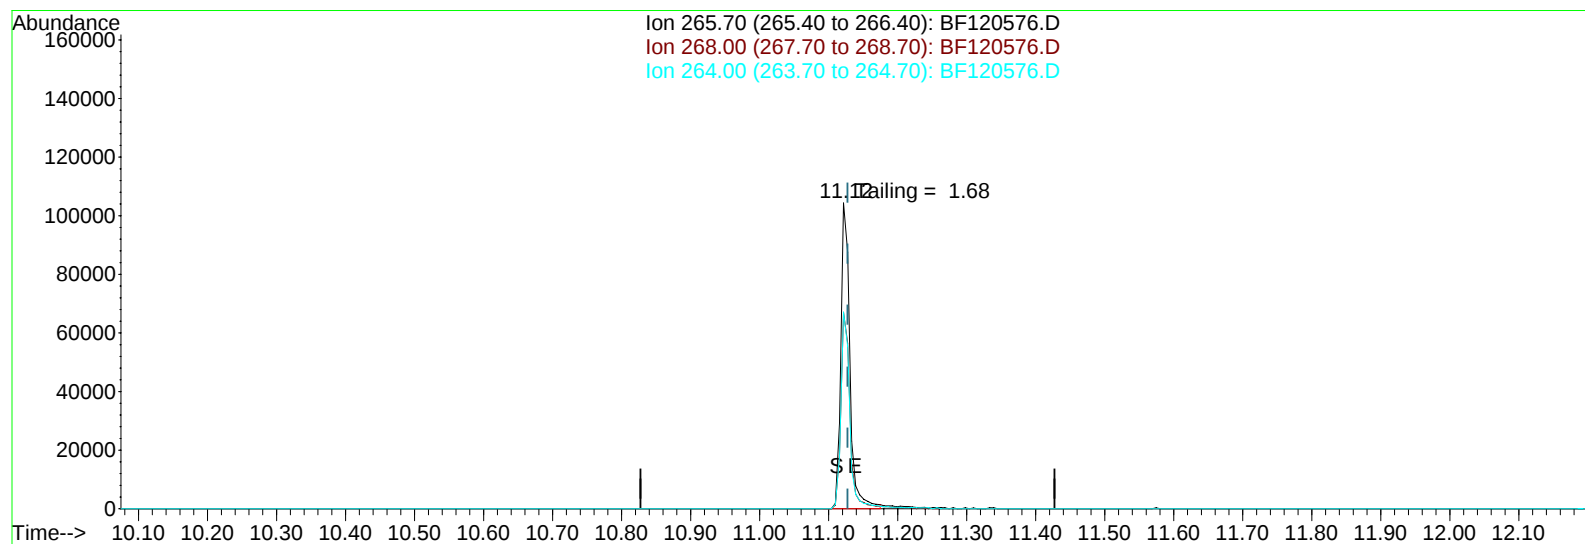

(70) Pentachlorophenol (C)




11.122min (-0.006) 40610.71ng

response 96224

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.10 | 64.28 |
| 264.00 | 61.80 | 64.34 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060920\  
 Data File : BF120576.D  
 Acq On : 9 Jun 2020 11:49  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 18:42:44 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF060920.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 09 18:08:31 2020  
 Response via : Initial Calibration

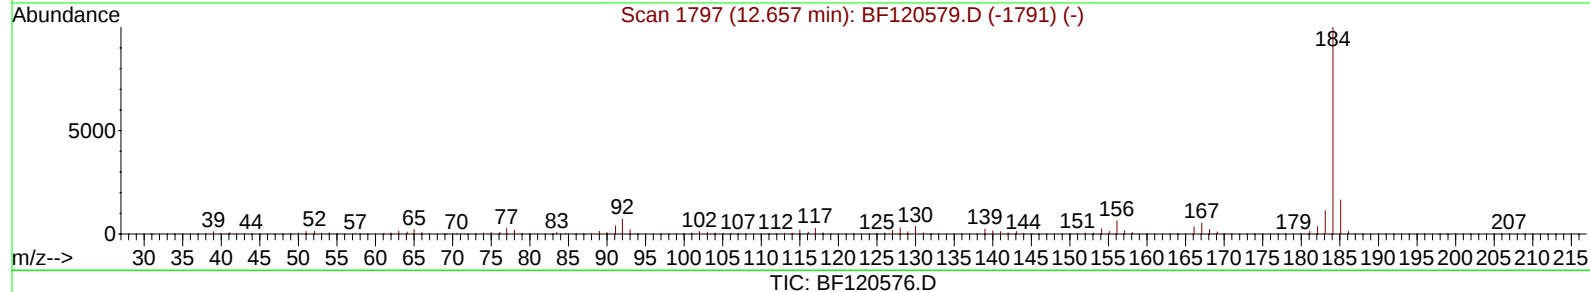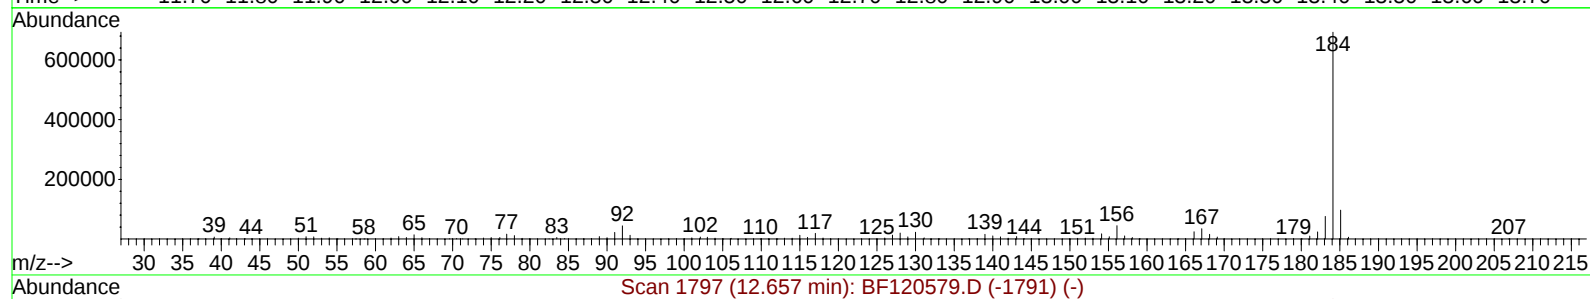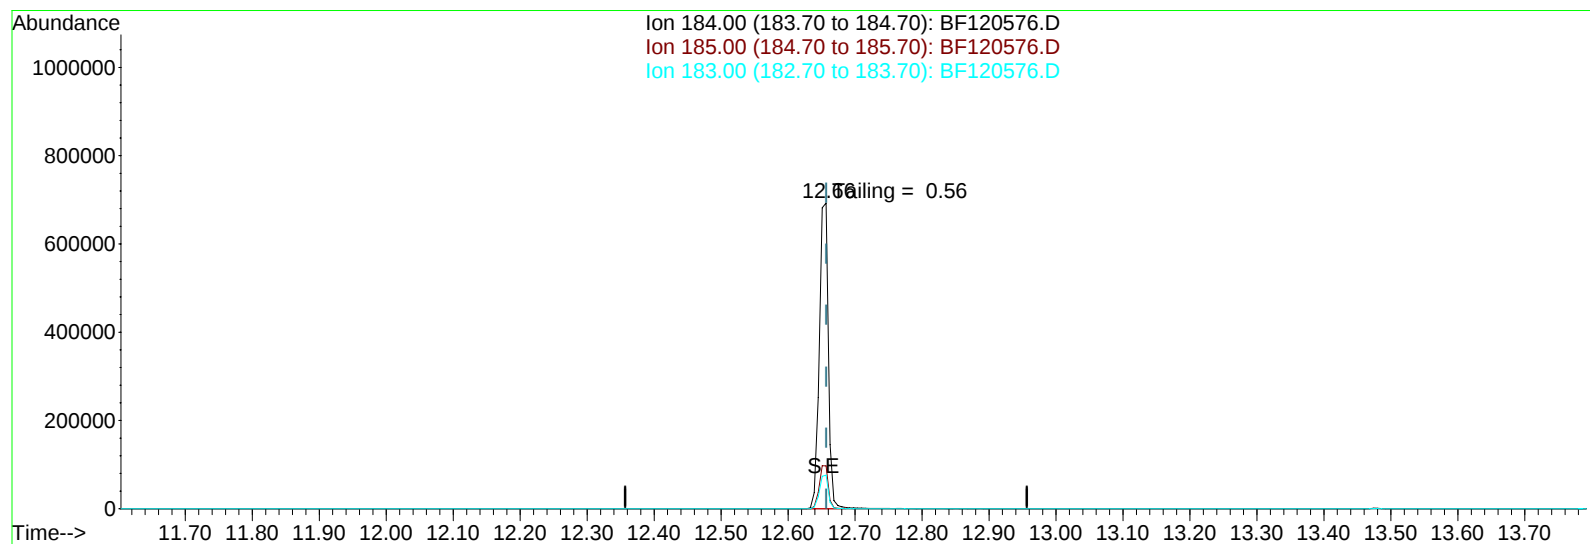

(77) Benzidine

12.657min (+0.000) 0.00ng

response 656348

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.50 | 14.01 |
| 183.00 | 11.30 | 10.98 |
| 0.00   | 0.00  | 0.00  |