


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060920\
 Data File : BF120576.D
 Acq On : 9 Jun 2020 11:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 18:08:31 2020

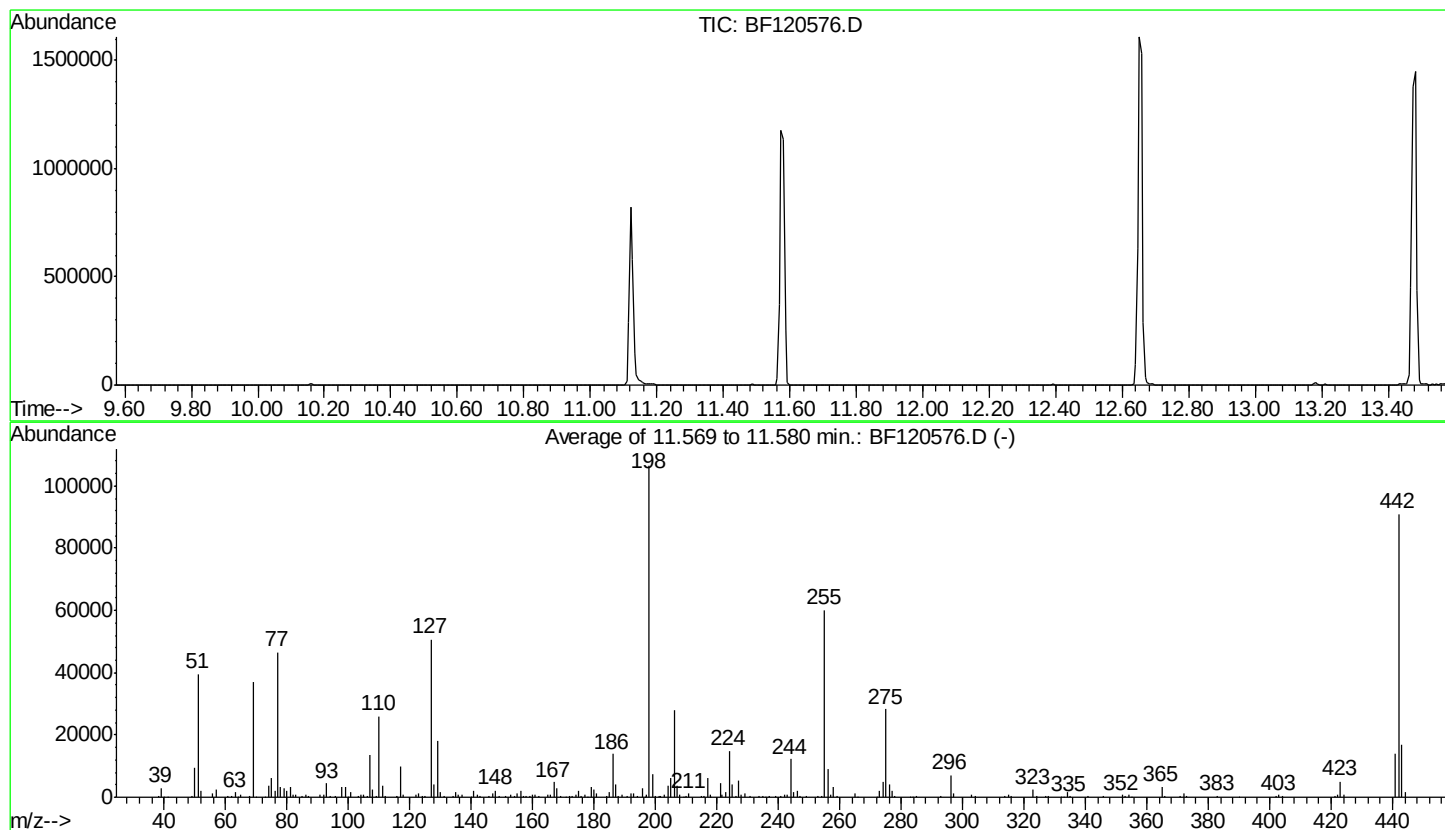

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	39690	PASS
68	69	0.00	2	1.2	445	PASS
69	198	0.00	100	34.8	37048	PASS
70	69	0.00	2	0.4	130	PASS
127	198	10	80	47.6	50698	PASS
197	198	0.00	2	0.6	665	PASS
198	198	100	100	100.0	106528	PASS
199	198	5	9	6.8	7244	PASS
275	198	10	60	26.5	28277	PASS
365	198	1	100	3.2	3364	PASS
441	198	0.01	100	13.3	14190	PASS
442	198	50	100	85.5	91049	PASS
443	442	15	24	18.4	16733	PASS