
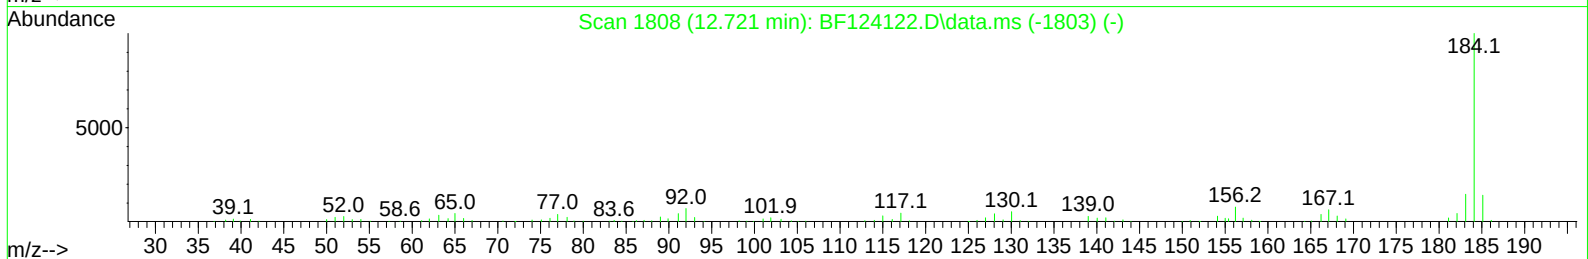
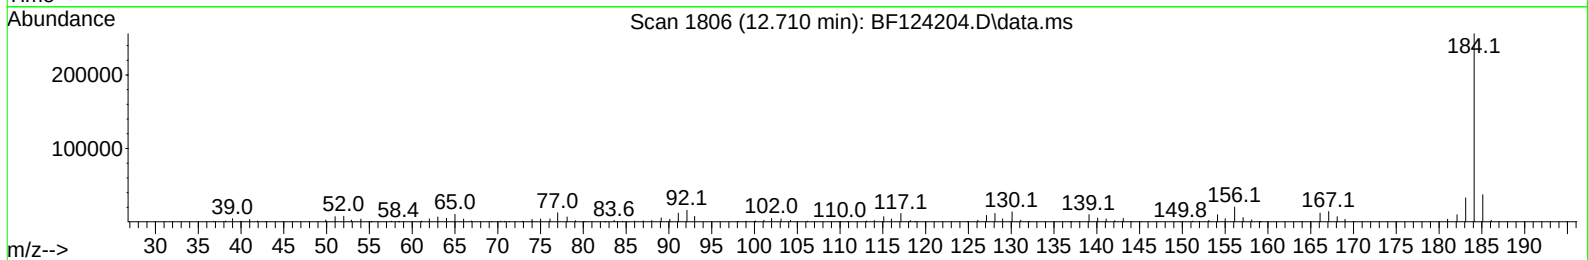


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060921\
 Data File : BF124204.D
 Acq On : 9 Jun 2021 11:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:29:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 07 13:32:21 2021
 Response via : Initial Calibration

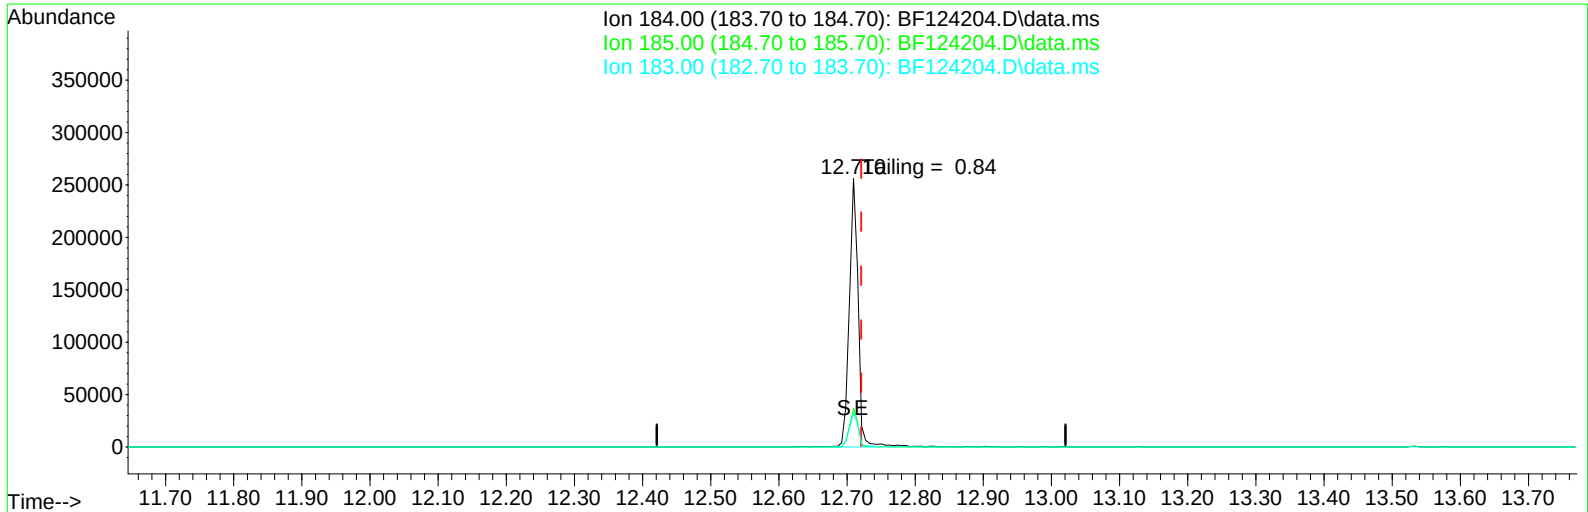

TIC: BF124204.D\data.ms

(77) Benzidine




12.710min (-0.011) 0.00 ng

response 232034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.46
183.00	9.80	12.77#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060921\
Data File : BF124204.D
Acq On : 9 Jun 2021 11:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:29:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 07 13:32:21 2021
Response via : Initial Calibration

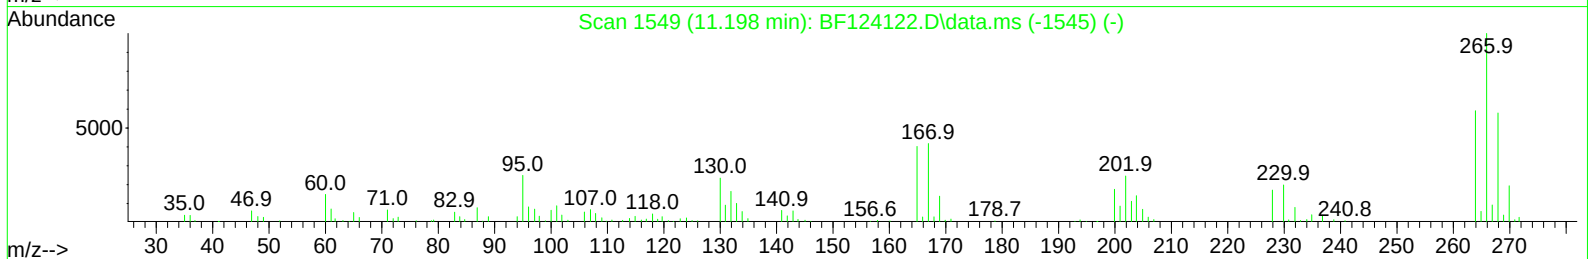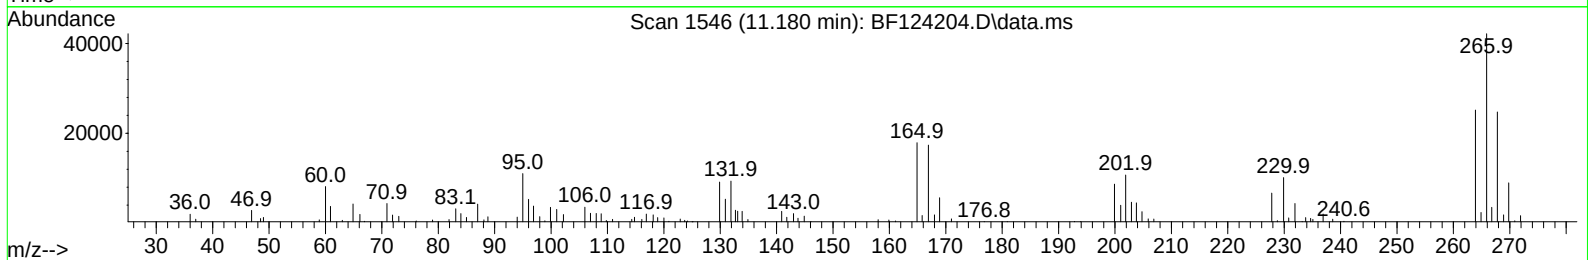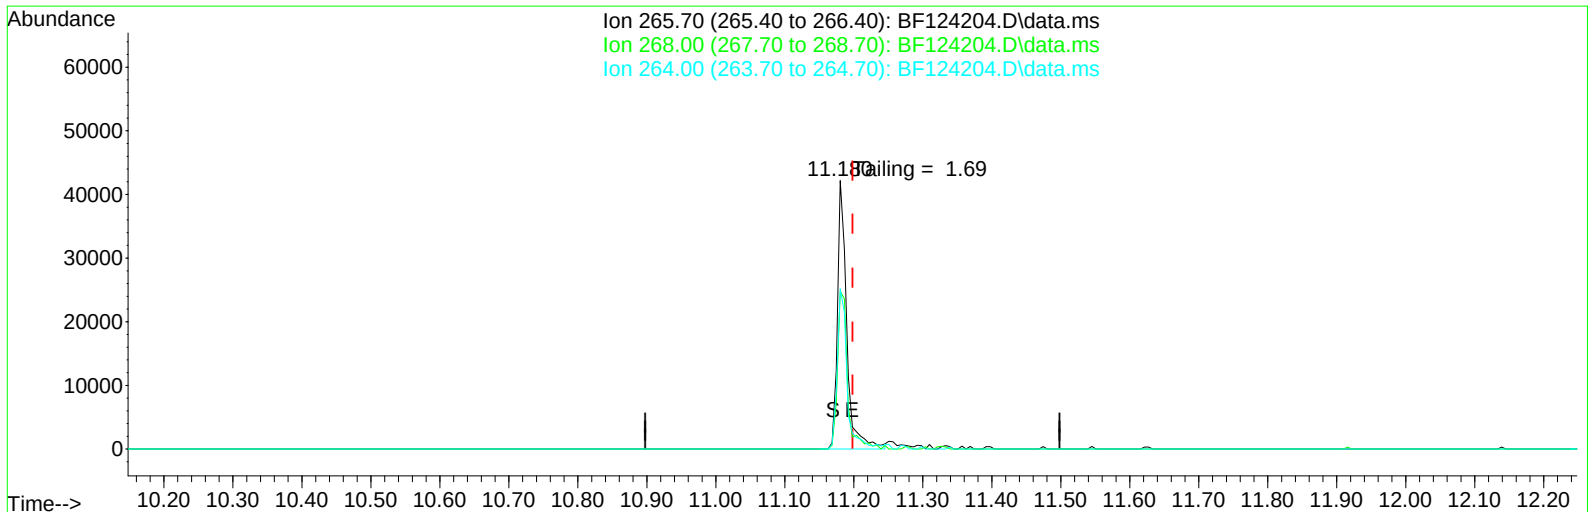

TIC: BF124204.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.018) 18127.15 ng

response 39257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.71
264.00	65.70	59.67
0.00	0.00	0.00