
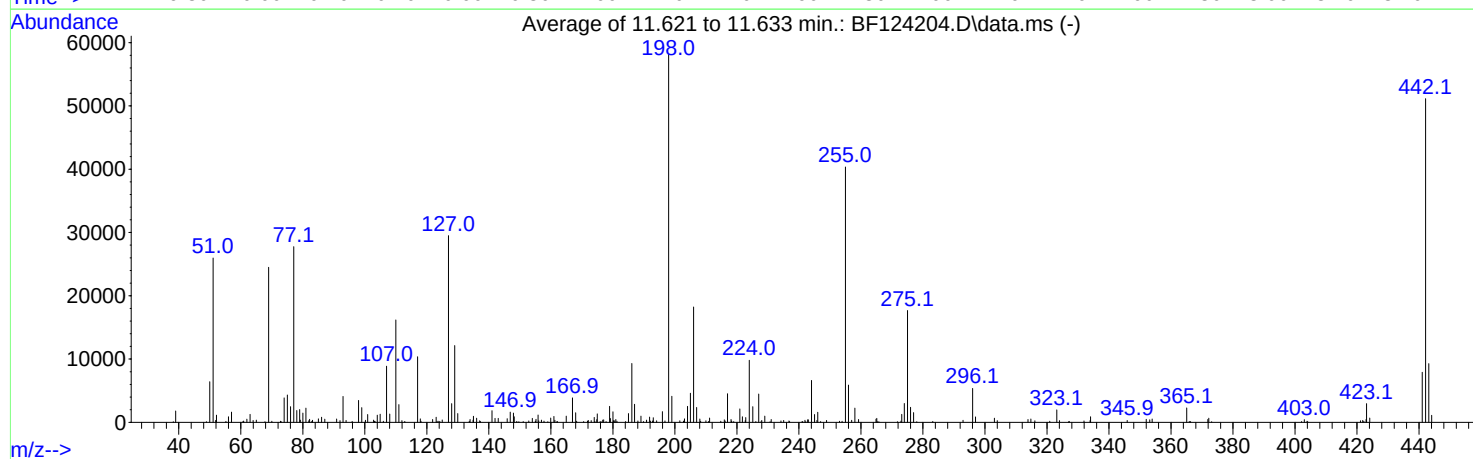


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060921\
 Data File : BF124204.D
 Acq On : 9 Jun 2021 11:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 10 01:53:56 2021

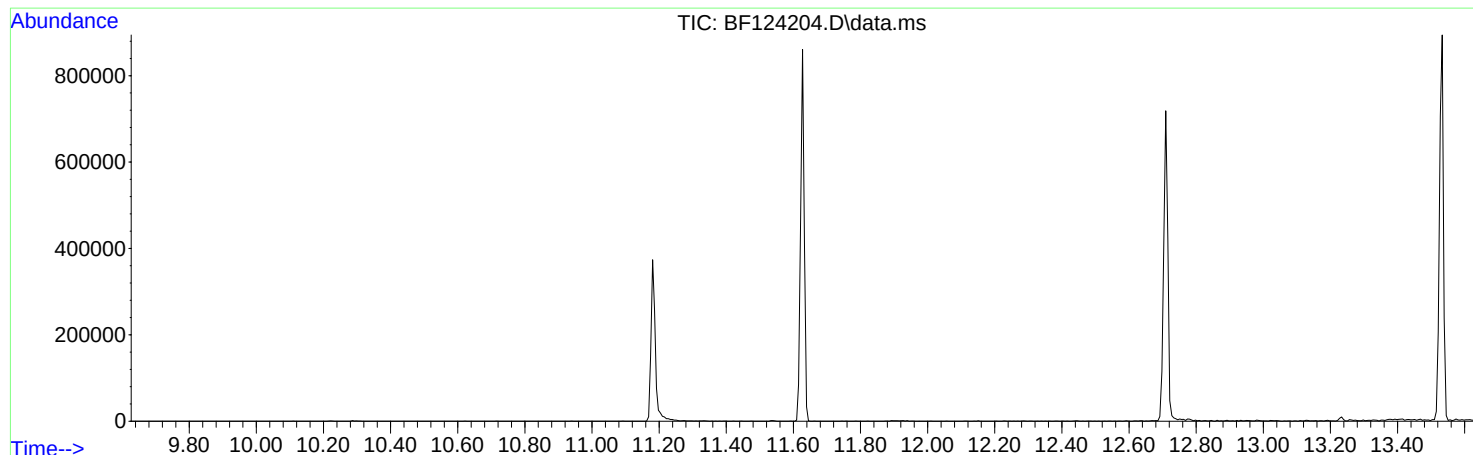




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	25975	PASS
68	69	0.00	2	0.5	115	PASS
69	198	0.00	100	42.2	24503	PASS
70	69	0.00	2	0.7	183	PASS
127	198	10	80	50.7	29490	PASS
197	198	0.00	2	0.4	226	PASS
198	198	100	100	100.0	58120	PASS
199	198	5	9	7.1	4119	PASS
275	198	10	60	30.4	17676	PASS
365	198	1	100	3.9	2267	PASS
441	198	0.01	100	13.6	7921	PASS
442	442	50	100	100.0	51136	PASS
443	442	15	24	18.2	9283	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060921\
 Data File : BF124204.D
 Acq On : 9 Jun 2021 11:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 14:29:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 07 13:32:21 2021
 Response via : Initial Calibration

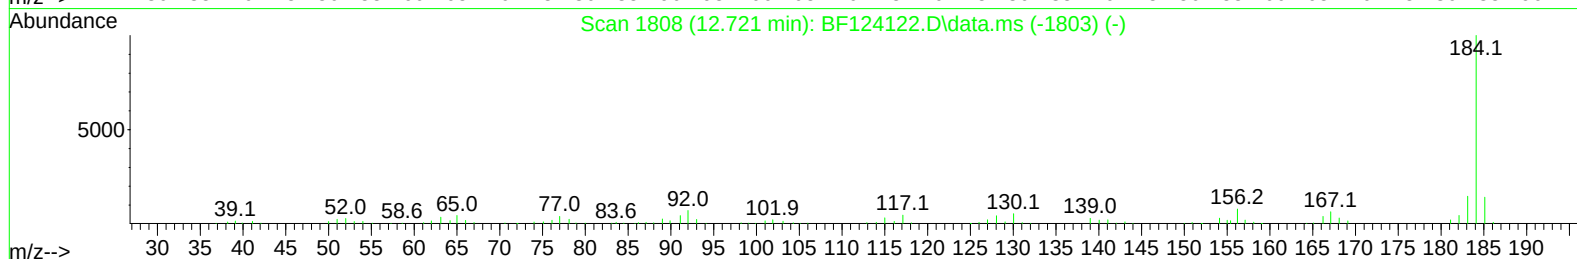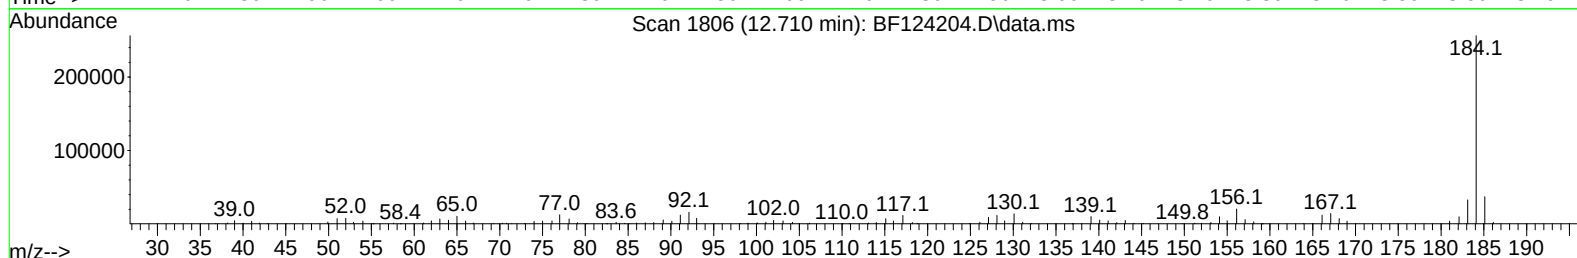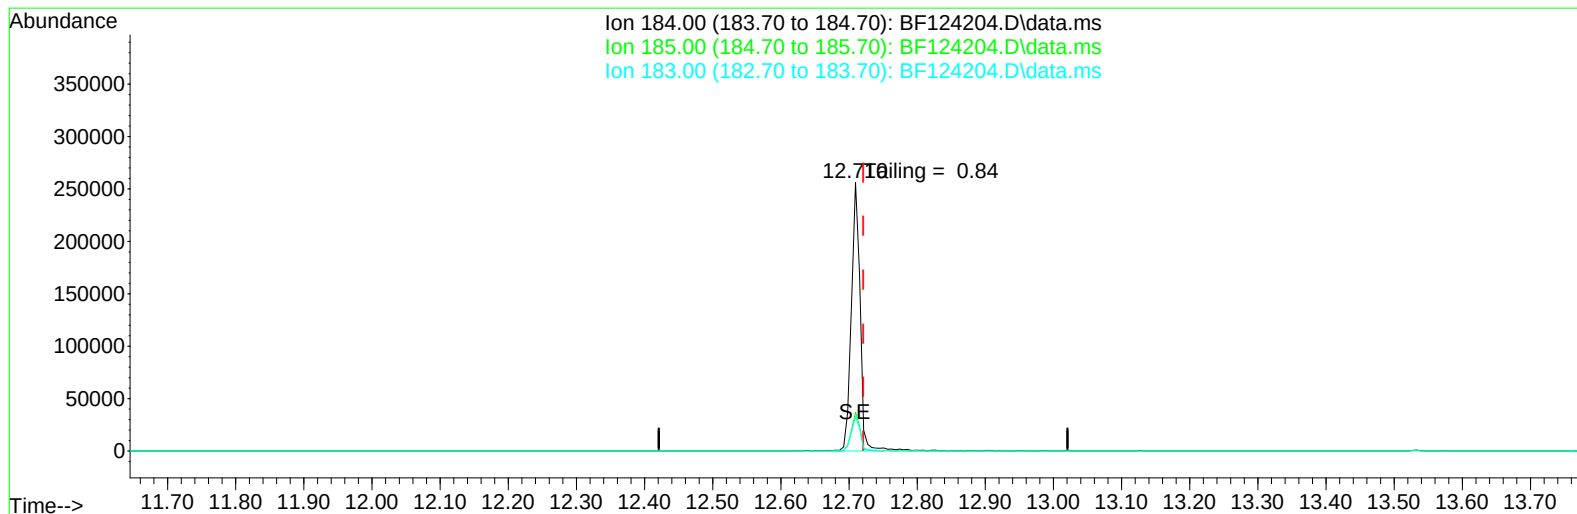

TIC: BF124204.D\data.ms

(77) Benzidine

12.710min (-0.011) 0.00 ng




response 232034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.46
183.00	9.80	12.77#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060921\
Data File : BF124204.D
Acq On : 9 Jun 2021 11:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 09 14:29:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 07 13:32:21 2021
Response via : Initial Calibration

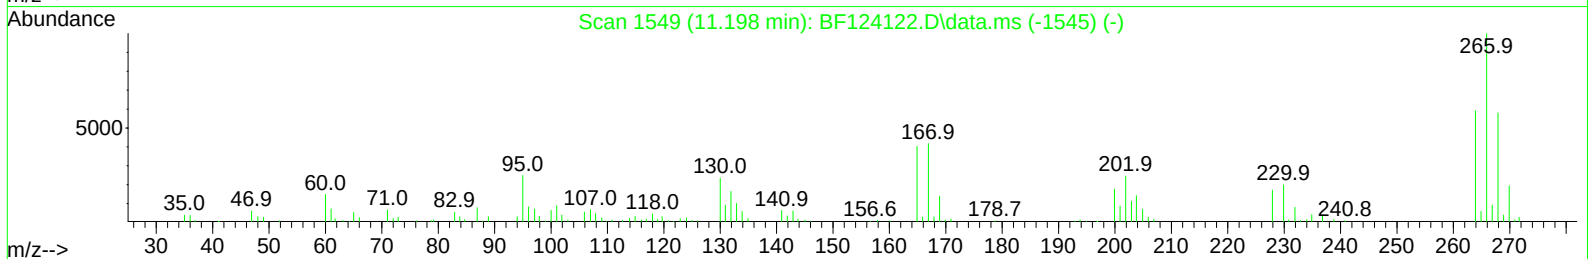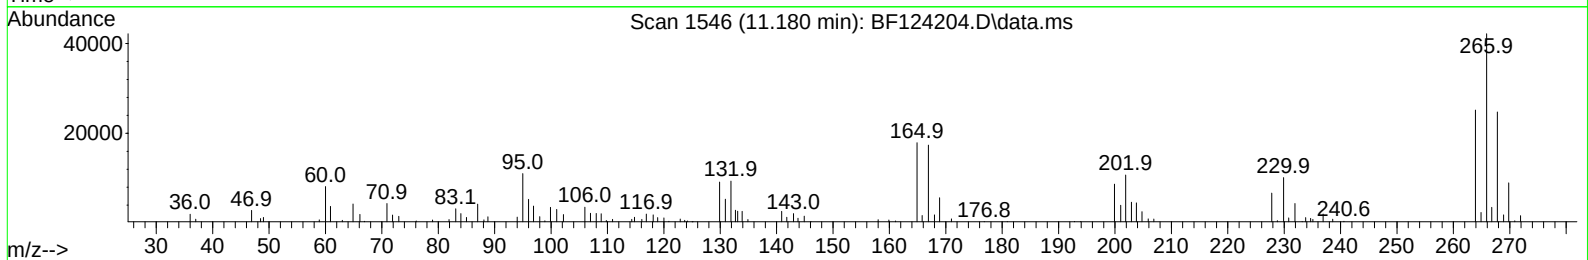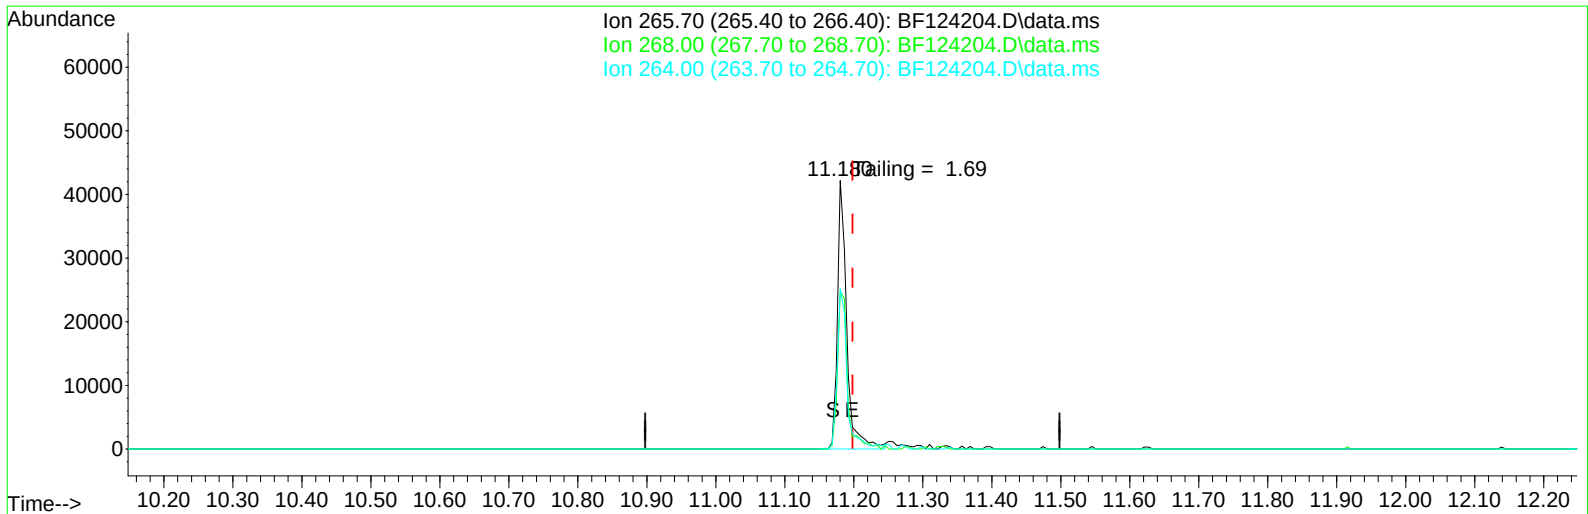

TIC: BF124204.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.018) 18127.15 ng

response 39257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.71
264.00	65.70	59.67
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/9/2021	BNA_F	<u>BF124204.D</u>
Compound Name	Response	Retention Time
DDT	129571	13.53
DDD	1932	13.22
DDE	223	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2155	131726	1.64