
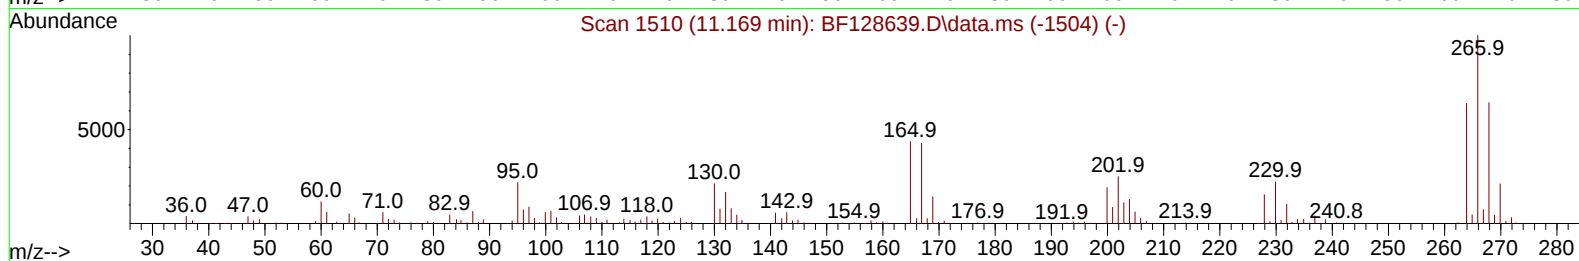
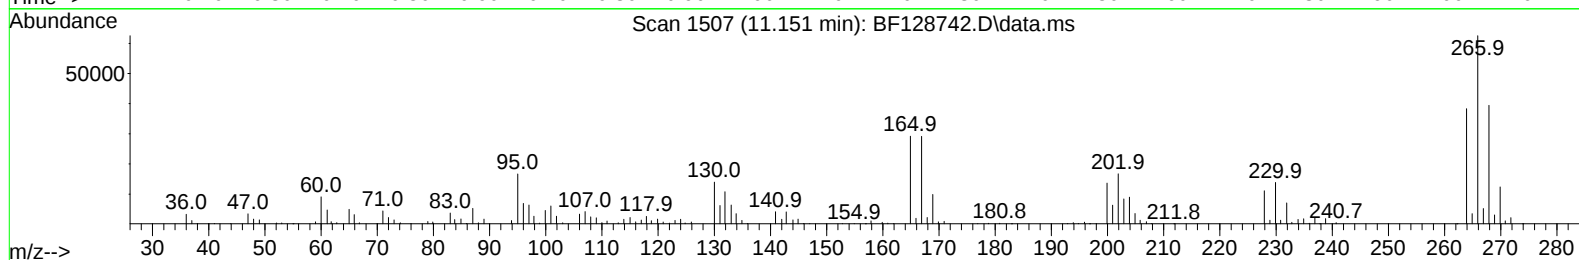


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
Data File : BF128742.D
Acq On : 09 Jun 2022 10:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 04:42:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 08 14:28:39 2022
Response via : Initial Calibration

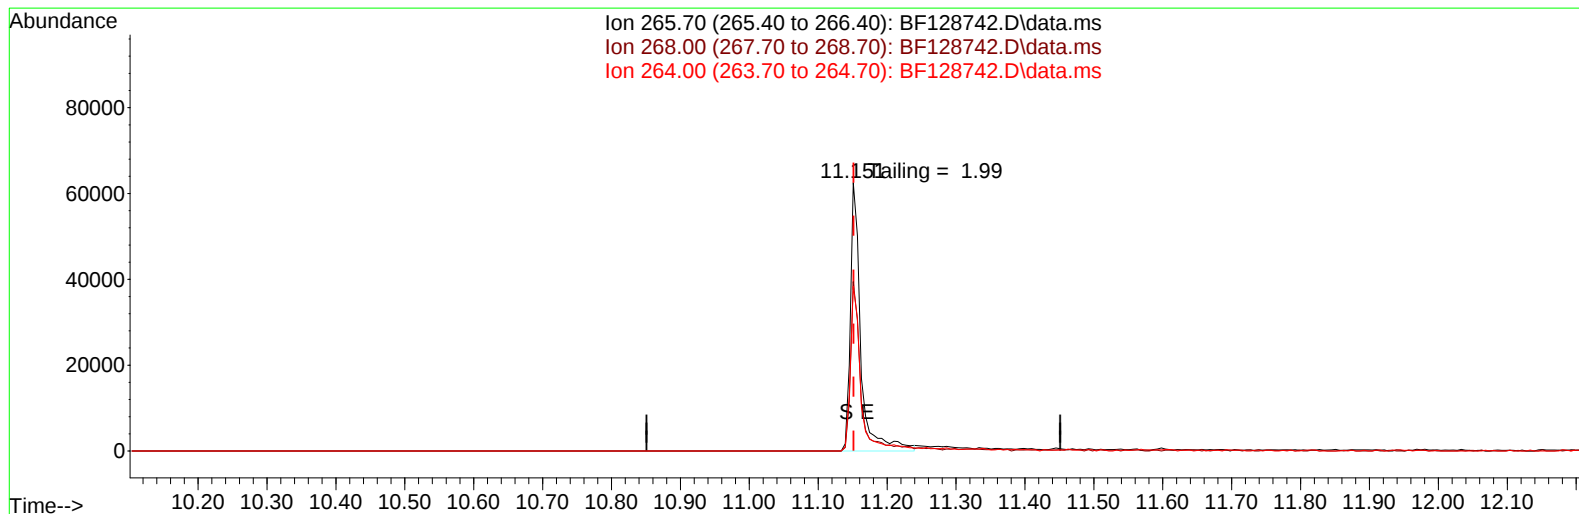

TIC: BF128742.D\data.ms

(70) Pentachlorophenol (C)




11.151min (-0.000) 13297.83 ng

response 62562

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.08
264.00	61.80	61.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
Data File : BF128742.D
Acq On : 09 Jun 2022 10:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 04:42:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 08 14:28:39 2022
Response via : Initial Calibration

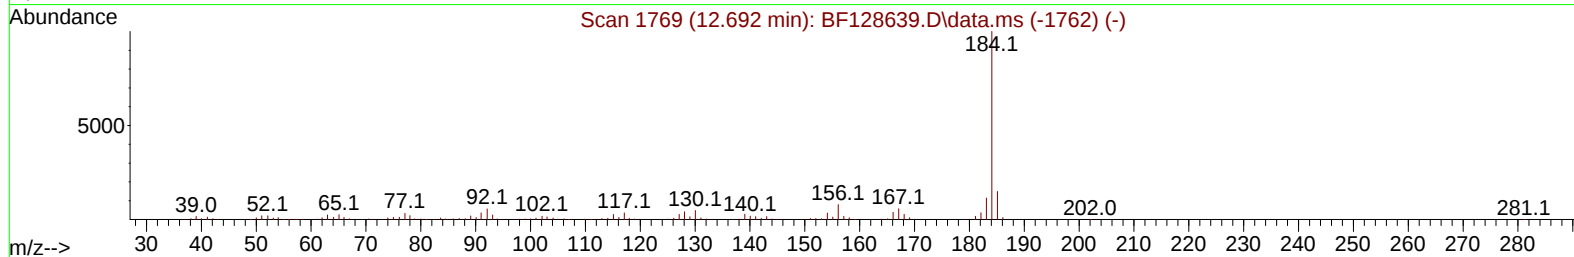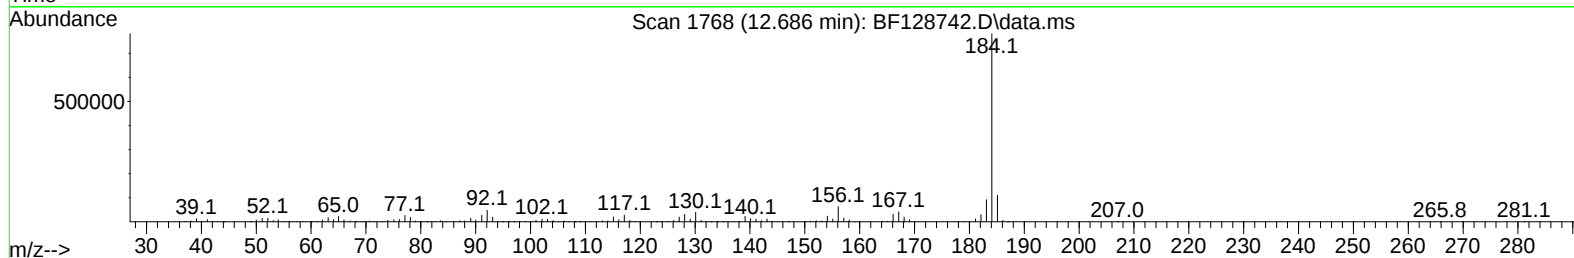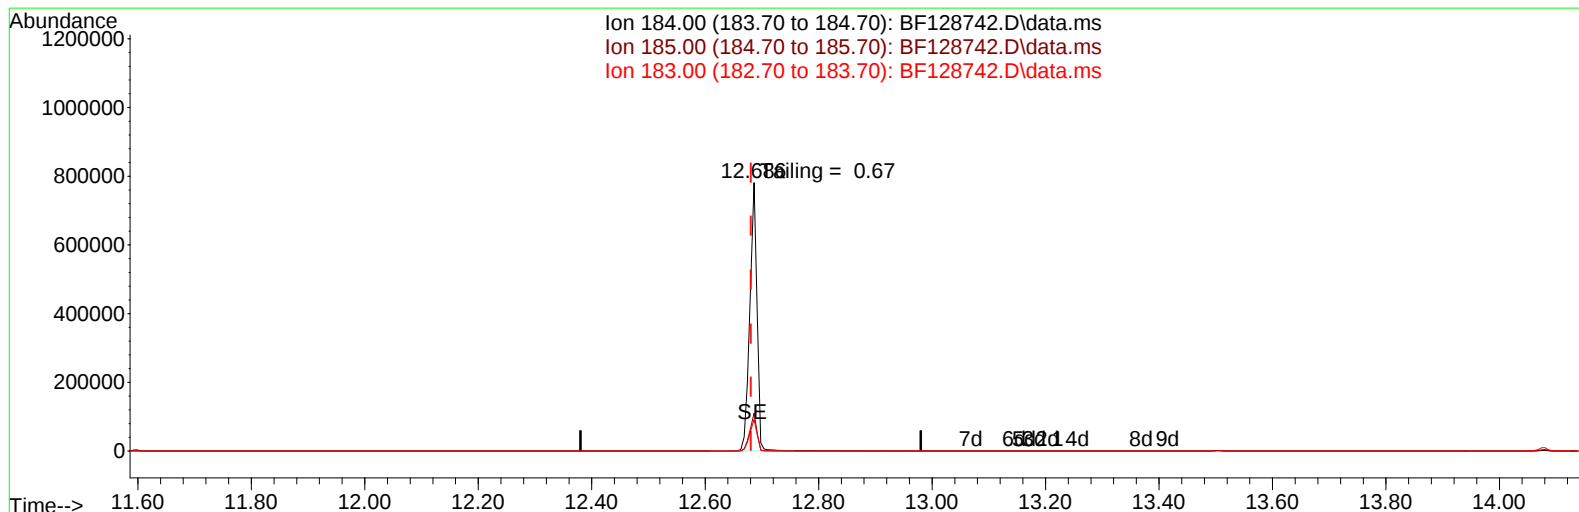

TIC: BF128742.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 611668.21 ng m

response 695017

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.18
183.00	11.60	11.77
0.00	0.00	0.00