

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
 Data File : BF128744.D
 Acq On : 09 Jun 2022 11:22
 Operator : CG\JU
 Sample : PB145411BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145411BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	537	541	553	rBV	3197478	3000648	73.90%	12.746%
2	6.475	707	712	715	rBV	2972022	2987200	73.57%	12.689%
3	6.810	765	769	772	rBV	784933	627977	15.47%	2.667%
4	7.381	859	866	869	rBV	1826391	2065341	50.87%	8.773%
5	8.092	981	987	991	rBV	801744	806591	19.87%	3.426%
6	9.175	1164	1171	1174	rBV	3754715	3875035	95.44%	16.460%
7	9.851	1280	1286	1289	rBV	1106605	936617	23.07%	3.978%
8	10.651	1414	1422	1425	rBV	2240112	2304790	56.76%	9.790%
9	11.339	1533	1539	1542	rBV	1212420	988949	24.36%	4.201%
10	12.933	1805	1810	1813	rBV	3957016	4060328	100.00%	17.247%
11	13.986	1984	1989	1992	rBV	958437	844665	20.80%	3.588%
12	14.074	1998	2004	2012	rBV	195653	252632	6.22%	1.073%
13	15.451	2232	2238	2246	rBV	586130	742354	18.28%	3.153%
14	15.904	2310	2315	2320	rVB	31502	49084	1.21%	0.208%




Sum of corrected areas: 23542211

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
Data File : BF128744.D
Acq On : 09 Jun 2022 11:22
Operator : CG\JU
Sample : PB145411BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

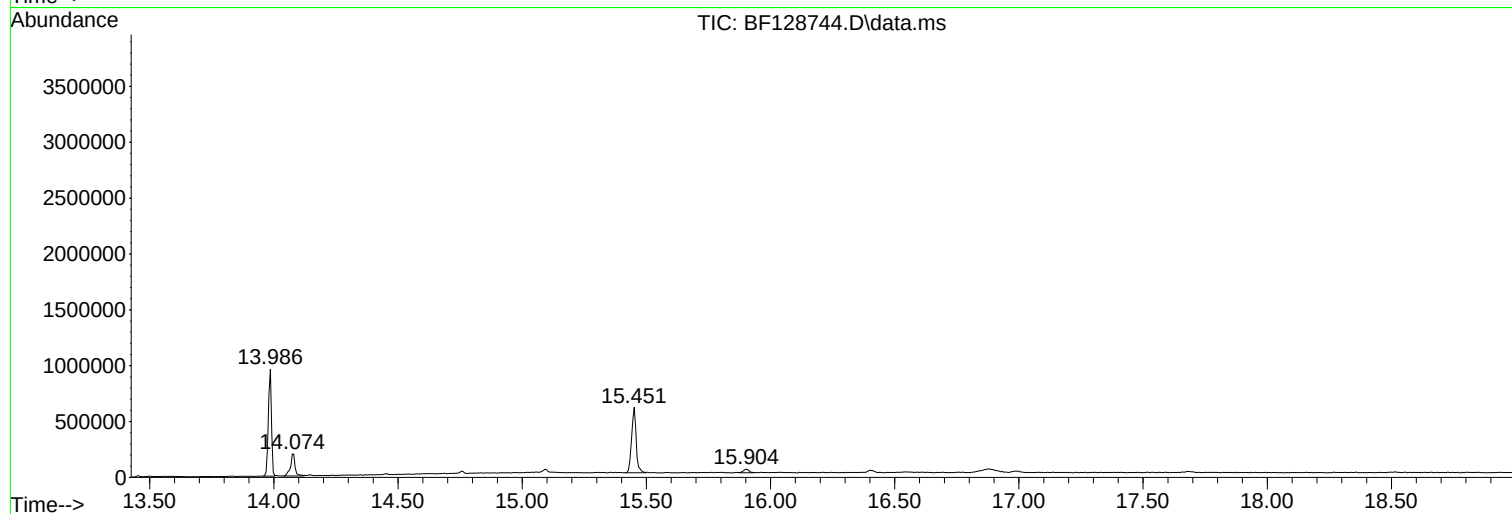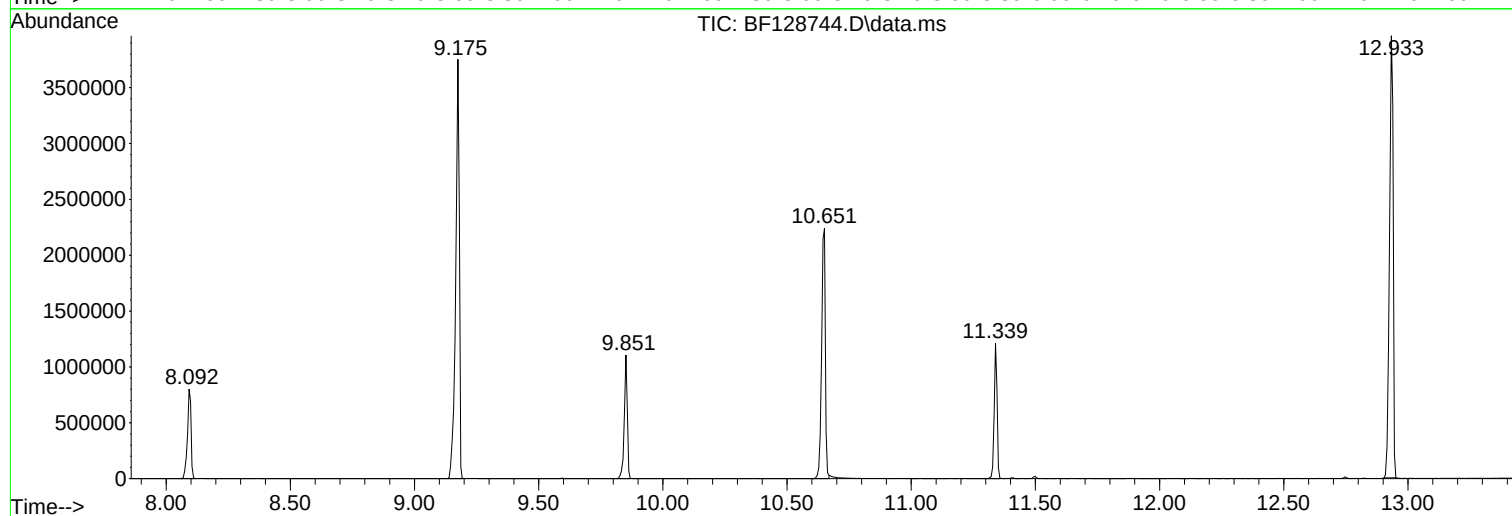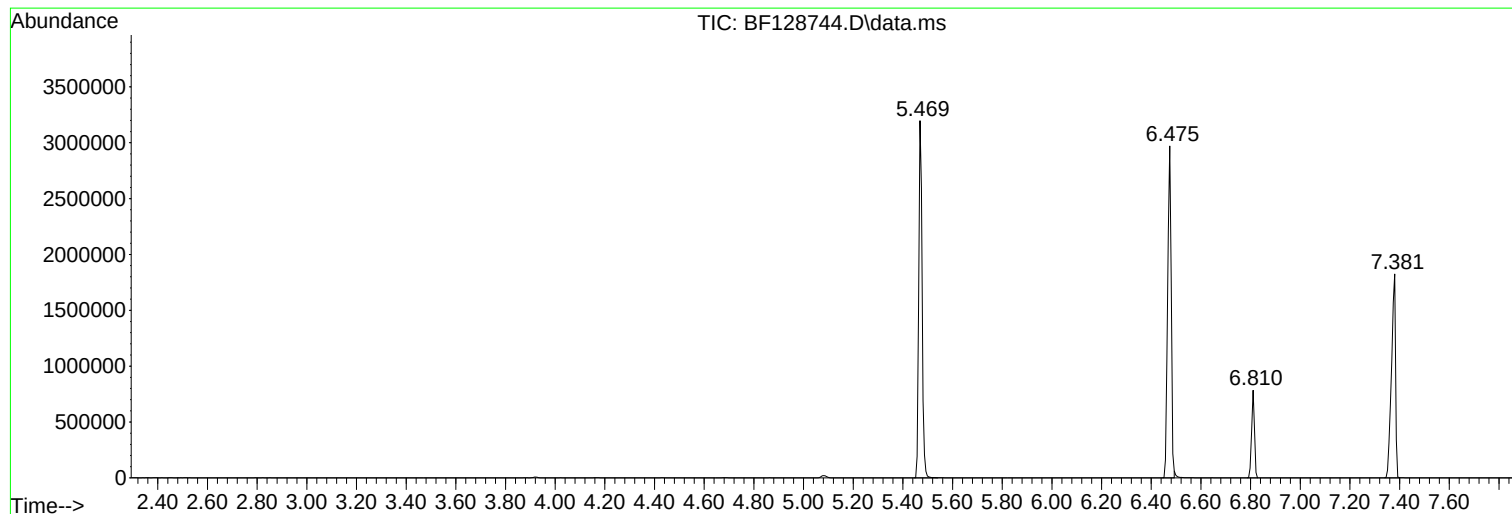

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
Data File : BF128744.D
Acq On : 09 Jun 2022 11:22
Operator : CG\JU
Sample : PB145411BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145411BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.074	5.98 ng	252632	Chrysene-d12	13.986

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	81
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	27
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	25

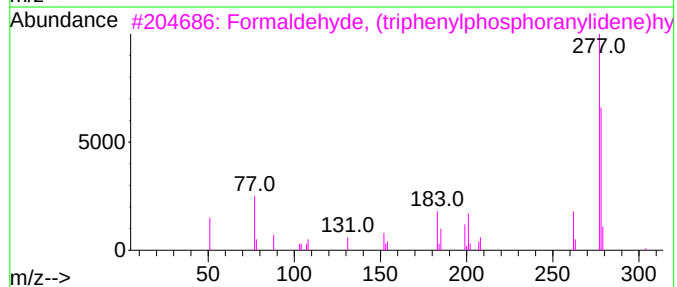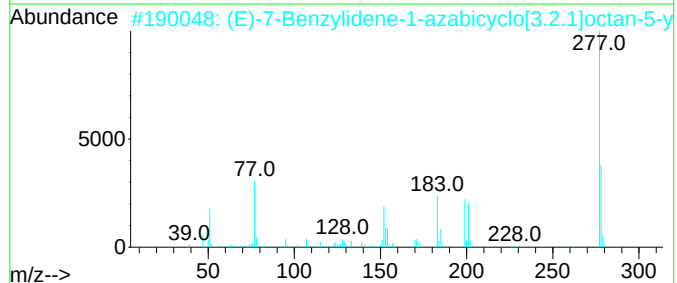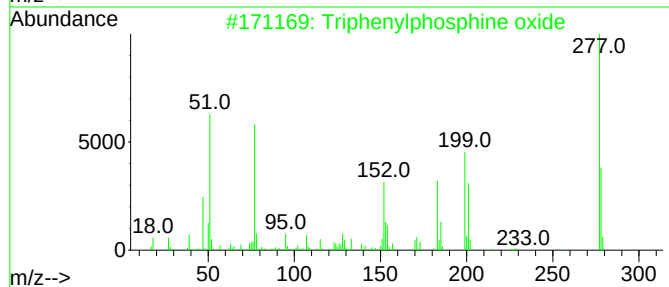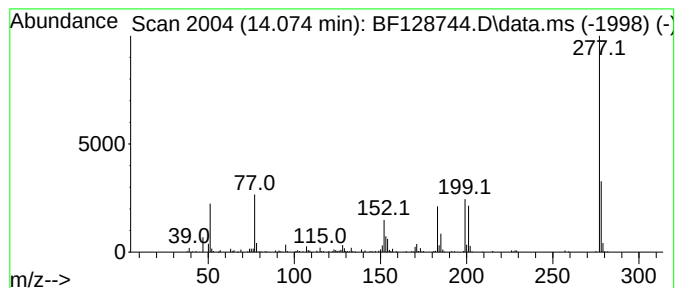

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
Data File : BF128744.D
Acq On : 09 Jun 2022 11:22
Operator : CG\JU
Sample : PB145411BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.074	6.0	ng	252632	5	13.986	844665	20.0