


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
 Data File : BF128742.D
 Acq On : 09 Jun 2022 10:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 08 14:28:39 2022

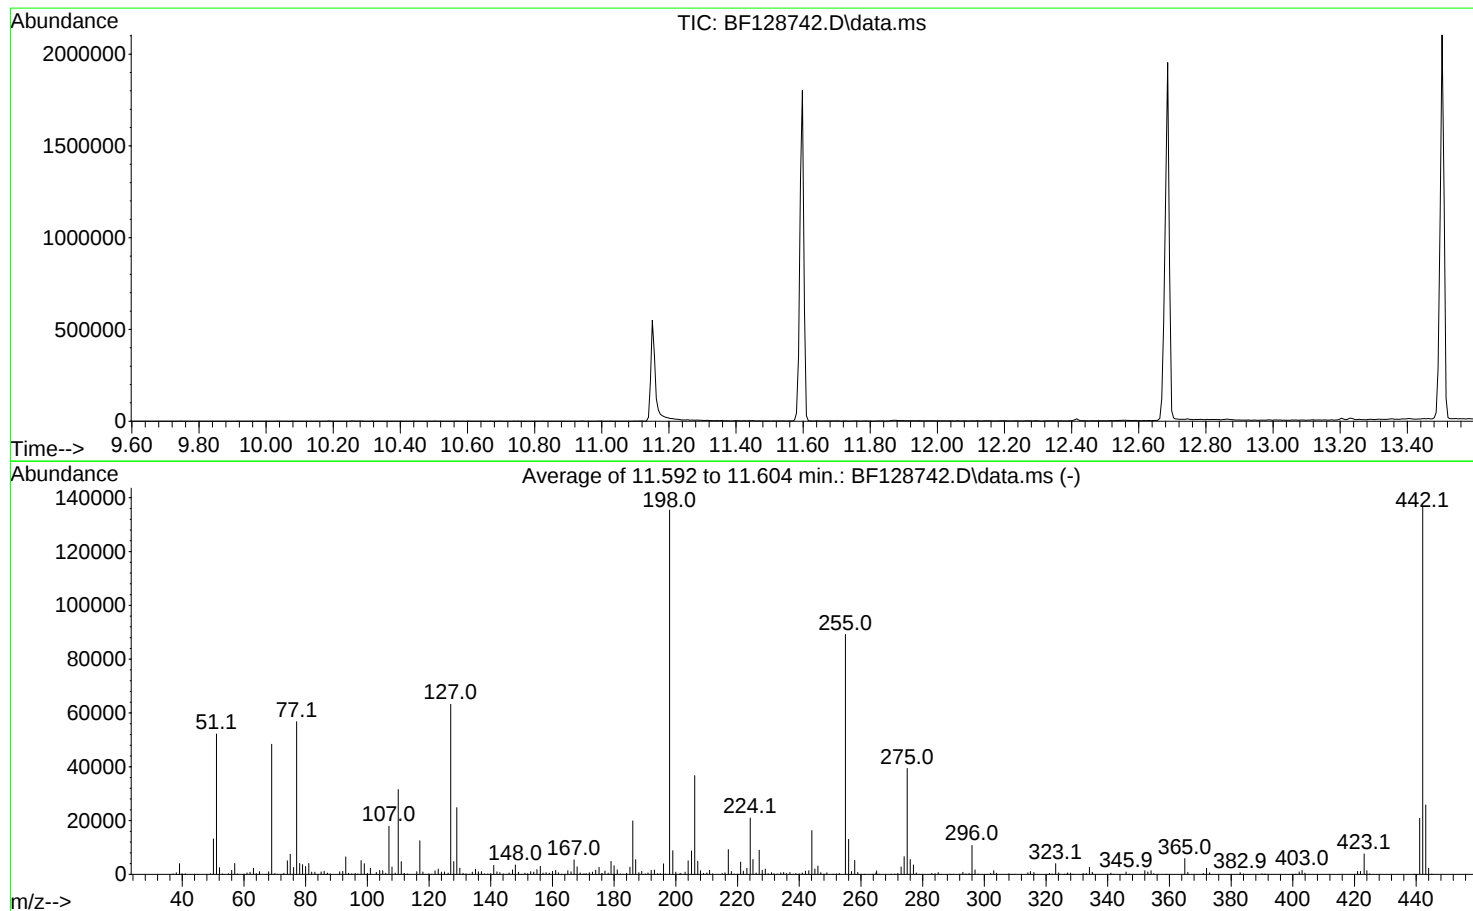




AutoFind: Scans 1582, 1583, 1584; Background Corrected with Scan 1576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	52179	PASS
68	69	0.00	2	1.9	932	PASS
69	198	0.00	100	35.7	48340	PASS
70	69	0.00	2	0.7	322	PASS
127	198	10	80	46.7	63216	PASS
197	198	0.00	2	0.1	142	PASS
198	198	100	100	100.0	135477	PASS
199	198	5	9	6.5	8836	PASS
275	198	10	60	29.1	39368	PASS
365	198	1	100	4.3	5884	PASS
441	198	0.01	100	15.4	20814	PASS
442	442	50	100	100.0	136757	PASS
443	442	15	24	18.9	25807	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
 Data File : BF128742.D
 Acq On : 09 Jun 2022 10:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 04:42:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 08 14:28:39 2022
 Response via : Initial Calibration

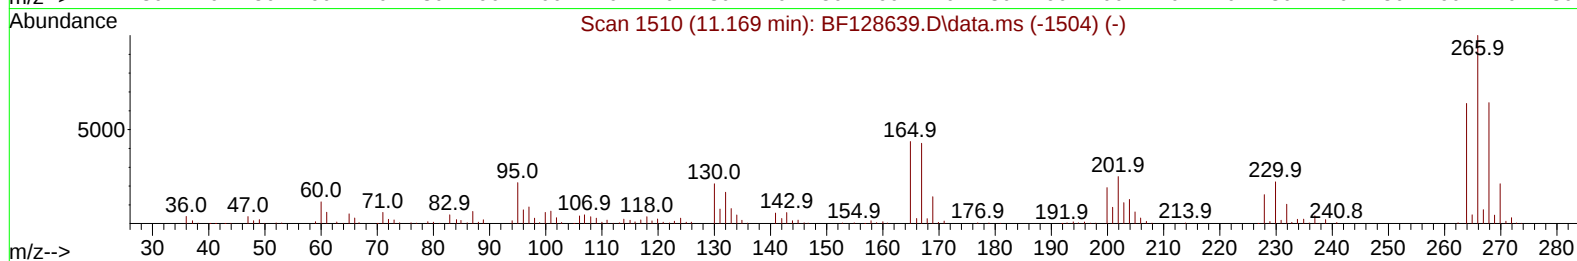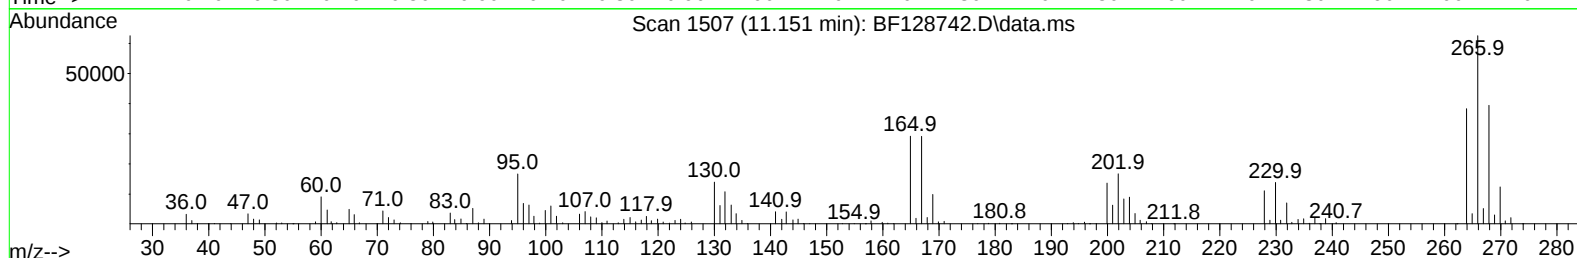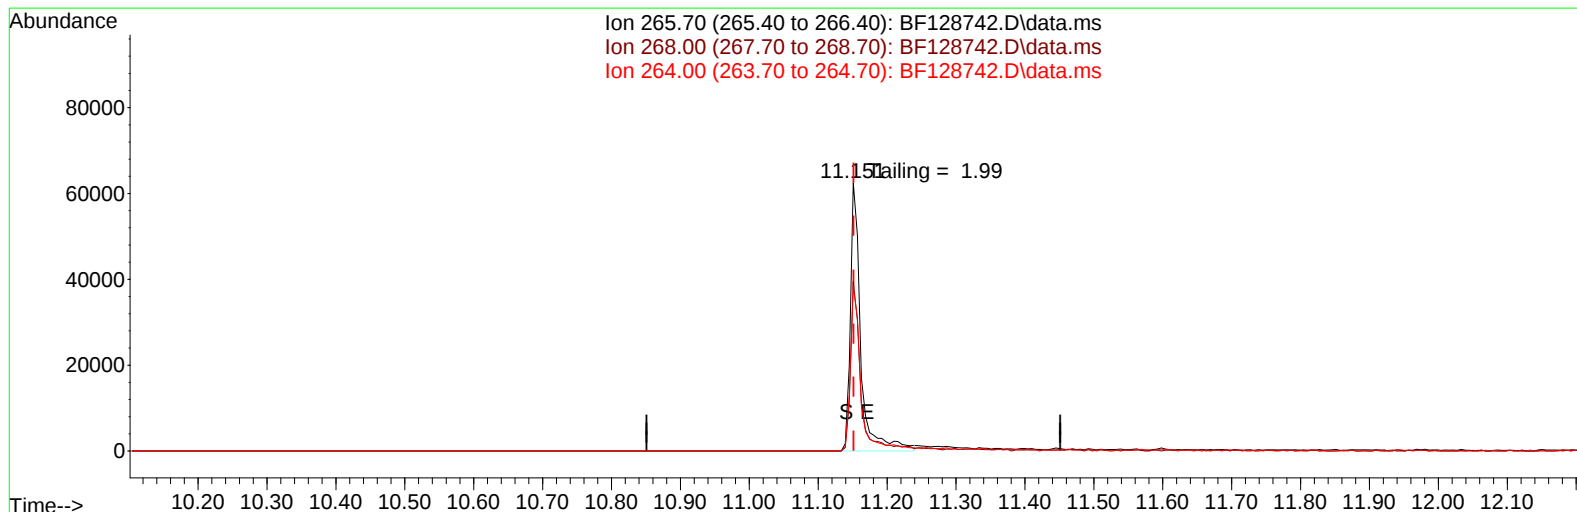

TIC: BF128742.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.000) 13297.83 ng




response 62562

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.08
264.00	61.80	61.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060922\
Data File : BF128742.D
Acq On : 09 Jun 2022 10:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 10 04:42:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 08 14:28:39 2022
Response via : Initial Calibration

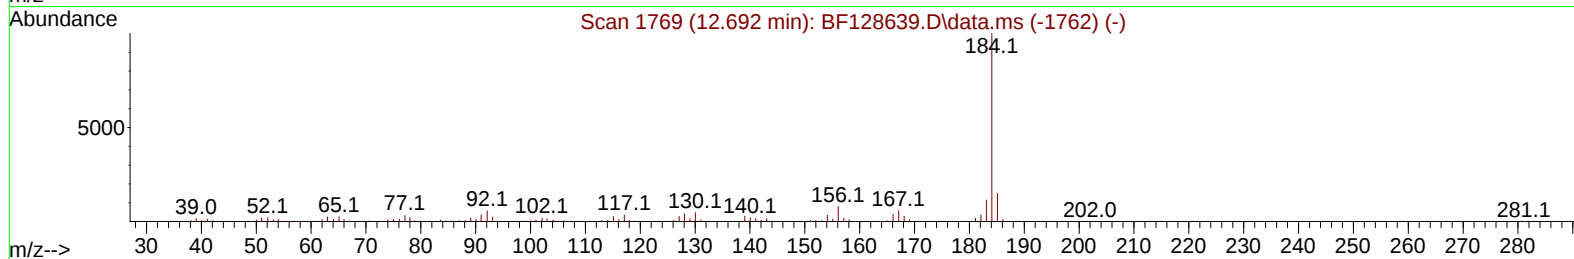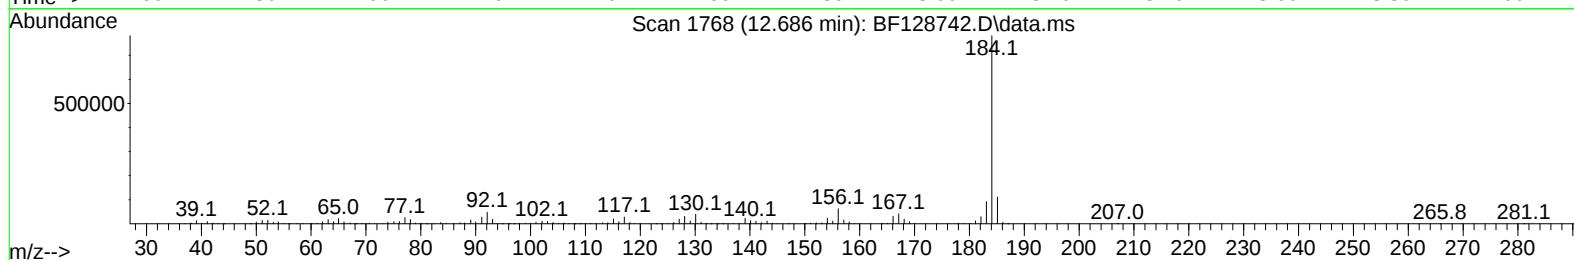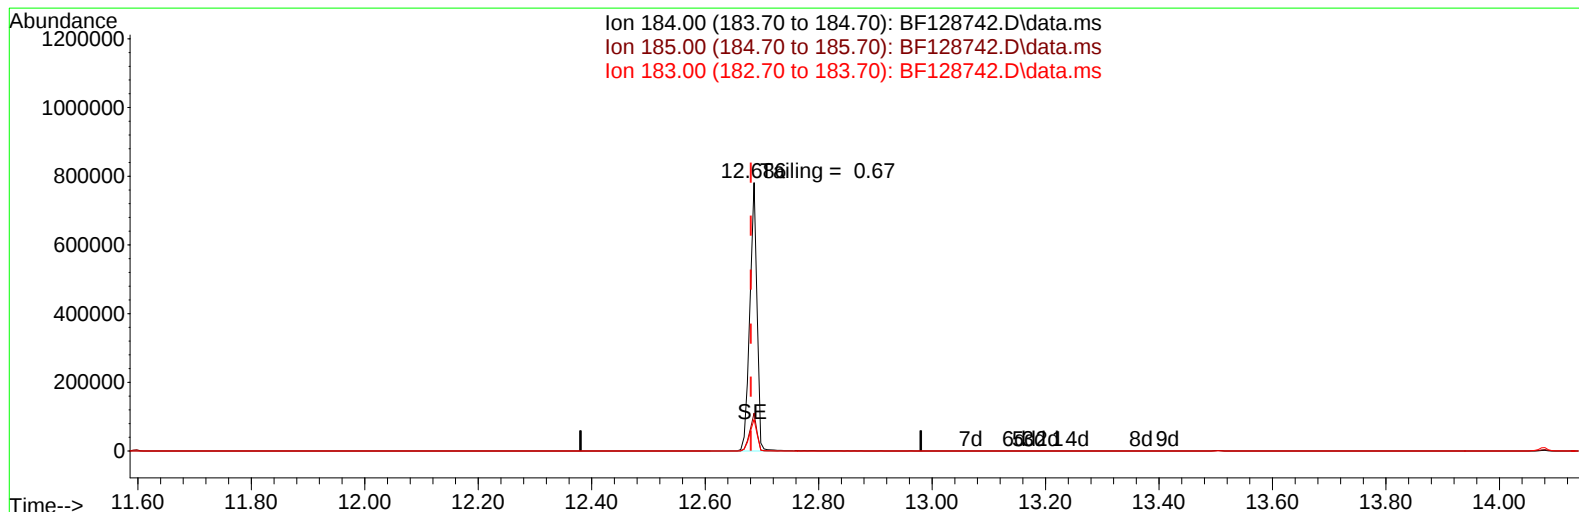

TIC: BF128742.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 611668.21 ng m

response 695017

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.18
183.00	11.60	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2022	BNA_F	<u>BF128742.D</u>
Compound Name	Response	Retention Time
DDT	329022	13.504
DDD	3966	13.227
DDE	462	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4428	333450	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP