
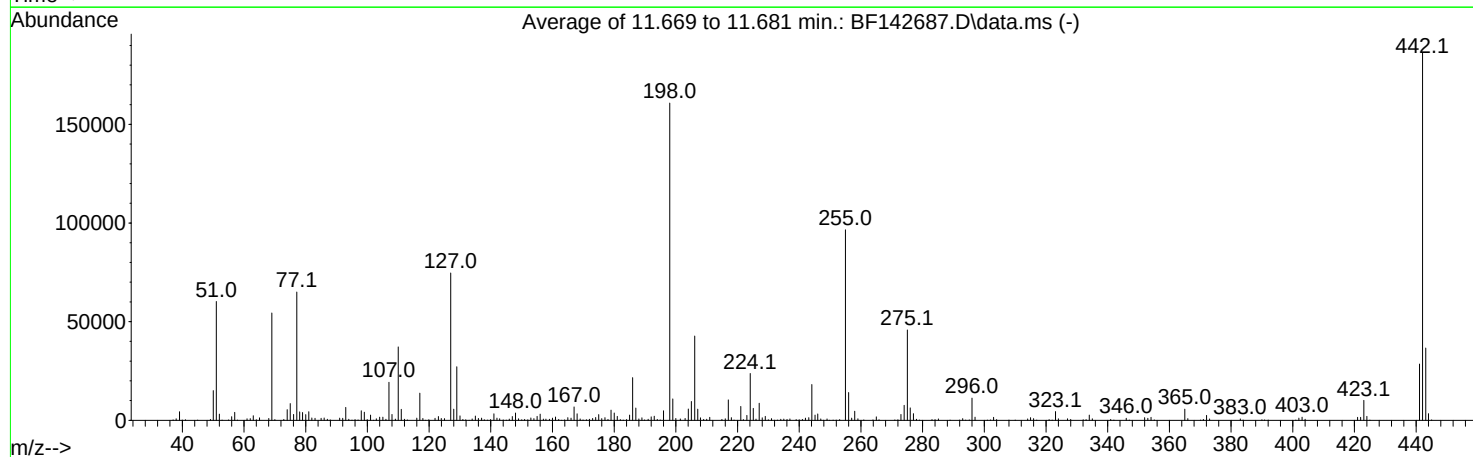


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060925\
Data File : BF142687.D
Acq On : 09 Jun 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 18:21:22 2025

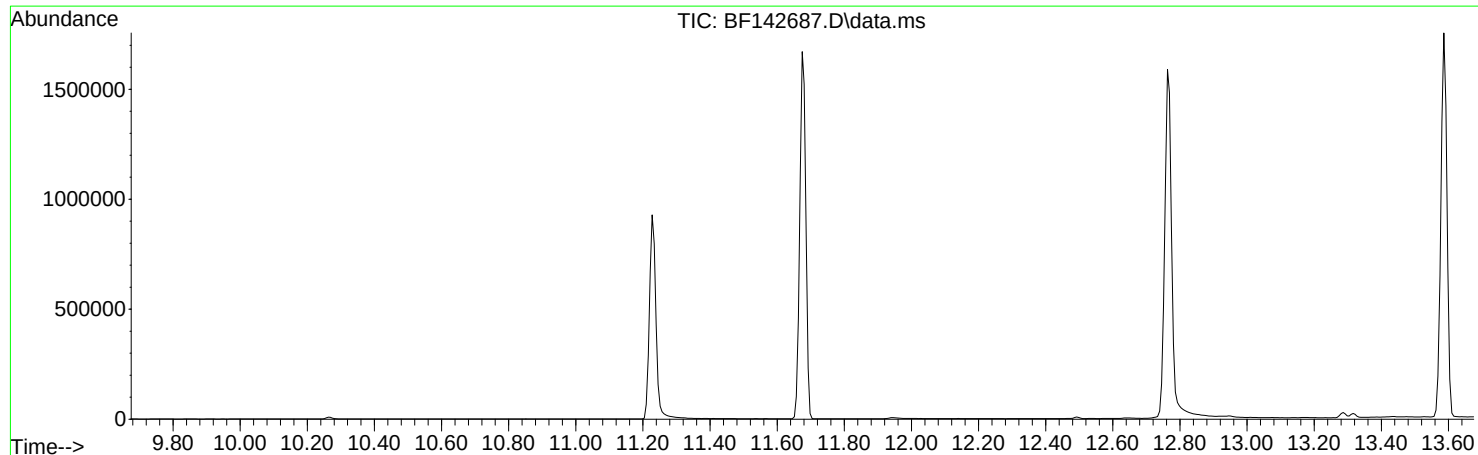




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	60256	PASS
68	69	0.00	2	1.7	923	PASS
69	198	0.00	100	33.8	54368	PASS
70	69	0.00	2	0.6	338	PASS
127	198	10	80	46.4	74659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	160765	PASS
199	198	5	9	6.8	10868	PASS
275	198	10	60	28.5	45829	PASS
365	198	1	100	3.5	5649	PASS
441	198	0.01	100	17.7	28523	PASS
442	442	50	100	100.0	186464	PASS
443	442	15	24	19.6	36635	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060925\
Data File : BF142687.D
Acq On : 09 Jun 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 09 18:43:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 18:21:22 2025
Response via : Initial Calibration

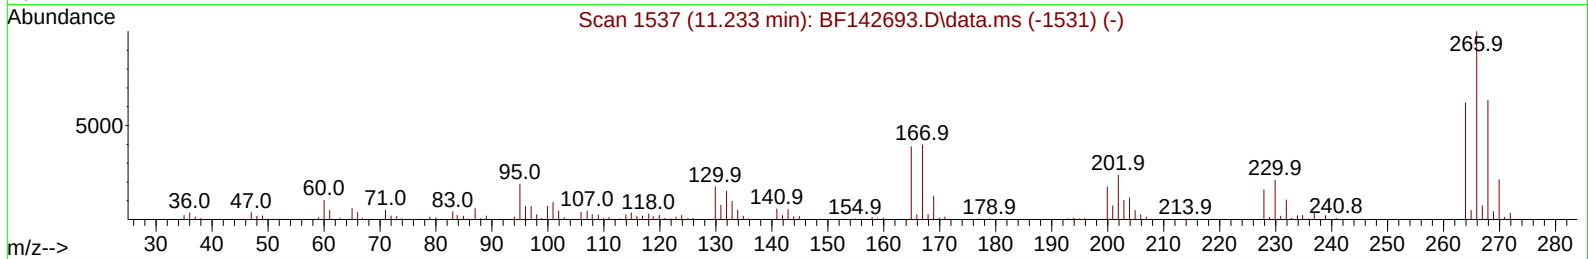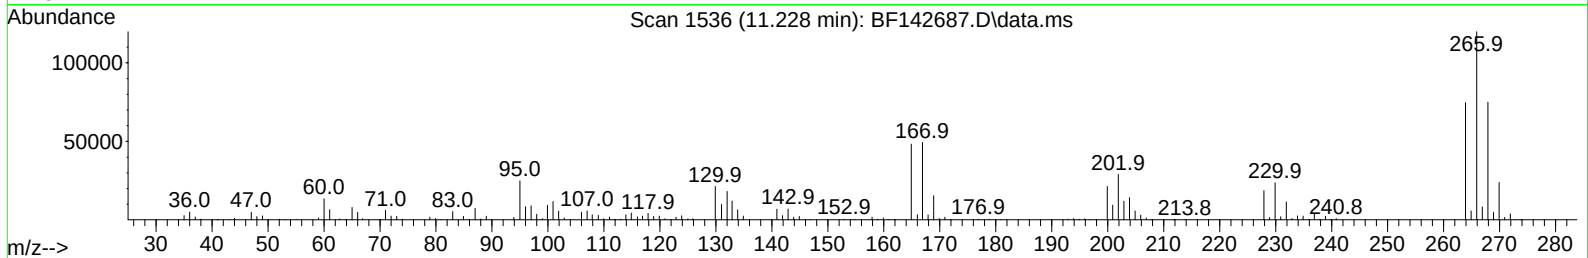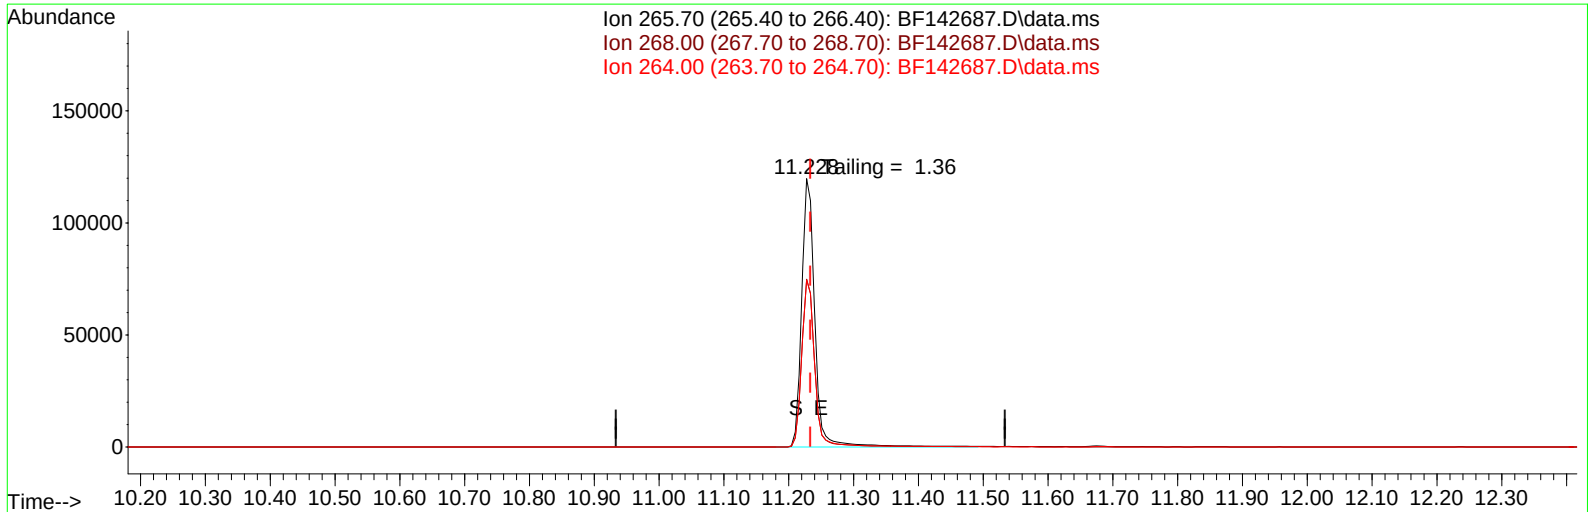

TIC: BF142687.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.006) 26620.89 ng




response 169012

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.56
264.00	62.10	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060925\
Data File : BF142687.D
Acq On : 09 Jun 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 09 18:43:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 18:21:22 2025
Response via : Initial Calibration

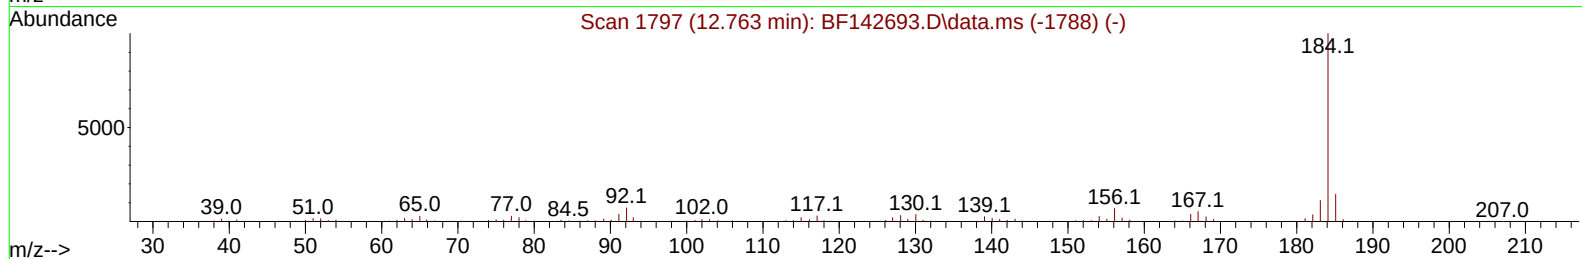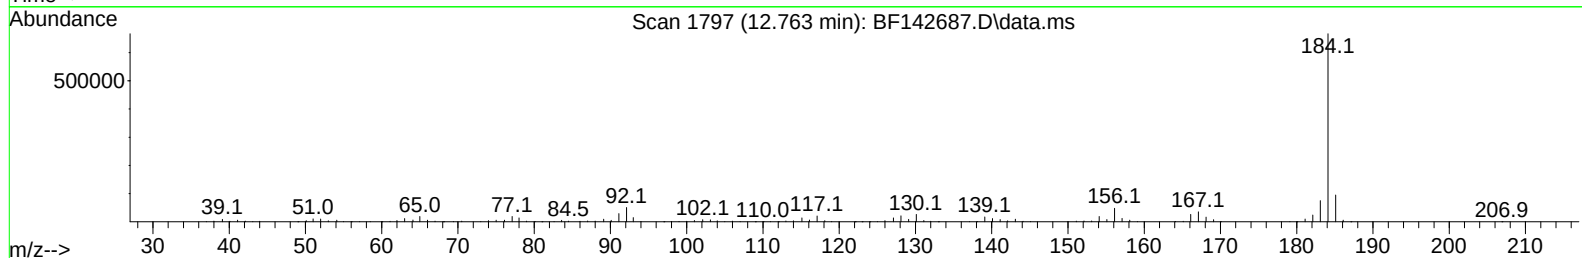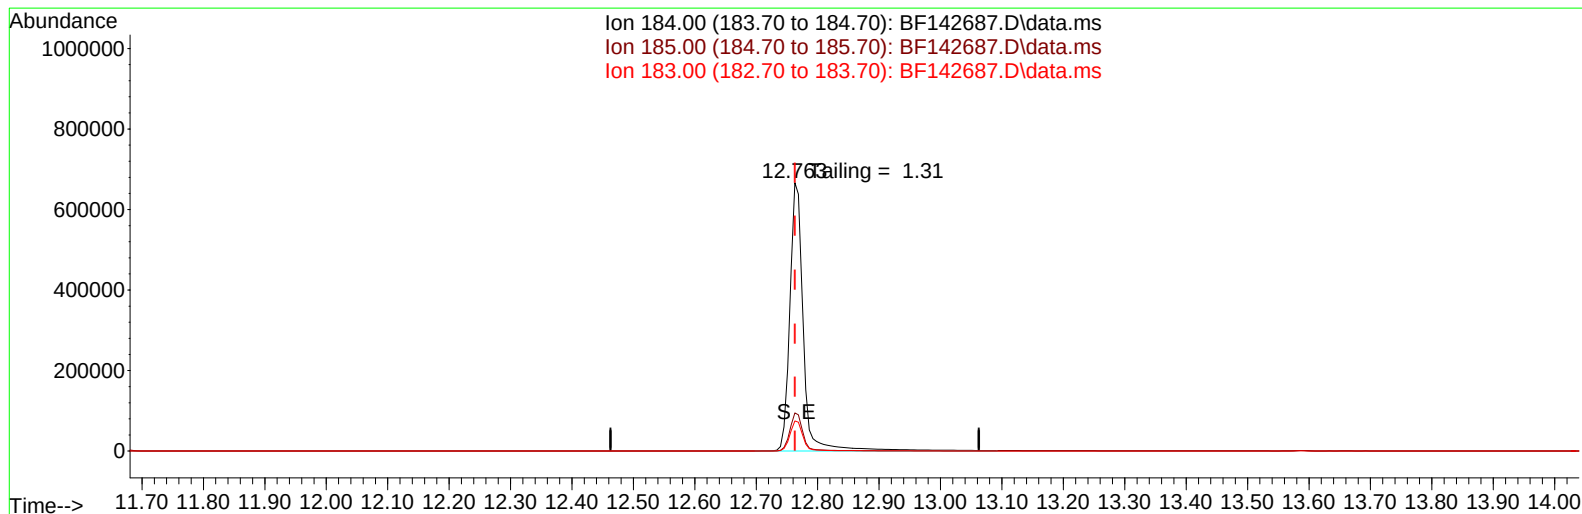

TIC: BF142687.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 1027528

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.21
183.00	11.10	11.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2025	BNA_F	<u>BF142687.D</u>
Compound Name	Response	Retention Time
DDT	456536	13.586
DDD	12637	13.286
DDE	1322	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13959	470495	2.97

Instrument :
BNA_F
ClientSampleId :
DFTPP