
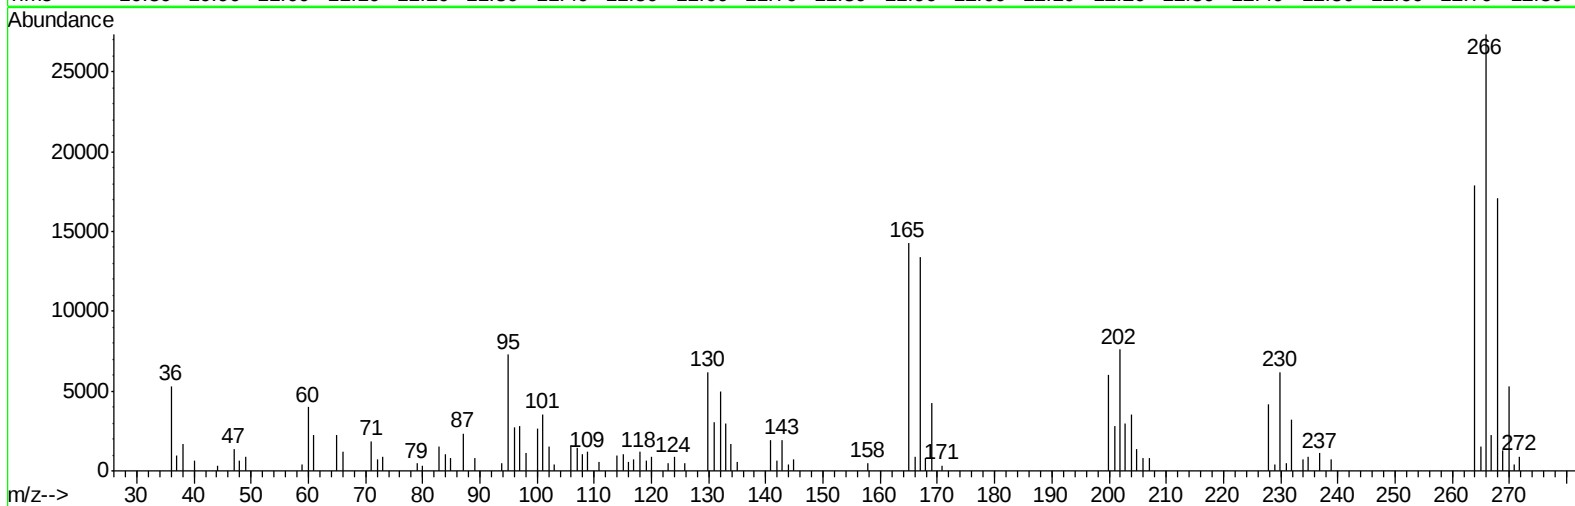


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079854.D
Acq On : 10 Jun 2015 8:41
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 08:05:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

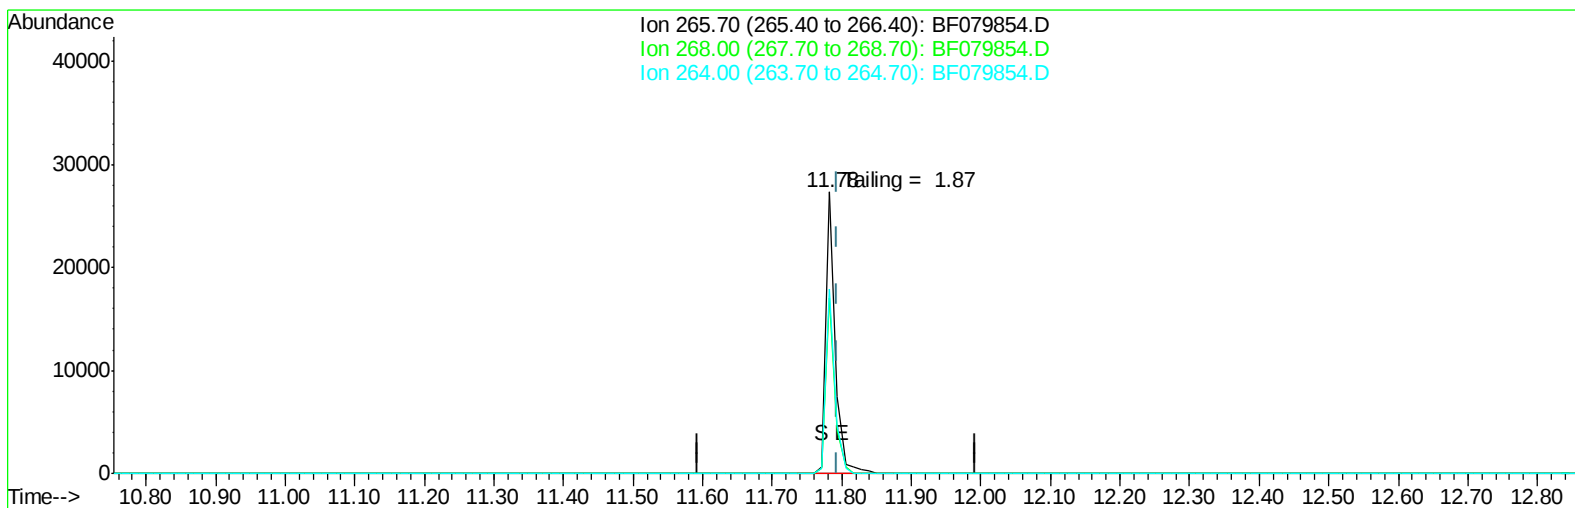

TIC: BF079854.D

(69) Pentachlorophenol (C)



11.782min (-0.011) 0.00ng

response 25746

Ion	Exp%	Act%
265.70	100	100
268.00	61.40	62.42
264.00	61.80	65.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079854.D
Acq On : 10 Jun 2015 8:41
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 08:05:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

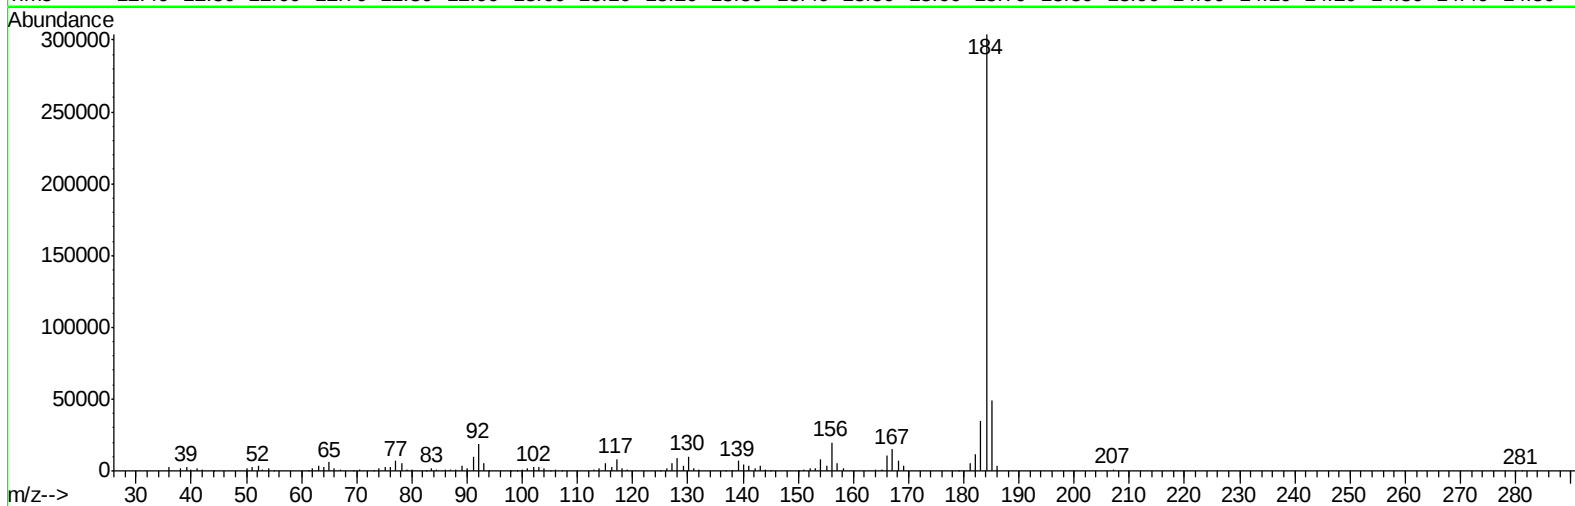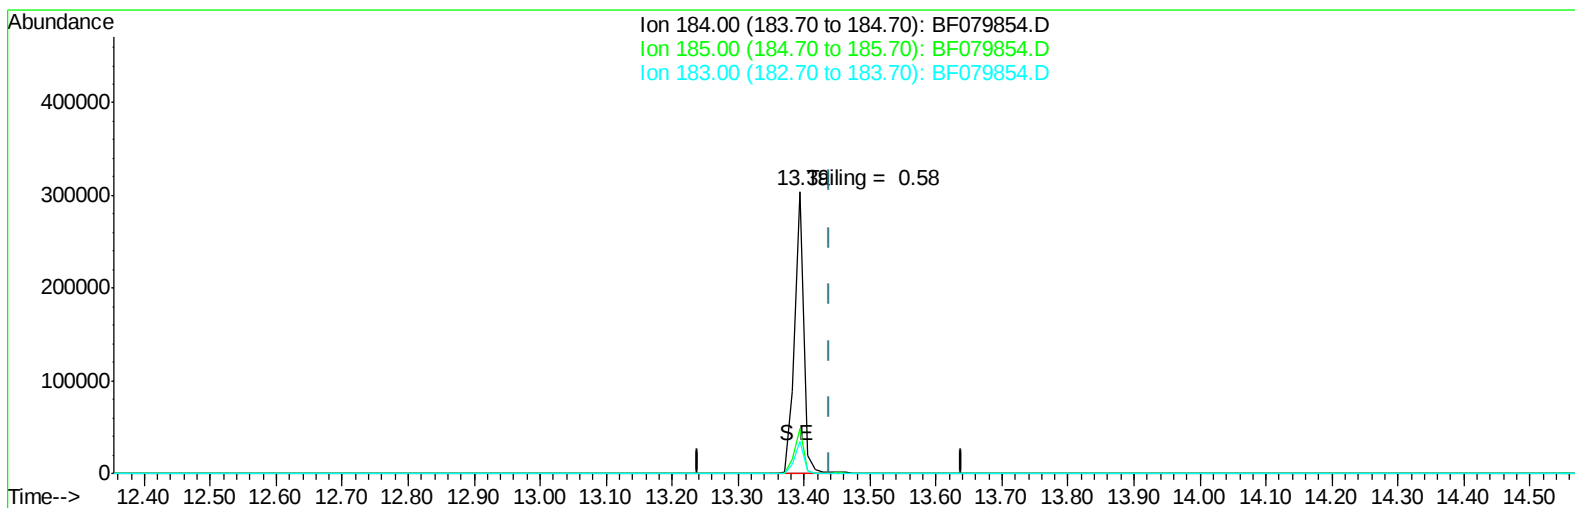

TIC: BF079854.D

(76) Benzidine

13.394min (-0.046) 0.00ng

response 291900

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.01
183.00	11.30	11.38
0.00	0.00	0.00