
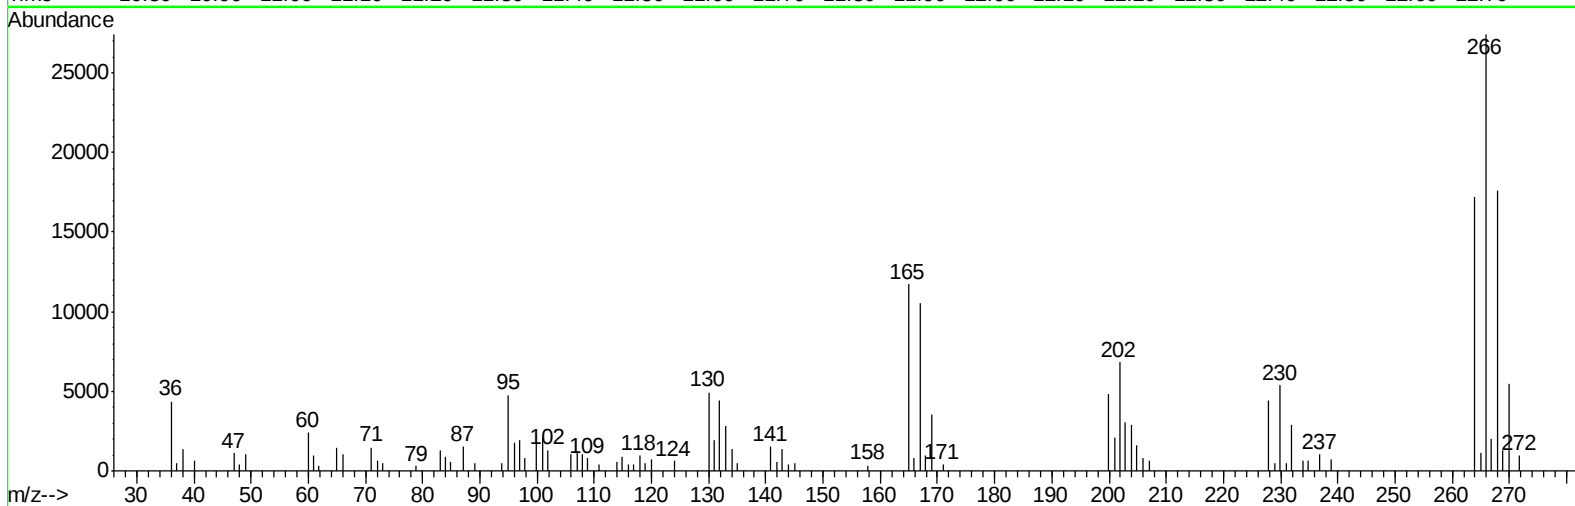


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079878.D
Acq On : 10 Jun 2015 23:08
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 08:06:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

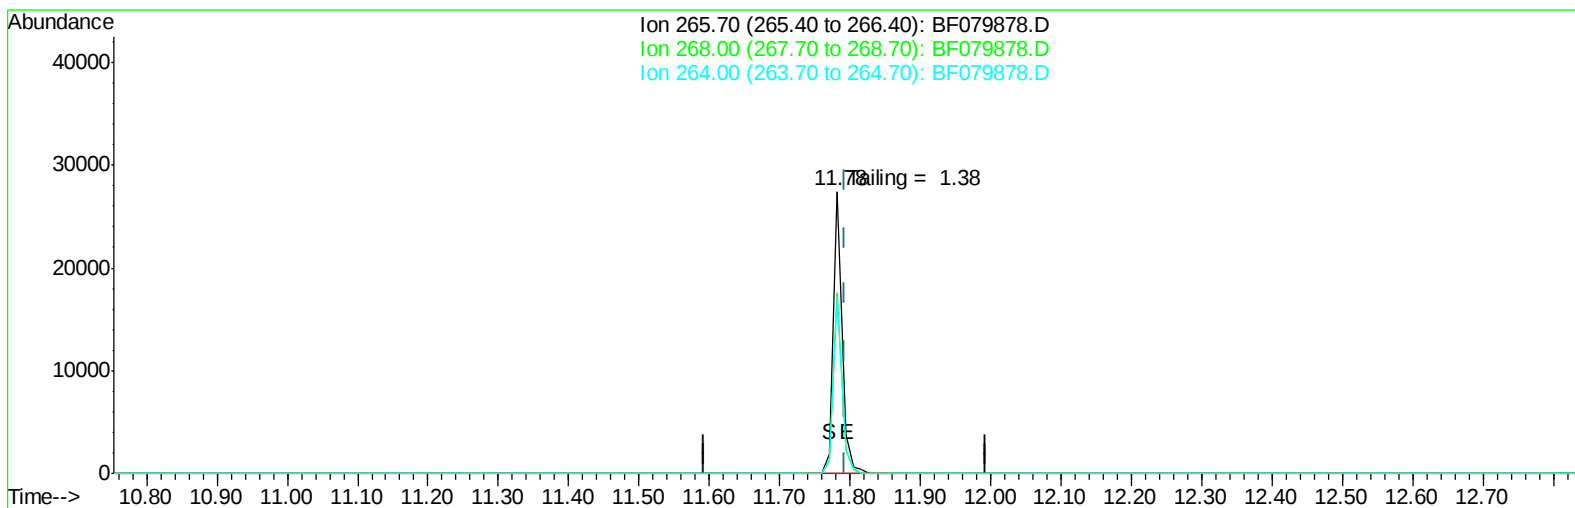

TIC: BF079878.D

(69) Pentachlorophenol (C)



11.782min (-0.012) 0.00ng

response 23374

Ion	Exp%	Act%
265.70	100	100
268.00	61.40	64.14
264.00	61.80	62.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079878.D
Acq On : 10 Jun 2015 23:08
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 08:06:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

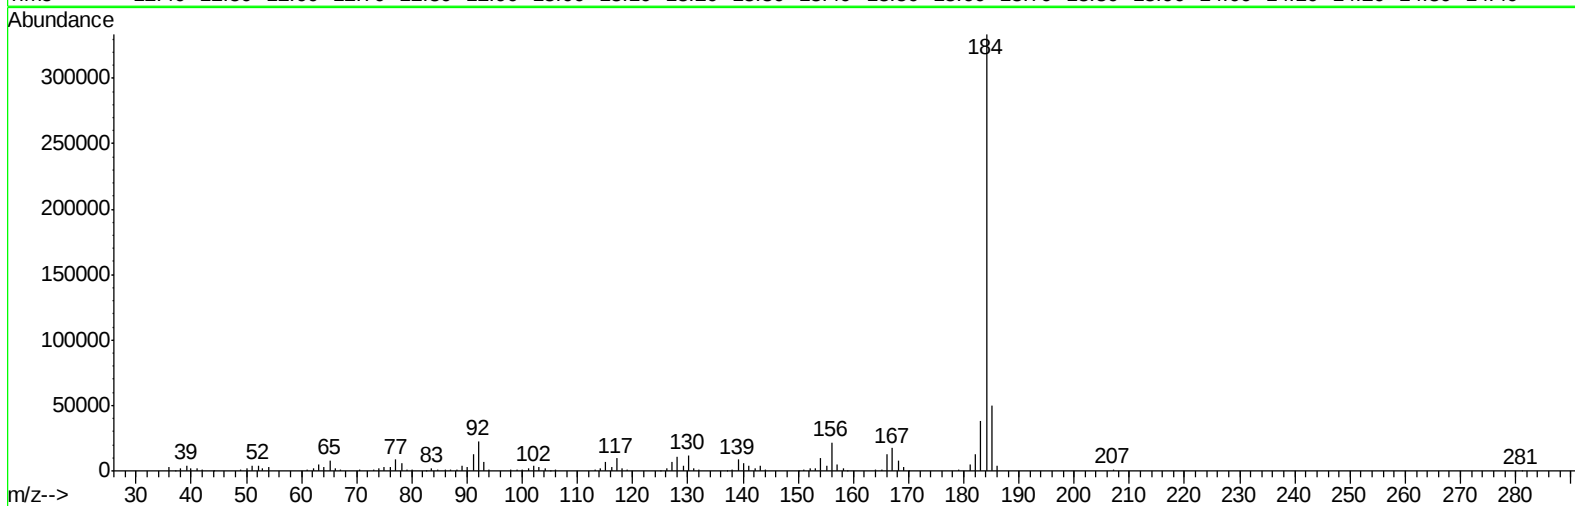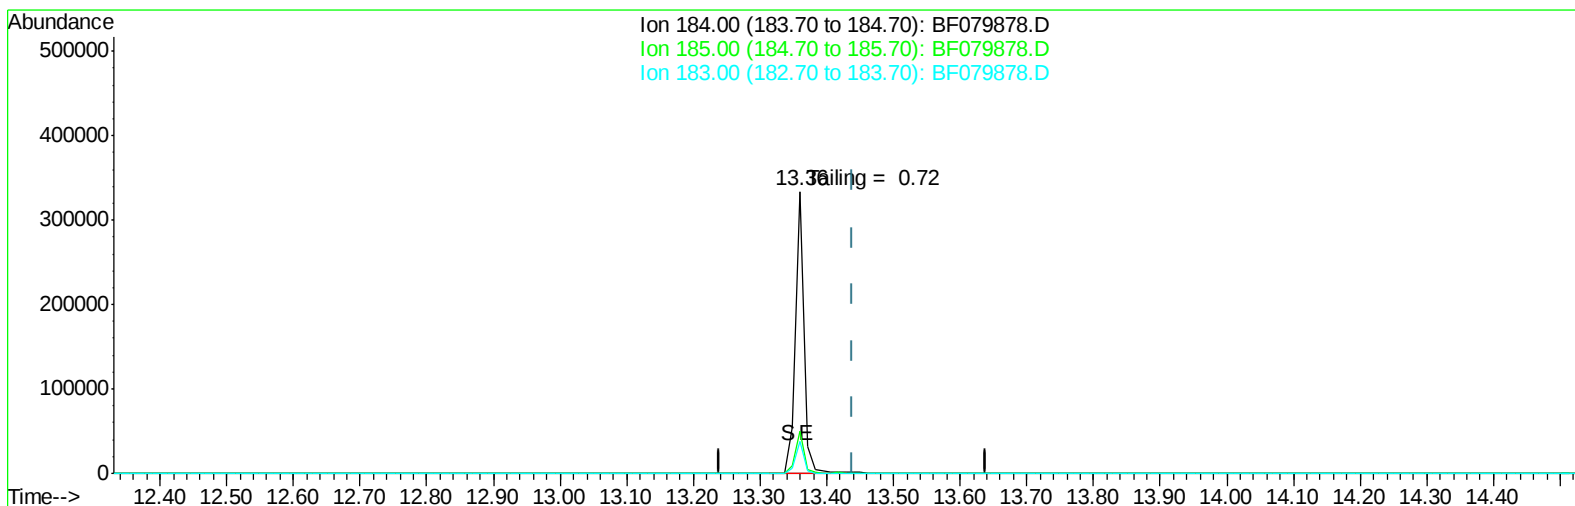

TIC: BF079878.D

(76) Benzidine

13.359min (-0.080) 0.00ng

response 299535

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.08
183.00	11.30	11.45
0.00	0.00	0.00