

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
 Data File : BF079856.D
 Acq On : 10 Jun 2015 10:59
 Operator : TP/IZ
 Sample : PB83906BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83906BL

Quant Time: Jun 11 01:37:16 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 00:53:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	45986	20.00	ng	0.00
21) Naphthalene-d8	8.71	136	182616	20.00	ng	0.00
38) Acenaphthene-d10	10.48	164	88782	20.00	ng	-0.01
63) Phenanthrene-d10	12.02	188	188266	20.00	ng	0.02
75) Chrysene-d12	15.26	240	180926m	20.00	ng	0.18
86) Perylene-d12	17.33	264	164675m	20.00	ng	0.30
System Monitoring Compounds						
5) 2-Fluorophenol	6.03	112	364472	130.62	ng	0.00
7) Phenol-d6	7.02	99	495351	137.20	ng	0.00
23) Nitrobenzene-d5	7.98	82	241001	76.24	ng	0.00
41) 2,4,6-Tribromophenol	11.29	330	88231	114.83	ng	0.01
44) 2-Fluorobiphenyl	9.78	172	562762	89.15	ng	0.00
78) Terphenyl-d14	13.85	244	706942	88.09	ng	0.11


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079856.D
Acq On : 10 Jun 2015 10:59
Operator : TP/IZ
Sample : PB83906BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83906BL

Quant Time: Jun 11 01:37:16 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

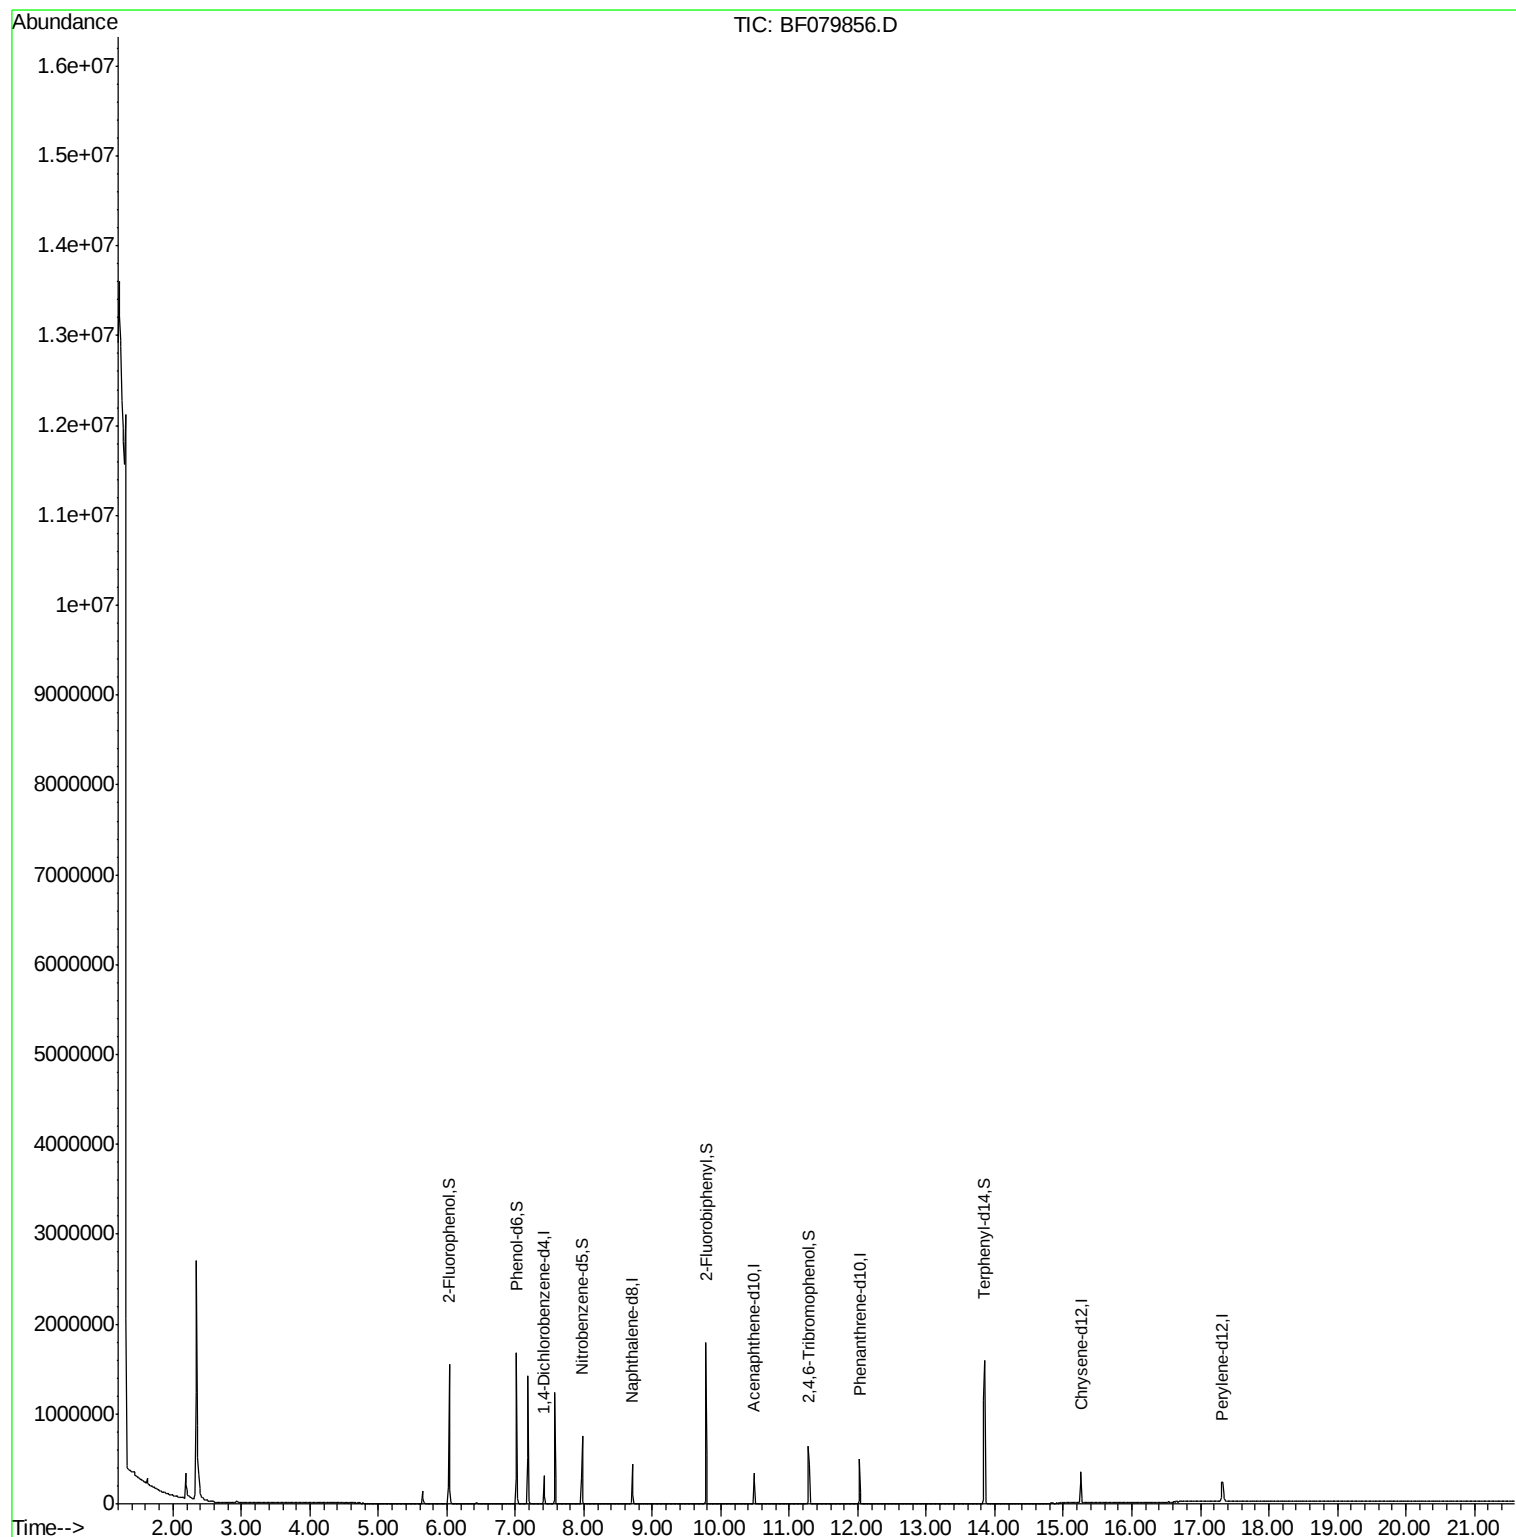

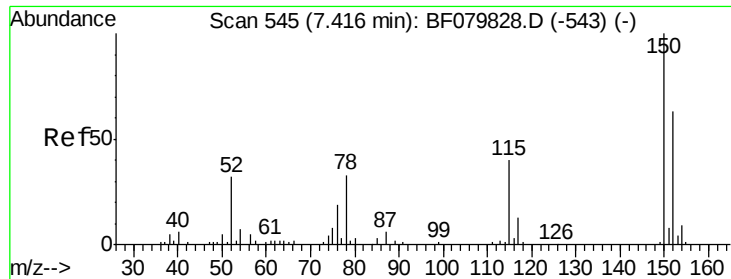


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.42 min Scan# 545
Delta R.T. 0.00 min
Lab File: BF079856.D
Acq: 10 Jun 2015 10:59

Instrument :
BNA_F
ClientSampleId :
PB83906BL

Tgt Ion:152 Resp: 45986
Ion Ratio Lower Upper
152 100
150 160.8 131.4 197.2
115 63.9 56.5 84.7

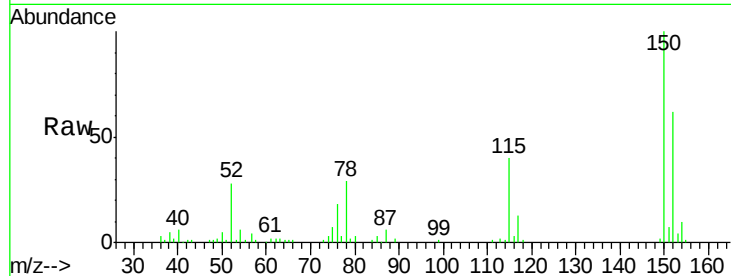


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

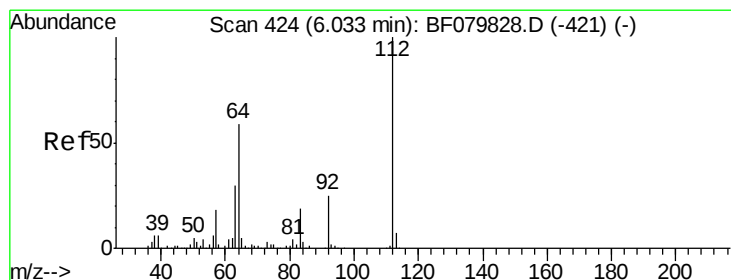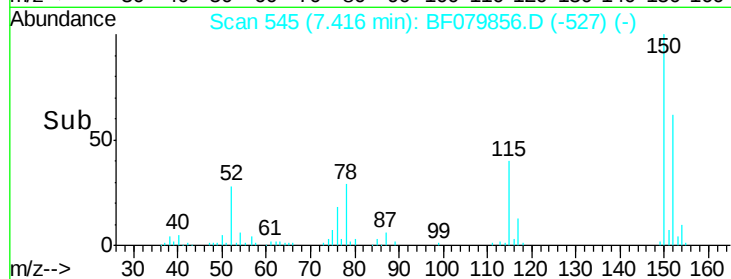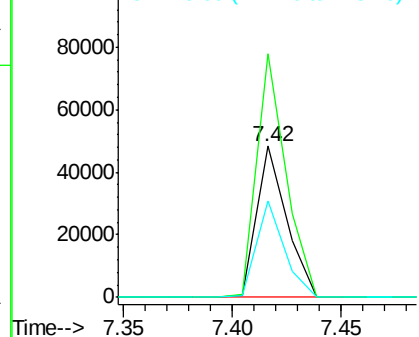



#5

2-Fluorophenol
Concen: 130.62 ng
RT: 6.03 min Scan# 424
Delta R.T. 0.00 min
Lab File: BF079856.D
Acq: 10 Jun 2015 10:59

Tgt Ion:112 Resp: 364472
Ion Ratio Lower Upper
112 100
64 63.2 44.2 66.4
63 32.0 22.8 34.2

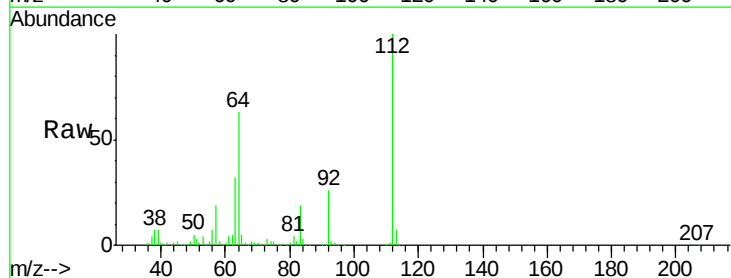

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

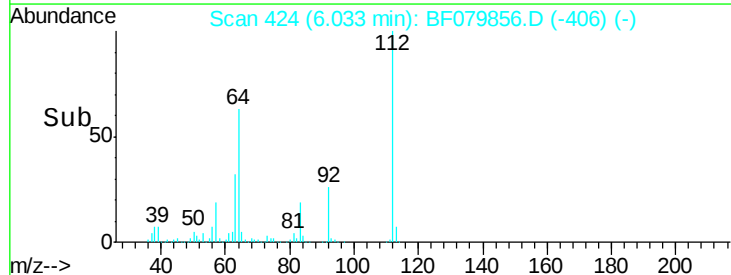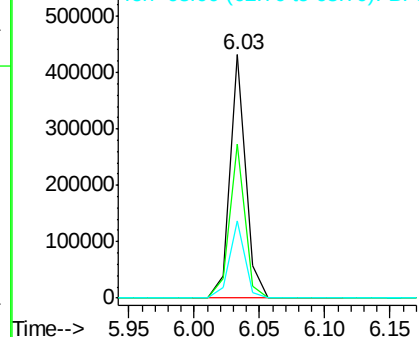



#7

Phenol-d6

Concen: 137.20 ng

RT: 7.02 min Scan# 510

Delta R.T. 0.00 min

Lab File: BF079856.D

Acq: 10 Jun 2015 10:59

Instrument :

BNA_F

ClientSampleId :

PB83906BL


Tgt Ion: 99 Resp: 495351

Ion Ratio Lower Upper

99 100

42 18.6 13.7 20.5




71 32.2 25.1 37.7

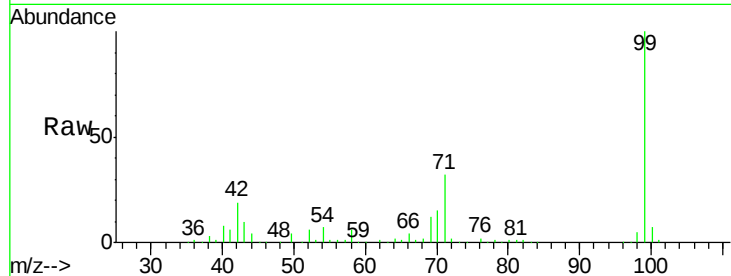

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

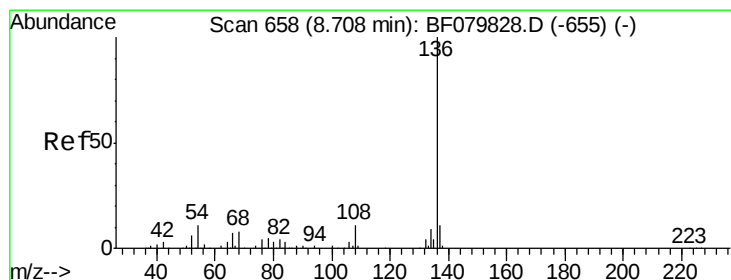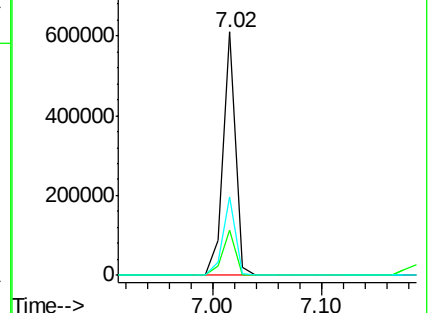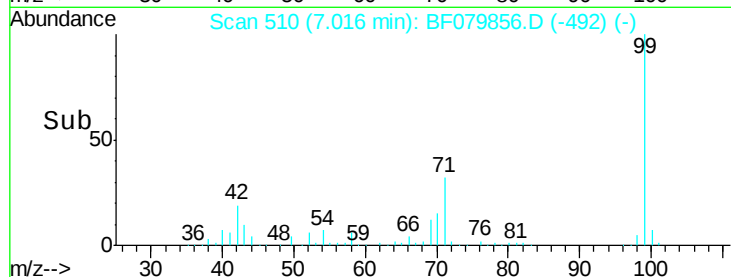

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.71 min Scan# 658

Delta R.T. 0.00 min

Lab File: BF079856.D

Acq: 10 Jun 2015 10:59

Tgt Ion: 136 Resp: 182616


Ion Ratio Lower Upper

136 100

137 10.7 9.3 13.9

54 10.2 8.1 12.1

68 7.1 4.8 7.2


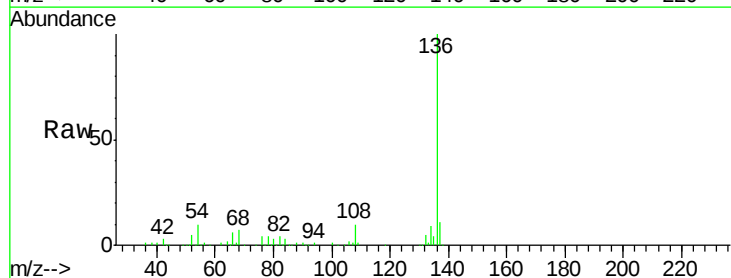



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



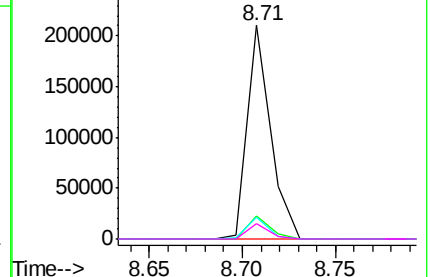
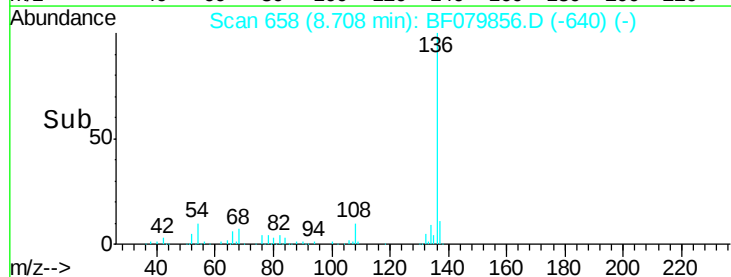


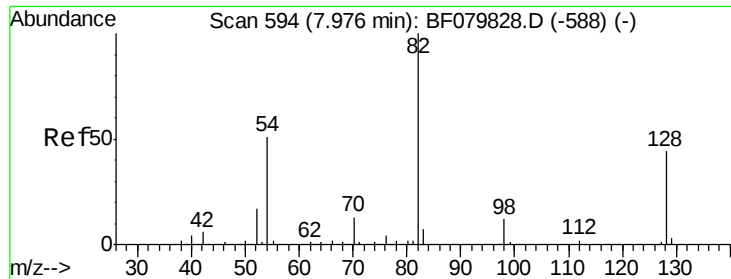

#23
 Nitrobenzene-d5
 Concen: 76.24 ng
 RT: 7.98 min Scan# 594
 Delta R.T. 0.00 min
 Lab File: BF079856.D
 Acq: 10 Jun 2015 10:59




Instrument :
 BNA_F
 ClientSampleId :
 PB83906BL


Tgt Ion: 82 Resp: 241001
 Ion Ratio Lower Upper
 82 100
 128 48.7 35.2 52.8
 54 46.8 39.2 58.8

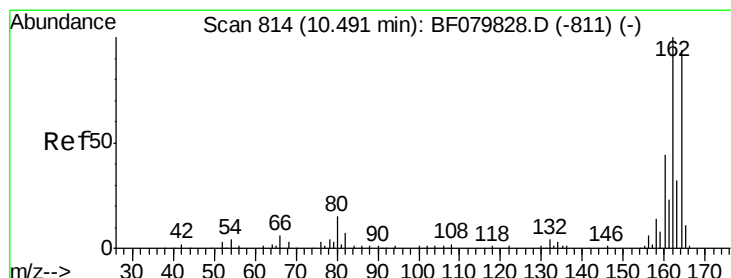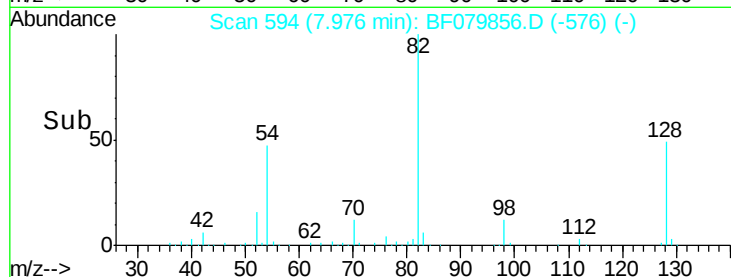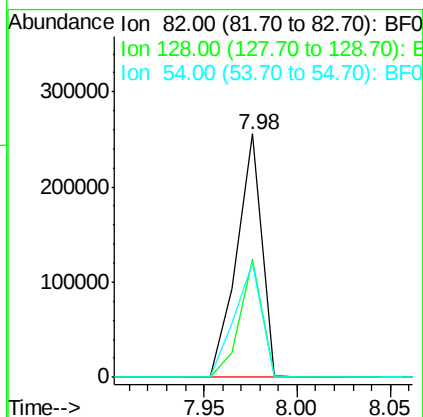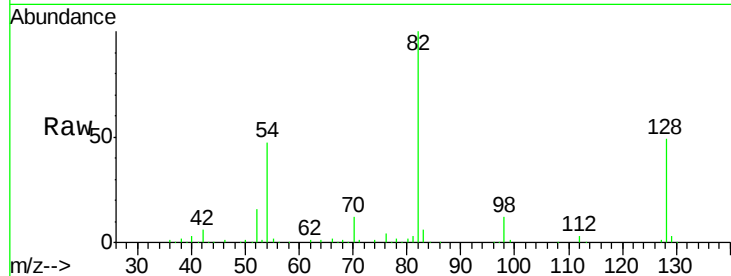

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.48 min Scan# 813
 Delta R.T. -0.01 min
 Lab File: BF079856.D
 Acq: 10 Jun 2015 10:59

Tgt Ion: 164 Resp: 88782
 Ion Ratio Lower Upper
 164 100
 162 101.6 89.8 134.8
 160 45.0 39.6 59.4

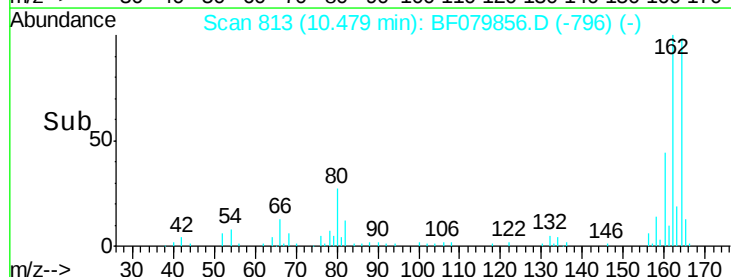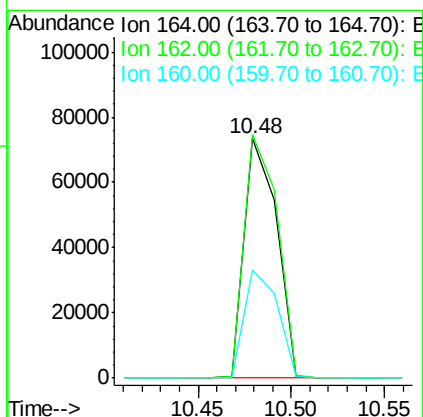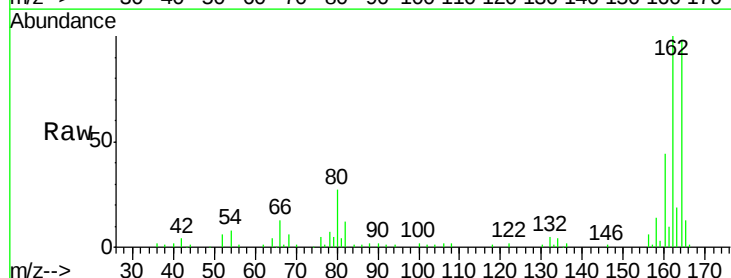


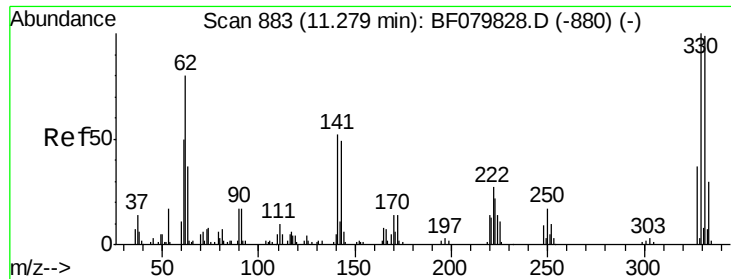




#41
 2,4,6-Tribromophenol
 Concen: 114.83 ng
 RT: 11.29 min Scan# 884
 Delta R.T. 0.01 min
 Lab File: BF079856.D
 Acq: 10 Jun 2015 10:59

Instrument :
 BNA_F
 ClientSampleId :
 PB83906BL

Tgt Ion:330 Resp: 88231
 Ion Ratio Lower Upper
 330 100
 332 96.0 76.8 115.2
 141 37.7 29.1 43.7

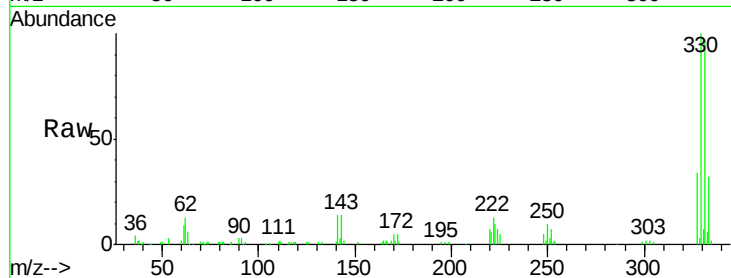


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

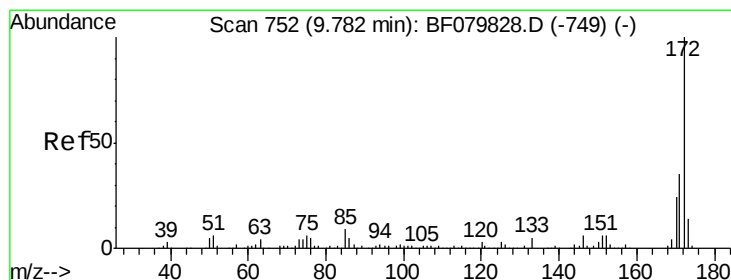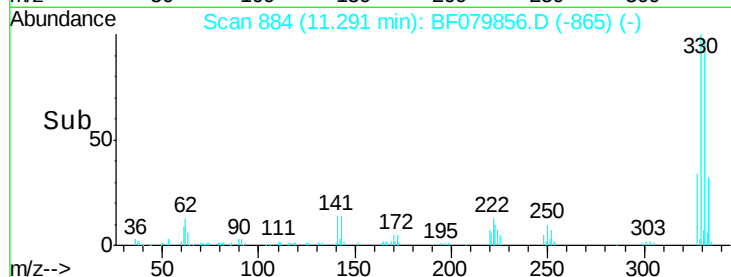
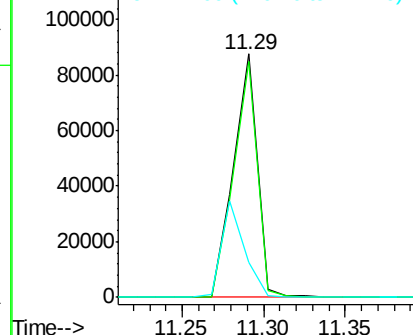



#44
 2-Fluorobiphenyl
 Concen: 89.15 ng
 RT: 9.78 min Scan# 752
 Delta R.T. 0.00 min
 Lab File: BF079856.D
 Acq: 10 Jun 2015 10:59

Tgt Ion:172 Resp: 562762
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.5 42.7
 170 23.5 18.8 28.2

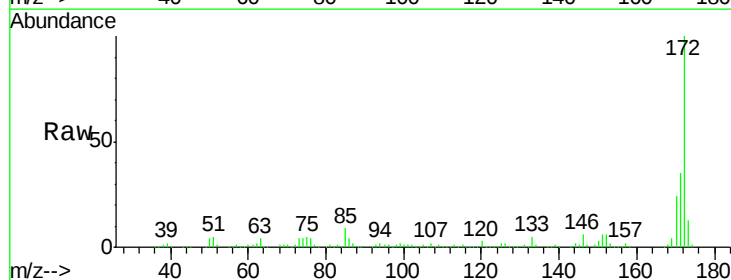

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



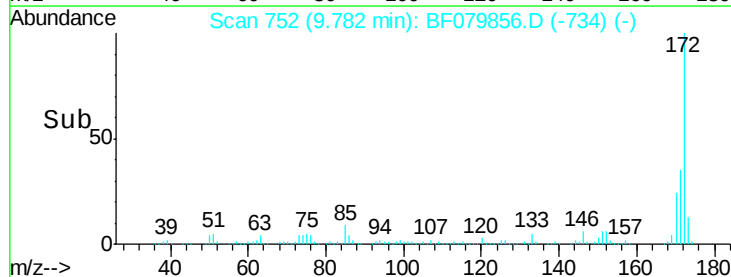
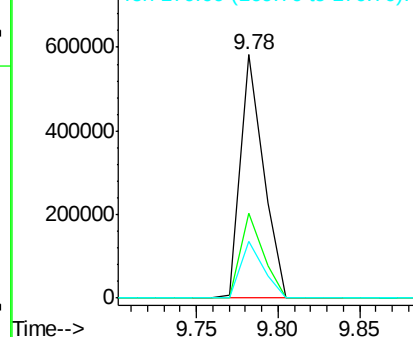


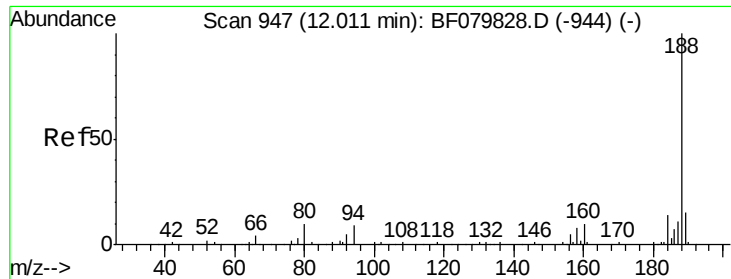

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.02 min Scan# 948
Delta R.T. 0.02 min
Lab File: BF079856.D
Acq: 10 Jun 2015 10:59




Instrument :
BNA_F
ClientSampled :
PB83906BL


Tgt Ion:188 Resp: 188266
Ion Ratio Lower Upper
188 100
94 10.3 7.4 11.0
80 12.1 8.0 12.0#

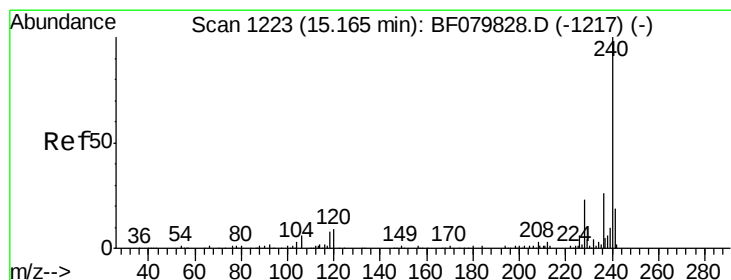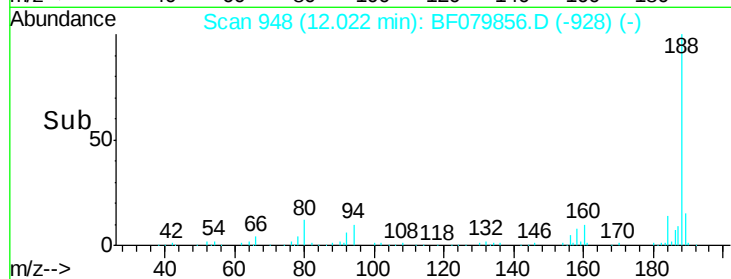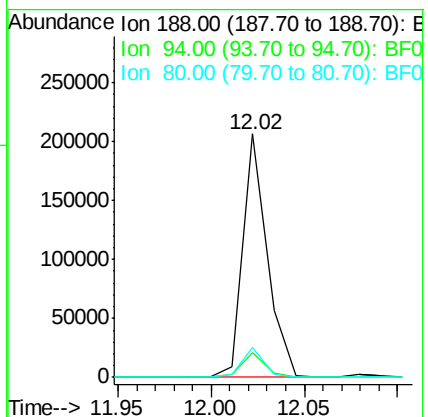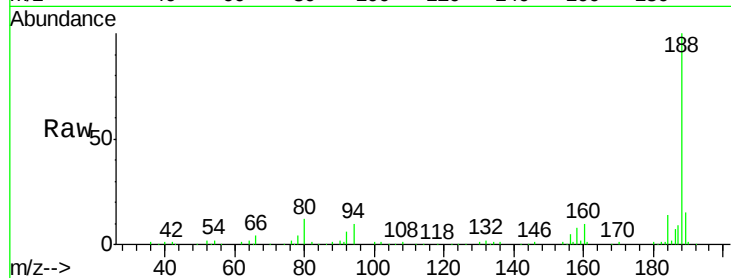

#75
Chrysene-d12
Concen: 20.00 ng m
RT: 15.26 min Scan# 1231
Delta R.T. 0.18 min
Lab File: BF079856.D
Acq: 10 Jun 2015 10:59

Tgt Ion:240 Resp: 180926
Ion Ratio Lower Upper
240 100
120 9.1 6.6 9.8
236 24.8 20.2 30.4

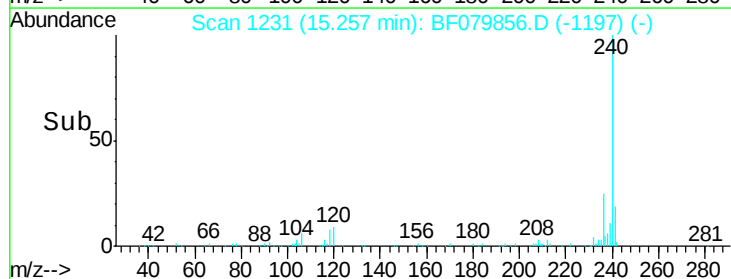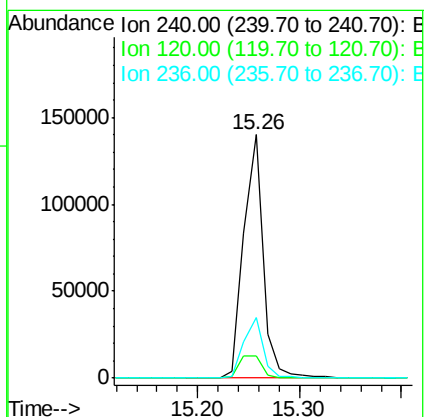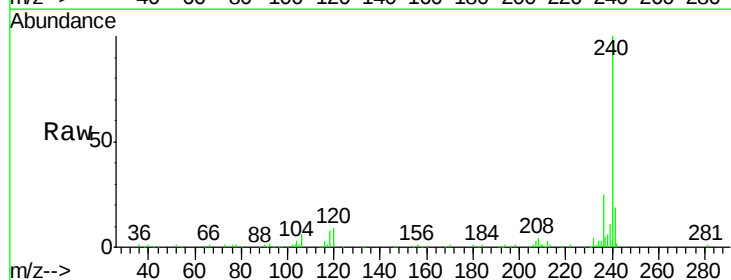

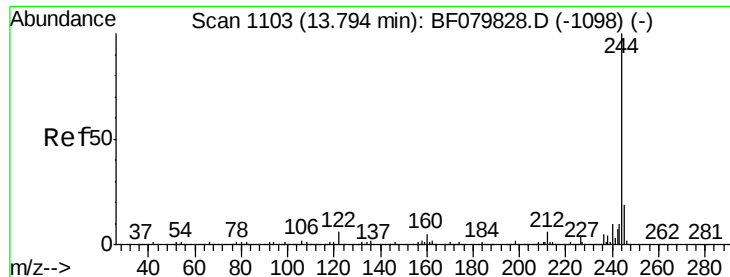

#78

Terphenyl-d14

Concen: 88.09 ng

RT: 13.85 min Scan# 1108

Delta R.T. 0.11 min

Lab File: BF079856.D

Acq: 10 Jun 2015 10:59

Instrument :

BNA_F

ClientSampleId :

PB83906BL


Tgt Ion:244 Resp: 706942

Ion Ratio Lower Upper

244 100

212 6.4 5.6 8.4


122 7.3 8.2 12.2#

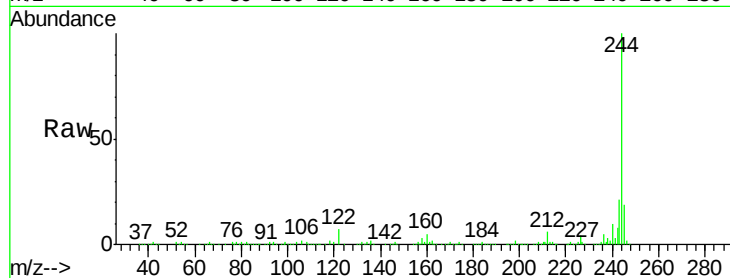



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

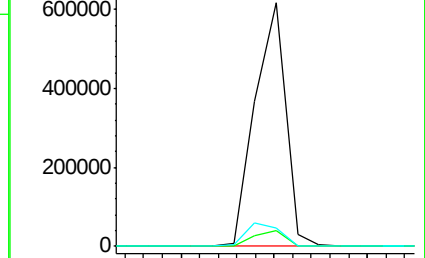

Time-->

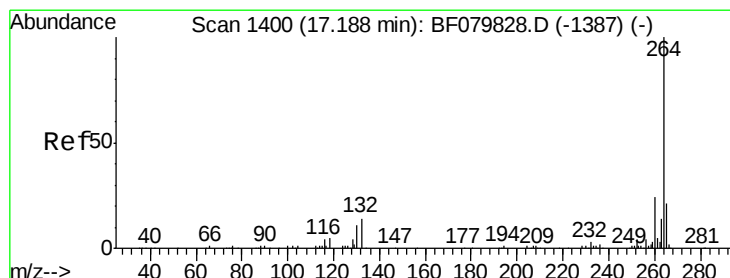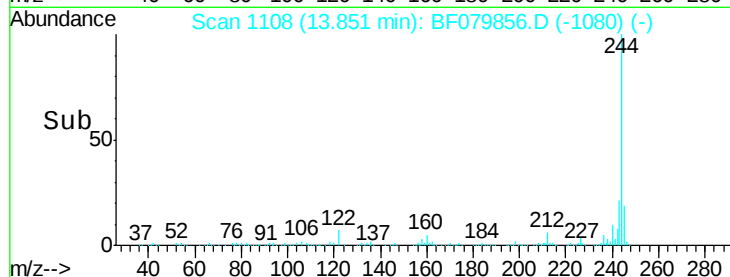

#86

Perylene-d12

Concen: 20.00 ng m

RT: 17.33 min Scan# 1412

Delta R.T. 0.30 min

Lab File: BF079856.D

Acq: 10 Jun 2015 10:59


Tgt Ion:264 Resp: 164675

Ion Ratio Lower Upper

264 100

260 24.0 19.5 29.3


265 22.2 18.0 27.0

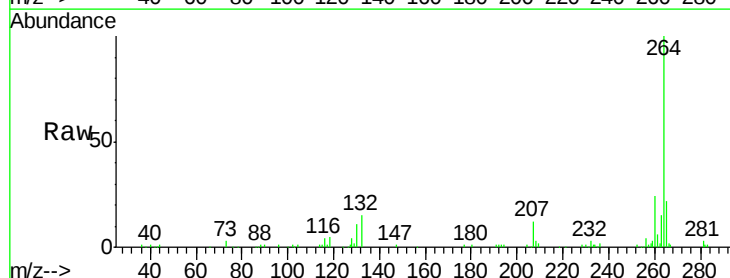

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

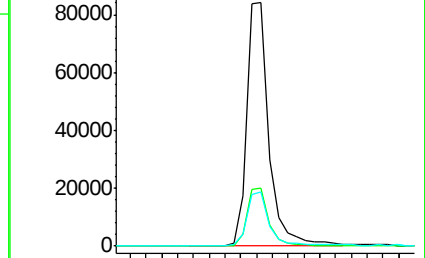

Time-->

