

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
 Data File : BF079864.D
 Acq On : 10 Jun 2015 14:51
 Operator : TP/IZ
 Sample : G2536-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P5-24(FILTERED)

Quant Time: Jun 11 01:56:52 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 00:53:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	48349	20.00	ng	0.00
21) Naphthalene-d8	8.71	136	194888	20.00	ng	0.00
38) Acenaphthene-d10	10.48	164	98030	20.00	ng	-0.01
63) Phenanthrene-d10	12.01	188	202100	20.00	ng	0.01
75) Chrysene-d12	15.06	240	202890	20.00	ng	-0.01
86) Perylene-d12	17.01	264	186563	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.03	112	182369	62.16	ng	0.00
7) Phenol-d6	7.02	99	150831	39.74	ng	0.00
23) Nitrobenzene-d5	7.98	82	265100	78.58	ng	0.00
41) 2,4,6-Tribromophenol	11.28	330	127118	149.84	ng	0.00
44) 2-Fluorobiphenyl	9.78	172	696311	99.90	ng	0.00
78) Terphenyl-d14	13.76	244	870894	96.77	ng	0.02


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079864.D
Acq On : 10 Jun 2015 14:51
Operator : TP/IZ
Sample : G2536-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P5-24(FILTERED)

Quant Time: Jun 11 01:56:52 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

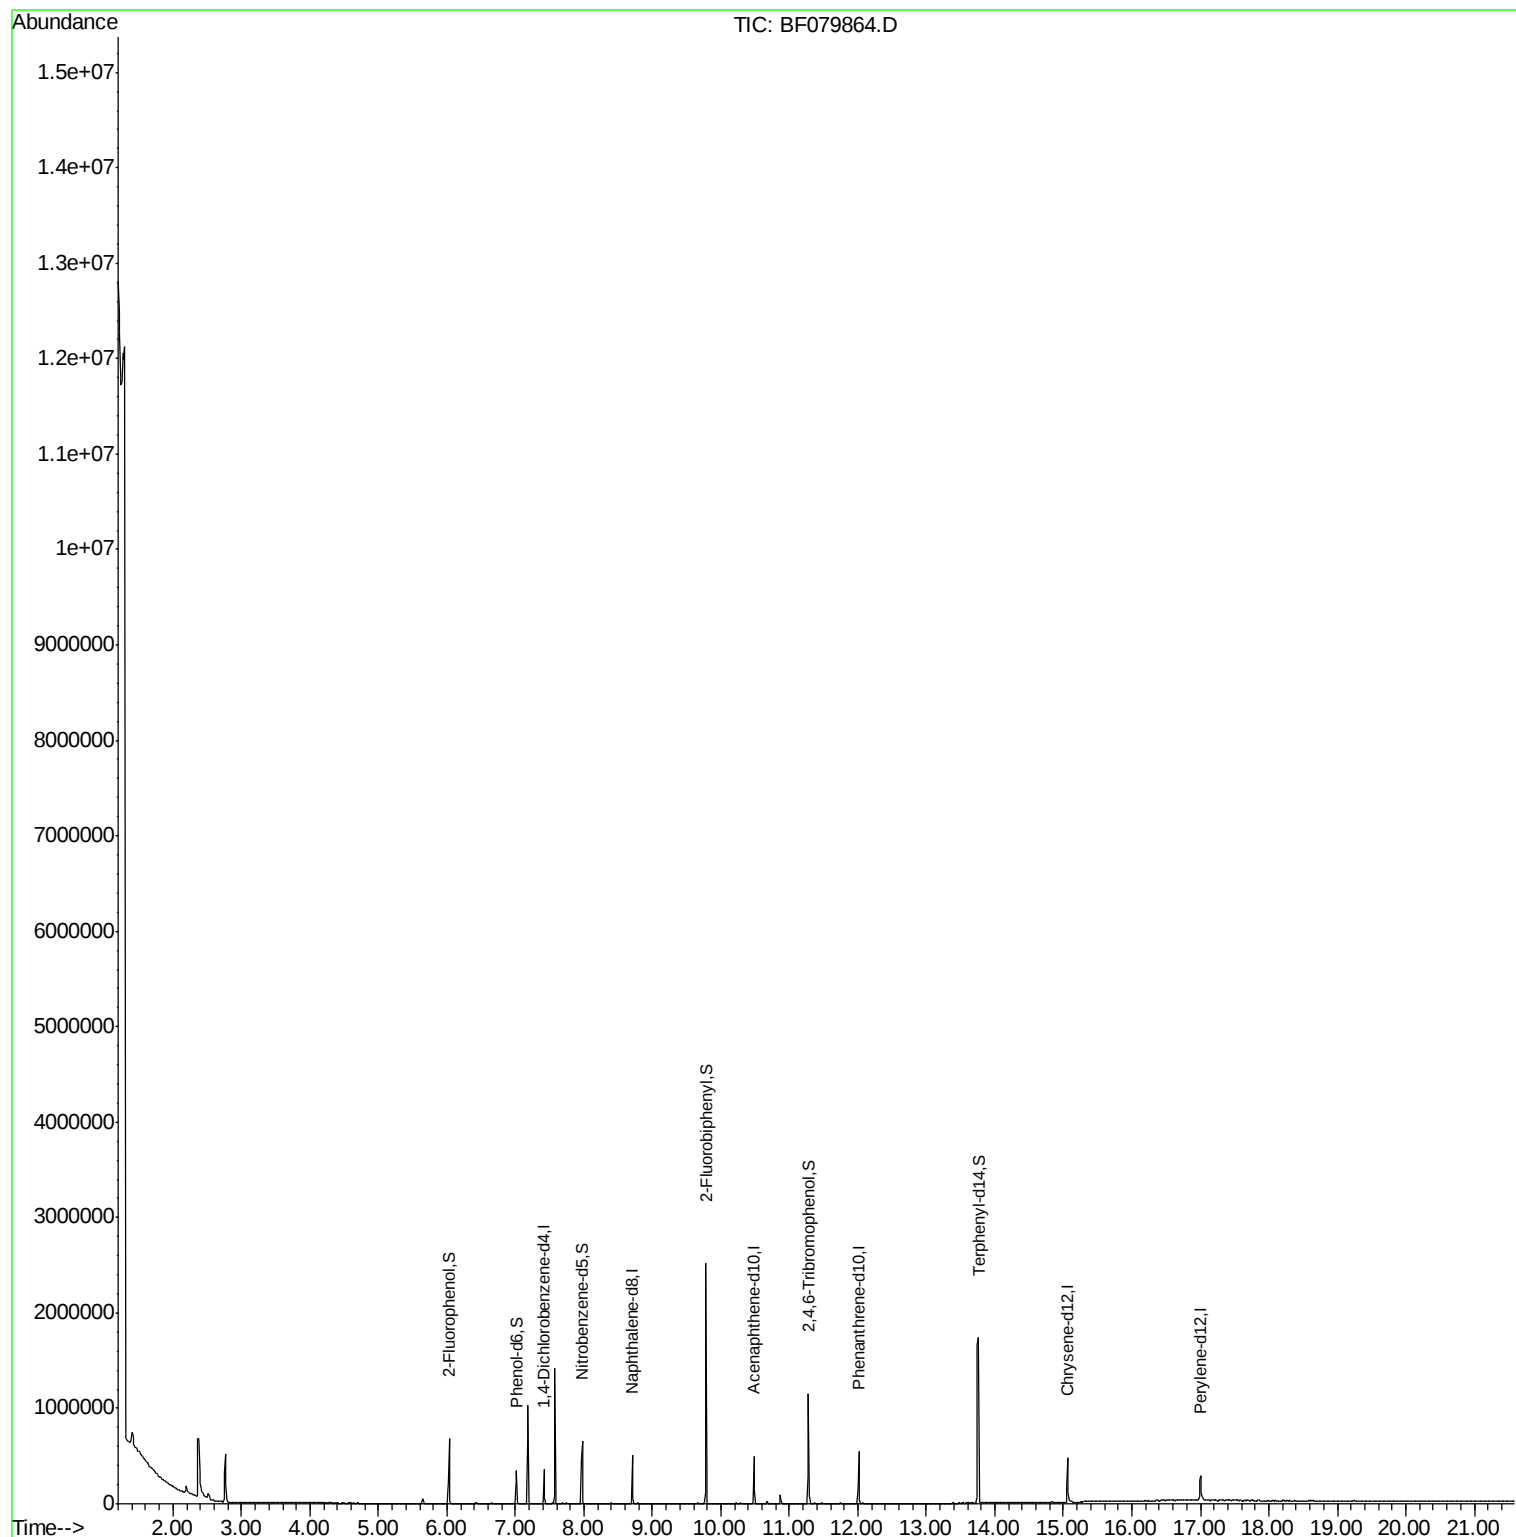




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.42 min Scan# 545
Delta R.T. 0.00 min
Lab File: BF079864.D
Acq: 10 Jun 2015 14:51

Instrument :
BNA_F
ClientSampleId :
P5-24(FILTERED)

Tgt Ion:152 Resp: 48349
Ion Ratio Lower Upper
152 100
150 157.7 131.4 197.2
115 62.3 56.5 84.7

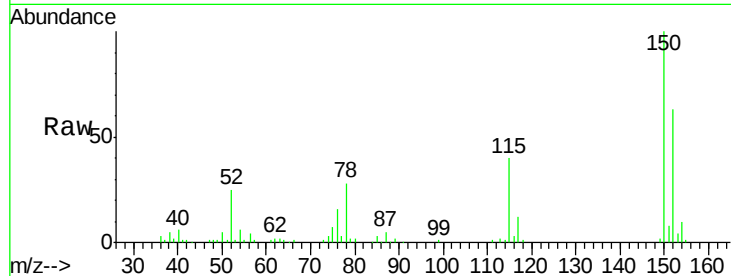


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

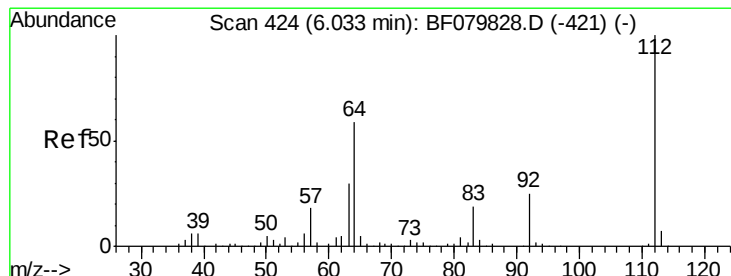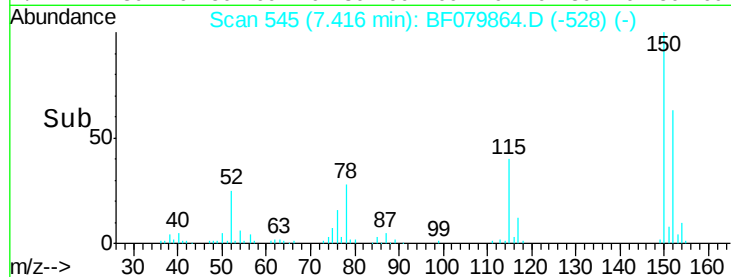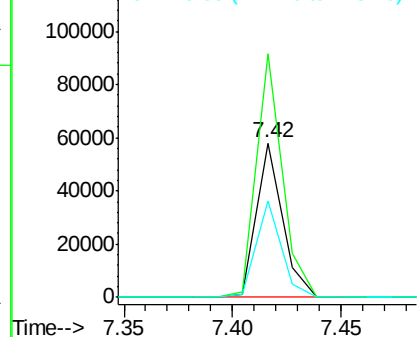



#5


2-Fluorophenol
Concen: 62.16 ng
RT: 6.03 min Scan# 424
Delta R.T. 0.00 min
Lab File: BF079864.D
Acq: 10 Jun 2015 14:51

Tgt Ion:112 Resp: 182369
Ion Ratio Lower Upper
112 100
64 55.0 44.2 66.4
63 27.9 22.8 34.2

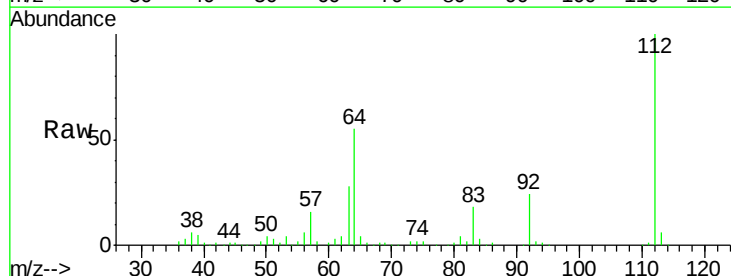

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

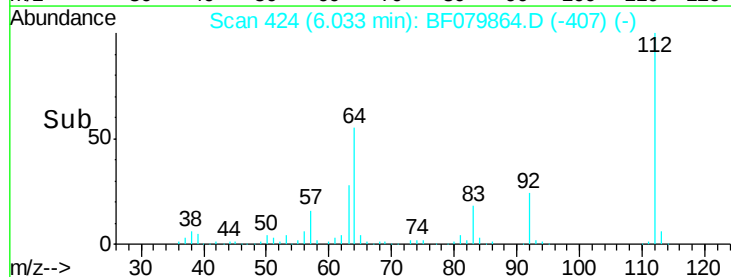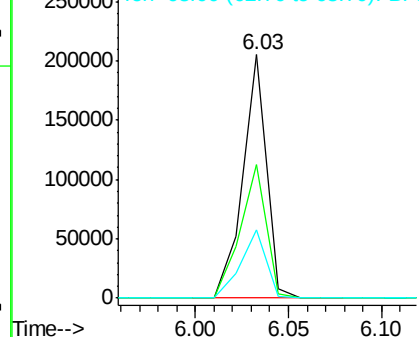

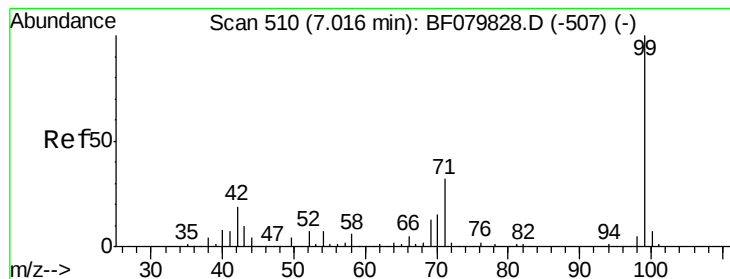

#7

Phenol-d6

Concen: 39.74 ng

RT: 7.02 min Scan# 510

Delta R.T. 0.00 min

Lab File: BF079864.D

Acq: 10 Jun 2015 14:51

Instrument :

BNA_F

ClientSampleId :

P5-24(FILTERED)


Tgt Ion: 99 Resp: 150831

Ion Ratio Lower Upper

99 100

42 15.3 13.7 20.5




71 29.5 25.1 37.7

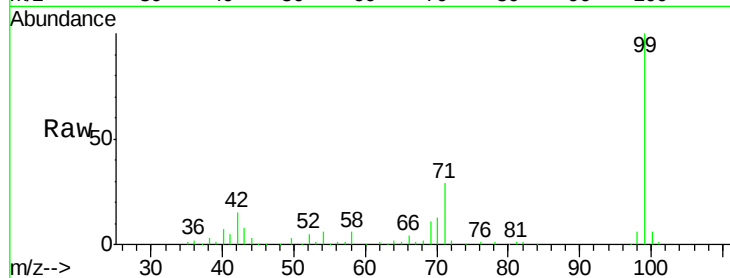

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

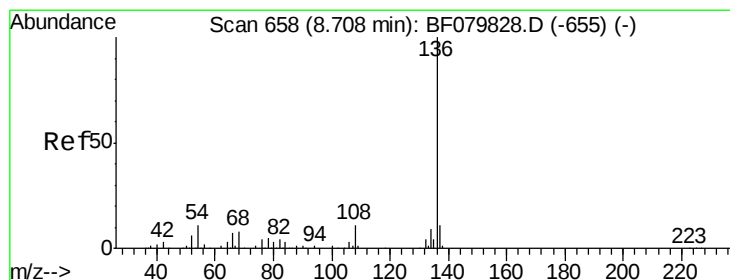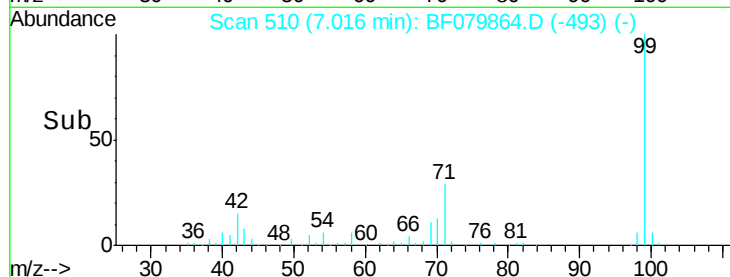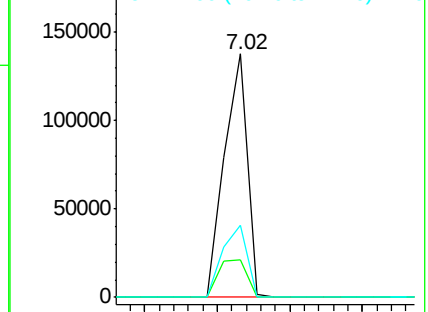

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.71 min Scan# 658

Delta R.T. 0.00 min

Lab File: BF079864.D

Acq: 10 Jun 2015 14:51

Tgt Ion: 136 Resp: 194888


Ion Ratio Lower Upper

136 100

137 11.0 9.3 13.9

54 8.7 8.1 12.1

68 6.5 4.8 7.2


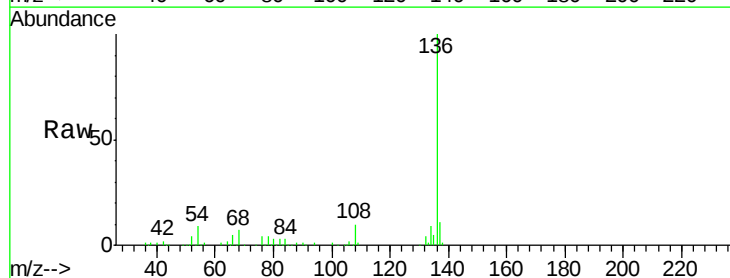


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

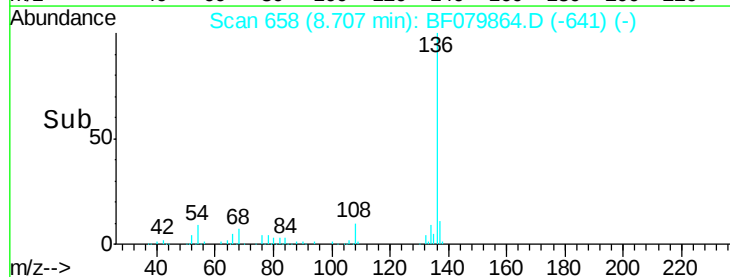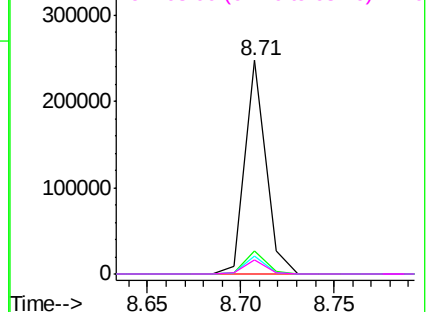



#23

Nitrobenzene-d5

Concen: 78.58 ng

RT: 7.98 min Scan# 594

Delta R.T. 0.00 min

Lab File: BF079864.D

Acq: 10 Jun 2015 14:51

Instrument :

BNA_F

ClientSampleId :

P5-24(FILTERED)


Tgt Ion: 82 Resp: 265100

Ion Ratio Lower Upper

82 100

128 51.8 35.2 52.8




54 44.9 39.2 58.8

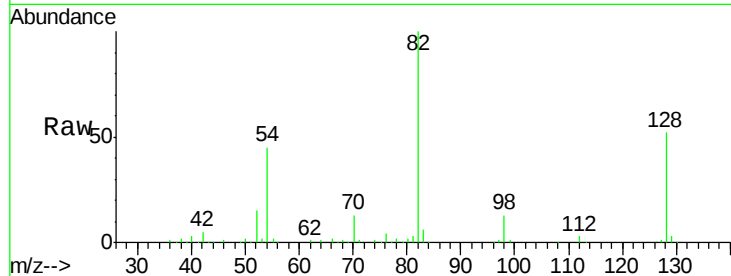

Abundance Ion 82.00 (81.70 to 82.70): BF079828.D (-588) (-)

Ion 128.00 (127.70 to 128.70): BF079828.D (-588) (-)

Ion 54.00 (53.70 to 54.70): BF079828.D (-588) (-)

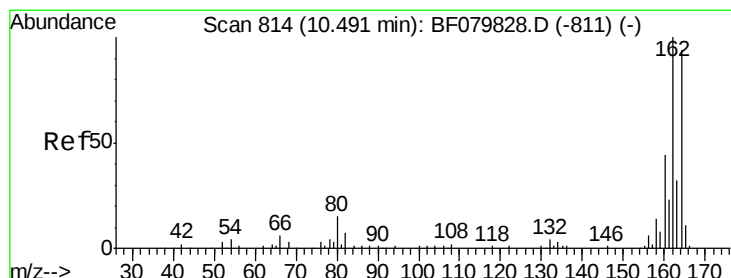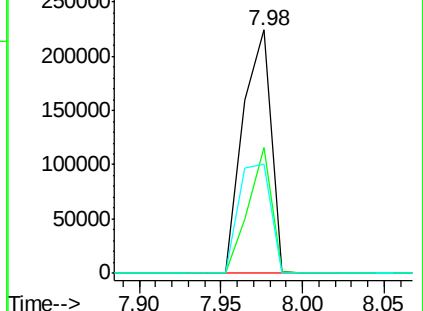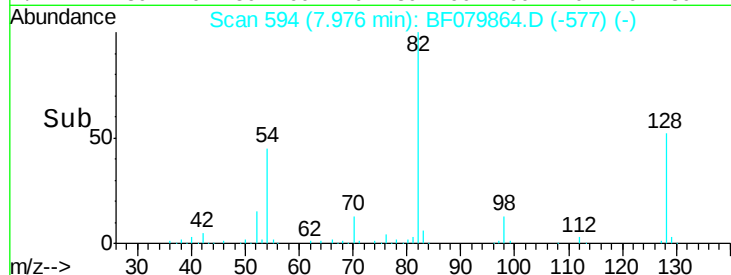

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.48 min Scan# 813

Delta R.T. -0.01 min

Lab File: BF079864.D

Acq: 10 Jun 2015 14:51


Tgt Ion: 164 Resp: 98030

Ion Ratio Lower Upper

164 100

162 101.4 89.8 134.8



160 45.0 39.6 59.4

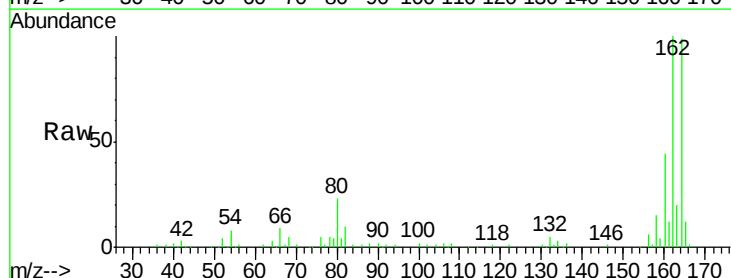


Abundance Ion 164.00 (163.70 to 164.70): BF079828.D (-811) (-)

Ion 162.00 (161.70 to 162.70): BF079828.D (-811) (-)

Ion 160.00 (159.70 to 160.70): BF079828.D (-811) (-)



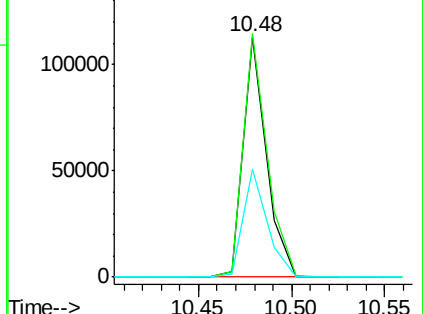
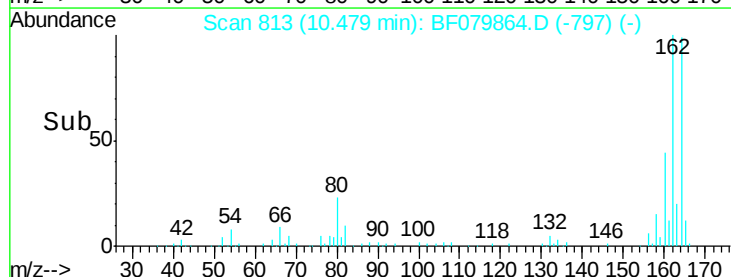


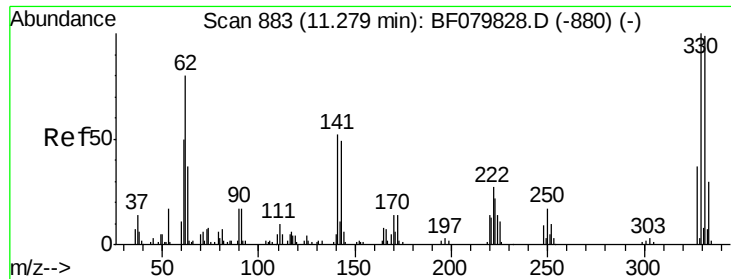

#41
 2,4,6-Tribromophenol
 Concen: 149.84 ng
 RT: 11.28 min Scan# 883
 Delta R.T. 0.00 min
 Lab File: BF079864.D
 Acq: 10 Jun 2015 14:51




Instrument :
 BNA_F
 ClientSampleId :
 P5-24(FILTERED)


Tgt Ion	Ratio	Lower	Upper
330	100		
332	93.3	76.8	115.2
141	35.6	29.1	43.7

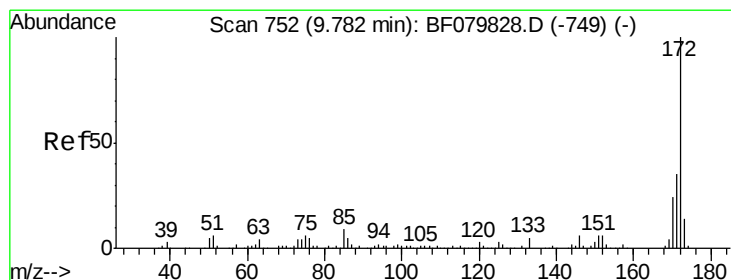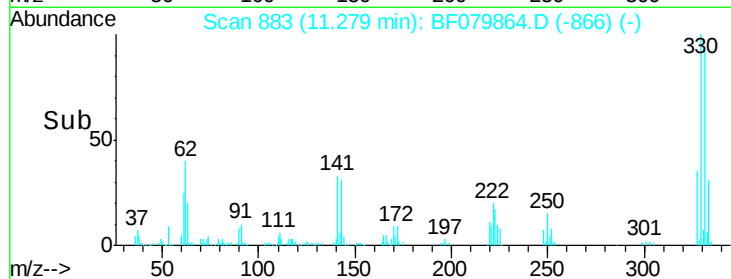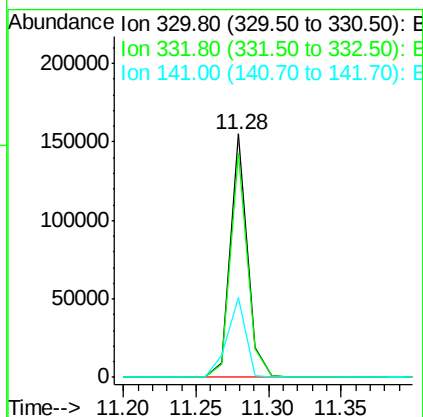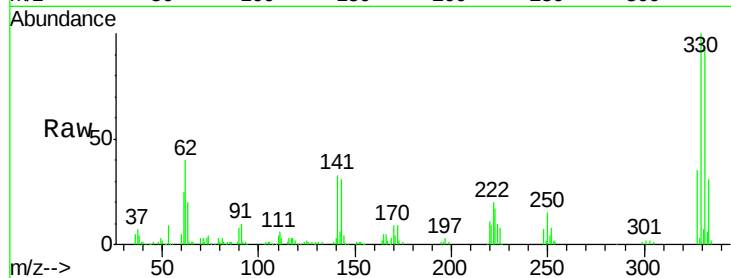

#44
 2-Fluorobiphenyl
 Concen: 99.90 ng
 RT: 9.78 min Scan# 752
 Delta R.T. 0.00 min
 Lab File: BF079864.D
 Acq: 10 Jun 2015 14:51

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.5	42.7
170	24.3	18.8	28.2

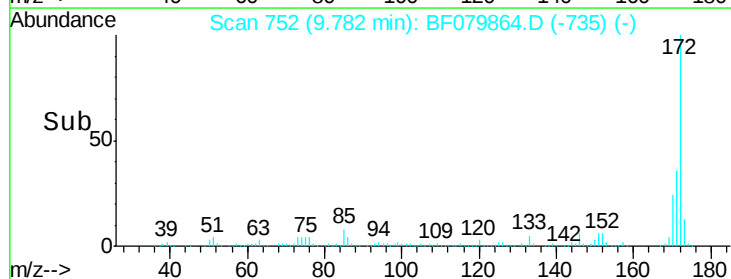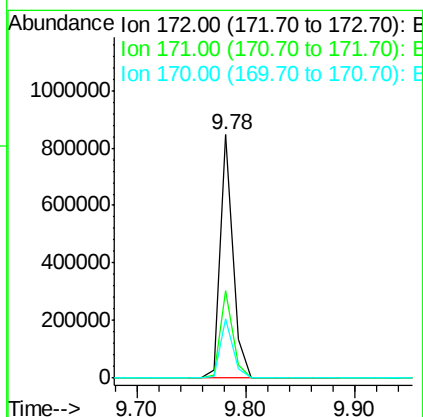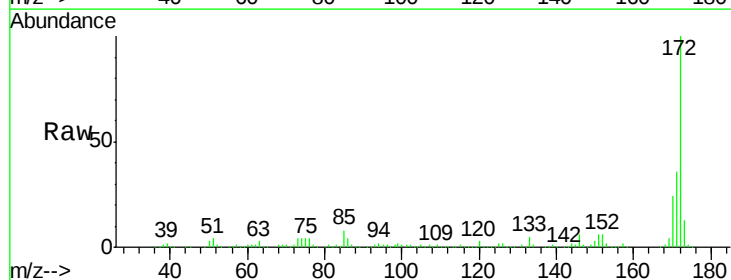


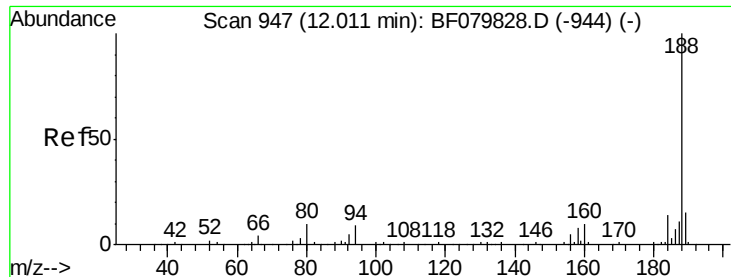




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.01 min Scan# 947
Delta R.T. 0.01 min
Lab File: BF079864.D
Acq: 10 Jun 2015 14:51

Instrument :
BNA_F
ClientSampleId :
P5-24(FILTERED)

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.2	7.4	11.0
80	8.8	8.0	12.0

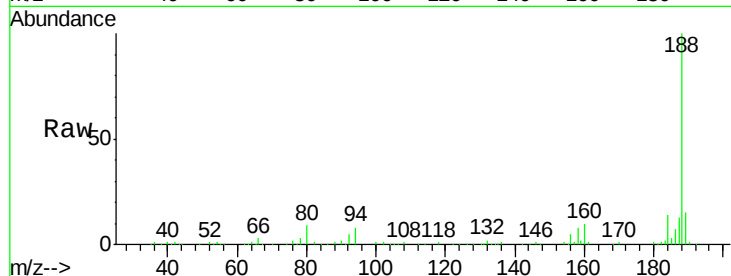


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

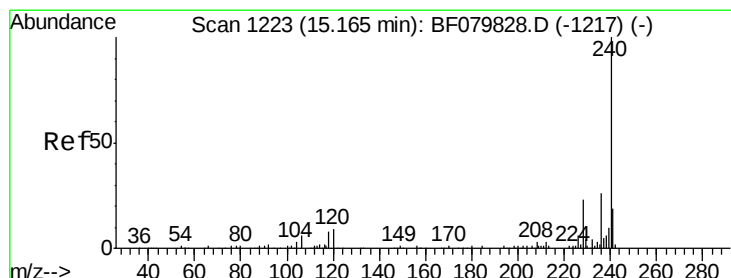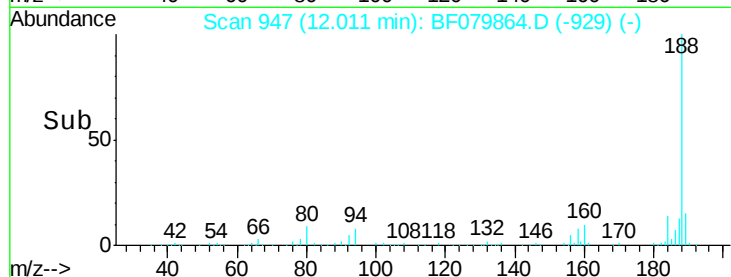
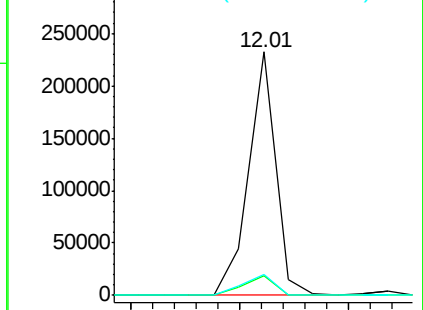



#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.06 min Scan# 1214
Delta R.T. -0.01 min
Lab File: BF079864.D
Acq: 10 Jun 2015 14:51

Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.8	6.6	9.8
236	26.1	20.2	30.4

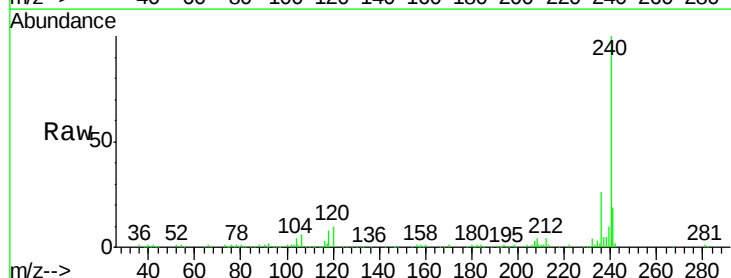

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

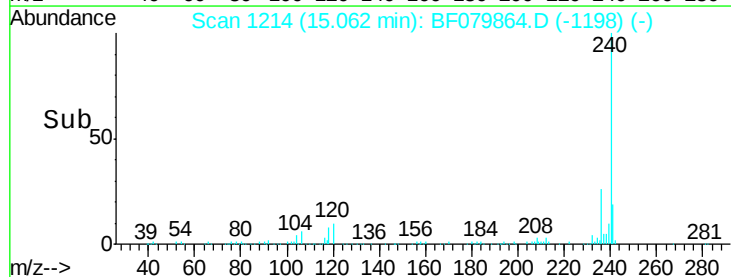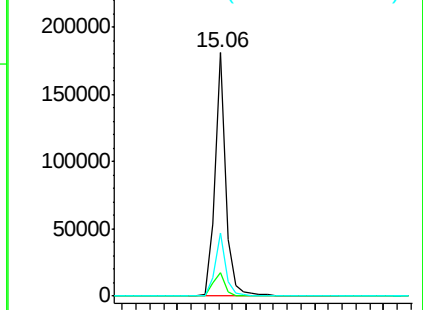

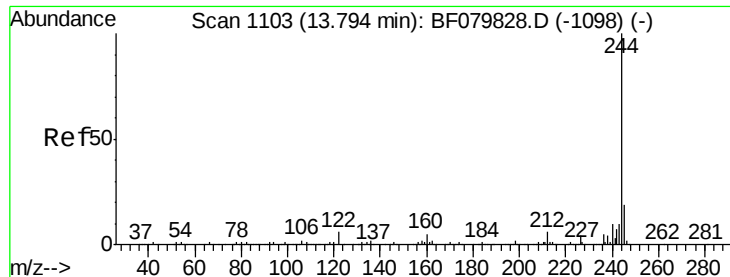

#78

Terphenyl-d14

Concen: 96.77 ng

RT: 13.76 min Scan# 1100

Delta R.T. 0.02 min

Lab File: BF079864.D

Acq: 10 Jun 2015 14:51

Instrument :

BNA_F

ClientSampleId :

P5-24(FILTERED)

Tgt Ion:244 Resp: 870894

Ion Ratio Lower Upper

244 100

212 6.4


5.6

8.4

122 6.7

8.2




12.2#

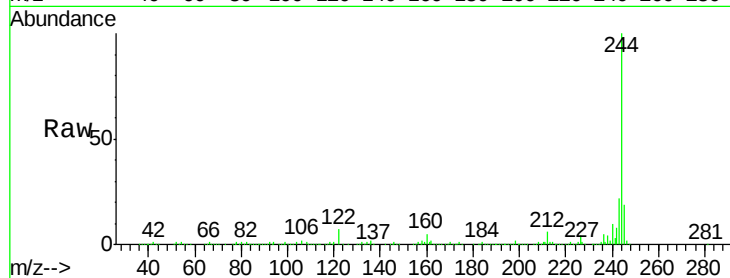

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

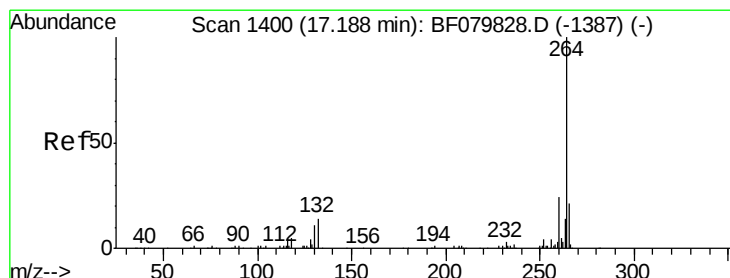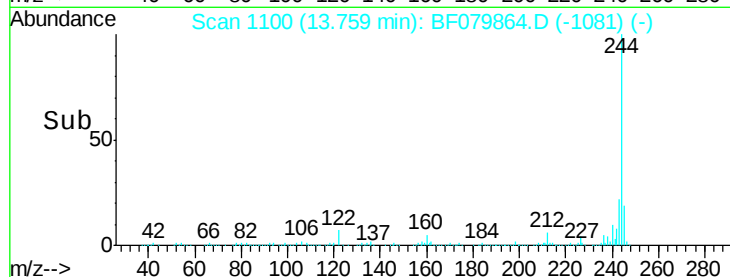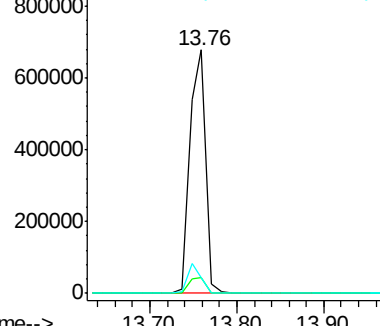

#86

Perylene-d12

Concen: 20.00 ng

RT: 17.01 min Scan# 1384

Delta R.T. -0.02 min

Lab File: BF079864.D

Acq: 10 Jun 2015 14:51

Tgt Ion:264 Resp: 186563

Ion Ratio Lower Upper

264 100

260 22.5


19.5

29.3

265 20.7

18.0

27.0

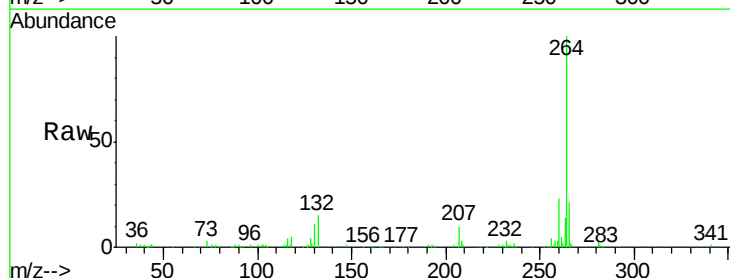

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

