

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
 Data File : BF079866.D
 Acq On : 10 Jun 2015 15:49
 Operator : TP/IZ
 Sample : G2536-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P5-19(FILTERED)

Quant Time: Jun 11 02:02:31 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 00:53:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	49615	20.00	ng	0.00
21) Naphthalene-d8	8.71	136	199395	20.00	ng	0.00
38) Acenaphthene-d10	10.48	164	99955	20.00	ng	-0.01
63) Phenanthrene-d10	11.99	188	207489	20.00	ng	-0.01
75) Chrysene-d12	14.96	240	202892	20.00	ng	-0.11
86) Perylene-d12	16.89	264	183570	20.00	ng	-0.14
System Monitoring Compounds						
5) 2-Fluorophenol	6.03	112	183939	61.10	ng	0.00
7) Phenol-d6	7.02	99	139510	35.81	ng	0.00
23) Nitrobenzene-d5	7.98	82	273880	79.35	ng	0.00
41) 2,4,6-Tribromophenol	11.28	330	114724	132.62	ng	0.00
44) 2-Fluorobiphenyl	9.78	172	690832	97.21	ng	0.00
78) Terphenyl-d14	13.68	244	789772	87.75	ng	-0.06


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF061015\
Data File : BF079866.D
Acq On : 10 Jun 2015 15:49
Operator : TP/IZ
Sample : G2536-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P5-19(FILTERED)

Quant Time: Jun 11 02:02:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 11 00:53:15 2015
Response via : Initial Calibration

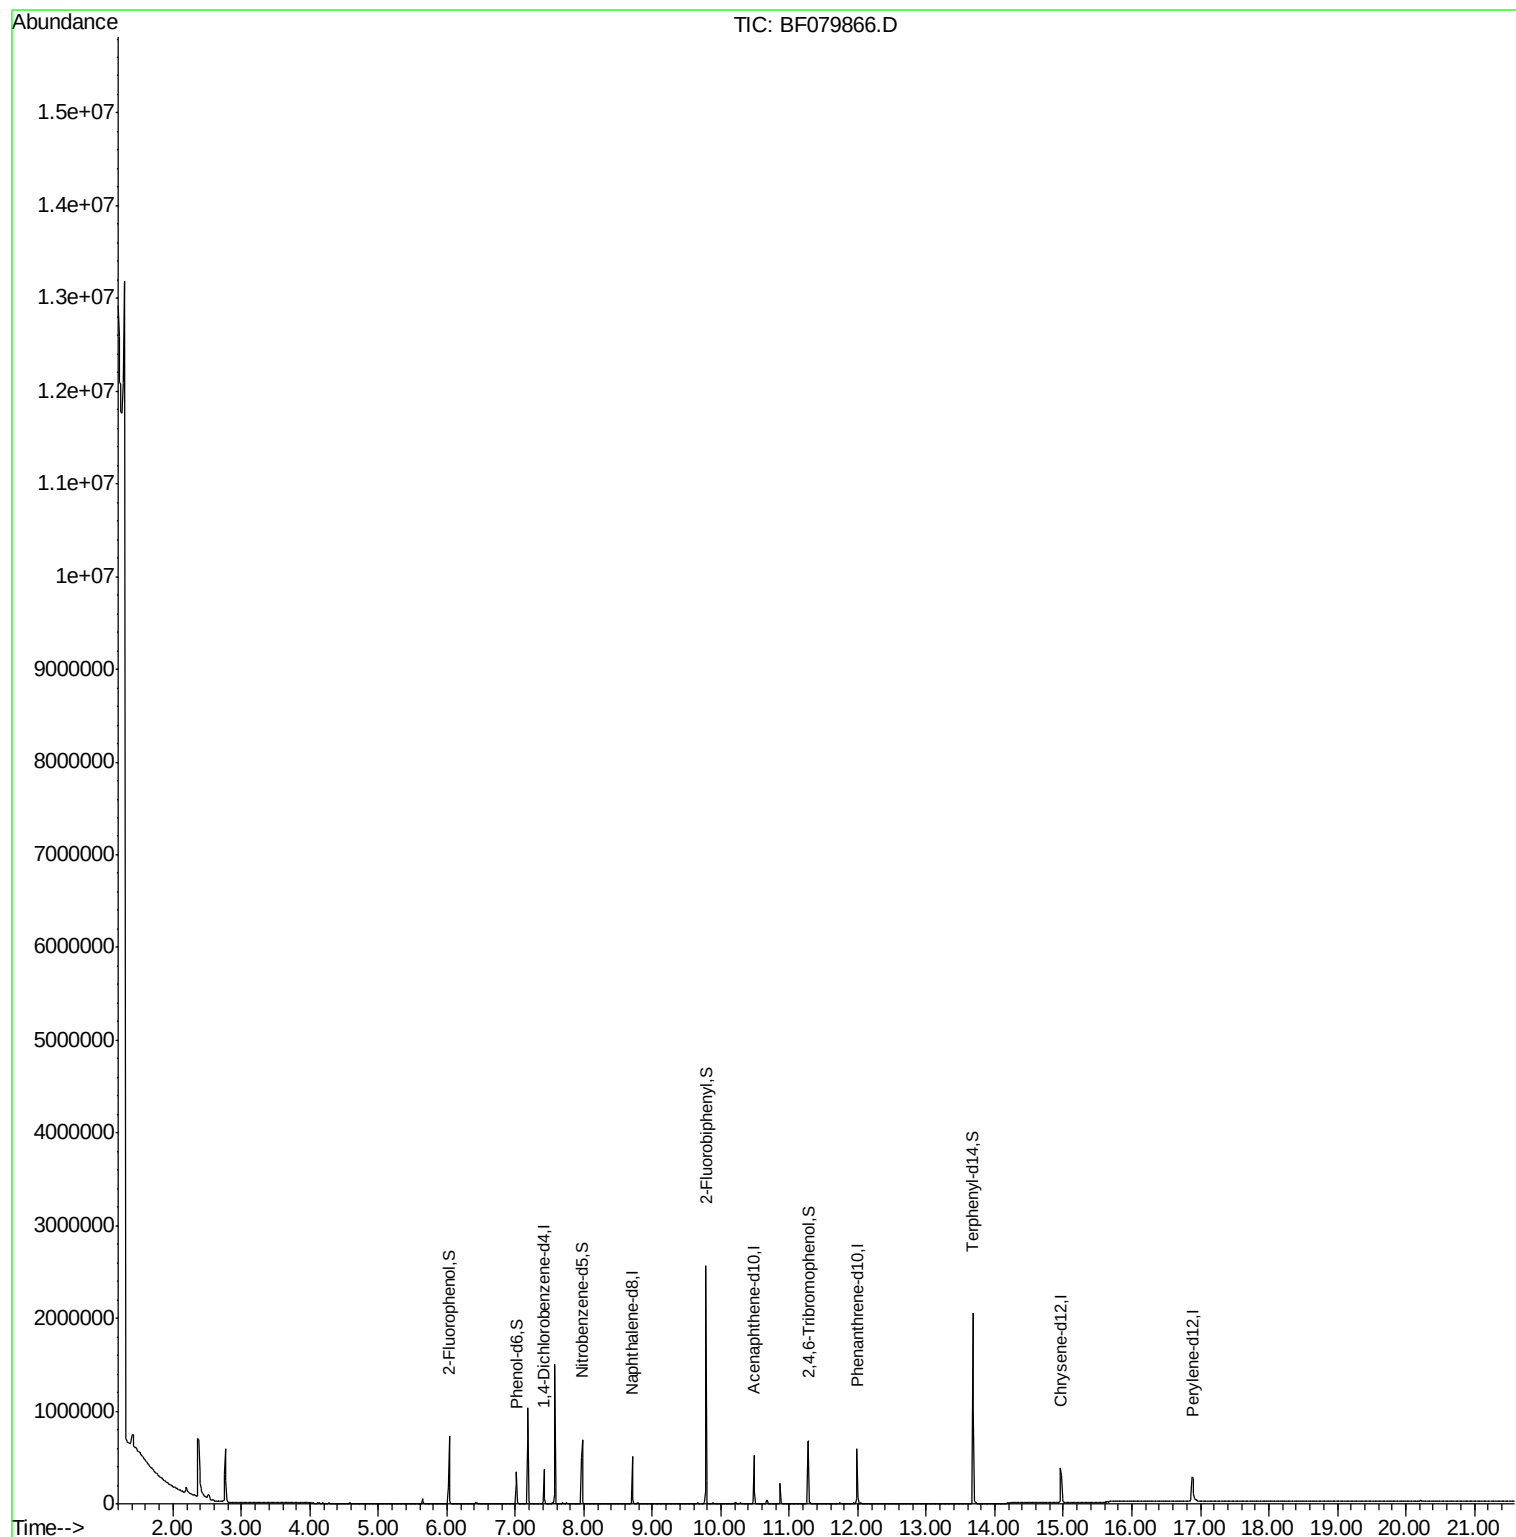




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.42 min Scan# 545
Delta R.T. 0.00 min
Lab File: BF079866.D
Acq: 10 Jun 2015 15:49

Instrument :
BNA_F
ClientSampleId :
P5-19(FILTERED)

Tgt Ion:152 Resp: 49615
Ion Ratio Lower Upper
152 100
150 159.8 131.4 197.2
115 61.1 56.5 84.7

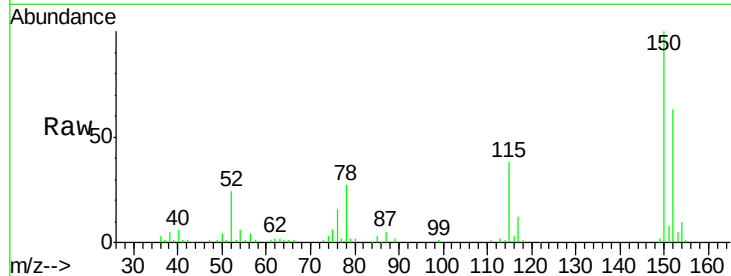


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

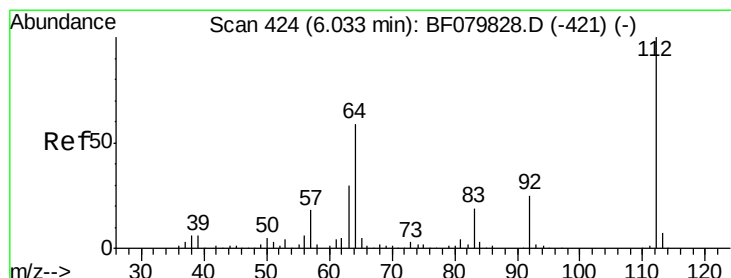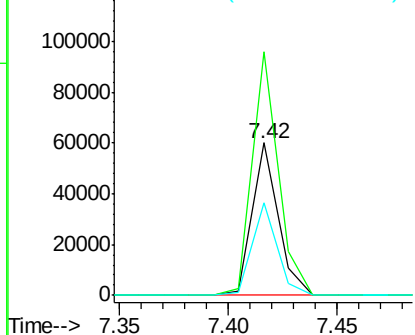



#5


2-Fluorophenol
Concen: 61.10 ng
RT: 6.03 min Scan# 424
Delta R.T. 0.00 min
Lab File: BF079866.D
Acq: 10 Jun 2015 15:49

Tgt Ion:112 Resp: 183939
Ion Ratio Lower Upper
112 100
64 57.0 44.2 66.4
63 29.1 22.8 34.2

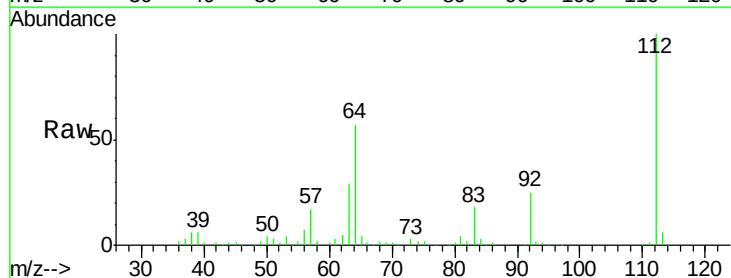

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

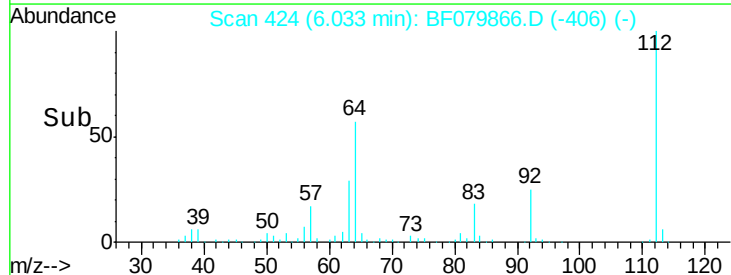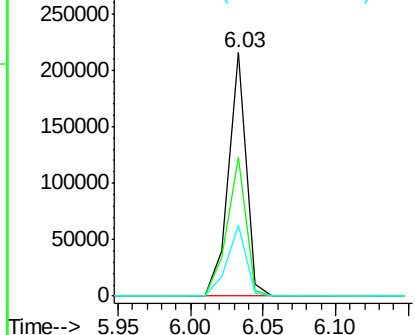

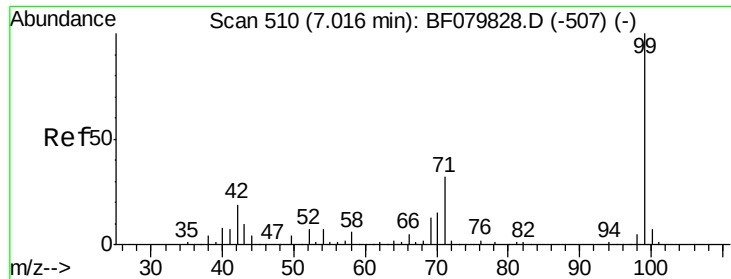

#7

Phenol-d6

Concen: 35.81 ng

RT: 7.02 min Scan# 510

Delta R.T. 0.00 min

Lab File: BF079866.D

Acq: 10 Jun 2015 15:49

Instrument :

BNA_F

ClientSampleId :

P5-19(FILTERED)


Tgt Ion: 99 Resp: 139510

Ion Ratio Lower Upper

99 100

42 15.2 13.7 20.5




71 29.2 25.1 37.7

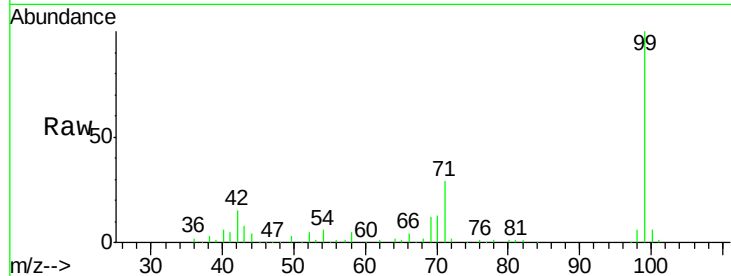

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

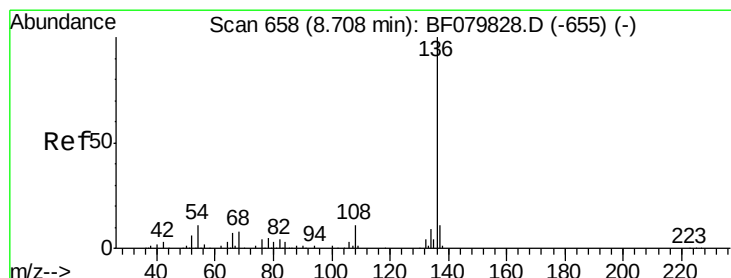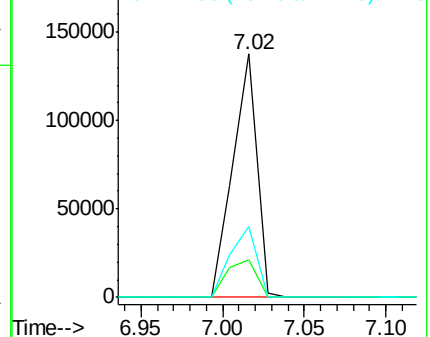

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.71 min Scan# 658

Delta R.T. 0.00 min

Lab File: BF079866.D

Acq: 10 Jun 2015 15:49

Tgt Ion: 136 Resp: 199395


Ion Ratio Lower Upper

136 100

137 10.7 9.3 13.9

54 8.4 8.1 12.1

68 6.5 4.8 7.2


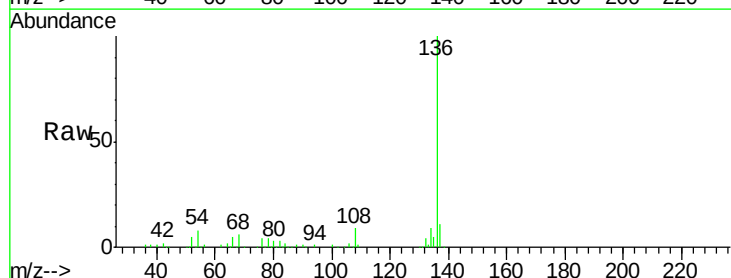



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

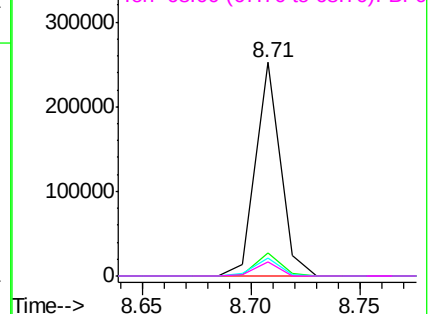



#23

Nitrobenzene-d5

Concen: 79.35 ng

RT: 7.98 min Scan# 594

Delta R.T. 0.00 min

Lab File: BF079866.D

Acq: 10 Jun 2015 15:49

Instrument :

BNA_F

ClientSampleId :

P5-19(FILTERED)


Tgt Ion: 82 Resp: 273880

Ion Ratio Lower Upper

82 100

128 52.1 35.2 52.8




54 46.1 39.2 58.8

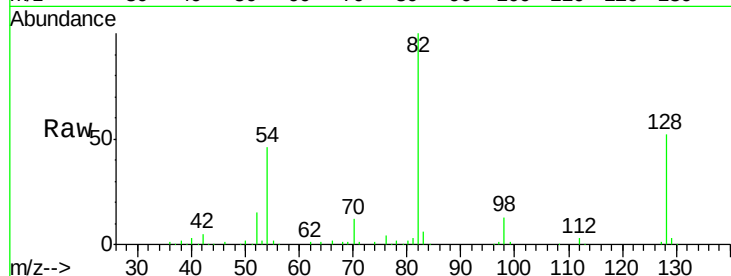

Abundance Ion 82.00 (81.70 to 82.70): BF079828.D (-588) (-)

Ion 128.00 (127.70 to 128.70): BF079828.D (-588) (-)

Ion 54.00 (53.70 to 54.70): BF079828.D (-588) (-)

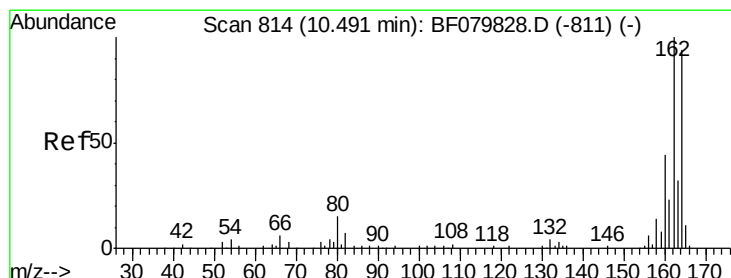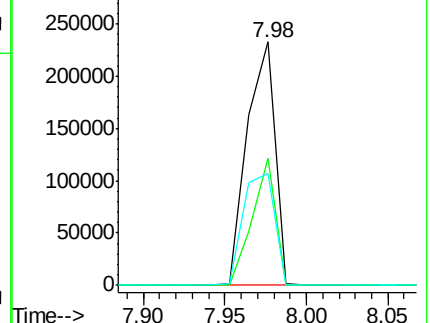

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.48 min Scan# 813

Delta R.T. -0.01 min

Lab File: BF079866.D

Acq: 10 Jun 2015 15:49


Tgt Ion: 164 Resp: 99955

Ion Ratio Lower Upper

164 100

162 102.0 89.8 134.8



160 44.7 39.6 59.4

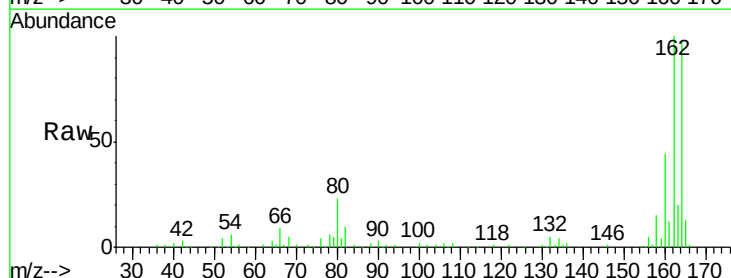


Abundance Ion 164.00 (163.70 to 164.70): BF079828.D (-811) (-)

Ion 162.00 (161.70 to 162.70): BF079828.D (-811) (-)

Ion 160.00 (159.70 to 160.70): BF079828.D (-811) (-)

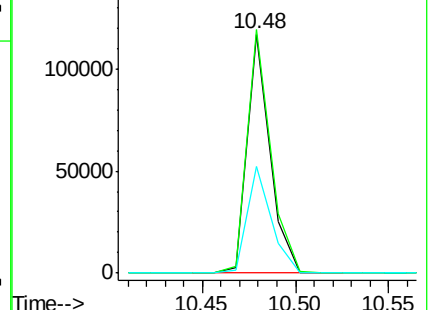


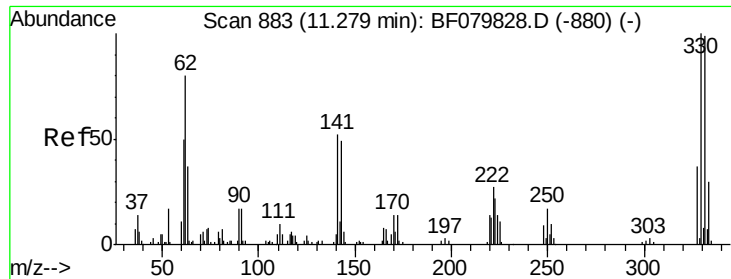




#41
 2,4,6-Tribromophenol
 Concen: 132.62 ng
 RT: 11.28 min Scan# 883
 Delta R.T. 0.00 min
 Lab File: BF079866.D
 Acq: 10 Jun 2015 15:49

Instrument :
 BNA_F
 ClientSampleId :
 P5-19(FILTERED)

Tgt Ion:330 Resp: 114724
 Ion Ratio Lower Upper
 330 100
 332 98.0 76.8 115.2
 141 34.4 29.1 43.7

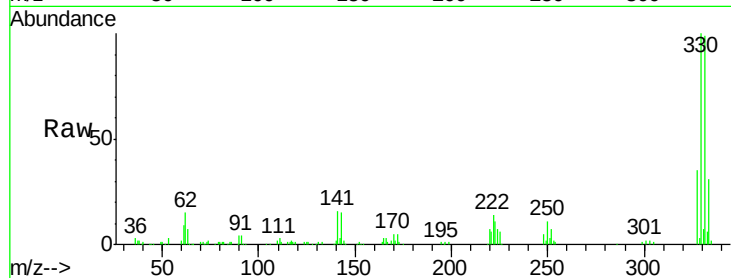


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

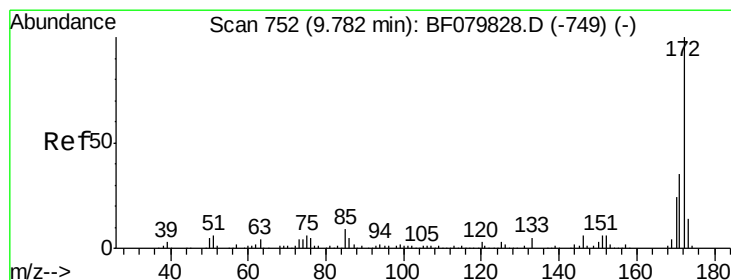
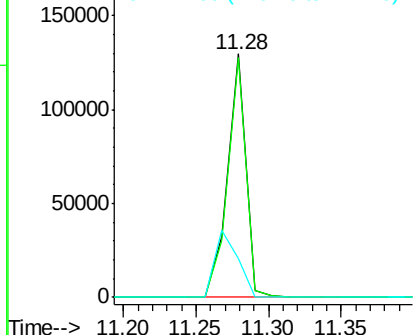



#44
 2-Fluorobiphenyl
 Concen: 97.21 ng
 RT: 9.78 min Scan# 752
 Delta R.T. 0.00 min
 Lab File: BF079866.D
 Acq: 10 Jun 2015 15:49

Tgt Ion:172 Resp: 690832
 Ion Ratio Lower Upper
 172 100
 171 36.3 28.5 42.7
 170 24.7 18.8 28.2

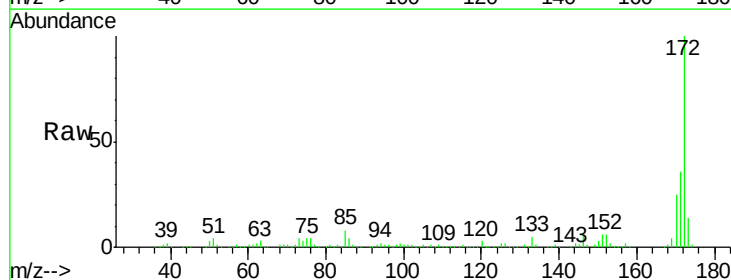

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




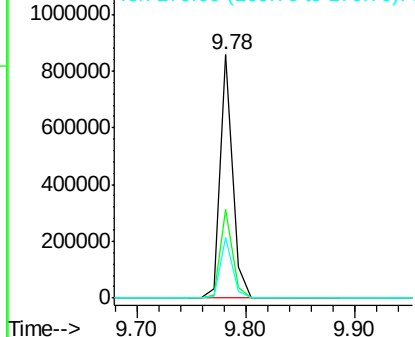




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.99 min Scan# 945
Delta R.T. -0.01 min
Lab File: BF079866.D
Acq: 10 Jun 2015 15:49




Instrument :
BNA_F
ClientSampleId :
P5-19(FILTERED)


Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.9	7.4	11.0
80	9.9	8.0	12.0

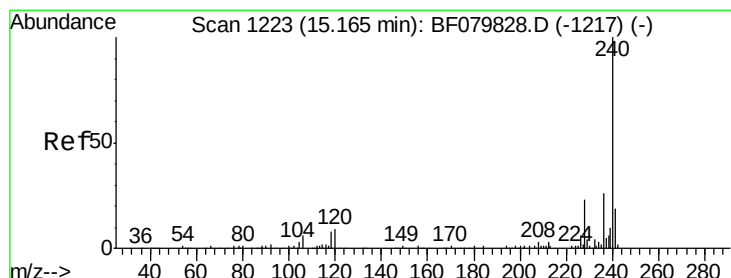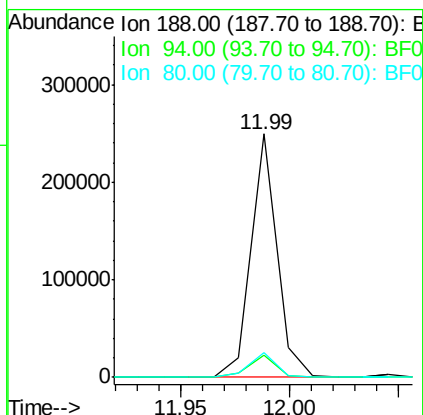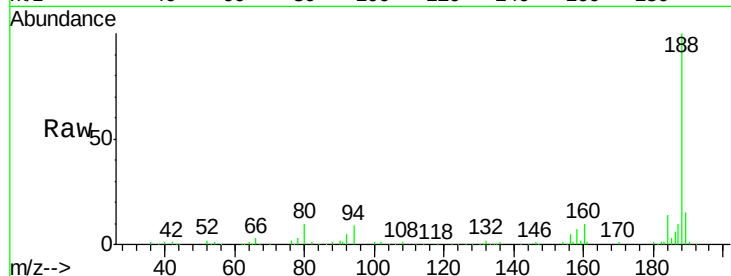

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.96 min Scan# 1205
Delta R.T. -0.11 min
Lab File: BF079866.D
Acq: 10 Jun 2015 15:49

Tgt Ion	Ratio	Lower	Upper
240	100		
120	13.3	6.6	9.8#
236	25.8	20.2	30.4

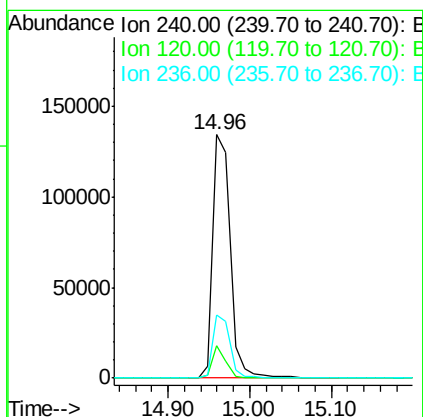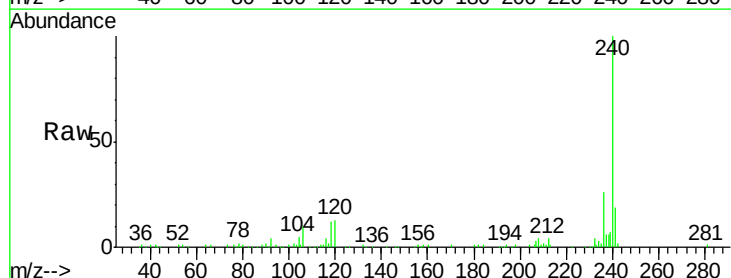

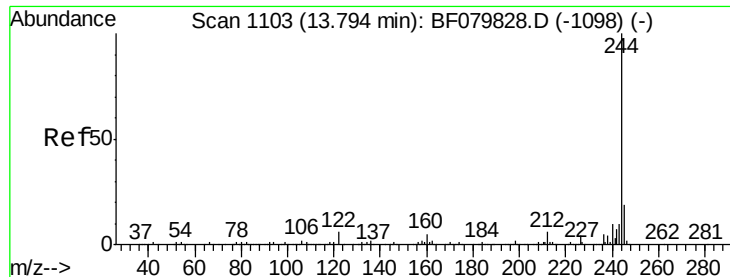

#78

Terphenyl-d14

Concen: 87.75 ng

RT: 13.68 min Scan# 1093

Delta R.T. -0.06 min

Lab File: BF079866.D

Acq: 10 Jun 2015 15:49

Instrument :

BNA_F

ClientSampleId :

P5-19(FILTERED)


Tgt Ion:244 Resp: 789772

Ion Ratio Lower Upper

244 100

212 7.4 5.6 8.4




122 14.5 8.2 12.2#

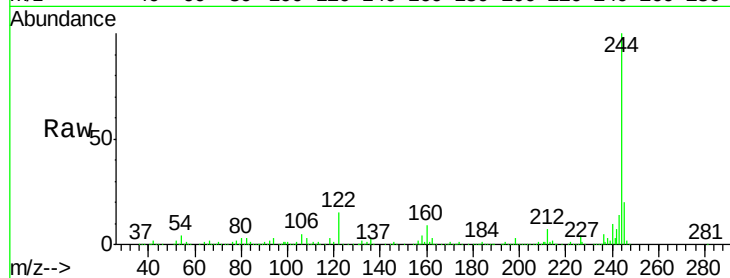

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

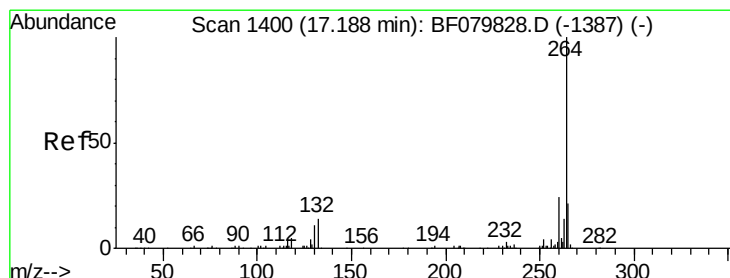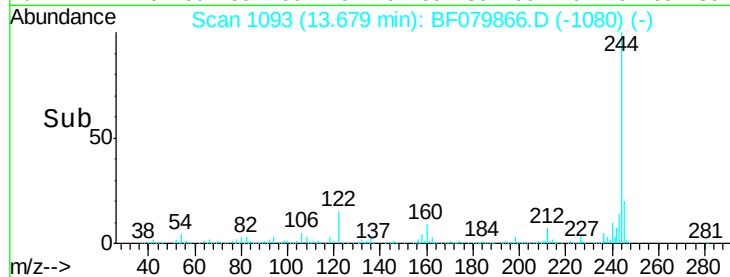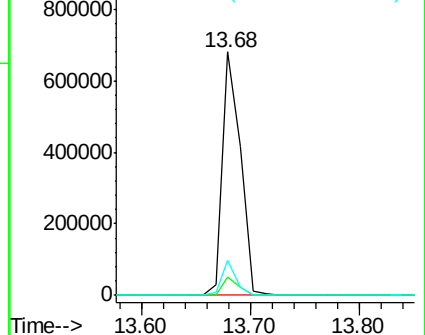

#86

Perylene-d12

Concen: 20.00 ng

RT: 16.89 min Scan# 1374

Delta R.T. -0.14 min

Lab File: BF079866.D

Acq: 10 Jun 2015 15:49


Tgt Ion:264 Resp: 183570

Ion Ratio Lower Upper

264 100

260 23.3 19.5 29.3

265 21.3 18.0 27.0

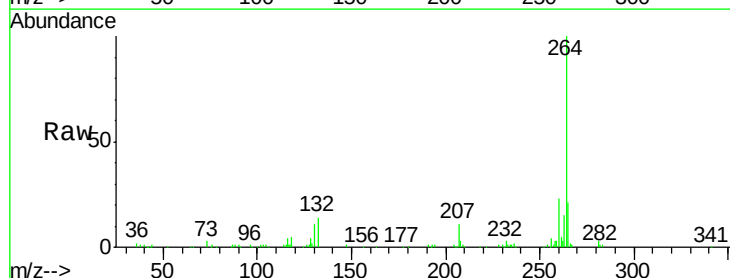

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

